

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031566.D
 Acq On : 27 Apr 2019 05:19
 Operator : JC/SP
 Sample : K2592-19 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X86

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	33	rBV2	17887	14821	0.12%	0.037%
2	1.396	88	95	106	rBV	511491	553445	4.39%	1.380%
3	1.678	175	183	197	rBV	403637	511059	4.06%	1.275%
4	1.881	240	246	257	rVB	62774	89120	0.71%	0.222%
5	2.270	356	367	380	rVB	861014	1307907	10.38%	3.262%
6	2.566	456	459	461	rBV2	1548	844	0.01%	0.002%
7	2.698	493	500	510	rVB9	4074	8443	0.07%	0.021%
8	2.955	576	580	583	rVB2	1246	859	0.01%	0.002%
9	2.981	583	588	593	rBV5	1962	2202	0.02%	0.005%
10	3.045	604	608	613	rVV5	1090	1144	0.01%	0.003%
11	3.100	617	625	630	rBV4	1196	1900	0.02%	0.005%
12	3.254	671	673	679	rVB5	1384	1224	0.01%	0.003%
13	3.350	698	703	709	rBV2	1700	1970	0.02%	0.005%
14	3.389	709	715	720	rBV4	2255	2489	0.02%	0.006%
15	3.469	735	740	745	rVB4	1246	1334	0.01%	0.003%
16	3.495	745	748	750	rBV3	1715	1171	0.01%	0.003%
17	3.797	838	842	845	rBV	1273	1084	0.01%	0.003%
18	3.823	846	850	853	rVV4	1092	840	0.01%	0.002%
19	3.849	853	858	861	rVV2	1666	1599	0.01%	0.004%
20	3.875	863	866	869	rVB	1589	930	0.01%	0.002%
21	3.894	869	872	874	rBV2	1870	1407	0.01%	0.004%
22	3.971	891	896	899	rBV6	1287	1373	0.01%	0.003%
23	4.003	903	906	910	rVV2	1005	983	0.01%	0.002%
24	4.186	950	963	999	rBV	344892	1113682	8.84%	2.778%
25	4.643	1088	1105	1127	rBV	608653	1439318	11.42%	3.590%
26	4.862	1170	1173	1175	rBV2	1483	1047	0.01%	0.003%
27	4.929	1192	1194	1198	rVB4	1458	827	0.01%	0.002%
28	4.990	1205	1213	1218	rBV9	2654	4362	0.03%	0.011%
29	5.013	1218	1220	1223	rVB3	1894	1060	0.01%	0.003%
30	5.061	1232	1235	1240	rVB4	954	892	0.01%	0.002%
31	5.116	1249	1252	1254	rBV3	1245	856	0.01%	0.002%
32	5.334	1297	1320	1349	rBV2	1243241	3751417	29.78%	9.357%
33	5.656	1417	1420	1424	rBV6	1486	1584	0.01%	0.004%
34	5.717	1436	1439	1441	rBV3	1542	1148	0.01%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031566.D
 Acq On : 27 Apr 2019 05:19
 Operator : JC/SP
 Sample : K2592-19 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X86

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.820	1467	1471	1475	rBV6	1414	1030	0.01%	0.003%
36	5.881	1475	1490	1521	rBV	966517	2013038	15.98%	5.021%
37	6.180	1567	1583	1616	rBV	6349175	12599042	100.00%	31.425%
38	6.325	1617	1628	1651	rVB	840132	1739417	13.81%	4.339%
39	6.633	1719	1724	1726	rBV4	1813	1862	0.01%	0.005%
40	6.675	1734	1737	1742	rVB5	1830	1376	0.01%	0.003%
41	6.723	1747	1752	1754	rBV5	987	977	0.01%	0.002%
42	6.771	1764	1767	1770	rVB3	1485	926	0.01%	0.002%
43	6.810	1775	1779	1781	rBV4	1147	836	0.01%	0.002%
44	6.900	1802	1807	1809	rBV5	874	837	0.01%	0.002%
45	7.058	1850	1856	1861	rVB8	1289	1759	0.01%	0.004%
46	7.093	1861	1867	1872	rBV5	1620	1637	0.01%	0.004%
47	7.141	1880	1882	1887	rVB4	1216	954	0.01%	0.002%
48	7.170	1887	1891	1895	rBV4	2026	1973	0.02%	0.005%
49	7.225	1896	1908	1941	rBV	422393	790167	6.27%	1.971%
50	7.427	1965	1971	1975	rBV7	1655	2516	0.02%	0.006%
51	7.498	1989	1993	1999	rVB5	1203	1106	0.01%	0.003%
52	7.562	1999	2013	2066	rBV	1480160	2830069	22.46%	7.059%
53	7.849	2090	2102	2119	rBV	278246	499551	3.96%	1.246%
54	8.093	2176	2178	2181	rVB2	1891	982	0.01%	0.002%
55	8.148	2192	2195	2199	rBV3	1606	1275	0.01%	0.003%
56	8.225	2205	2219	2234	rBV2	149185	268772	2.13%	0.670%
57	8.312	2235	2246	2297	rVV	1175810	2317546	18.39%	5.781%
58	8.797	2393	2397	2401	rBV6	1278	1497	0.01%	0.004%
59	8.836	2405	2409	2414	rBV6	1079	951	0.01%	0.002%
60	8.996	2455	2459	2465	rVB5	1568	1532	0.01%	0.004%
61	9.087	2473	2487	2526	rBV	1377559	2430167	19.29%	6.061%
62	9.466	2602	2605	2608	rBV4	1564	1093	0.01%	0.003%
63	9.701	2674	2678	2681	rBV3	1663	1407	0.01%	0.004%
64	9.784	2698	2704	2709	rVB6	1379	1695	0.01%	0.004%
65	10.045	2783	2785	2791	rVB3	1055	901	0.01%	0.002%
66	10.074	2791	2794	2797	rVB2	1478	910	0.01%	0.002%
67	10.135	2805	2813	2816	rBV7	1732	1880	0.01%	0.005%
68	10.157	2816	2820	2823	rBV2	1277	1091	0.01%	0.003%
69	10.302	2858	2865	2868	rBV4	1335	1771	0.01%	0.004%
70	10.360	2877	2883	2888	rBV4	1404	1414	0.01%	0.004%
71	10.427	2892	2904	2929	rVV	1053026	1723894	13.68%	4.300%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031566.D
 Acq On : 27 Apr 2019 05:19
 Operator : JC/SP
 Sample : K2592-19 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X86

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.627	2963	2966	2971	rBV4	1210	1314	0.01%	0.003%
73	10.672	2976	2980	2984	rBV4	867	917	0.01%	0.002%
74	10.829	3024	3029	3030	rBV2	1197	972	0.01%	0.002%
75	10.945	3060	3065	3067	rBV4	1109	1098	0.01%	0.003%
76	10.974	3072	3074	3079	rBV2	1185	1021	0.01%	0.003%
77	11.006	3079	3084	3091	rVB4	2350	3140	0.02%	0.008%
78	11.041	3091	3095	3097	rBV2	1704	1432	0.01%	0.004%
79	11.160	3128	3132	3134	rBV3	1264	1087	0.01%	0.003%
80	11.221	3147	3151	3154	rBV4	1763	1471	0.01%	0.004%
81	11.260	3161	3163	3166	rVB4	1648	998	0.01%	0.002%
82	11.340	3186	3188	3193	rVV3	929	825	0.01%	0.002%
83	11.366	3193	3196	3199	rVV2	1340	855	0.01%	0.002%
84	11.482	3219	3232	3258	rBV	1143540	1878971	14.91%	4.687%
85	11.855	3334	3348	3371	rBV	1258031	2103935	16.70%	5.248%
86	12.299	3483	3486	3490	rBV2	1705	1364	0.01%	0.003%
87	12.398	3512	3517	3519	rVB3	1463	1185	0.01%	0.003%
88	12.620	3584	3586	3591	rBV3	1260	840	0.01%	0.002%
89	12.736	3618	3622	3625	rBV4	1600	1224	0.01%	0.003%
90	12.820	3644	3648	3654	rBV4	2447	2955	0.02%	0.007%
91	12.938	3680	3685	3689	rVB3	1747	1625	0.01%	0.004%
92	12.961	3689	3692	3695	rVB3	1394	990	0.01%	0.002%
93	12.977	3695	3697	3705	rBV6	1711	2209	0.02%	0.006%
94	13.041	3713	3717	3719	rBV3	1228	900	0.01%	0.002%
95	13.186	3759	3762	3768	rVB4	1567	1499	0.01%	0.004%
96	13.418	3831	3834	3837	rBV2	1449	1175	0.01%	0.003%
97	13.537	3868	3871	3875	rVB2	1797	1178	0.01%	0.003%
98	13.868	3971	3974	3975	rBV3	1413	821	0.01%	0.002%
99	14.315	4111	4113	4121	rBV4	1566	2015	0.02%	0.005%
100	14.440	4148	4152	4155	rBV3	2849	2245	0.02%	0.006%


Sum of corrected areas: 40092453

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042719\
Data File : VU031566.D
Acq On : 27 Apr 2019 05:19
Operator : JC/SP
Sample : K2592-19 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X86

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

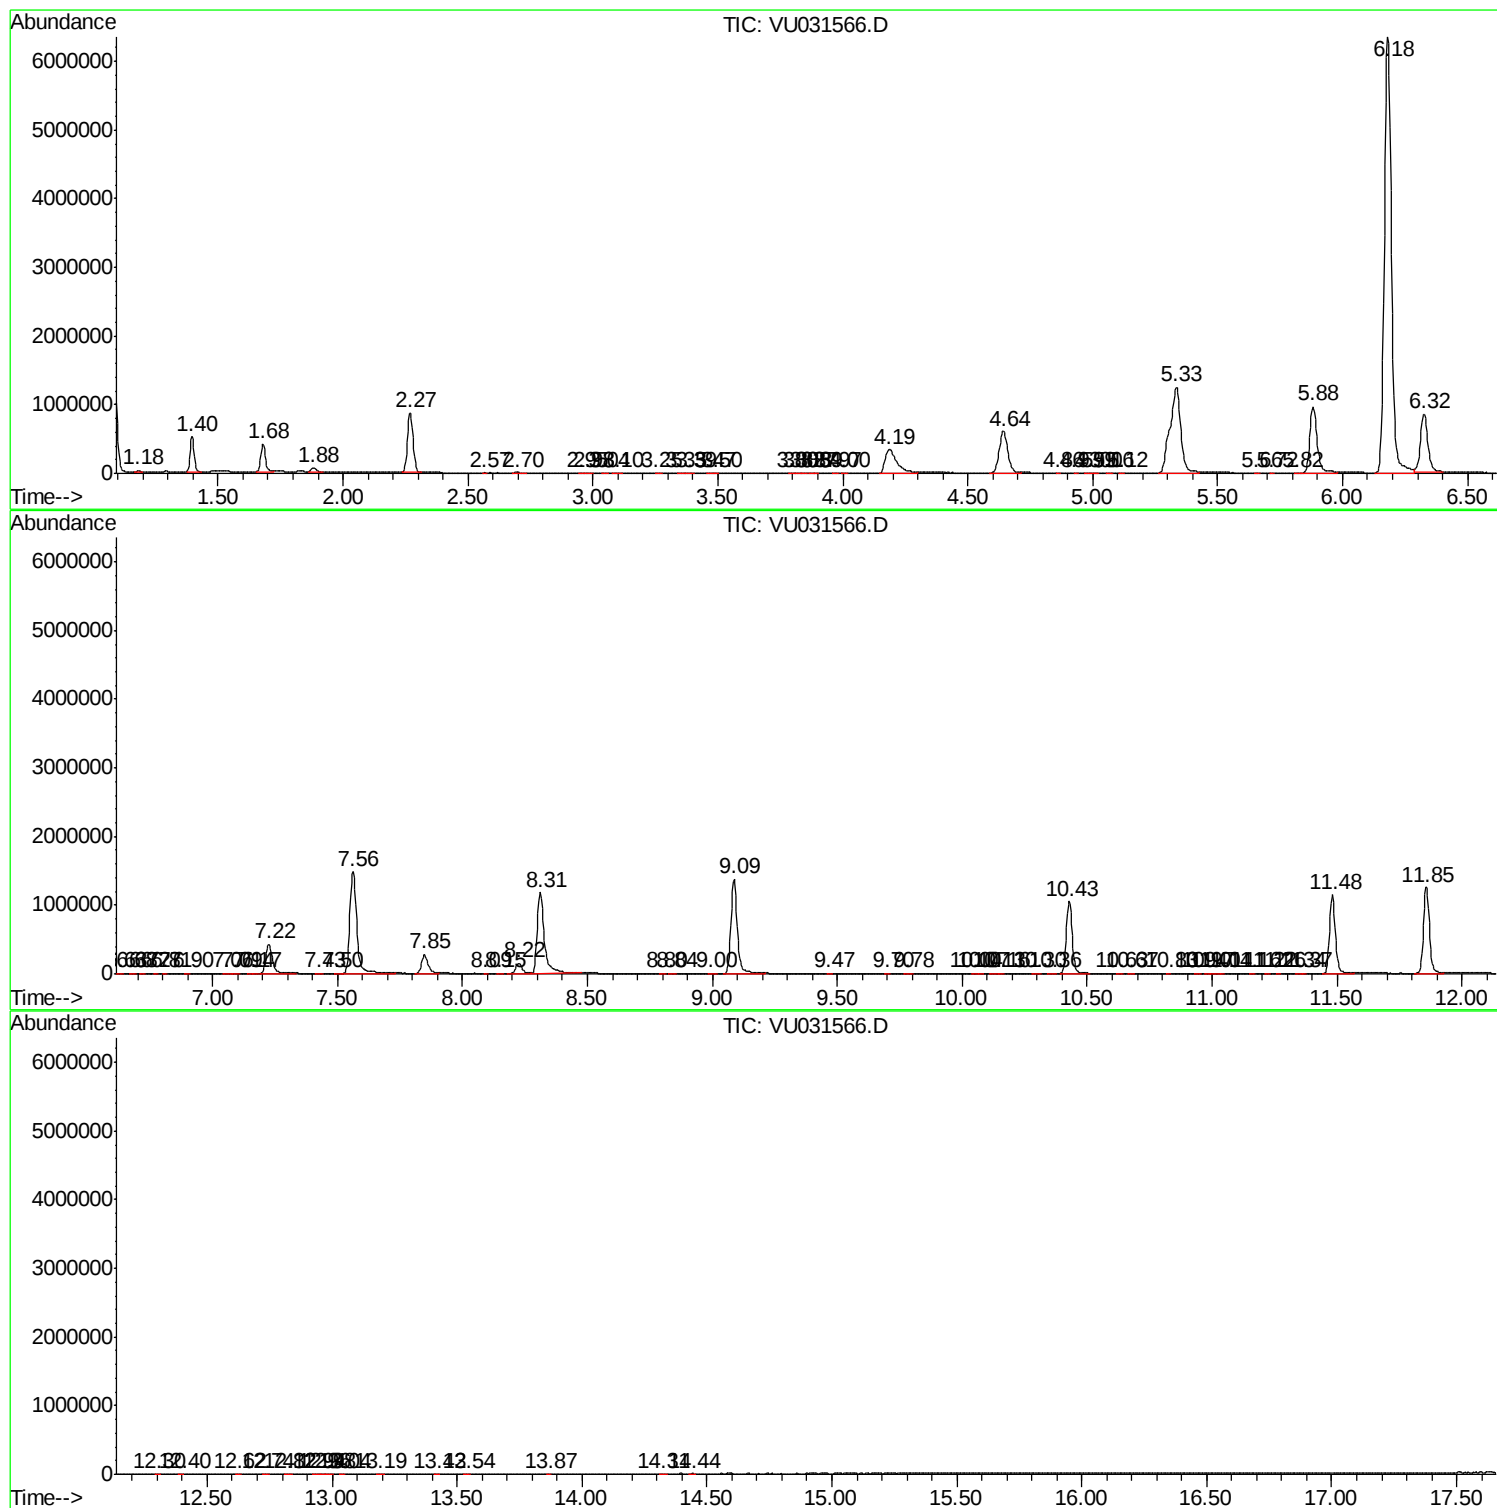

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031566.D
Acq On : 27 Apr 2019 05:19
Operator : JC/SP
Sample : K2592-19 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X86

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031566.D
Acq On : 27 Apr 2019 05:19
Operator : JC/SP
Sample : K2592-19 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X86

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc