

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031567.D
 Acq On : 27 Apr 2019 05:42
 Operator : JC/SP
 Sample : K2592-20 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X87

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	36	rVB2	17910	16804	0.13%	0.043%
2	1.396	88	95	111	rBV	497088	542098	4.35%	1.380%
3	1.679	175	183	195	rBV	412774	508381	4.08%	1.294%
4	1.881	240	246	256	rVB	60426	82428	0.66%	0.210%
5	2.270	356	367	380	rVB	829707	1277046	10.24%	3.251%
6	2.704	495	502	509	rBV7	3877	5834	0.05%	0.015%
7	2.785	523	527	533	rBV2	1190	1543	0.01%	0.004%
8	2.810	533	535	538	rBV2	1076	882	0.01%	0.002%
9	2.910	564	566	570	rVB2	1349	929	0.01%	0.002%
10	2.965	578	583	585	rBV4	2153	1879	0.02%	0.005%
11	3.019	597	600	603	rVB4	1882	1325	0.01%	0.003%
12	3.058	608	612	617	rVB3	2014	1639	0.01%	0.004%
13	3.090	617	622	626	rBV6	1393	1631	0.01%	0.004%
14	3.199	652	656	665	rVB5	1586	2291	0.02%	0.006%
15	3.241	665	669	672	rBV2	1105	1053	0.01%	0.003%
16	3.296	680	686	689	rBV5	1260	1453	0.01%	0.004%
17	3.357	697	705	710	rBV4	1378	1632	0.01%	0.004%
18	3.502	746	750	754	rVB2	1611	1215	0.01%	0.003%
19	3.534	754	760	766	rBV3	1438	1731	0.01%	0.004%
20	3.566	766	770	773	rVB3	1090	930	0.01%	0.002%
21	3.595	773	779	785	rBV4	1619	2548	0.02%	0.006%
22	3.656	792	798	804	rBV2	1722	2251	0.02%	0.006%
23	3.685	804	807	813	rVB3	950	1133	0.01%	0.003%
24	3.859	858	861	864	rVV2	1362	1068	0.01%	0.003%
25	3.945	883	888	892	rVV4	1344	1482	0.01%	0.004%
26	4.135	942	947	950	rBV2	1673	1645	0.01%	0.004%
27	4.183	950	962	1001	rBV	353105	1109809	8.90%	2.826%
28	4.643	1088	1105	1131	rBV	599393	1407505	11.29%	3.584%
29	4.849	1165	1169	1171	rBV3	1655	1365	0.01%	0.003%
30	4.888	1178	1181	1184	rBV2	1720	1177	0.01%	0.003%
31	5.077	1236	1240	1243	rBV2	1021	921	0.01%	0.002%
32	5.251	1290	1294	1296	rBV3	1203	1034	0.01%	0.003%
33	5.334	1296	1320	1345	rBV2	1202594	3659152	29.35%	9.316%
34	5.666	1420	1423	1425	rBV	2143	1431	0.01%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031567.D
 Acq On : 27 Apr 2019 05:42
 Operator : JC/SP
 Sample : K2592-20 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X87

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.881	1477	1490	1514	rBV	939650	1918812	15.39%	4.885%
36	6.180	1568	1583	1616	rBV	6329512	12468586	100.00%	31.746%
37	6.325	1617	1628	1651	rVB	828456	1697112	13.61%	4.321%
38	6.614	1715	1718	1722	rVB5	2092	1354	0.01%	0.003%
39	6.730	1750	1754	1758	rBV4	1906	1728	0.01%	0.004%
40	6.762	1761	1764	1767	rBV2	1520	1017	0.01%	0.003%
41	6.810	1774	1779	1780	rBV4	1782	1538	0.01%	0.004%
42	6.994	1833	1836	1840	rVV3	1831	1561	0.01%	0.004%
43	7.016	1840	1843	1847	rVV3	1137	957	0.01%	0.002%
44	7.225	1896	1908	1934	rVV	404577	774480	6.21%	1.972%
45	7.485	1987	1989	1995	rVB3	2298	1647	0.01%	0.004%
46	7.563	1995	2013	2063	rBV	1424183	2754899	22.09%	7.014%
47	7.849	2091	2102	2124	rBV	269575	491302	3.94%	1.251%
48	8.039	2158	2161	2165	rVB3	2090	1482	0.01%	0.004%
49	8.109	2180	2183	2190	rVB6	1623	1417	0.01%	0.004%
50	8.164	2197	2200	2205	rBV6	1352	1552	0.01%	0.004%
51	8.225	2208	2219	2232	rBV2	154632	275573	2.21%	0.702%
52	8.312	2235	2246	2290	rVV	1157427	2273354	18.23%	5.788%
53	8.646	2347	2350	2353	rBV3	1399	1025	0.01%	0.003%
54	8.701	2361	2367	2370	rBV4	1862	1979	0.02%	0.005%
55	8.727	2373	2375	2379	rVB4	1579	1075	0.01%	0.003%
56	8.852	2410	2414	2419	rVB7	1834	2027	0.02%	0.005%
57	8.887	2419	2425	2427	rBV3	1773	1646	0.01%	0.004%
58	8.977	2450	2453	2457	rVB3	1394	1043	0.01%	0.003%
59	9.087	2472	2487	2514	rBV	1326211	2323947	18.64%	5.917%
60	9.231	2530	2532	2540	rVB7	1907	2388	0.02%	0.006%
61	9.383	2575	2579	2581	rBV4	1051	923	0.01%	0.002%
62	9.437	2591	2596	2600	rBV3	2231	2387	0.02%	0.006%
63	9.456	2600	2602	2606	rVB3	2186	1332	0.01%	0.003%
64	9.485	2606	2611	2613	rBV3	1524	1291	0.01%	0.003%
65	9.579	2638	2640	2646	rVB4	1619	1389	0.01%	0.004%
66	9.608	2646	2649	2653	rVB2	1545	1064	0.01%	0.003%
67	9.630	2653	2656	2660	rBV4	1195	884	0.01%	0.002%
68	9.682	2667	2672	2674	rBV3	1077	973	0.01%	0.002%
69	9.842	2719	2722	2725	rBV4	1098	907	0.01%	0.002%
70	9.910	2741	2743	2746	rVB3	2072	1249	0.01%	0.003%
71	9.932	2746	2750	2753	rBV2	1670	1521	0.01%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042719\
 Data File : VU031567.D
 Acq On : 27 Apr 2019 05:42
 Operator : JC/SP
 Sample : K2592-20 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X87

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.026	2776	2779	2781	rBV2	2516	1601	0.01%	0.004%
73	10.231	2839	2843	2845	rBV	1586	1339	0.01%	0.003%
74	10.276	2855	2857	2860	rBV	1572	877	0.01%	0.002%
75	10.427	2892	2904	2928	rBV	1056544	1704905	13.67%	4.341%
76	10.598	2954	2957	2959	rBV3	1619	1002	0.01%	0.003%
77	10.791	3011	3017	3019	rVB2	952	962	0.01%	0.002%
78	10.897	3047	3050	3057	rBV5	1131	1139	0.01%	0.003%
79	11.087	3106	3109	3115	rVB4	2129	2042	0.02%	0.005%
80	11.222	3147	3151	3155	rBV4	1445	1451	0.01%	0.004%
81	11.408	3203	3209	3211	rBV3	1330	1518	0.01%	0.004%
82	11.479	3218	3231	3262	rBV	1098478	1826401	14.65%	4.650%
83	11.855	3336	3348	3380	rBV	1213913	2046611	16.41%	5.211%
84	12.206	3454	3457	3461	rBV2	1818	1642	0.01%	0.004%
85	12.386	3510	3513	3518	rBV5	2052	1314	0.01%	0.003%
86	12.707	3608	3613	3616	rBV4	1195	1370	0.01%	0.003%
87	12.749	3622	3626	3630	rBV4	2106	1976	0.02%	0.005%
88	12.833	3646	3652	3656	rBV6	2152	2788	0.02%	0.007%
89	13.077	3725	3728	3732	rVV3	1265	1216	0.01%	0.003%
90	13.231	3773	3776	3778	rVB2	1471	877	0.01%	0.002%
91	13.286	3790	3793	3795	rBV2	1250	937	0.01%	0.002%
92	13.443	3837	3842	3845	rBV2	2144	2032	0.02%	0.005%
93	13.511	3860	3863	3866	rVB2	1664	1014	0.01%	0.003%
94	13.775	3941	3945	3949	rBV3	1482	1289	0.01%	0.003%
95	13.797	3949	3952	3955	rBV2	1320	977	0.01%	0.002%
96	13.955	3998	4001	4004	rBV2	1807	1294	0.01%	0.003%
97	14.080	4037	4040	4041	rBV2	2058	1096	0.01%	0.003%
98	14.128	4051	4055	4058	rBV3	2155	1895	0.02%	0.005%
99	14.585	4194	4197	4199	rBV2	1652	1090	0.01%	0.003%
100	15.289	4414	4416	4418	rBV2	1732	974	0.01%	0.002%


Sum of corrected areas: 39276295

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042719\
Data File : VU031567.D
Acq On : 27 Apr 2019 05:42
Operator : JC/SP
Sample : K2592-20 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X87

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

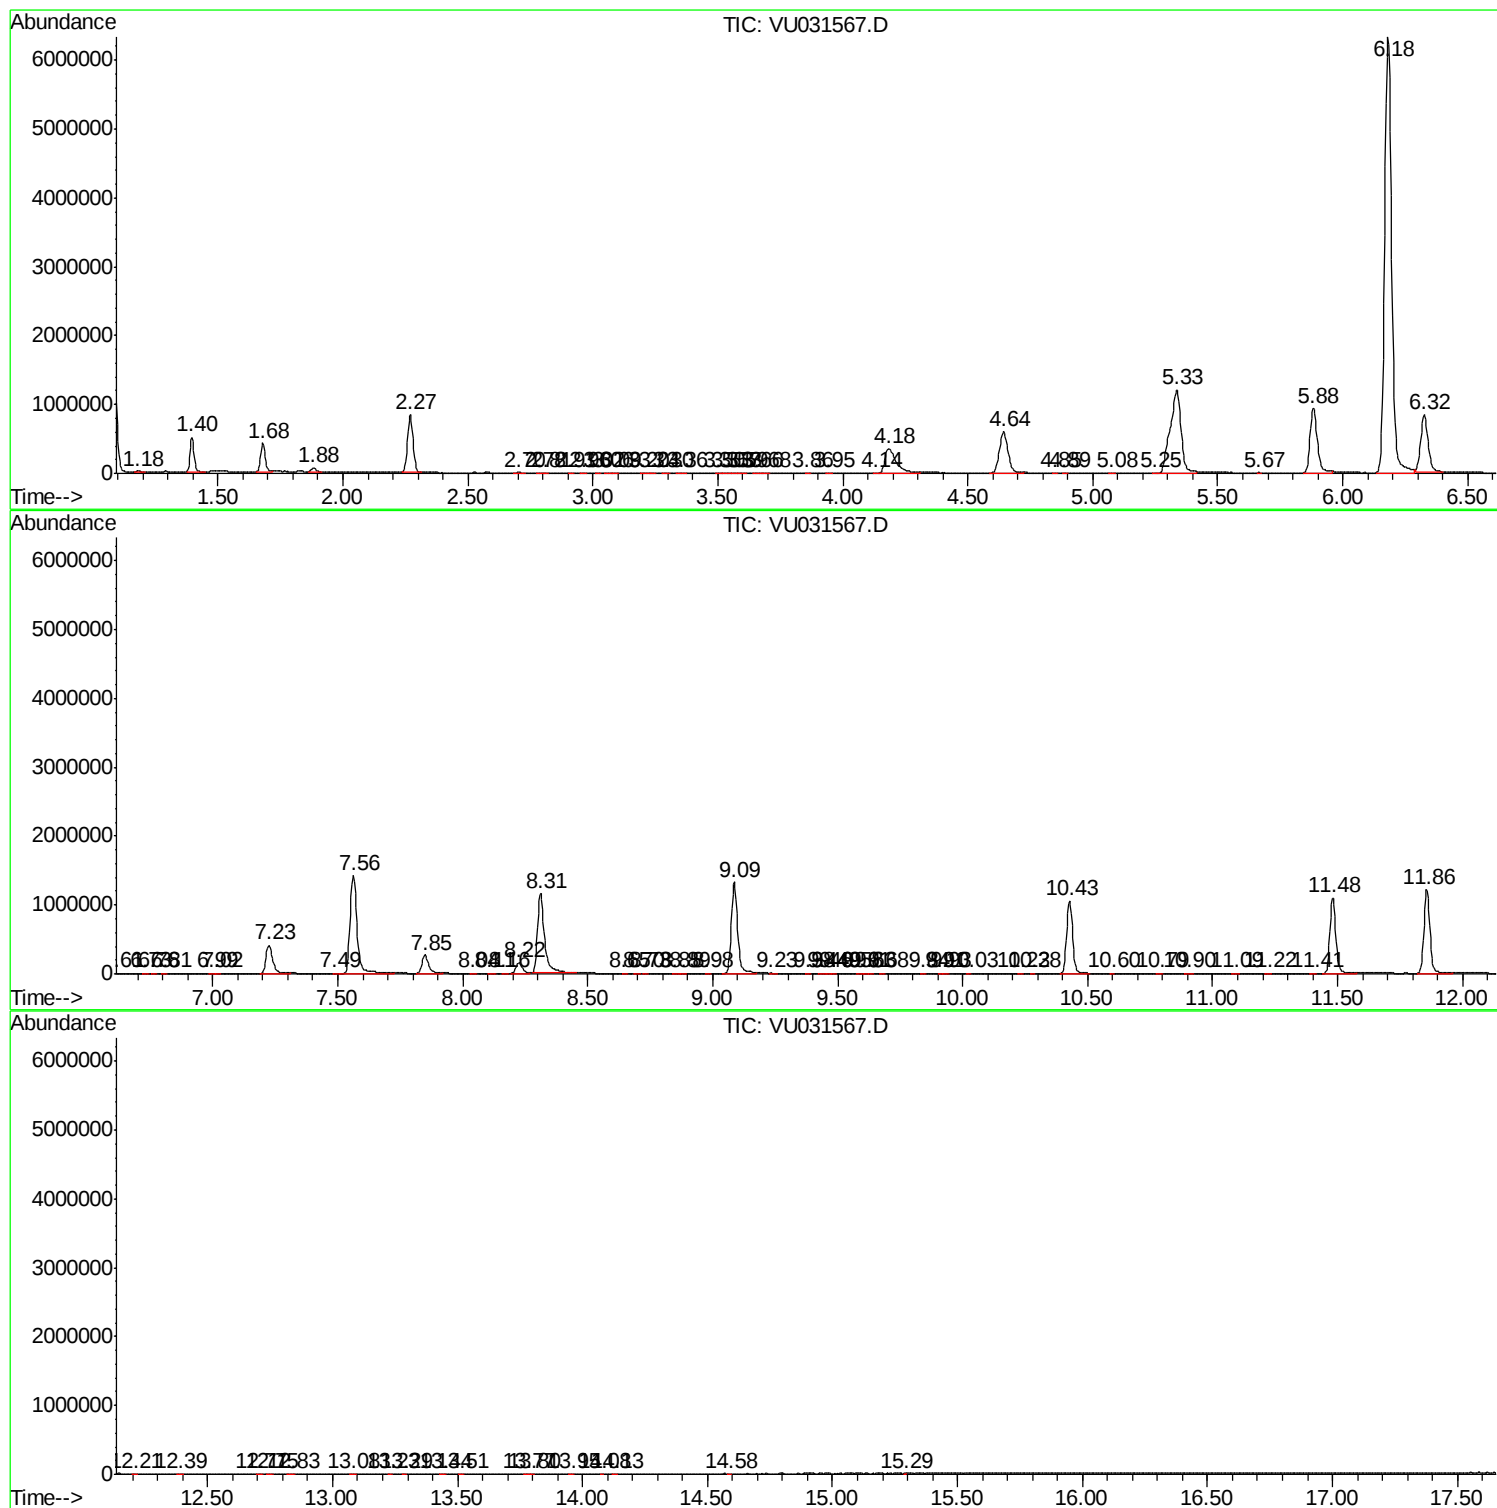

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031567.D
Acq On : 27 Apr 2019 05:42
Operator : JC/SP
Sample : K2592-20 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X87

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042719\
Data File : VU031567.D
Acq On : 27 Apr 2019 05:42
Operator : JC/SP
Sample : K2592-20 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 52 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X87

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc