


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042719\
 Data File : VU031519.D
 Acq On : 26 Apr 2019 08:55
 Operator : JC/SP
 Sample : BFB99
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB99

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis
 Last Update : Mon Apr 29 01:00:30 2019

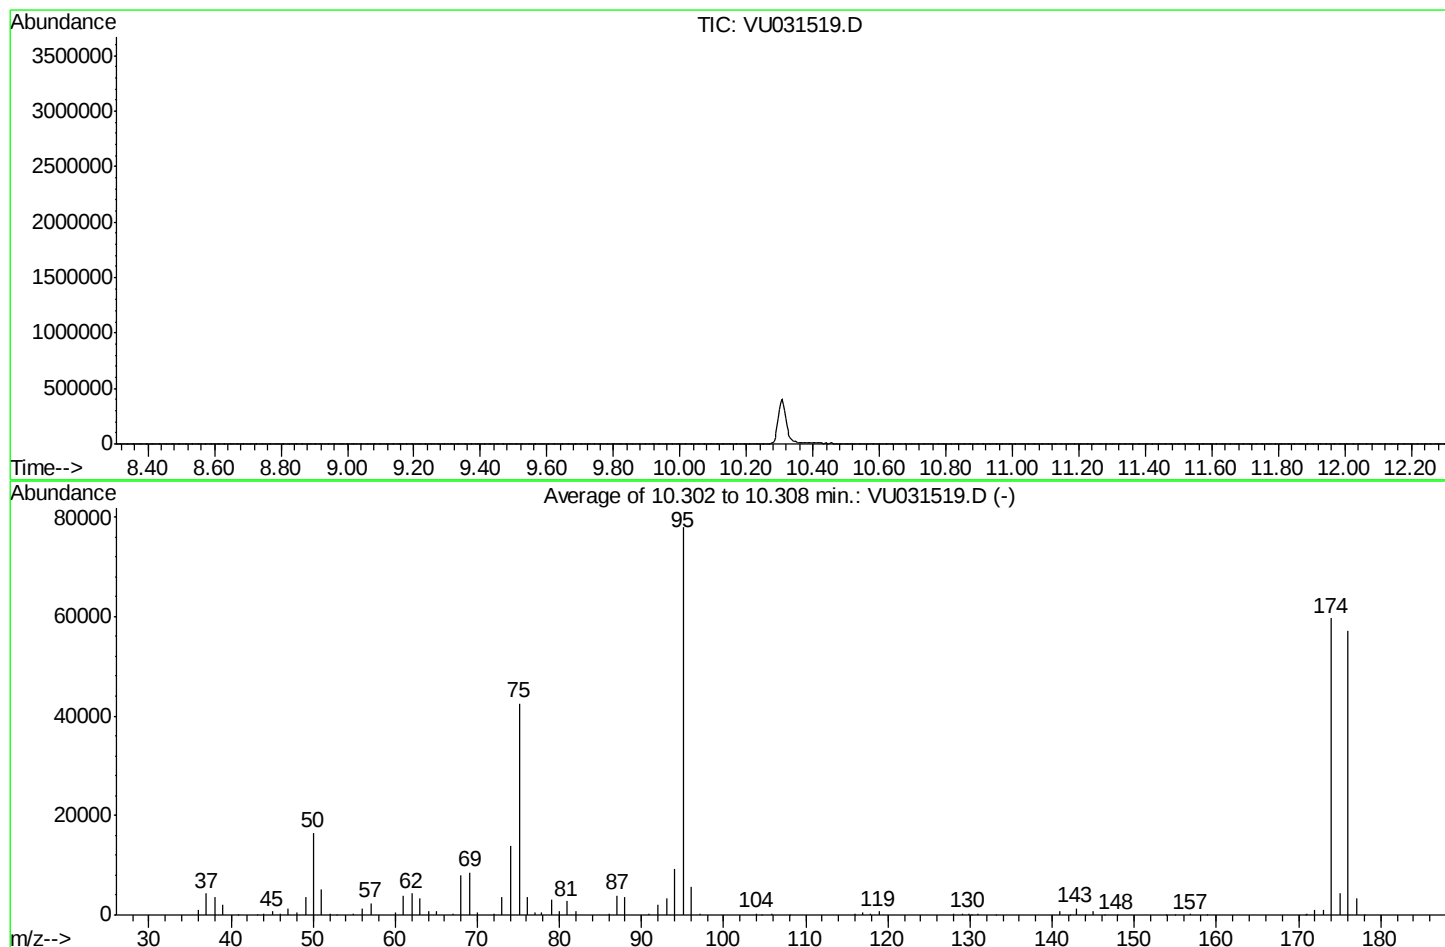

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2854

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.3	16603	PASS
75	95	30	80	54.6	42530	PASS
95	95	100	100	100.0	77912	PASS
96	95	5	9	7.3	5697	PASS
173	174	0.00	2	1.7	1011	PASS
174	95	50	120	76.5	59602	PASS
175	174	5	9	7.6	4503	PASS
176	174	95	101	96.0	57221	PASS
177	176	5	9	5.7	3269	PASS

Scan 2854 (10.267 min): VU031519.D
BFB99

m/z	Abundance
39.90	3876.0
43.90	846.0

Instrument :
MSVOA_U
ClientSampleId :
BFB99

m/z	Abundance
36.10	1124.0
37.00	4238.0
38.00	3263.0
39.00	2106.0
40.00	3156.0
40.80	101.0
43.20	100.0
44.00	1070.0
45.10	725.0
46.10	382.0
47.00	1114.0
48.10	476.0
49.10	3461.0
50.00	15987.0
51.00	4962.0
52.00	219.0
54.90	280.0
56.00	1198.0
57.00	2352.0
60.10	572.0
61.00	3683.0
62.10	4066.0
63.00	3293.0
64.00	827.0
65.00	1003.0
67.10	282.0
68.00	7584.0
69.10	8168.0
70.00	667.0
72.00	337.0
73.00	3636.0
74.10	13294.0
75.10	41224.0
76.10	3141.0
77.00	409.0
77.80	288.0
79.00	3291.0
80.00	640.0
80.90	2663.0
82.00	781.0
87.00	3694.0
88.00	3395.0
91.10	192.0
92.00	2083.0
93.00	3203.0
94.00	8755.0
95.10	73824.0
96.10	5462.0
97.20	156.0
104.00	504.0
105.90	236.0
116.10	118.0
116.90	580.0
117.80	255.0
118.90	604.0
128.00	281.0
129.00	165.0
129.80	230.0
130.10	229.0
131.00	161.0
133.20	123.0
140.90	767.0
143.00	1118.0
143.90	106.0
145.00	564.0
153.80	100.0
156.90	126.0
171.00	320.0
171.90	901.0
174.00	56360.0
175.00	4485.0
176.00	53296.0
177.00	2927.0

Instrument :
MSVOA_U
ClientSampleId :
BFB99

m/z	Abundance
36.00	1150.0
37.00	4527.0
38.00	3656.0
39.00	2206.0
40.00	2840.0
44.00	1160.0
45.10	799.0
46.00	294.0
47.00	1336.0
48.00	533.0
49.10	3611.0
50.10	17216.0
51.00	5218.0
52.10	217.0
54.90	331.0
56.00	1394.0
57.00	2481.0
60.10	602.0
61.00	3863.0
62.10	4445.0
63.00	3526.0
64.00	900.0
65.00	928.0
67.10	300.0
68.10	8249.0
69.10	8813.0
70.00	641.0
72.00	369.0
73.00	3697.0
74.10	14282.0
75.10	44192.0
76.10	3669.0
77.10	458.0
77.90	392.0
79.00	3265.0
80.00	670.0
80.90	2928.0
82.00	719.0
86.10	280.0
87.00	3958.0
88.00	3940.0
90.90	190.0
92.00	2049.0
93.10	3569.0
94.10	9487.0
95.10	80336.0
96.10	6004.0
97.20	155.0
104.00	393.0
105.90	226.0
115.90	146.0
116.90	582.0
117.90	313.0
118.90	707.0
128.00	334.0
129.00	175.0
129.90	374.0
131.00	144.0
140.90	824.0
142.20	118.0
142.90	1381.0
144.00	119.0
144.90	679.0
146.30	105.0
147.90	103.0
156.80	171.0
171.10	244.0
172.00	1178.0
173.10	1549.0
174.00	61400.0
175.00	4705.0
176.00	59096.0
177.10	3355.0
178.00	110.0

Instrument :
MSVOA_U
ClientSampleId :
BFB99

m/z	Abundance
36.00	1098.0
37.00	4219.0
38.00	3728.0
39.00	2142.0
40.00	2847.0
44.00	1354.0
45.00	777.0
46.00	201.0
46.90	1345.0
48.00	497.0
49.10	3705.0
50.10	16608.0
51.10	5177.0
52.10	182.0
52.90	132.0
54.90	290.0
56.00	1286.0
57.00	2392.0
60.10	532.0
61.00	3901.0
62.00	4377.0
63.00	3343.0
64.00	913.0
65.10	730.0
67.10	326.0
68.10	8358.0
69.10	8818.0
70.00	535.0
72.00	393.0
73.00	3495.0
74.10	13804.0
75.10	42176.0
76.10	3678.0
77.10	481.0
77.90	549.0
79.00	2906.0
79.90	656.0
80.90	2873.0
82.00	659.0
86.10	313.0
87.00	3991.0
88.00	3856.0
90.90	211.0
92.00	1873.0
93.10	3353.0
94.10	9723.0
95.10	79576.0
96.00	5626.0
97.20	177.0
103.90	263.0
104.60	124.0
105.90	220.0
108.00	104.0
115.90	215.0
116.90	622.0
117.90	312.0
118.90	743.0
127.80	312.0
129.00	139.0
129.90	473.0
131.00	147.0
140.90	815.0
142.20	179.0
143.00	1548.0
144.10	146.0
145.00	778.0
147.90	157.0
155.00	125.0
156.80	172.0
158.90	112.0
170.80	171.0
172.00	1237.0
173.10	1484.0
174.00	61048.0
175.00	4319.0
176.00	59272.0
177.10	3525.0
178.00	129.0

Instrument :
MSVOA_U
ClientSampleId :
BFB99