

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042721\
 Data File : VU043347.D
 Acq On : 27 Apr 2021 12:27
 Operator : SY/MD
 Sample : M2127-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 E0AA9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU043347.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	73	82	92	rVB	36800	44480	8.71%	1.243%
2	1.919	172	180	193	rVB	33775	43144	8.45%	1.206%
3	2.575	372	384	397	rBV	82611	133334	26.11%	3.727%
4	2.662	397	411	438	rVV	17943	63048	12.34%	1.762%
5	3.057	524	534	545	rVB4	3655	7822	1.53%	0.219%
6	4.652	1013	1030	1076	rBV2	61642	223031	43.67%	6.234%
7	5.073	1146	1161	1182	rBV	83884	193761	37.94%	5.415%
8	5.735	1344	1367	1387	rBV3	149551	395440	77.42%	11.052%
9	6.170	1491	1502	1512	rBV3	3430	7259	1.42%	0.203%
10	6.256	1516	1529	1551	rVB	145098	269442	52.75%	7.531%
11	6.700	1651	1667	1683	rBV	98645	193462	37.88%	5.407%
12	7.571	1924	1938	1954	rBV3	46360	82720	16.20%	2.312%
13	7.906	2028	2042	2055	rBV	166008	287294	56.25%	8.030%
14	7.977	2057	2064	2081	rVB	8622	17089	3.35%	0.478%
15	8.186	2119	2129	2143	rBV	31075	51443	10.07%	1.438%
16	8.645	2258	2272	2300	rBV	252115	510748	100.00%	14.275%
17	9.423	2502	2514	2533	rBV	209353	344035	67.36%	9.615%
18	10.764	2920	2931	2949	rVB	75047	121665	23.82%	3.400%
19	11.819	3247	3259	3274	rBV	196103	305900	59.89%	8.550%
20	12.070	3328	3337	3349	rVB3	5833	9925	1.94%	0.277%
21	12.201	3362	3378	3393	rBV	168520	272889	53.43%	7.627%




Sum of corrected areas: 3577931

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042721\
Data File : VU043347.D
Acq On : 27 Apr 2021 12:27
Operator : SY/MD
Sample : M2127-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0AA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

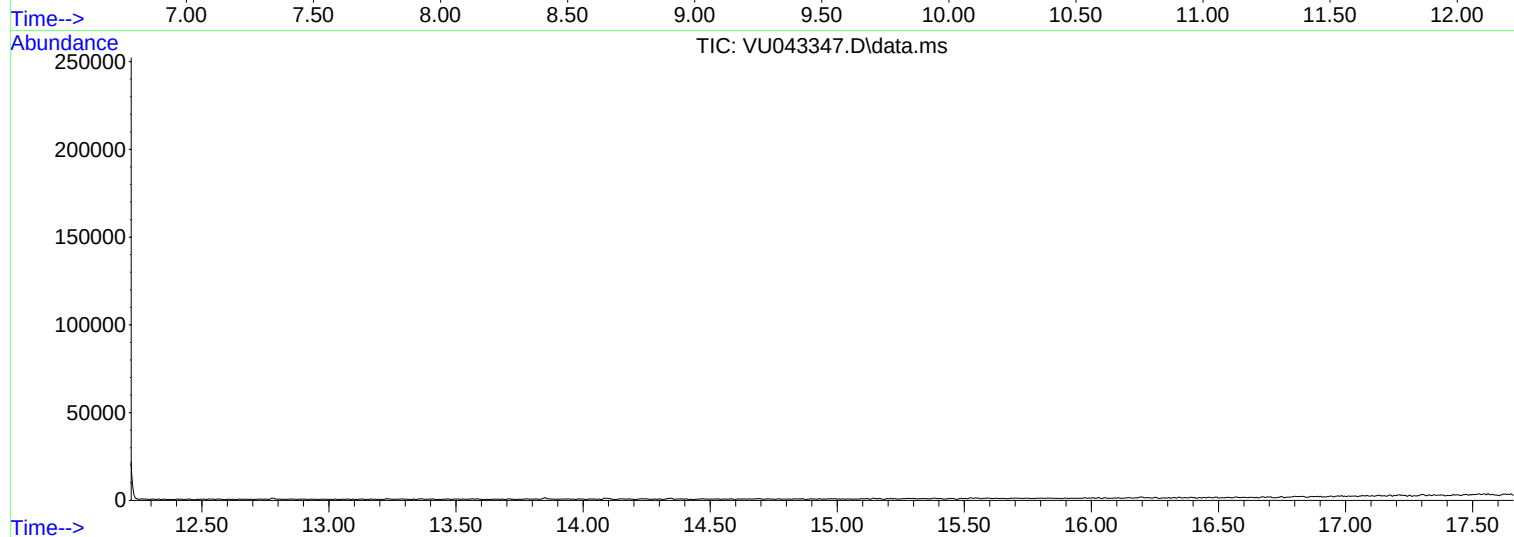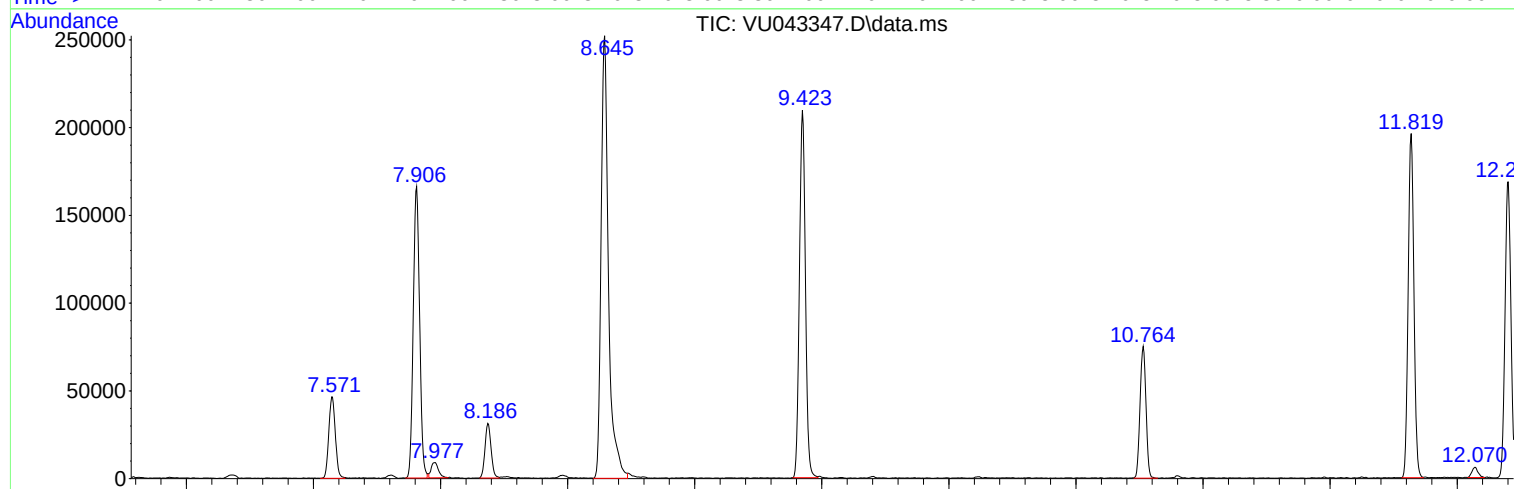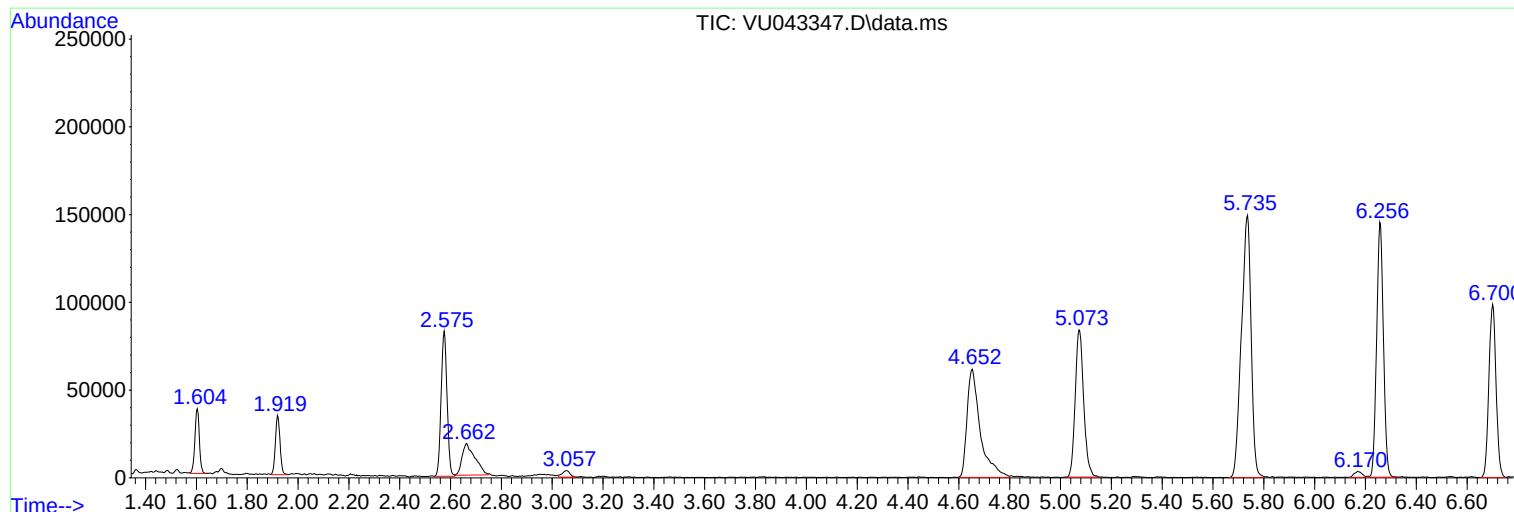

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042721\
Data File : VU043347.D
Acq On : 27 Apr 2021 12:27
Operator : SY/MD
Sample : M2127-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0AA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042721\
Data File : VU043347.D
Acq On : 27 Apr 2021 12:27
Operator : SY/MD
Sample : M2127-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
E0AA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
