


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042721\
Data File : VU043341.D
Acq On : 27 Apr 2021 09:08
Operator : SY/MD
Sample : BFB37
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB137

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR041521WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Tue Apr 27 23:46:47 2021

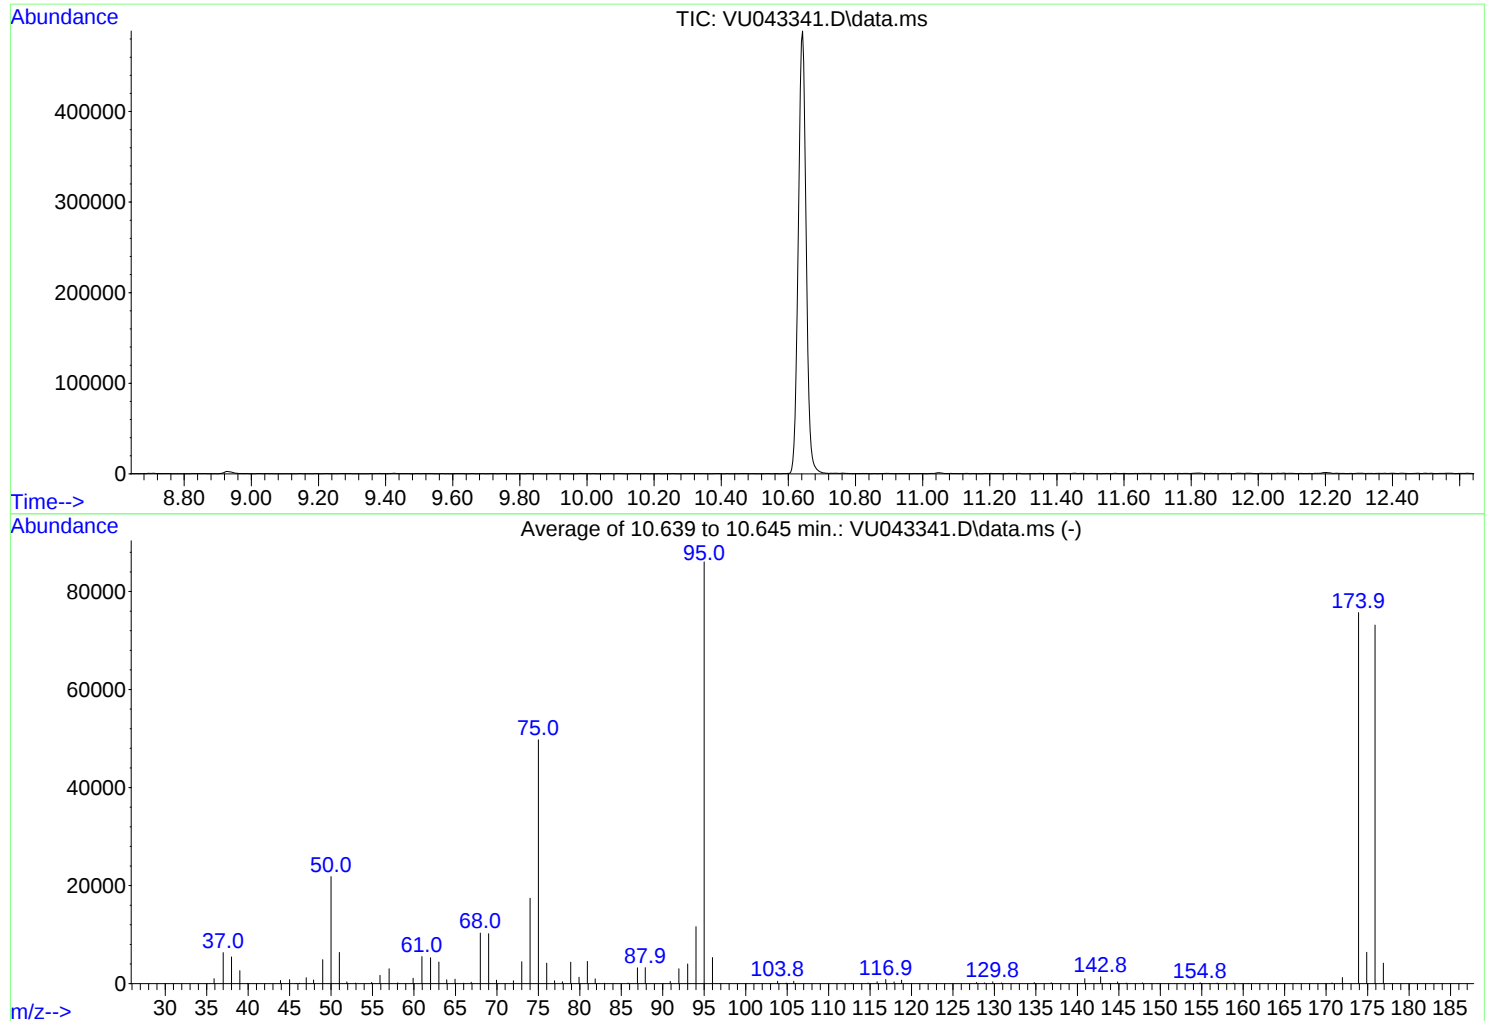

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.4	21840	PASS
75	95	30	80	57.8	49744	PASS
95	95	100	100	100.0	86048	PASS
96	95	5	9	6.2	5320	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	88.0	75683	PASS
175	174	5	9	8.4	6388	PASS
176	174	95	101	96.7	73157	PASS
177	176	5	9	5.7	4195	PASS

m/z	Abundance
35.90	1076.0
37.00	6479.0
38.00	5593.0
39.00	2637.0
39.90	192.0
44.00	1023.0
45.00	927.0
45.80	164.0
47.00	1107.0
47.90	795.0
49.00	4912.0
50.00	22416.0
51.00	6349.0
51.90	341.0
52.90	128.0
54.90	288.0
55.90	1803.0
57.00	3064.0
58.00	156.0
59.90	1135.0
60.90	5833.0
62.00	5337.0
63.00	4693.0
64.00	840.0
64.90	872.0
66.00	148.0
66.90	287.0
68.00	10478.0
69.00	10455.0
70.00	729.0
72.00	617.0
73.00	4593.0
74.00	17496.0
75.00	49840.0
76.00	4184.0
76.90	602.0
77.90	435.0
78.90	4501.0
79.90	1427.0
80.90	4642.0
81.90	940.0
83.00	102.0
85.80	140.0
86.90	3320.0
87.90	3165.0
90.90	470.0
91.90	2980.0
93.00	4361.0
94.00	11739.0
95.00	85880.0
96.00	5713.0
103.90	507.0
104.90	151.0
105.80	531.0
112.80	161.0
114.80	147.0
115.80	347.0
116.90	917.0
117.90	353.0
118.80	847.0
127.80	241.0
128.80	160.0
129.80	382.0
130.80	156.0
134.80	213.0
136.80	209.0
140.90	1034.0
142.80	1438.0
144.90	314.0
145.80	140.0
147.90	126.0
154.80	186.0
155.90	102.0
156.80	150.0
158.90	132.0
160.60	106.0
170.70	187.0
172.00	1269.0
173.90	75496.0
174.90	6425.0
175.90	72856.0
176.90	4313.0

Instrument :
MSVOA_U
ClientSampleId :
BFB137

m/z	Abundance
39.90	109.0
43.90	318.0

Instrument :
MSVOA_U
ClientSampleId :
BFB137

m/z	Abundance
35.90	951.0
37.00	6022.0
38.00	5119.0
39.00	2483.0
39.90	191.0
43.90	933.0
45.00	733.0
46.20	175.0
47.00	1274.0
47.90	679.0
49.00	4754.0
50.00	20624.0
51.00	6054.0
51.90	375.0
53.00	150.0
54.90	259.0
55.90	1580.0
57.00	2837.0
58.10	164.0
59.90	994.0
61.00	5037.0
62.00	5098.0
63.00	3989.0
63.90	707.0
65.00	919.0
66.90	270.0
68.00	9759.0
69.00	9593.0
70.00	667.0
72.00	532.0
73.00	4254.0
74.00	16968.0
75.00	48160.0
76.00	4040.0
77.00	564.0
77.90	304.0
78.90	4013.0
79.90	1130.0
80.90	4306.0
81.80	1025.0
82.90	105.0
85.80	109.0
87.00	3055.0
87.90	3143.0
90.90	435.0
92.00	2960.0
93.00	3588.0
94.00	11106.0
95.00	83584.0
96.00	4820.0
96.90	110.0
103.80	473.0
104.90	120.0
105.80	431.0
114.70	142.0
115.90	433.0
116.90	765.0
117.90	363.0
118.80	574.0
127.80	281.0
128.80	148.0
129.80	411.0
130.90	144.0
134.80	207.0
136.90	178.0
140.00	120.0
140.90	988.0
142.80	1331.0
143.90	125.0
144.80	373.0
146.00	130.0
147.80	199.0
148.80	101.0
149.70	104.0
154.80	193.0
156.90	141.0
158.80	146.0
170.80	174.0
171.90	1247.0
173.90	73376.0
174.90	5994.0
175.90	71024.0
176.90	4029.0

Instrument :
MSVOA_U
ClientSampleId :
BFB137

m/z	Abundance
35.90	1040.0
37.00	6463.0
38.00	5600.0
39.00	2804.0
39.90	188.0
44.00	1006.0
45.00	811.0
46.20	147.0
47.00	1207.0
47.90	777.0
49.00	5040.0
50.00	22480.0
51.00	6656.0
51.90	394.0
52.90	145.0
54.90	267.0
55.90	1701.0
57.00	3191.0
58.10	182.0
59.90	1160.0
60.90	5710.0
62.00	5463.0
63.00	4554.0
63.90	838.0
65.00	928.0
66.00	108.0
66.90	311.0
68.00	10709.0
69.00	10548.0
69.90	760.0
72.00	586.0
73.00	4605.0
74.00	17848.0
75.00	51232.0
76.00	4297.0
76.90	623.0
77.90	402.0
78.90	4579.0
79.90	1349.0
80.90	4681.0
81.80	1003.0
82.90	102.0
85.80	135.0
86.90	3343.0
87.90	3473.0
90.90	497.0
91.90	3191.0
93.00	4131.0
94.00	11995.0
95.00	88680.0
96.00	5427.0
103.80	532.0
104.90	140.0
105.80	503.0
112.80	126.0
114.80	148.0
115.90	401.0
116.90	893.0
117.90	357.0
118.80	746.0
127.90	257.0
128.80	174.0
129.80	414.0
130.90	148.0
134.80	241.0
136.90	207.0
138.80	113.0
140.90	1070.0
142.80	1453.0
143.90	113.0
144.90	359.0
145.90	135.0
147.80	153.0
154.80	204.0
156.90	122.0
158.90	146.0
170.60	184.0
171.90	1258.0
173.90	78176.0
174.90	6744.0
175.90	75592.0
176.90	4244.0
177.80	106.0

Instrument :
MSVOA_U
ClientSampleId :
BFB137