




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
 Data File : VU048311.D
 Acq On : 27 Apr 2022 13:54
 Operator : SY/MD
 Sample : N2562-02ME
 Misc : 7.25g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW462ME

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/28/2022
 Supervised By :Mahesh Dadoda 04/28/2022

Quant Time: Apr 28 04:37:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 28 04:33:44 2022
 Response via : Initial Calibration

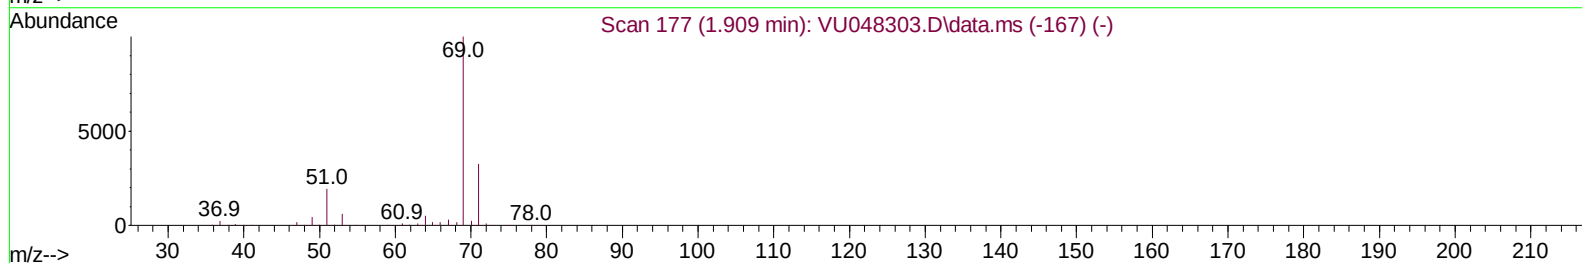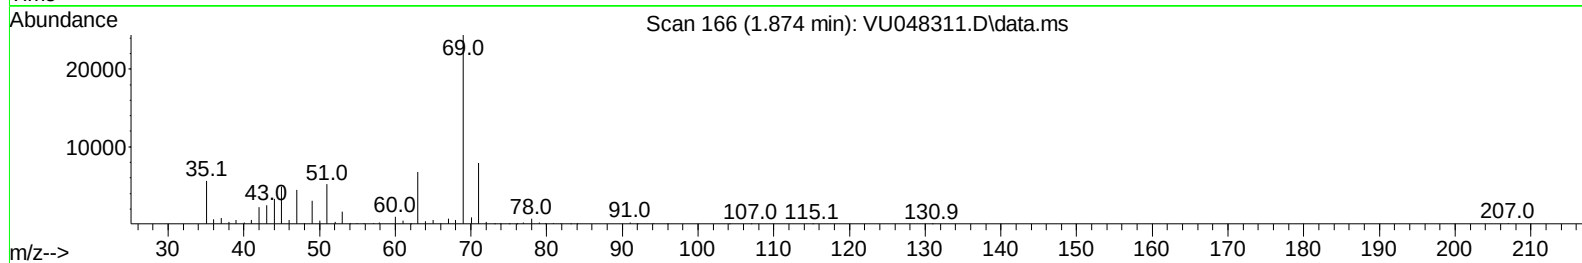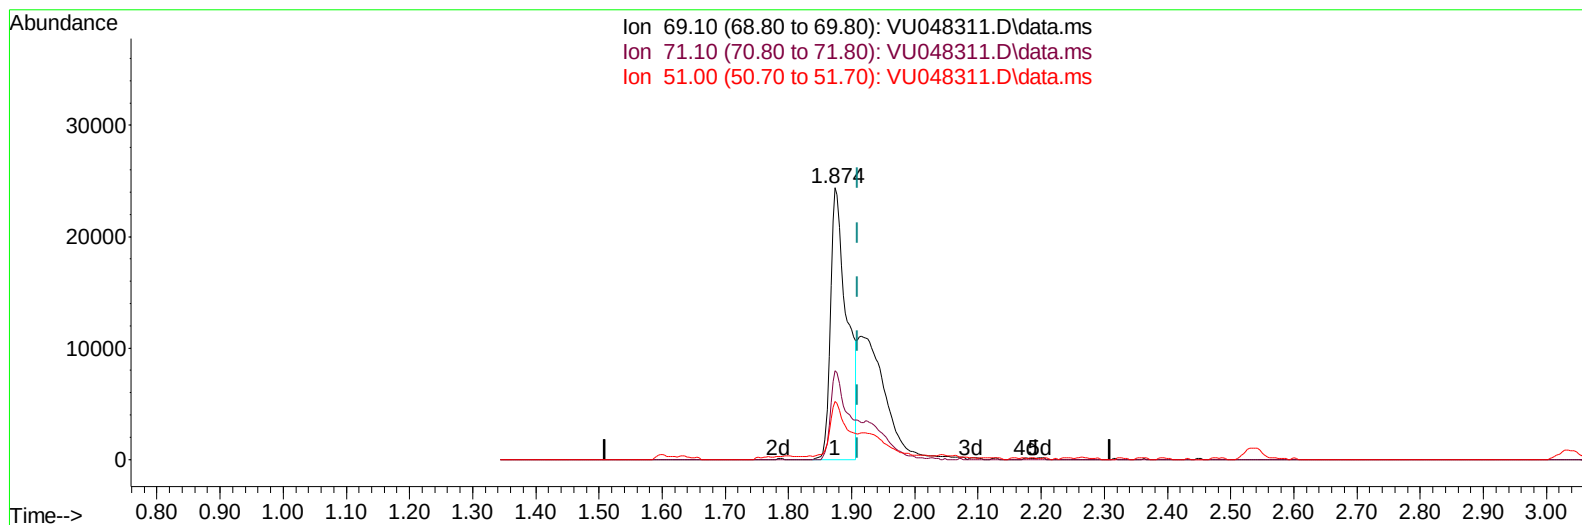

TIC: VU048311.D\data.ms

(7) Chloroethane-d5 (S)

1.874min (-0.035) 17.79 ug/L

response 43560

Ion	Exp%	Act%
69.10	100.00	100.00
71.10	31.60	32.65
51.00	22.10	21.28
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
 Data File : VU048311.D
 Acq On : 27 Apr 2022 13:54
 Operator : SY/MD
 Sample : N2562-02ME
 Misc : 7.25g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW462ME

Manual IntegrationsAPPROVED

Quant Time: Apr 28 04:37:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 28 04:33:44 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/28/2022
 Supervised By :Mahesh Dadoda 04/28/2022

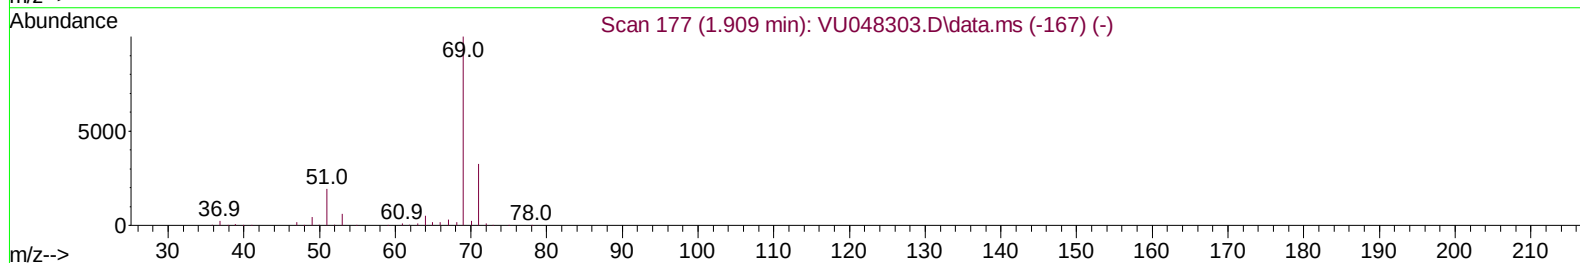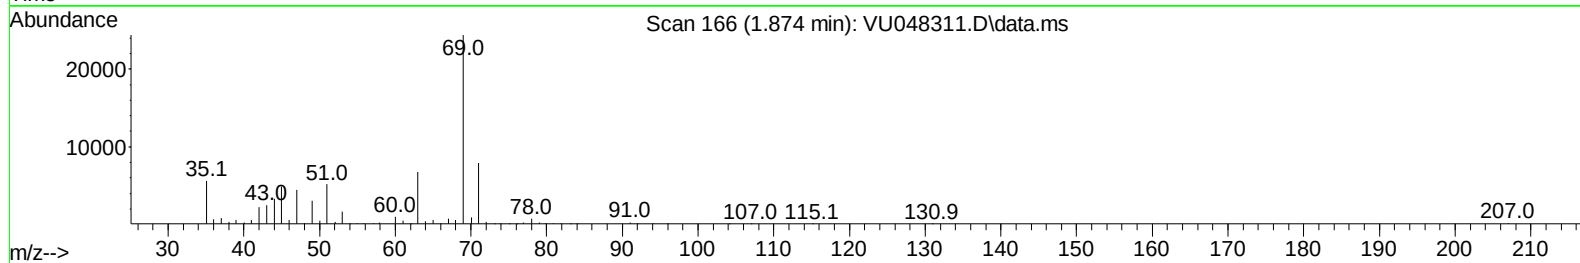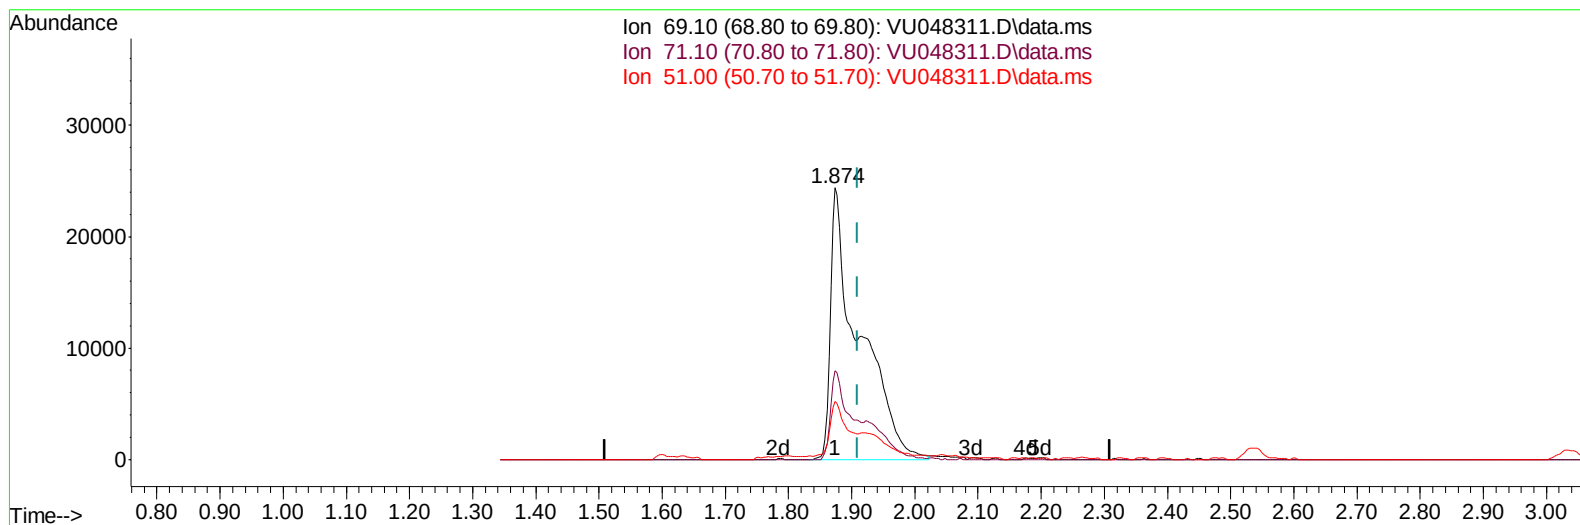

TIC: VU048311.D\data.ms

(7) Chloroethane-d5 (S)

1.874min (-0.035) 31.40 ug/L m

response 76886

Ion	Exp%	Act%
69.10	100.00	100.00
71.10	31.60	18.50#
51.00	22.10	12.06#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
 Data File : VU048311.D
 Acq On : 27 Apr 2022 13:54
 Operator : SY/MD
 Sample : N2562-02ME
 Misc : 7.25g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EW462ME

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/28/2022
 Supervised By :Mahesh Dadoda 04/28/2022

Quant Time: Apr 28 04:37:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Apr 28 04:33:44 2022
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.247	114		379370	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.423	117		390052	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.816	152		184184	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.601	65		187067	53.623	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery	=	107.240%	
7) Chloroethane-d5	1.874	69		76886m	31.398	ug/L	-0.04
Spiked Amount 50.000	Range 70	- 130		Recovery	=	62.800%#	
11) 1,1-Dichloroethene-d2	2.536	63		253556	45.361	ug/L	-0.03
Spiked Amount 50.000	Range 60	- 125		Recovery	=	90.720%	
21) 2-Butanone-d5	4.636	46		325667	109.452	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130		Recovery	=	109.450%	
24) Chloroform-d	5.060	84		356394	56.323	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	112.640%	
26) 1,2-Dichloroethane-d4	5.700	65		230020	61.267	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	122.540%	
32) Benzene-d6	5.719	84		760968	61.859	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	123.720%	
36) 1,2-Dichloropropane-d6	6.690	67		243763	59.937	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery	=	119.880%	
41) Toluene-d8	7.896	98		698703	62.660	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	125.320%#	
43) trans-1,3-Dichloroprop...	8.182	79		107727	60.029	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	120.060%	
47) 2-Hexanone-d5	8.658	63		245175	111.736	ug/L	0.02
Spiked Amount 100.000	Range 45	- 130		Recovery	=	111.740%	
56) 1,1,2,2-Tetrachloroeth...	10.764	84		390341	54.725	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery	=	109.460%	
66) 1,2-Dichlorobenzene-d4	12.198	152		273049	65.902	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	131.800%#	
Target Compounds							
22) 2-Butanone	4.719	43		33268	11.778	ug/L	Qvalue 94

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
Data File : VU048311.D
Acq On : 27 Apr 2022 13:54
Operator : SY/MD
Sample : N2562-02ME
Misc : 7.25g/5.0mL/100uL/5.0mL/MSVOA_U/MEOH
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EW462ME

Manual IntegrationsAPPROVED

Quant Time: Apr 28 04:37:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Apr 28 04:33:44 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/28/2022
Supervised By :Mahesh Dadoda 04/28/2022

