

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
 Data File : VU048305.D
 Acq On : 27 Apr 2022 11:29
 Operator : SY/MD
 Sample : VU0427WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK103

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048305.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	39	45	51	rBV4	4133	6002	0.37%	0.050%
2	1.600	73	81	98	rBV	191111	243860	15.23%	2.028%
3	1.883	162	169	191	rVB	131788	211504	13.21%	1.759%
4	2.475	350	353	354	rBV	375	248	0.02%	0.002%
5	2.562	367	380	398	rBV	332453	547447	34.19%	4.554%
6	2.710	423	426	428	rBV2	321	207	0.01%	0.002%
7	2.787	445	450	453	rBV5	724	736	0.05%	0.006%
8	2.867	472	475	478	rBV2	267	218	0.01%	0.002%
9	2.957	500	503	509	rVB2	770	659	0.04%	0.005%
10	3.047	520	531	540	rBV4	4641	8505	0.53%	0.071%
11	3.099	544	547	551	rVB3	447	273	0.02%	0.002%
12	3.144	558	561	563	rBV3	282	175	0.01%	0.001%
13	3.179	563	572	589	rBV	3616	8458	0.53%	0.070%
14	3.276	599	602	604	rBV	231	177	0.01%	0.001%
15	3.350	623	625	627	rVV2	387	235	0.01%	0.002%
16	3.375	631	633	638	rVB2	229	190	0.01%	0.002%
17	3.694	729	732	735	rBV	249	227	0.01%	0.002%
18	3.755	747	751	755	rVB2	225	223	0.01%	0.002%
19	3.838	769	777	781	rBV2	257	355	0.02%	0.003%
20	3.925	801	804	807	rVB	276	215	0.01%	0.002%
21	4.018	828	833	837	rVB2	249	281	0.02%	0.002%
22	4.041	837	840	843	rBV2	223	182	0.01%	0.002%
23	4.462	965	971	974	rBV2	266	382	0.02%	0.003%
24	4.620	1007	1020	1050	rBV	165326	413267	25.81%	3.438%
25	5.063	1140	1158	1184	rBV	288804	628015	39.22%	5.224%
26	5.192	1195	1198	1201	rVB3	303	232	0.01%	0.002%
27	5.214	1201	1205	1207	rBV2	358	283	0.02%	0.002%
28	5.227	1207	1209	1213	rVV2	262	173	0.01%	0.001%
29	5.417	1264	1268	1270	rBV	226	181	0.01%	0.002%
30	5.722	1341	1363	1393	rBV2	598288	1601080	100.00%	13.318%
31	5.964	1433	1438	1441	rBV3	979	1066	0.07%	0.009%
32	6.038	1457	1461	1464	rBV3	458	454	0.03%	0.004%
33	6.057	1464	1467	1469	rVB3	369	226	0.01%	0.002%
34	6.124	1486	1488	1492	rVB3	569	359	0.02%	0.003%
35	6.169	1498	1502	1512	rVB3	318	372	0.02%	0.003%
36	6.250	1512	1527	1550	rBV	377484	717542	44.82%	5.969%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
 Data File : VU048305.D
 Acq On : 27 Apr 2022 11:29
 Operator : SY/MD
 Sample : VU0427WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK103

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.423	1578	1581	1585	rVB2	382	314	0.02%	0.003%
38	6.526	1606	1613	1616	rBV2	1773	2344	0.15%	0.019%
39	6.578	1625	1629	1630	rBV2	237	156	0.01%	0.001%
40	6.690	1648	1664	1691	rVV	369668	723588	45.19%	6.019%
41	6.928	1736	1738	1742	rVB2	292	168	0.01%	0.001%
42	6.960	1742	1748	1753	rBV3	366	521	0.03%	0.004%
43	7.050	1774	1776	1781	rVV2	323	273	0.02%	0.002%
44	7.105	1790	1793	1797	rBV3	297	239	0.01%	0.002%
45	7.176	1804	1815	1826	rBV3	3643	8145	0.51%	0.068%
46	7.327	1859	1862	1870	rBV2	190	226	0.01%	0.002%
47	7.565	1916	1936	1959	rBV	194128	343008	21.42%	2.853%
48	7.645	1959	1961	1968	rVV3	818	981	0.06%	0.008%
49	7.677	1968	1971	1972	rVV3	797	490	0.03%	0.004%
50	7.690	1973	1975	1986	rVB5	1324	1711	0.11%	0.014%
51	7.783	2000	2004	2006	rBV2	772	560	0.03%	0.005%
52	7.899	2025	2040	2056	rBV	732950	1260561	78.73%	10.485%
53	8.179	2115	2127	2146	rBV	139734	237716	14.85%	1.977%
54	8.385	2187	2191	2194	rBV4	464	395	0.02%	0.003%
55	8.407	2194	2198	2201	rVV3	405	370	0.02%	0.003%
56	8.459	2211	2214	2216	rBV2	431	342	0.02%	0.003%
57	8.475	2216	2219	2221	rVV2	328	216	0.01%	0.002%
58	8.549	2239	2242	2244	rBV2	259	179	0.01%	0.001%
59	8.636	2254	2269	2307	rBV	524391	1005188	62.78%	8.361%
60	8.954	2366	2368	2373	rVB3	487	318	0.02%	0.003%
61	8.999	2374	2382	2384	rBV2	442	453	0.03%	0.004%
62	9.012	2384	2386	2390	rVV2	420	285	0.02%	0.002%
63	9.070	2400	2404	2409	rVB3	501	397	0.02%	0.003%
64	9.137	2422	2425	2429	rBV	227	191	0.01%	0.002%
65	9.166	2429	2434	2441	rVB4	469	637	0.04%	0.005%
66	9.198	2441	2444	2448	rBV3	425	301	0.02%	0.003%
67	9.417	2499	2512	2542	rVV	571335	955674	59.69%	7.949%
68	9.645	2581	2583	2586	rVV3	444	266	0.02%	0.002%
69	9.697	2591	2599	2605	rBV3	916	1412	0.09%	0.012%
70	9.835	2639	2642	2646	rBV	246	166	0.01%	0.001%
71	9.925	2666	2670	2671	rBV	271	208	0.01%	0.002%
72	10.044	2702	2707	2710	rBV2	290	274	0.02%	0.002%
73	10.099	2719	2724	2725	rBV2	768	628	0.04%	0.005%
74	10.491	2840	2846	2852	rVB2	544	706	0.04%	0.006%
75	10.671	2895	2902	2910	rBV4	2446	3018	0.19%	0.025%
76	10.758	2916	2929	2952	rBV	631086	1011499	63.18%	8.414%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
 Data File : VU048305.D
 Acq On : 27 Apr 2022 11:29
 Operator : SY/MD
 Sample : VU0427WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK103

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.867	2960	2963	2965	rBV4	314	205	0.01%	0.002%
78	10.893	2965	2971	2975	rVV5	611	825	0.05%	0.007%
79	11.095	3030	3034	3036	rBV3	276	261	0.02%	0.002%
80	11.185	3059	3062	3065	rBV2	211	170	0.01%	0.001%
81	11.417	3132	3134	3139	rVB4	336	198	0.01%	0.002%
82	11.455	3139	3146	3147	rBV3	1353	1220	0.08%	0.010%
83	11.507	3159	3162	3164	rBV	367	248	0.02%	0.002%
84	11.655	3206	3208	3215	rVB3	313	241	0.02%	0.002%
85	11.693	3216	3220	3228	rVB4	899	991	0.06%	0.008%
86	11.748	3232	3237	3244	rVB2	1267	1356	0.08%	0.011%
87	11.812	3244	3257	3278	rBV	555742	883234	55.16%	7.347%
88	11.973	3303	3307	3314	rVB4	1850	2002	0.13%	0.017%
89	12.012	3316	3319	3323	rVV2	319	239	0.01%	0.002%
90	12.195	3362	3376	3402	rBV	712161	1155471	72.17%	9.611%
91	12.481	3462	3465	3469	rVB	398	253	0.02%	0.002%
92	12.770	3548	3555	3560	rBV3	1232	1650	0.10%	0.014%
93	12.844	3576	3578	3584	rVB2	442	406	0.03%	0.003%
94	12.893	3590	3593	3594	rBV	411	237	0.01%	0.002%
95	12.915	3598	3600	3603	rVV2	315	179	0.01%	0.001%
96	13.124	3662	3665	3670	rBV3	485	517	0.03%	0.004%
97	13.848	3884	3890	3900	rBV5	2029	3032	0.19%	0.025%
98	14.098	3960	3968	3979	rVB2	3809	6787	0.42%	0.056%
99	14.240	4010	4012	4015	rBV	399	311	0.02%	0.003%
100	14.333	4035	4041	4051	rVB5	2626	3835	0.24%	0.032%




Sum of corrected areas: 12022001

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
Data File : VU048305.D
Acq On : 27 Apr 2022 11:29
Operator : SY/MD
Sample : VU0427WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK103

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

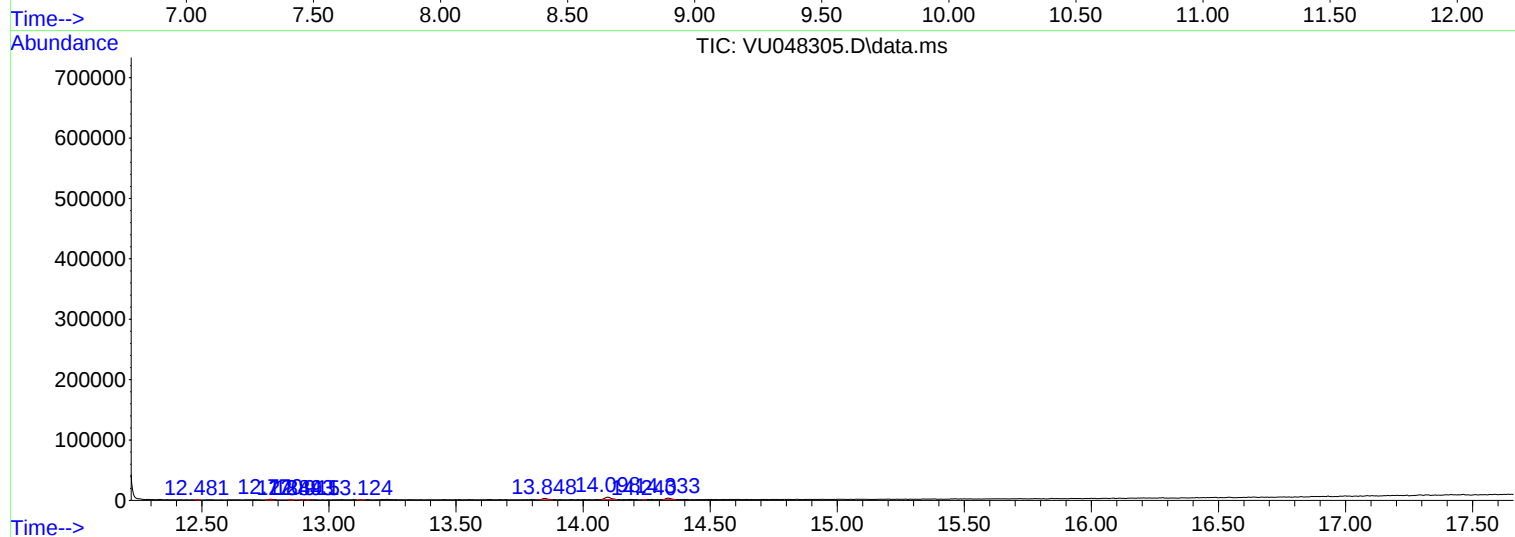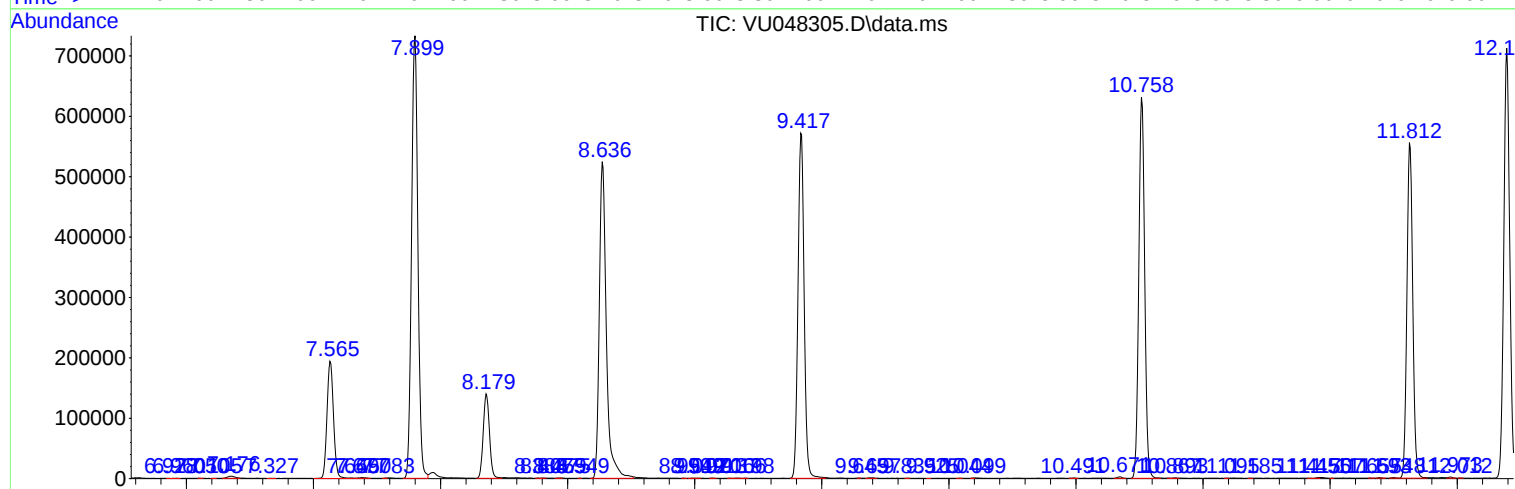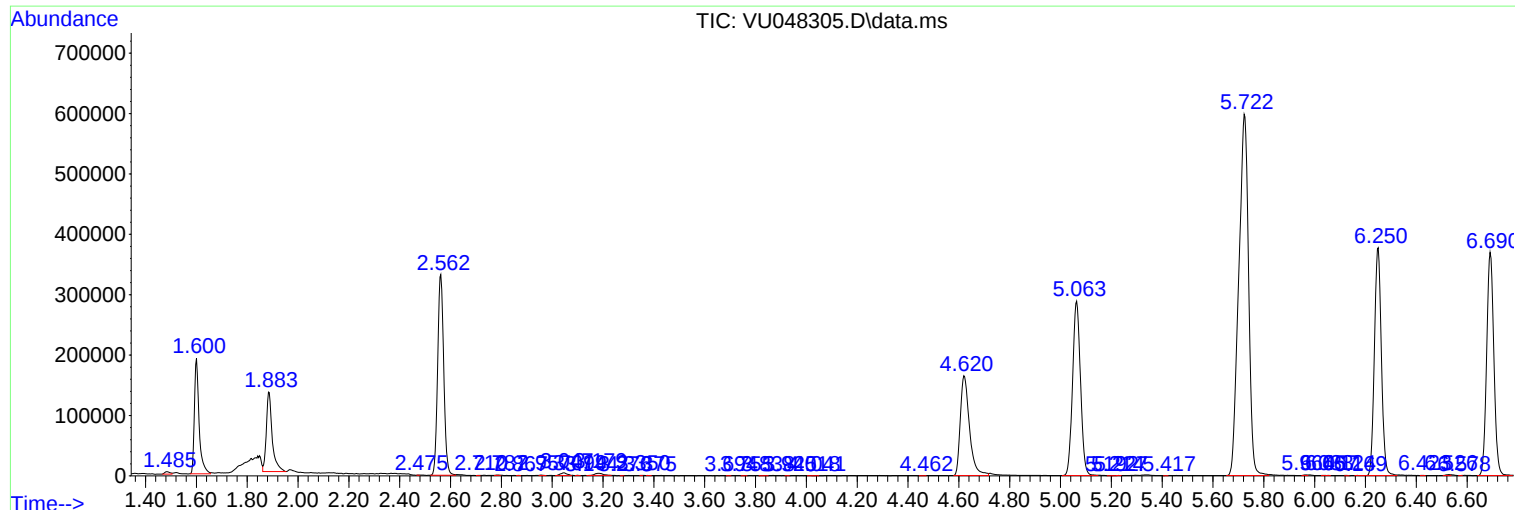

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
Data File : VU048305.D
Acq On : 27 Apr 2022 11:29
Operator : SY/MD
Sample : VU0427WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK103

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
Data File : VU048305.D
Acq On : 27 Apr 2022 11:29
Operator : SY/MD
Sample : VU0427WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK103

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------