

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
 Data File : VU048306.D
 Acq On : 27 Apr 2022 11:53
 Operator : SY/MD
 Sample : VU0427WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK104

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M

Title : VOC Analysis

Signal : TIC: VU048306.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.482	41	44	51	rVB2	3639	3489	0.22%	0.030%
2	1.601	73	81	100	rBV	186427	236817	15.17%	2.041%
3	1.896	165	173	187	rBV	126866	182718	11.70%	1.575%
4	2.491	355	358	361	rBV	424	204	0.01%	0.002%
5	2.565	368	381	400	rBV	317593	525516	33.66%	4.530%
6	2.736	430	434	440	rBV3	346	495	0.03%	0.004%
7	2.945	497	499	501	rBV2	284	181	0.01%	0.002%
8	3.044	518	530	546	rBV3	4612	9519	0.61%	0.082%
9	3.186	559	574	596	rBV	9234	22464	1.44%	0.194%
10	3.356	624	627	630	rBV2	334	188	0.01%	0.002%
11	3.385	633	636	640	rVB2	290	218	0.01%	0.002%
12	3.578	694	696	701	rVB2	237	220	0.01%	0.002%
13	3.613	701	707	711	rBV	317	377	0.02%	0.003%
14	3.642	711	716	721	rBV2	147	205	0.01%	0.002%
15	3.768	751	755	757	rBV2	209	183	0.01%	0.002%
16	3.832	769	775	780	rVB2	217	252	0.02%	0.002%
17	3.861	780	784	788	rBV2	236	248	0.02%	0.002%
18	4.121	862	865	871	rVB	260	278	0.02%	0.002%
19	4.160	874	877	879	rVV	255	166	0.01%	0.001%
20	4.182	880	884	887	rVV2	217	203	0.01%	0.002%
21	4.462	968	971	976	rBV	209	173	0.01%	0.001%
22	4.620	1006	1020	1044	rBV	178226	434647	27.84%	3.746%
23	4.829	1083	1085	1089	rBV3	323	218	0.01%	0.002%
24	5.063	1140	1158	1179	rBV	281429	612712	39.24%	5.281%
25	5.211	1200	1204	1207	rBV	375	339	0.02%	0.003%
26	5.276	1220	1224	1225	rBV	283	209	0.01%	0.002%
27	5.327	1236	1240	1243	rBV2	621	615	0.04%	0.005%
28	5.391	1255	1260	1265	rVB2	235	206	0.01%	0.002%
29	5.530	1297	1303	1307	rBV	187	204	0.01%	0.002%
30	5.645	1334	1339	1341	rBV2	171	165	0.01%	0.001%
31	5.726	1342	1364	1389	rBV2	576353	1561475	100.00%	13.459%
32	5.970	1437	1440	1442	rBV	274	158	0.01%	0.001%
33	6.076	1470	1473	1476	rVB2	362	227	0.01%	0.002%
34	6.112	1476	1484	1486	rBV3	483	456	0.03%	0.004%
35	6.157	1491	1498	1503	rBV	245	264	0.02%	0.002%
36	6.250	1509	1527	1549	rBV	377246	719280	46.06%	6.200%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
 Data File : VU048306.D
 Acq On : 27 Apr 2022 11:53
 Operator : SY/MD
 Sample : VU0427WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK104

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.375	1562	1566	1569	rBV3	403	258	0.02%	0.002%
38	6.420	1577	1580	1586	rVB2	355	342	0.02%	0.003%
39	6.491	1598	1602	1607	rBV2	214	261	0.02%	0.002%
40	6.571	1624	1627	1630	rBV2	236	185	0.01%	0.002%
41	6.690	1649	1664	1684	rBV	361931	703814	45.07%	6.066%
42	6.806	1696	1700	1708	rVB3	1075	1339	0.09%	0.012%
43	7.115	1793	1796	1798	rBV2	240	160	0.01%	0.001%
44	7.173	1804	1814	1818	rBV3	2268	3827	0.25%	0.033%
45	7.333	1860	1864	1866	rBV	429	237	0.02%	0.002%
46	7.394	1878	1883	1888	rBV2	192	240	0.02%	0.002%
47	7.565	1923	1936	1954	rBV	192958	335163	21.46%	2.889%
48	7.690	1969	1975	1983	rVB6	854	1356	0.09%	0.012%
49	7.787	2001	2005	2015	rVB5	1106	1418	0.09%	0.012%
50	7.899	2025	2040	2056	rBV	706542	1215890	77.87%	10.480%
51	8.050	2084	2087	2090	rBV2	394	291	0.02%	0.003%
52	8.179	2115	2127	2144	rBV	137301	227974	14.60%	1.965%
53	8.266	2151	2154	2157	rBV4	444	331	0.02%	0.003%
54	8.513	2228	2231	2235	rBV3	449	370	0.02%	0.003%
55	8.587	2249	2254	2256	rBV2	273	182	0.01%	0.002%
56	8.636	2256	2269	2304	rBV	526857	985272	63.10%	8.492%
57	8.857	2335	2338	2340	rBV2	416	232	0.01%	0.002%
58	8.877	2340	2344	2346	rVV2	259	165	0.01%	0.001%
59	9.015	2384	2387	2391	rBV2	257	203	0.01%	0.002%
60	9.050	2395	2398	2401	rBV2	303	214	0.01%	0.002%
61	9.073	2401	2405	2408	rVB3	241	197	0.01%	0.002%
62	9.105	2412	2415	2421	rVB3	317	241	0.02%	0.002%
63	9.234	2452	2455	2457	rBV	269	161	0.01%	0.001%
64	9.417	2498	2512	2545	rBV	563044	940053	60.20%	8.103%
65	9.568	2555	2559	2562	rBV3	451	411	0.03%	0.004%
66	9.645	2580	2583	2590	rVB3	656	491	0.03%	0.004%
67	9.697	2591	2599	2604	rBV2	1089	1449	0.09%	0.012%
68	9.787	2623	2627	2630	rBV2	181	166	0.01%	0.001%
69	9.890	2655	2659	2666	rBV3	366	477	0.03%	0.004%
70	9.947	2675	2677	2680	rVB2	407	172	0.01%	0.001%
71	10.105	2717	2726	2728	rBV3	569	801	0.05%	0.007%
72	10.259	2770	2774	2778	rBV2	294	256	0.02%	0.002%
73	10.282	2778	2781	2785	rBV2	307	251	0.02%	0.002%
74	10.468	2835	2839	2840	rBV	275	217	0.01%	0.002%
75	10.574	2870	2872	2875	rBV2	292	184	0.01%	0.002%
76	10.671	2894	2902	2910	rVB3	1895	2627	0.17%	0.023%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
 Data File : VU048306.D
 Acq On : 27 Apr 2022 11:53
 Operator : SY/MD
 Sample : VU0427WBL02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK104

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.706	2910	2913	2916	rBV2	238	168	0.01%	0.001%
78	10.758	2916	2929	2947	rBV	596251	959391	61.44%	8.269%
79	10.861	2957	2961	2965	rBV4	449	381	0.02%	0.003%
80	10.880	2965	2967	2974	rVV5	348	359	0.02%	0.003%
81	11.012	3006	3008	3012	rVB2	304	182	0.01%	0.002%
82	11.099	3030	3035	3038	rBV3	348	279	0.02%	0.002%
83	11.115	3038	3040	3042	rBV2	379	199	0.01%	0.002%
84	11.205	3066	3068	3071	rVB	326	176	0.01%	0.002%
85	11.462	3140	3148	3157	rVB4	1592	2543	0.16%	0.022%
86	11.613	3191	3195	3203	rVB	401	510	0.03%	0.004%
87	11.655	3203	3208	3210	rBV2	225	228	0.01%	0.002%
88	11.697	3217	3221	3224	rVB2	588	485	0.03%	0.004%
89	11.745	3231	3236	3242	rBV3	663	600	0.04%	0.005%
90	11.812	3245	3257	3279	rBV	509774	832487	53.31%	7.175%
91	12.028	3321	3324	3331	rVB	287	195	0.01%	0.002%
92	12.060	3331	3334	3335	rBV2	355	188	0.01%	0.002%
93	12.195	3361	3376	3396	rBV	644088	1056464	67.66%	9.106%
94	12.520	3474	3477	3482	rBV3	301	277	0.02%	0.002%
95	12.590	3497	3499	3504	rVB2	419	181	0.01%	0.002%
96	12.684	3524	3528	3531	rBV3	394	403	0.03%	0.003%
97	12.748	3545	3548	3549	rBV2	288	161	0.01%	0.001%
98	12.764	3549	3553	3554	rBV	671	408	0.03%	0.004%
99	12.970	3612	3617	3620	rBV3	359	382	0.02%	0.003%
100	14.095	3963	3967	3975	rVB3	1544	2189	0.14%	0.019%




Sum of corrected areas: 11602003

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
Data File : VU048306.D
Acq On : 27 Apr 2022 11:53
Operator : SY/MD
Sample : VU0427WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK104

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

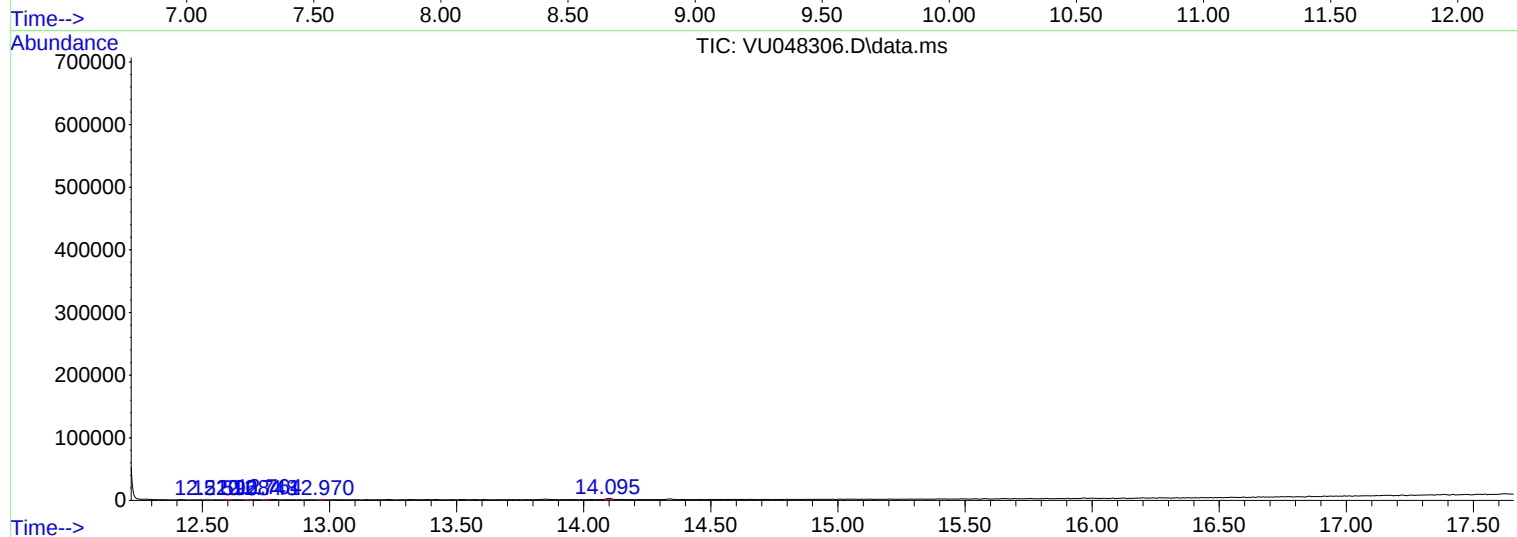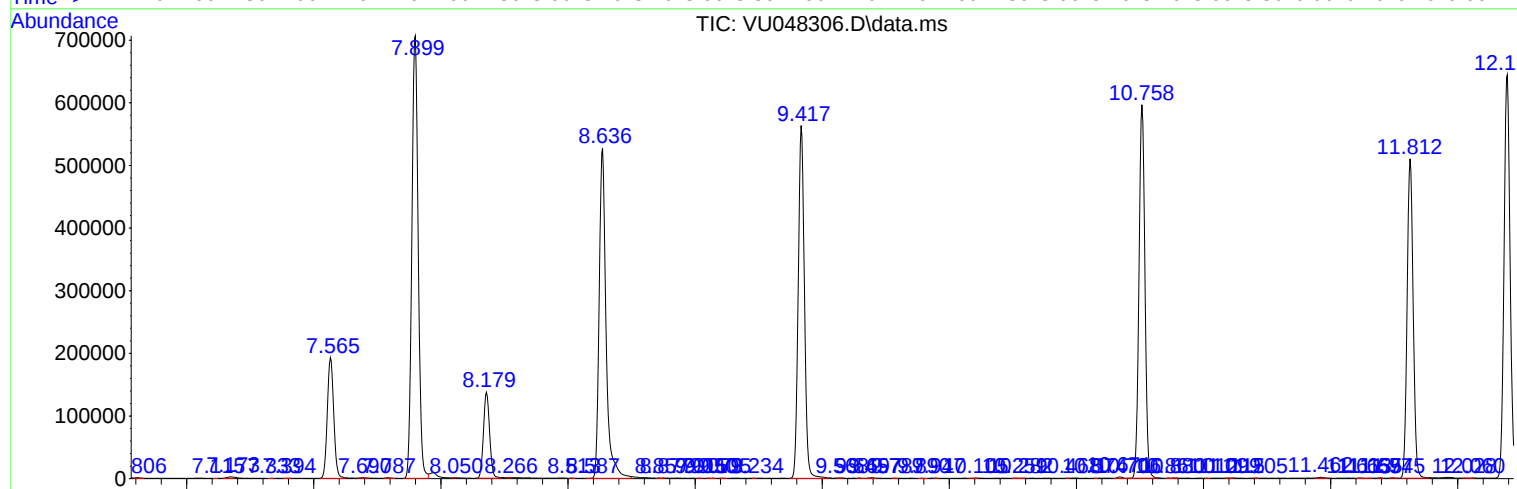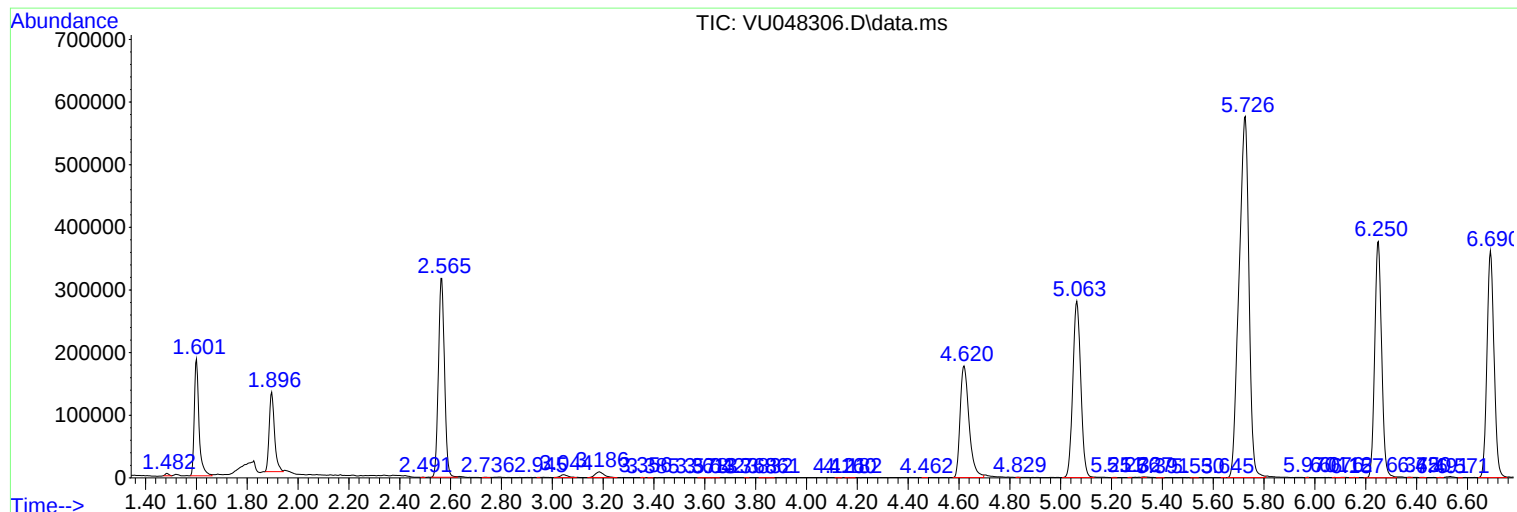

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
Data File : VU048306.D
Acq On : 27 Apr 2022 11:53
Operator : SY/MD
Sample : VU0427WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK104

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
Data File : VU048306.D
Acq On : 27 Apr 2022 11:53
Operator : SY/MD
Sample : VU0427WBL02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK104

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------