

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
 Data File : VU048310.D
 Acq On : 27 Apr 2022 13:31
 Operator : SY/MD
 Sample : N2518-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXES7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048310.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.491	40	47	53	rBV2	24549	29625	1.80%	0.238%
2	1.600	73	81	99	rVB	195118	244098	14.85%	1.962%
3	1.890	163	171	190	rVB	137480	206617	12.57%	1.660%
4	2.469	349	351	355	rBV3	295	162	0.01%	0.001%
5	2.562	367	380	393	rBV	339592	553618	33.68%	4.449%
6	2.626	394	400	415	rVB	17958	29762	1.81%	0.239%
7	2.780	445	448	449	rBV2	396	229	0.01%	0.002%
8	2.825	460	462	465	rVB2	284	177	0.01%	0.001%
9	2.851	465	470	472	rBV3	286	269	0.02%	0.002%
10	2.899	476	485	486	rBV2	1574	1714	0.10%	0.014%
11	2.951	498	501	509	rVB2	999	1224	0.07%	0.010%
12	3.041	524	529	536	rBV4	1100	1435	0.09%	0.012%
13	3.079	539	541	544	rVB	314	171	0.01%	0.001%
14	3.096	544	546	549	rBV	322	167	0.01%	0.001%
15	3.189	560	575	590	rBV2	5219	12639	0.77%	0.102%
16	3.317	611	615	618	rBV2	218	179	0.01%	0.001%
17	3.427	646	649	653	rVB2	354	225	0.01%	0.002%
18	3.575	688	695	697	rBV5	817	775	0.05%	0.006%
19	3.639	710	715	720	rVB2	271	275	0.02%	0.002%
20	3.739	742	746	749	rBV2	257	282	0.02%	0.002%
21	3.980	818	821	826	rBV2	170	170	0.01%	0.001%
22	4.398	947	951	954	rBV2	271	270	0.02%	0.002%
23	4.433	958	962	965	rBV	361	359	0.02%	0.003%
24	4.555	987	1000	1006	rBV3	2736	6246	0.38%	0.050%
25	4.620	1007	1020	1042	rBV	165152	406493	24.73%	3.267%
26	4.964	1124	1127	1133	rVB	294	242	0.01%	0.002%
27	5.063	1138	1158	1186	rBV	294258	641698	39.04%	5.157%
28	5.282	1224	1226	1228	rBV	304	212	0.01%	0.002%
29	5.491	1288	1291	1296	rVB	259	250	0.02%	0.002%
30	5.578	1313	1318	1321	rBV2	332	373	0.02%	0.003%
31	5.726	1341	1364	1405	rVV2	608269	1643626	100.00%	13.209%
32	5.970	1435	1440	1447	rVB5	1165	1463	0.09%	0.012%
33	6.038	1460	1461	1468	rVB	314	188	0.01%	0.002%
34	6.095	1474	1479	1481	rBV	294	216	0.01%	0.002%
35	6.128	1486	1489	1492	rVB2	350	260	0.02%	0.002%
36	6.160	1496	1499	1503	rBV2	422	296	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
 Data File : VU048310.D
 Acq On : 27 Apr 2022 13:31
 Operator : SY/MD
 Sample : N2518-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXES7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.250	1511	1527	1558	rBV	418009	795218	48.38%	6.391%
38	6.365	1561	1563	1565	rVV2	962	572	0.03%	0.005%
39	6.391	1569	1571	1576	rVB4	329	255	0.02%	0.002%
40	6.488	1597	1601	1602	rBV2	334	179	0.01%	0.001%
41	6.526	1605	1613	1622	rVB5	1360	2259	0.14%	0.018%
42	6.562	1622	1624	1627	rVB2	486	208	0.01%	0.002%
43	6.581	1627	1630	1631	rBV3	348	197	0.01%	0.002%
44	6.690	1649	1664	1691	rBV	381540	731697	44.52%	5.880%
45	6.835	1708	1709	1716	rVB	467	366	0.02%	0.003%
46	6.893	1716	1727	1730	rBV3	435	622	0.04%	0.005%
47	6.931	1737	1739	1742	rVB	350	230	0.01%	0.002%
48	7.037	1765	1772	1773	rBV2	485	472	0.03%	0.004%
49	7.121	1796	1798	1804	rVB3	290	273	0.02%	0.002%
50	7.173	1804	1814	1825	rBV4	3340	7077	0.43%	0.057%
51	7.246	1833	1837	1840	rBV2	365	359	0.02%	0.003%
52	7.330	1859	1863	1865	rBV	289	218	0.01%	0.002%
53	7.488	1907	1912	1914	rBV2	319	369	0.02%	0.003%
54	7.565	1923	1936	1952	rBV	200403	344150	20.94%	2.766%
55	7.764	1996	1998	2002	rVB	389	239	0.01%	0.002%
56	7.803	2002	2010	2015	rBV2	627	997	0.06%	0.008%
57	7.899	2026	2040	2055	rBV	747500	1291546	78.58%	10.379%
58	8.134	2108	2113	2115	rBV2	275	226	0.01%	0.002%
59	8.179	2115	2127	2145	rBV	142990	237875	14.47%	1.912%
60	8.304	2164	2166	2170	rBV3	360	262	0.02%	0.002%
61	8.439	2205	2208	2210	rVV2	460	313	0.02%	0.003%
62	8.472	2211	2218	2228	rVB3	3758	5488	0.33%	0.044%
63	8.635	2254	2269	2309	rBV	521988	1010554	61.48%	8.121%
64	8.902	2350	2352	2354	rBV3	241	173	0.01%	0.001%
65	8.941	2362	2364	2369	rBV2	435	319	0.02%	0.003%
66	9.163	2429	2433	2435	rBV2	744	622	0.04%	0.005%
67	9.208	2441	2447	2452	rBV5	787	906	0.06%	0.007%
68	9.320	2478	2482	2487	rVB3	451	545	0.03%	0.004%
69	9.349	2487	2491	2493	rBV	300	205	0.01%	0.002%
70	9.417	2499	2512	2549	rBV	628614	1046233	63.65%	8.408%
71	9.642	2576	2582	2588	rVB3	624	853	0.05%	0.007%
72	9.671	2588	2591	2592	rBV	274	175	0.01%	0.001%
73	9.693	2593	2598	2612	rVB4	1020	1865	0.11%	0.015%
74	9.764	2616	2620	2625	rBV2	372	465	0.03%	0.004%
75	10.192	2751	2753	2760	rVB2	268	268	0.02%	0.002%
76	10.359	2799	2805	2810	rBV3	288	391	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
 Data File : VU048310.D
 Acq On : 27 Apr 2022 13:31
 Operator : SY/MD
 Sample : N2518-11
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXES7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.414	2820	2822	2826	rVB2	325	224	0.01%	0.002%
78	10.452	2830	2834	2837	rBV2	282	189	0.01%	0.002%
79	10.539	2857	2861	2864	rBV2	251	195	0.01%	0.002%
80	10.671	2895	2902	2910	rBV2	2629	3308	0.20%	0.027%
81	10.758	2915	2929	2949	rBV	630769	1016930	61.87%	8.172%
82	10.893	2962	2971	2984	rVB2	6069	10940	0.67%	0.088%
83	11.414	3131	3133	3137	rVB3	603	433	0.03%	0.003%
84	11.452	3137	3145	3146	rBV2	1668	1437	0.09%	0.012%
85	11.696	3215	3221	3226	rVB4	743	988	0.06%	0.008%
86	11.812	3244	3257	3281	rBV	599137	959691	58.39%	7.712%
87	12.060	3332	3334	3336	rVV2	557	304	0.02%	0.002%
88	12.073	3336	3338	3341	rVB2	417	255	0.02%	0.002%
89	12.195	3362	3376	3397	rBV	713616	1170837	71.24%	9.409%
90	12.333	3415	3419	3423	rBV4	608	515	0.03%	0.004%
91	12.500	3467	3471	3473	rBV2	392	320	0.02%	0.003%
92	12.561	3488	3490	3494	rVB2	460	317	0.02%	0.003%
93	12.590	3494	3499	3502	rBV3	418	362	0.02%	0.003%
94	12.777	3547	3557	3563	rVB3	1905	3157	0.19%	0.025%
95	13.089	3650	3654	3656	rBV2	430	293	0.02%	0.002%
96	13.278	3710	3713	3716	rVB3	305	204	0.01%	0.002%
97	13.532	3790	3792	3795	rBV2	283	185	0.01%	0.001%
98	14.278	4021	4024	4027	rBV2	441	278	0.02%	0.002%
99	14.333	4038	4041	4048	rBV3	455	585	0.04%	0.005%
100	14.934	4226	4228	4232	rBV3	527	358	0.02%	0.003%


Sum of corrected areas: 12443551

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
Data File : VU048310.D
Acq On : 27 Apr 2022 13:31
Operator : SY/MD
Sample : N2518-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXES7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

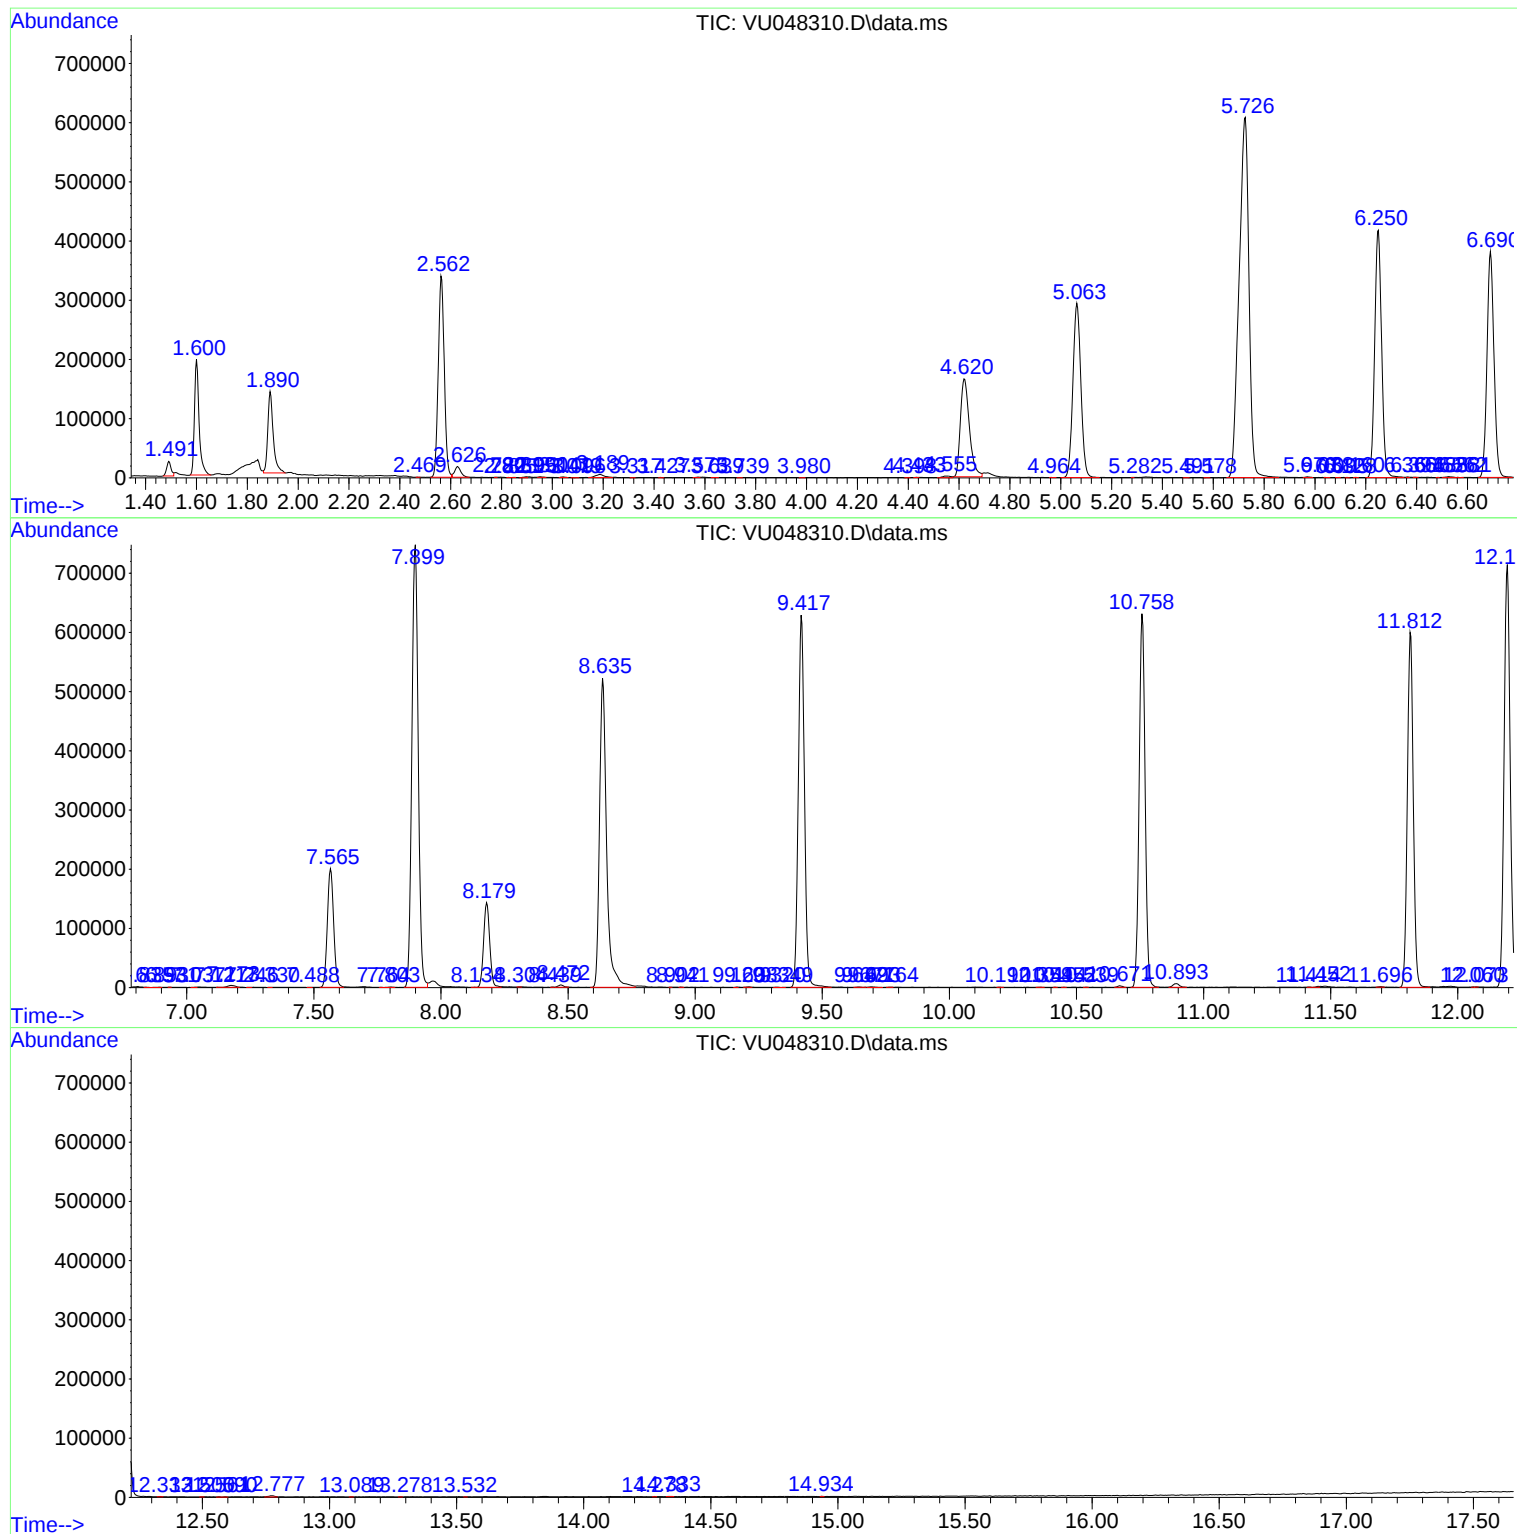

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
Data File : VU048310.D
Acq On : 27 Apr 2022 13:31
Operator : SY/MD
Sample : N2518-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXES7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
Data File : VU048310.D
Acq On : 27 Apr 2022 13:31
Operator : SY/MD
Sample : N2518-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXES7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc