

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
 Data File : VU048315.D
 Acq On : 27 Apr 2022 15:26
 Operator : SY/MD
 Sample : N2587-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXES9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048315.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.488	40	46	52	rBV4	6860	10027	0.63%	0.084%
2	1.520	53	56	66	rVB	5589	6201	0.39%	0.052%
3	1.601	72	81	101	rBV	189240	242286	15.34%	2.024%
4	1.890	163	171	189	rVB	127923	196772	12.46%	1.644%
5	2.562	367	380	392	rBV	328912	533383	33.78%	4.456%
6	2.626	393	400	413	rVV	25524	46321	2.93%	0.387%
7	2.674	413	415	419	rVV3	1162	872	0.06%	0.007%
8	2.710	423	426	428	rBV2	360	208	0.01%	0.002%
9	2.797	448	453	457	rVV5	672	727	0.05%	0.006%
10	2.816	457	459	462	rVB	352	186	0.01%	0.002%
11	2.896	477	484	486	rBV2	1373	1445	0.09%	0.012%
12	3.006	516	518	522	rBV2	388	188	0.01%	0.002%
13	3.044	522	530	539	rVV6	978	1818	0.12%	0.015%
14	3.189	560	575	587	rBV3	4645	12386	0.78%	0.103%
15	3.343	619	623	625	rBV2	248	195	0.01%	0.002%
16	3.427	645	649	652	rVB	324	199	0.01%	0.002%
17	3.446	652	655	657	rBV2	312	213	0.01%	0.002%
18	3.520	674	678	680	rBV2	295	212	0.01%	0.002%
19	3.568	688	693	695	rBV2	866	709	0.04%	0.006%
20	3.867	785	786	792	rVB2	181	162	0.01%	0.001%
21	3.903	792	797	802	rBV2	131	177	0.01%	0.001%
22	4.047	840	842	848	rBV2	234	178	0.01%	0.001%
23	4.144	866	872	874	rBV2	287	252	0.02%	0.002%
24	4.269	908	911	916	rVB3	289	241	0.02%	0.002%
25	4.440	952	964	975	rVB6	1622	3177	0.20%	0.027%
26	4.523	985	990	991	rBV	404	274	0.02%	0.002%
27	4.555	991	1000	1005	rBV4	1376	2611	0.17%	0.022%
28	4.620	1007	1020	1041	rBV	172395	419001	26.53%	3.501%
29	5.063	1141	1158	1181	rBV	278932	611215	38.71%	5.107%
30	5.179	1192	1194	1197	rVB3	449	203	0.01%	0.002%
31	5.289	1222	1228	1232	rBV3	405	567	0.04%	0.005%
32	5.388	1256	1259	1261	rBV	288	180	0.01%	0.002%
33	5.440	1270	1275	1279	rBV2	314	427	0.03%	0.004%
34	5.723	1341	1363	1396	rBV2	586902	1579155	100.00%	13.194%
35	5.980	1434	1443	1448	rVB5	1004	1486	0.09%	0.012%
36	6.025	1453	1457	1464	rBV3	546	789	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
 Data File : VU048315.D
 Acq On : 27 Apr 2022 15:26
 Operator : SY/MD
 Sample : N2587-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXES9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.115	1482	1485	1486	rBV	273	183	0.01%	0.002%
38	6.160	1494	1499	1503	rVB	371	424	0.03%	0.004%
39	6.247	1512	1526	1546	rBV	390186	740293	46.88%	6.185%
40	6.362	1559	1562	1567	rBV4	769	603	0.04%	0.005%
41	6.391	1567	1571	1573	rBV3	558	381	0.02%	0.003%
42	6.452	1586	1590	1599	rVB6	500	634	0.04%	0.005%
43	6.530	1607	1614	1619	rBV4	1683	2348	0.15%	0.020%
44	6.581	1627	1630	1631	rBV	525	261	0.02%	0.002%
45	6.690	1649	1664	1689	rBV	362917	710972	45.02%	5.940%
46	6.803	1696	1699	1709	rVB4	1057	1432	0.09%	0.012%
47	7.083	1785	1786	1790	rVB	340	189	0.01%	0.002%
48	7.124	1790	1799	1806	rBV7	858	1757	0.11%	0.015%
49	7.179	1807	1816	1828	rVB5	2905	5863	0.37%	0.049%
50	7.259	1837	1841	1844	rBV	210	190	0.01%	0.002%
51	7.372	1872	1876	1879	rBV2	400	378	0.02%	0.003%
52	7.420	1887	1891	1895	rVB3	195	161	0.01%	0.001%
53	7.507	1915	1918	1921	rBV	274	188	0.01%	0.002%
54	7.565	1921	1936	1954	rBV	189484	329891	20.89%	2.756%
55	7.687	1966	1974	1976	rBV5	1051	1183	0.07%	0.010%
56	7.748	1989	1993	2000	rBV2	300	405	0.03%	0.003%
57	7.790	2000	2006	2009	rBV2	432	518	0.03%	0.004%
58	7.896	2025	2039	2055	rBV	719871	1237417	78.36%	10.339%
59	8.179	2115	2127	2143	rBV	135348	226847	14.37%	1.895%
60	8.337	2174	2176	2181	rVB4	438	313	0.02%	0.003%
61	8.391	2191	2193	2198	rBV2	256	239	0.02%	0.002%
62	8.433	2204	2206	2209	rBV3	326	234	0.01%	0.002%
63	8.468	2210	2217	2226	rVV2	1939	2708	0.17%	0.023%
64	8.552	2240	2243	2247	rVB3	373	238	0.02%	0.002%
65	8.575	2247	2250	2253	rBV	283	161	0.01%	0.001%
66	8.636	2256	2269	2301	rBV2	521482	999265	63.28%	8.349%
67	9.012	2383	2386	2390	rVB	349	220	0.01%	0.002%
68	9.034	2390	2393	2397	rBV	440	267	0.02%	0.002%
69	9.095	2408	2412	2414	rBV2	348	294	0.02%	0.002%
70	9.317	2474	2481	2483	rBV3	290	331	0.02%	0.003%
71	9.417	2498	2512	2552	rVB	584160	976101	61.81%	8.155%
72	9.642	2579	2582	2589	rVB3	561	576	0.04%	0.005%
73	9.697	2592	2599	2605	rBV3	800	1158	0.07%	0.010%
74	9.899	2658	2662	2665	rBV2	392	354	0.02%	0.003%
75	10.021	2696	2700	2703	rBV2	225	159	0.01%	0.001%
76	10.176	2745	2748	2752	rVB2	335	225	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
 Data File : VU048315.D
 Acq On : 27 Apr 2022 15:26
 Operator : SY/MD
 Sample : N2587-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXES9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.353	2797	2803	2804	rBV3	653	593	0.04%	0.005%
78	10.671	2895	2902	2910	rVB4	2496	2969	0.19%	0.025%
79	10.758	2916	2929	2947	rBV	614751	983573	62.28%	8.218%
80	10.864	2960	2962	2963	rVV2	451	216	0.01%	0.002%
81	10.890	2963	2970	2981	rVB2	4152	6284	0.40%	0.053%
82	10.960	2989	2992	2994	rBV	313	196	0.01%	0.002%
83	11.105	3035	3037	3038	rBV	421	197	0.01%	0.002%
84	11.414	3129	3133	3134	rBV	516	283	0.02%	0.002%
85	11.481	3138	3154	3169	rBV5	7030	16274	1.03%	0.136%
86	11.562	3177	3179	3180	rBV5	333	163	0.01%	0.001%
87	11.648	3203	3206	3209	rVB	312	182	0.01%	0.002%
88	11.697	3215	3221	3227	rBV4	1039	1265	0.08%	0.011%
89	11.751	3233	3238	3241	rBV3	649	620	0.04%	0.005%
90	11.812	3245	3257	3278	rBV	566136	900885	57.05%	7.527%
91	11.912	3285	3288	3291	rBV3	434	351	0.02%	0.003%
92	11.944	3296	3298	3301	rVV3	1017	666	0.04%	0.006%
93	11.973	3301	3307	3314	rVB7	2019	2603	0.16%	0.022%
94	12.021	3320	3322	3326	rBV2	223	183	0.01%	0.002%
95	12.063	3326	3335	3348	rVV5	3032	6463	0.41%	0.054%
96	12.195	3362	3376	3398	rBV	683596	1122583	71.09%	9.379%
97	12.481	3463	3465	3468	rVB2	330	190	0.01%	0.002%
98	12.549	3482	3486	3488	rBV	364	244	0.02%	0.002%
99	12.774	3550	3556	3563	rVB2	1020	1582	0.10%	0.013%
100	13.224	3693	3696	3700	rVB2	447	314	0.02%	0.003%




Sum of corrected areas: 11968683

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
Data File : VU048315.D
Acq On : 27 Apr 2022 15:26
Operator : SY/MD
Sample : N2587-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXES9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

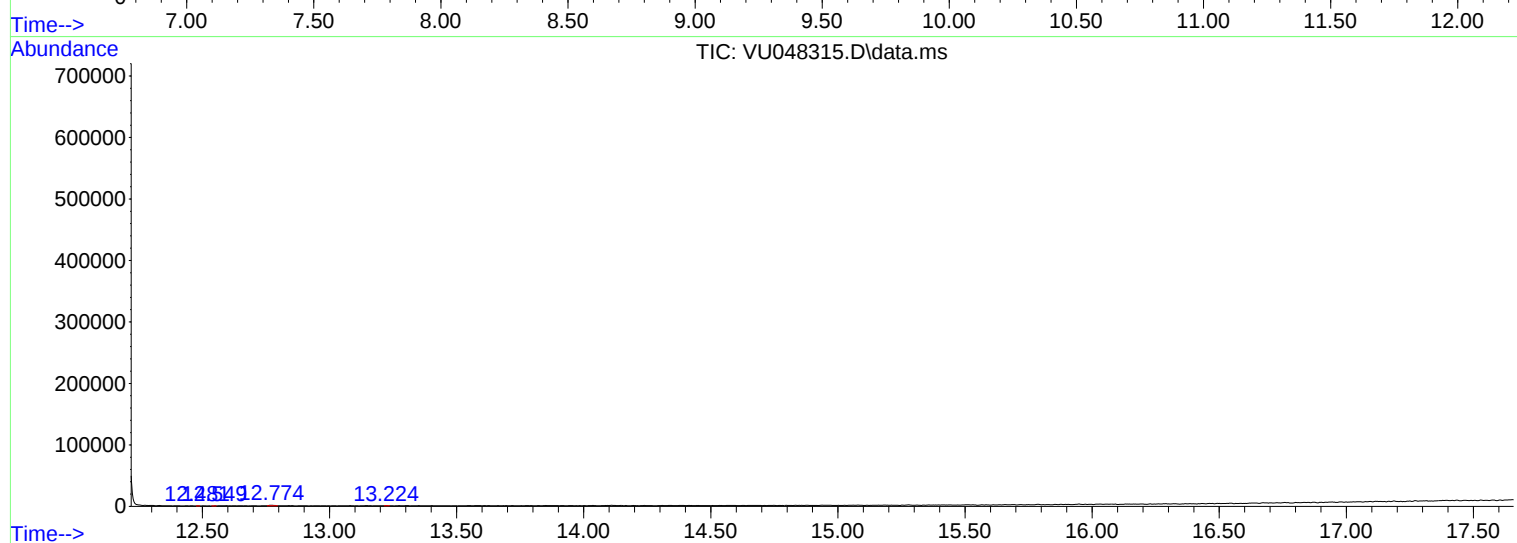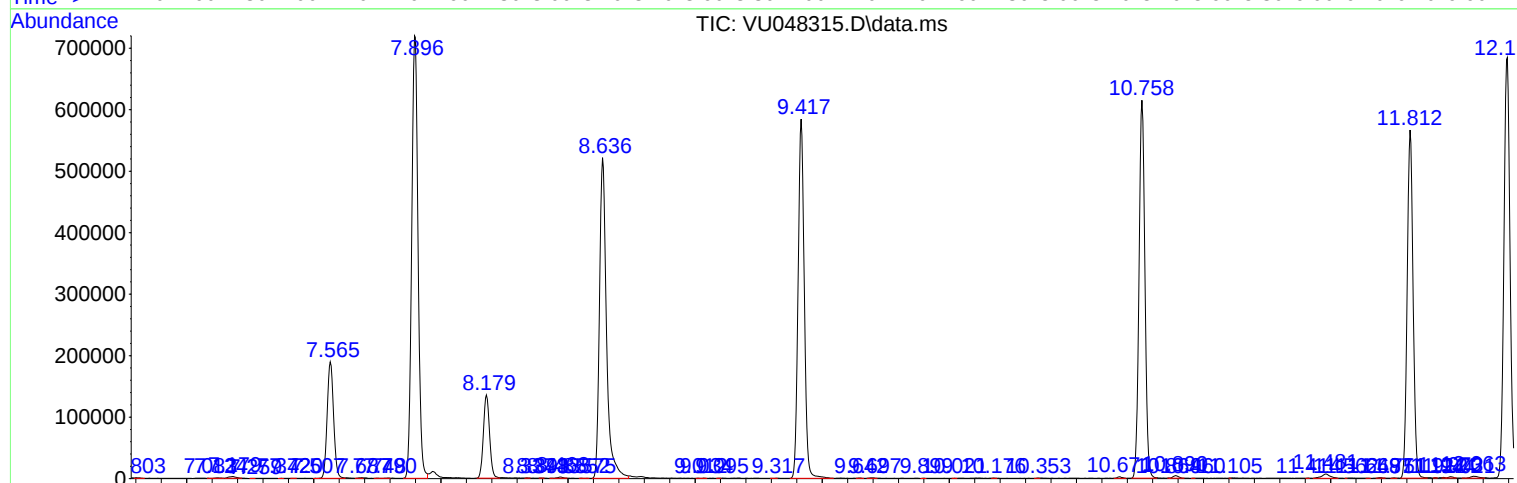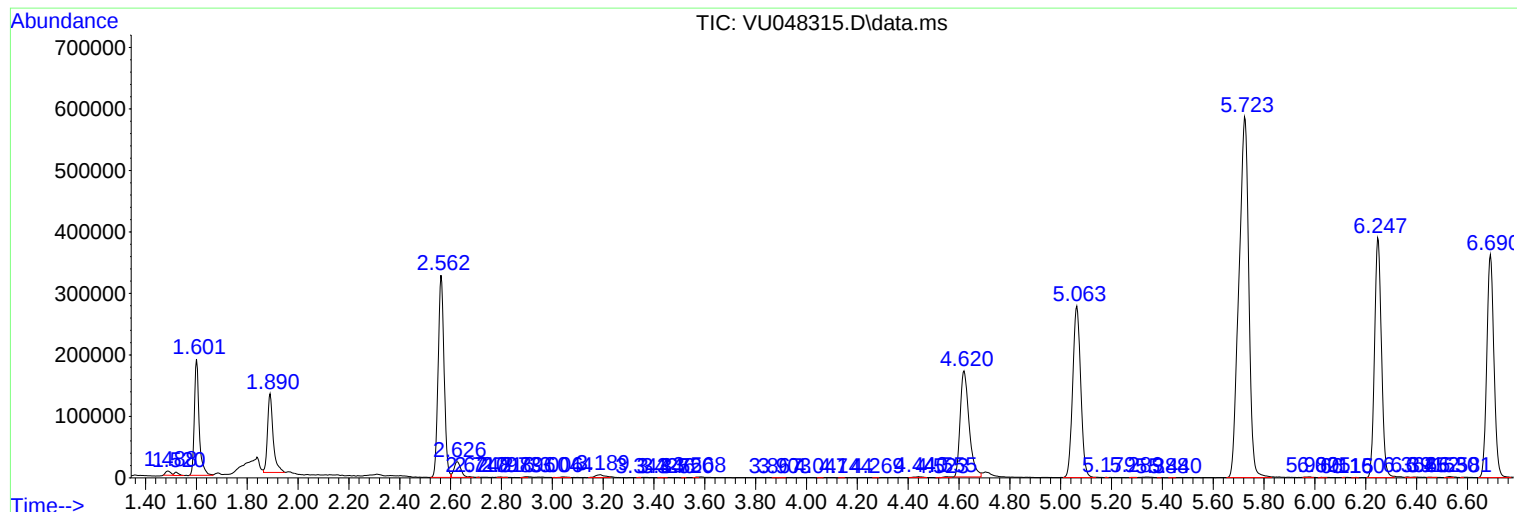

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
Data File : VU048315.D
Acq On : 27 Apr 2022 15:26
Operator : SY/MD
Sample : N2587-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXES9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
Data File : VU048315.D
Acq On : 27 Apr 2022 15:26
Operator : SY/MD
Sample : N2587-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXES9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------