

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
 Data File : VU048317.D
 Acq On : 27 Apr 2022 16:14
 Operator : SY/MD
 Sample : N2542-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048317.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.482	40	44	50	rBV	3920	4123	0.26%	0.035%
2	1.601	73	81	100	rBV	179868	231322	14.36%	1.947%
3	1.896	165	173	200	rVB	136814	213910	13.28%	1.800%
4	2.511	359	364	368	rBV3	525	554	0.03%	0.005%
5	2.565	368	381	397	rBV	329336	539653	33.49%	4.542%
6	2.720	425	429	433	rBV3	282	233	0.01%	0.002%
7	2.787	444	450	453	rBV3	539	723	0.04%	0.006%
8	2.803	453	455	458	rVV3	296	190	0.01%	0.002%
9	2.848	465	469	472	rVB2	293	227	0.01%	0.002%
10	2.880	477	479	490	rVB4	405	465	0.03%	0.004%
11	2.935	492	496	497	rBV2	209	153	0.01%	0.001%
12	3.048	517	531	551	rBV2	13000	28398	1.76%	0.239%
13	3.186	560	574	586	rBV	19677	49013	3.04%	0.412%
14	3.295	605	608	611	rBV2	261	150	0.01%	0.001%
15	3.340	619	622	625	rVB	366	266	0.02%	0.002%
16	3.446	651	655	658	rBV2	191	170	0.01%	0.001%
17	3.485	665	667	672	rVB2	190	154	0.01%	0.001%
18	3.585	695	698	702	rBV2	268	223	0.01%	0.002%
19	3.610	702	706	712	rBV2	155	204	0.01%	0.002%
20	3.729	730	743	749	rBV3	426	814	0.05%	0.007%
21	3.777	754	758	761	rVB2	271	196	0.01%	0.002%
22	3.855	777	782	785	rBV	201	237	0.01%	0.002%
23	4.015	830	832	835	rVB	278	171	0.01%	0.001%
24	4.038	835	839	843	rBV2	278	275	0.02%	0.002%
25	4.060	843	846	851	rBB2	268	218	0.01%	0.002%
26	4.173	879	881	885	rBV2	214	165	0.01%	0.001%
27	4.224	893	897	900	rBV2	242	159	0.01%	0.001%
28	4.401	949	952	957	rVB2	408	359	0.02%	0.003%
29	4.430	957	961	963	rBV	176	160	0.01%	0.001%
30	4.498	979	982	987	rBV2	204	198	0.01%	0.002%
31	4.552	996	999	1001	rBV2	325	206	0.01%	0.002%
32	4.572	1001	1005	1007	rBV2	250	212	0.01%	0.002%
33	4.623	1007	1021	1063	rBV	163592	423305	26.27%	3.562%
34	4.932	1112	1117	1119	rBV2	444	422	0.03%	0.004%
35	4.996	1133	1137	1141	rVB2	252	214	0.01%	0.002%
36	5.064	1141	1158	1182	rBV	290598	629554	39.07%	5.298%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
 Data File : VU048317.D
 Acq On : 27 Apr 2022 16:14
 Operator : SY/MD
 Sample : N2542-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	5.289	1216	1228	1231	rBV4	586	964	0.06%	0.008%
38	5.330	1234	1241	1242	rBV	438	465	0.03%	0.004%
39	5.388	1257	1259	1262	rBV	452	192	0.01%	0.002%
40	5.726	1342	1364	1395	rBV2	603589	1611203	100.00%	13.559%
41	5.967	1434	1439	1440	rBV3	853	611	0.04%	0.005%
42	6.025	1453	1457	1459	rBV	272	196	0.01%	0.002%
43	6.105	1480	1482	1485	rVV	247	147	0.01%	0.001%
44	6.154	1494	1497	1504	rVB2	485	443	0.03%	0.004%
45	6.250	1509	1527	1551	rBV	378072	725607	45.04%	6.107%
46	6.388	1567	1570	1574	rBV4	283	225	0.01%	0.002%
47	6.498	1602	1604	1606	rBV	370	156	0.01%	0.001%
48	6.536	1606	1616	1622	rBV6	1874	3165	0.20%	0.027%
49	6.691	1648	1664	1691	rBV	374337	726669	45.10%	6.115%
50	6.793	1692	1696	1698	rBV4	486	326	0.02%	0.003%
51	7.051	1771	1776	1782	rVB2	630	858	0.05%	0.007%
52	7.083	1782	1786	1787	rBV	433	286	0.02%	0.002%
53	7.105	1790	1793	1795	rVV2	282	175	0.01%	0.001%
54	7.176	1805	1815	1836	rVB6	2742	6528	0.41%	0.055%
55	7.285	1846	1849	1852	rBV	294	192	0.01%	0.002%
56	7.565	1923	1936	1955	rBV	190541	335212	20.81%	2.821%
57	7.690	1966	1975	1981	rBV6	1166	1654	0.10%	0.014%
58	7.793	1999	2007	2015	rVB4	1594	2558	0.16%	0.022%
59	7.832	2015	2019	2022	rBV2	214	210	0.01%	0.002%
60	7.899	2025	2040	2056	rBV	727202	1257010	78.02%	10.579%
61	8.179	2115	2127	2145	rBV	136579	229447	14.24%	1.931%
62	8.346	2177	2179	2182	rVB2	470	212	0.01%	0.002%
63	8.420	2199	2202	2210	rVB3	405	427	0.03%	0.004%
64	8.462	2210	2215	2216	rBV2	551	434	0.03%	0.004%
65	8.549	2239	2242	2252	rVB2	333	464	0.03%	0.004%
66	8.636	2256	2269	2306	rBV2	499640	954819	59.26%	8.035%
67	8.877	2342	2344	2349	rVB3	323	195	0.01%	0.002%
68	8.915	2349	2356	2363	rBV4	944	1636	0.10%	0.014%
69	9.115	2413	2418	2420	rBV2	308	249	0.02%	0.002%
70	9.308	2473	2478	2481	rBV3	420	453	0.03%	0.004%
71	9.417	2498	2512	2530	rBV	552179	912501	56.63%	7.679%
72	9.571	2557	2560	2565	rVB	639	517	0.03%	0.004%
73	9.623	2574	2576	2577	rBV	342	149	0.01%	0.001%
74	9.687	2592	2596	2597	rBV	482	332	0.02%	0.003%
75	9.887	2654	2658	2660	rBV	221	179	0.01%	0.002%
76	9.951	2674	2678	2682	rBV2	245	322	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
 Data File : VU048317.D
 Acq On : 27 Apr 2022 16:14
 Operator : SY/MD
 Sample : N2542-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.208	2754	2758	2759	rBV	283	174	0.01%	0.001%
78	10.256	2770	2773	2776	rBV	230	227	0.01%	0.002%
79	10.382	2809	2812	2815	rBV3	345	212	0.01%	0.002%
80	10.671	2895	2902	2911	rVB3	2398	3250	0.20%	0.027%
81	10.710	2911	2914	2916	rBV2	352	264	0.02%	0.002%
82	10.758	2916	2929	2948	rBV	609052	977594	60.67%	8.227%
83	10.848	2953	2957	2959	rBV3	323	235	0.01%	0.002%
84	10.893	2966	2971	2975	rBV3	864	773	0.05%	0.007%
85	11.150	3048	3051	3053	rBV	278	177	0.01%	0.001%
86	11.173	3056	3058	3062	rVB2	299	153	0.01%	0.001%
87	11.321	3102	3104	3109	rBV2	277	178	0.01%	0.001%
88	11.414	3128	3133	3135	rBV3	473	304	0.02%	0.003%
89	11.462	3141	3148	3156	rVB7	1647	2385	0.15%	0.020%
90	11.587	3180	3187	3193	rBV3	515	568	0.04%	0.005%
91	11.700	3214	3222	3226	rVV5	895	1213	0.08%	0.010%
92	11.742	3233	3235	3236	rBV	416	170	0.01%	0.001%
93	11.812	3244	3257	3279	rBV	549945	852055	52.88%	7.171%
94	11.973	3302	3307	3313	rVB3	2033	2244	0.14%	0.019%
95	12.057	3330	3333	3335	rBV	288	186	0.01%	0.002%
96	12.105	3345	3348	3352	rBV2	278	242	0.02%	0.002%
97	12.195	3360	3376	3397	rBV	691961	1132491	70.29%	9.531%
98	12.456	3455	3457	3458	rBV	339	155	0.01%	0.001%
99	12.584	3493	3497	3498	rBV2	257	164	0.01%	0.001%
100	12.771	3549	3555	3566	rVB4	1786	2736	0.17%	0.023%


Sum of corrected areas: 11882534

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
Data File : VU048317.D
Acq On : 27 Apr 2022 16:14
Operator : SY/MD
Sample : N2542-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

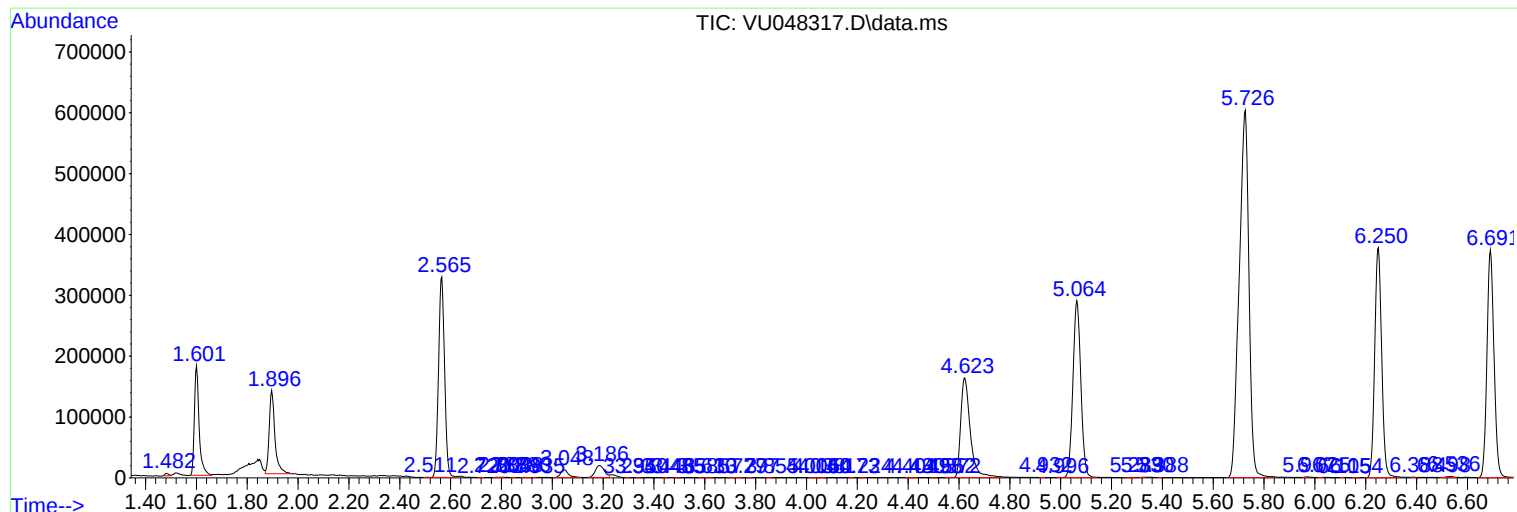

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
Data File : VU048317.D
Acq On : 27 Apr 2022 16:14
Operator : SY/MD
Sample : N2542-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
Data File : VU048317.D
Acq On : 27 Apr 2022 16:14
Operator : SY/MD
Sample : N2542-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------