


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042722\
 Data File : VU048302.D
 Acq On : 27 Apr 2022 09:26
 Operator : SY/MD
 Sample : BFB074
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB074

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis
 Last Update : Fri Apr 29 04:27:14 2022

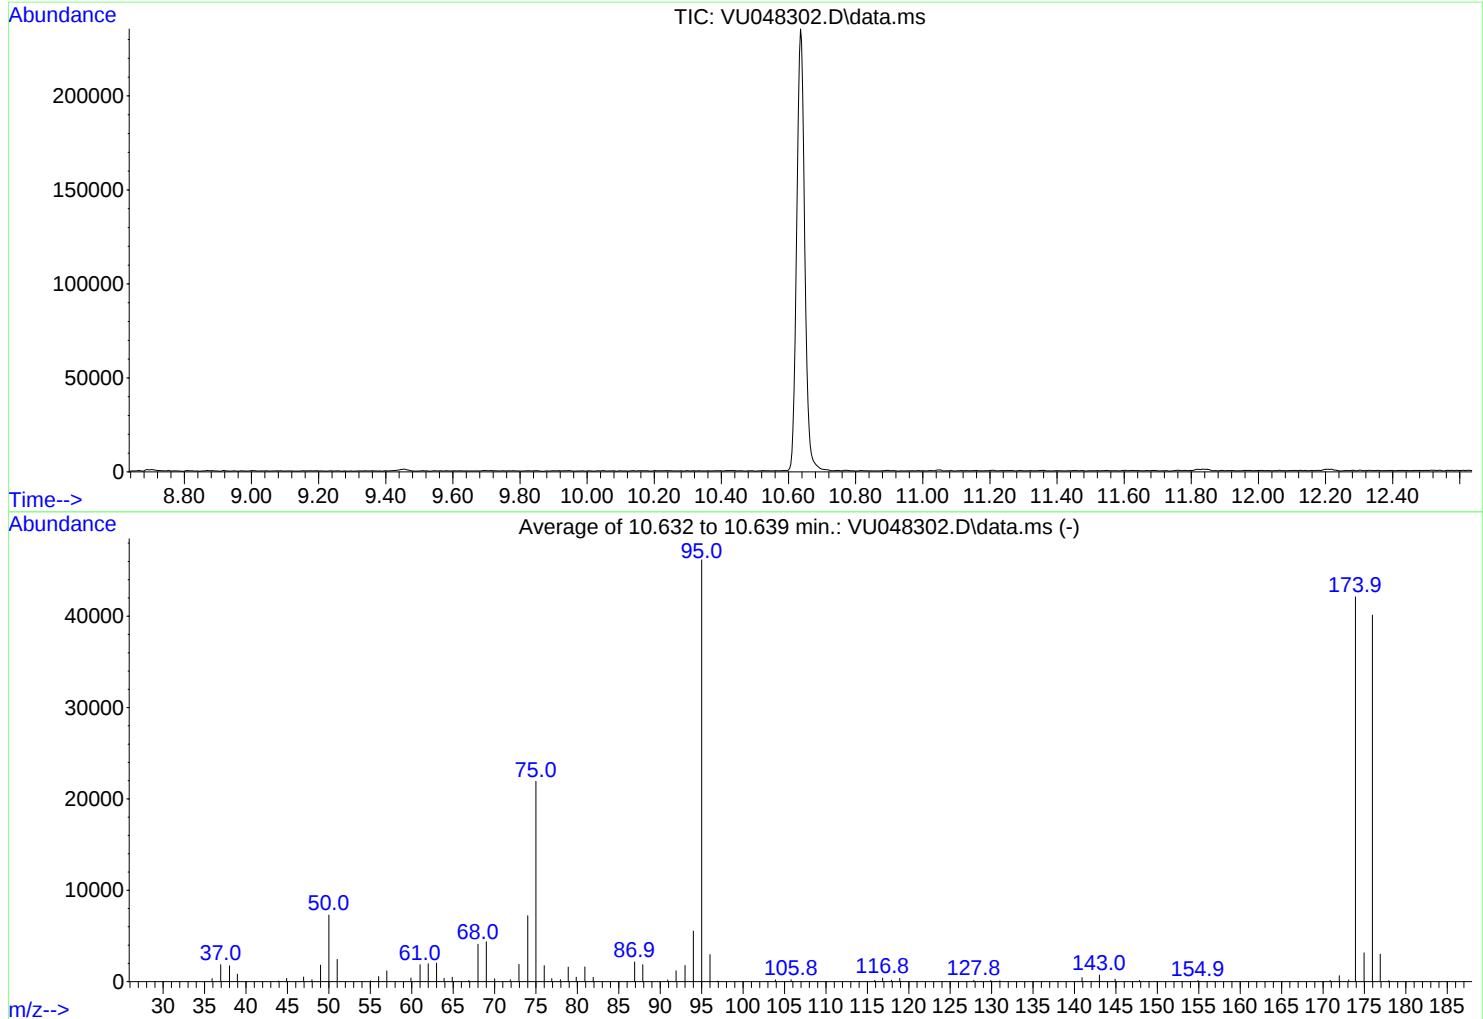

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.8	7281	PASS
75	95	30	80	47.5	21920	PASS
95	95	100	100	100.0	46171	PASS
96	95	5	9	6.4	2954	PASS
173	174	0.00	2	0.5	197	PASS
174	95	50	120	91.2	42131	PASS
175	174	5	9	7.5	3153	PASS
176	174	95	101	95.2	40125	PASS
177	176	5	9	7.5	3007	PASS

m/z	Abundance
39.90	155.0
43.90	526.0

Instrument :
MSVOA_U
ClientSampleId :
BFB074

m/z	Abundance
35.90	343.0
36.90	1895.0
38.00	1764.0
39.00	848.0
39.90	170.0
43.90	608.0
44.90	358.0
46.90	464.0
48.00	186.0
49.00	1683.0
50.00	7264.0
51.00	2417.0
55.00	134.0
56.00	500.0
57.00	1167.0
59.90	389.0
61.00	1897.0
62.00	1976.0
63.00	1943.0
63.90	403.0
64.90	477.0
66.90	113.0
68.00	4024.0
69.00	4173.0
70.00	340.0
71.90	194.0
72.90	1854.0
74.00	6954.0
75.00	21664.0
76.00	1697.0
76.90	274.0
78.00	195.0
78.90	1639.0
79.90	486.0
80.90	1616.0
81.90	413.0
86.90	1997.0
87.90	1895.0
90.90	182.0
91.90	1154.0
93.00	1779.0
94.00	5491.0
95.00	44816.0
96.00	2786.0
97.00	114.0
103.90	173.0
105.80	210.0
115.90	183.0
116.80	406.0
117.90	132.0
118.90	349.0
127.90	155.0
130.00	141.0
131.00	110.0
140.90	440.0
143.00	687.0
144.90	272.0
147.90	126.0
155.00	114.0
156.80	103.0
170.80	180.0
171.90	589.0
173.90	39816.0
175.00	3248.0
175.90	38392.0
176.90	2915.0
177.90	119.0

Instrument :
MSVOA_U
ClientSampleId :
BFB074

m/z	Abundance
35.90	348.0
37.00	1899.0
38.00	1808.0
39.00	860.0
40.00	163.0
43.90	585.0
44.90	357.0
46.90	532.0
47.90	210.0
49.00	1857.0
50.00	7497.0
51.00	2466.0
55.10	117.0
56.00	584.0
57.00	1259.0
59.90	427.0
61.00	1900.0
62.00	2009.0
63.00	2077.0
63.90	387.0
64.90	492.0
66.90	134.0
68.00	4227.0
69.00	4489.0
70.00	338.0
71.90	231.0
72.90	1957.0
74.00	7456.0
75.00	22592.0
76.00	1786.0
76.90	332.0
78.00	218.0
78.90	1638.0
79.80	495.0
80.90	1613.0
81.90	496.0
86.90	2236.0
87.90	1898.0
90.90	214.0
91.90	1221.0
93.00	1780.0
94.00	5704.0
95.00	47664.0
96.00	3021.0
96.90	101.0
103.90	212.0
105.80	239.0
115.90	164.0
116.90	390.0
117.90	158.0
118.90	374.0
127.80	170.0
128.80	106.0
129.90	145.0
131.00	114.0
140.90	462.0
143.00	763.0
144.90	295.0
147.90	156.0
154.90	145.0
170.80	146.0
171.90	666.0
173.90	43344.0
175.00	3226.0
175.90	41328.0
176.90	3135.0
178.00	138.0

Instrument :
MSVOA_U
ClientSampleId :
BFB074

m/z	Abundance
35.90	324.0
37.00	1798.0
38.00	1649.0
38.90	749.0
40.10	163.0
43.90	598.0
44.90	326.0
47.00	544.0
47.90	210.0
49.00	1856.0
50.00	7081.0
51.00	2424.0
56.00	617.0
57.00	1100.0
59.90	419.0
61.00	1771.0
62.00	1911.0
63.00	2058.0
63.90	338.0
64.90	524.0
66.90	128.0
68.00	4048.0
69.00	4418.0
70.00	284.0
71.90	224.0
73.00	1884.0
74.00	7233.0
75.00	21504.0
76.00	1785.0
76.90	386.0
77.90	236.0
78.90	1505.0
79.90	498.0
80.90	1596.0
81.90	500.0
86.00	116.0
86.90	2251.0
87.90	1796.0
90.90	181.0
91.90	1177.0
93.00	1745.0
94.00	5417.0
95.00	46032.0
96.00	3054.0
103.90	216.0
105.80	200.0
115.90	128.0
116.90	364.0
117.90	179.0
118.90	339.0
127.90	153.0
129.80	128.0
131.00	103.0
140.90	422.0
143.00	712.0
144.90	290.0
147.80	156.0
154.80	146.0
170.90	120.0
172.00	695.0
173.10	591.0
173.90	43232.0
174.90	2984.0
176.00	40656.0
176.90	2972.0
177.90	112.0

Instrument :
MSVOA_U
ClientSampleId :
BFB074