


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042723\
Data File : VU053926.D
Acq On : 26 Apr 2023 20:32
Operator : JC/MD
Sample : BFB020
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB020

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUSIM042723.M
Title : TRACE VOA SOM01.0
Last Update : Thu Apr 27 08:10:40 2023

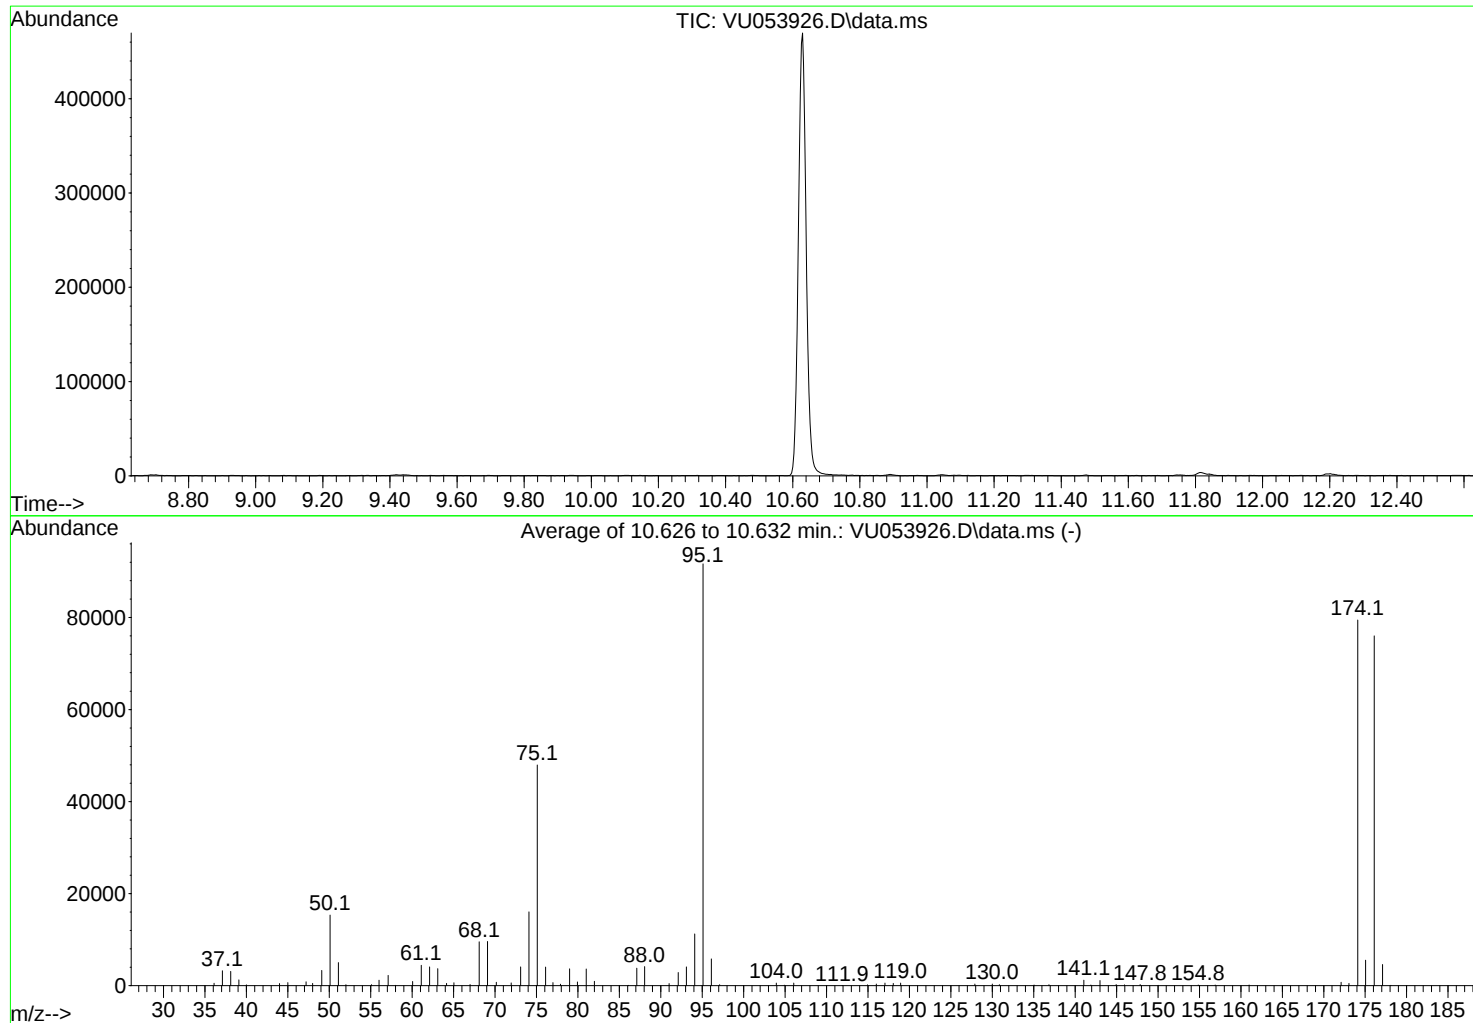

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.7	15326	PASS
75	95	30	80	52.3	47963	PASS
95	95	100	100	100.0	91669	PASS
96	95	5	9	6.3	5792	PASS
173	174	0.00	2	0.6	492	PASS
174	95	50	120	86.7	79469	PASS
175	174	5	9	7.0	5535	PASS
176	174	95	101	95.7	76029	PASS
177	176	5	9	6.1	4603	PASS

m/z	Abundance
44.00	248.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

m/z	Abundance
36.10	561.0
37.10	3230.0
38.10	3267.0
39.10	1276.0
40.00	166.0
44.00	725.0
45.00	733.0
47.20	875.0
48.00	497.0
49.10	3611.0
50.10	15739.0
51.10	5035.0
52.00	175.0
55.10	232.0
56.00	1126.0
57.10	2295.0
60.10	842.0
61.10	4671.0
62.10	4049.0
63.10	3837.0
64.20	495.0
65.10	634.0
67.00	298.0
68.10	9618.0
69.10	9469.0
70.20	723.0
71.90	592.0
73.10	4254.0
74.10	16744.0
75.10	49104.0
76.10	4143.0
77.00	723.0
77.80	360.0
79.00	3742.0
79.90	832.0
81.00	3825.0
82.00	936.0
86.10	110.0
87.10	3995.0
88.00	4086.0
91.00	467.0
92.10	2841.0
93.10	4075.0
94.10	11343.0
95.10	93704.0
96.10	5886.0
97.10	198.0
103.90	565.0
106.10	559.0
114.90	197.0
116.00	365.0
117.00	596.0
118.10	525.0
119.00	573.0
127.90	318.0
129.90	411.0
130.80	214.0
135.00	131.0
136.80	198.0
141.10	1104.0
141.90	144.0
143.00	1095.0
144.90	224.0
145.90	161.0
147.90	247.0
154.90	102.0
156.90	124.0
161.00	145.0
172.10	845.0
173.10	529.0
174.10	78536.0
175.10	5562.0
176.10	74024.0
177.10	4722.0
178.10	139.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

m/z	Abundance
36.10	525.0
37.10	3336.0
38.10	3178.0
39.10	1273.0
40.00	173.0
44.10	724.0
45.00	698.0
47.20	872.0
48.00	499.0
49.10	3430.0
50.10	15771.0
51.10	5174.0
52.00	224.0
55.10	227.0
56.00	1237.0
57.10	2221.0
58.00	108.0
60.10	925.0
61.10	4556.0
62.10	4163.0
63.10	3808.0
64.10	522.0
65.00	624.0
67.00	262.0
68.10	9820.0
69.10	9974.0
70.20	777.0
72.00	609.0
73.10	4191.0
74.10	16544.0
75.10	49664.0
76.10	4113.0
77.00	671.0
77.90	322.0
79.00	3783.0
80.00	819.0
81.00	3728.0
82.00	997.0
86.10	112.0
87.10	3847.0
88.10	4274.0
91.00	472.0
92.10	3001.0
93.10	4186.0
94.10	11602.0
95.10	94776.0
96.10	5875.0
97.10	214.0
103.90	605.0
104.90	114.0
106.10	563.0
115.00	186.0
116.00	365.0
117.10	565.0
118.10	501.0
118.90	587.0
127.90	345.0
130.00	352.0
130.80	218.0
135.10	153.0
136.80	221.0
141.00	1230.0
141.90	157.0
143.00	1168.0
145.00	264.0
146.00	178.0
147.90	244.0
150.00	113.0
154.80	153.0
156.90	130.0
161.00	134.0
172.10	767.0
173.00	502.0
174.10	81992.0
175.00	5624.0
176.10	78448.0
177.10	4759.0
178.10	103.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020

m/z	Abundance
36.10	495.0
37.10	3133.0
38.10	2895.0
39.10	1245.0
40.00	175.0
44.10	627.0
45.00	598.0
47.20	756.0
48.00	485.0
49.10	2892.0
50.10	14467.0
51.10	4839.0
52.00	223.0
55.10	182.0
56.00	1181.0
57.10	2119.0
58.00	119.0
60.00	899.0
61.10	4051.0
62.10	4043.0
63.10	3377.0
64.20	464.0
65.00	595.0
67.00	192.0
68.10	9151.0
69.10	9334.0
70.10	661.0
72.00	551.0
73.10	3783.0
74.10	14816.0
75.10	45120.0
76.10	3810.0
77.00	630.0
78.00	303.0
79.00	3396.0
80.00	765.0
81.00	3353.0
82.00	943.0
87.10	3568.0
88.10	4117.0
91.00	393.0
92.10	2722.0
93.10	3946.0
94.10	10710.0
95.10	86528.0
96.10	5614.0
97.10	219.0
104.00	548.0
104.90	161.0
106.00	533.0
111.90	103.0
115.00	137.0
116.00	367.0
117.10	491.0
118.00	453.0
118.90	539.0
127.90	358.0
130.10	338.0
130.90	160.0
135.10	170.0
136.90	209.0
141.00	1183.0
141.90	109.0
143.00	1117.0
145.00	270.0
146.00	146.0
147.80	207.0
150.00	117.0
154.90	216.0
156.90	132.0
161.00	102.0
172.10	641.0
173.00	444.0
174.10	77880.0
175.00	5418.0
176.10	75616.0
177.10	4327.0

Instrument :
MSVOA_U
ClientSampleId :
BFB020