
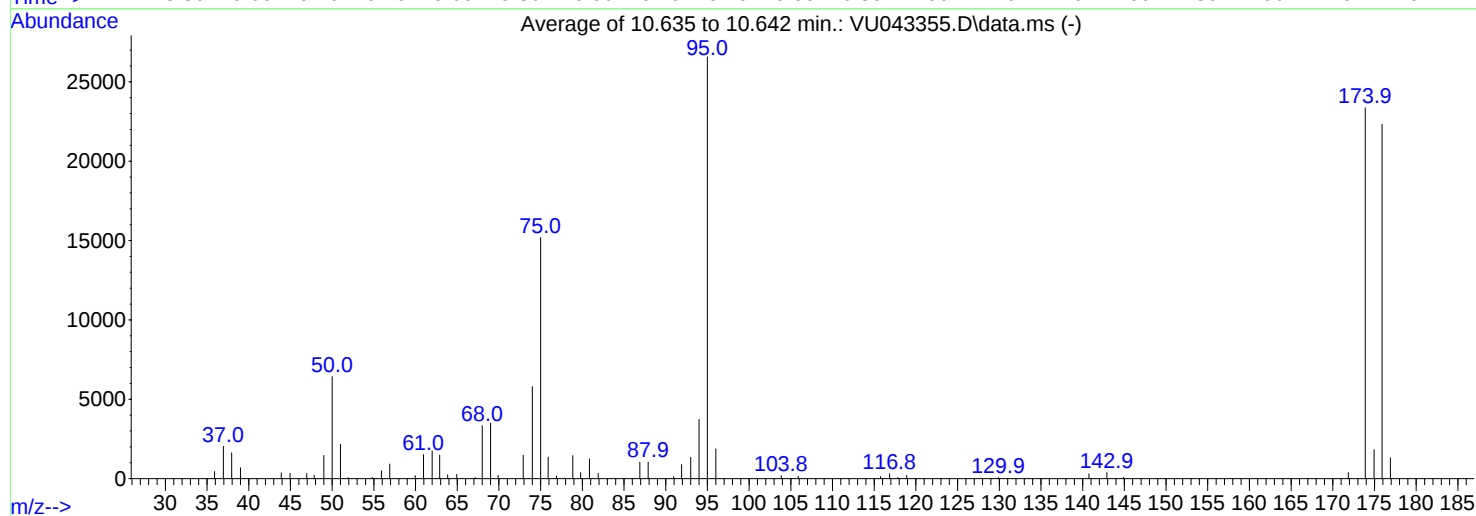


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042821\
 Data File : VU043355.D
 Acq On : 27 Apr 2021 15:39
 Operator : SY/MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U041221W.M
 Title : SW846 8260
 Last Update : Mon Apr 12 13:17:29 2021

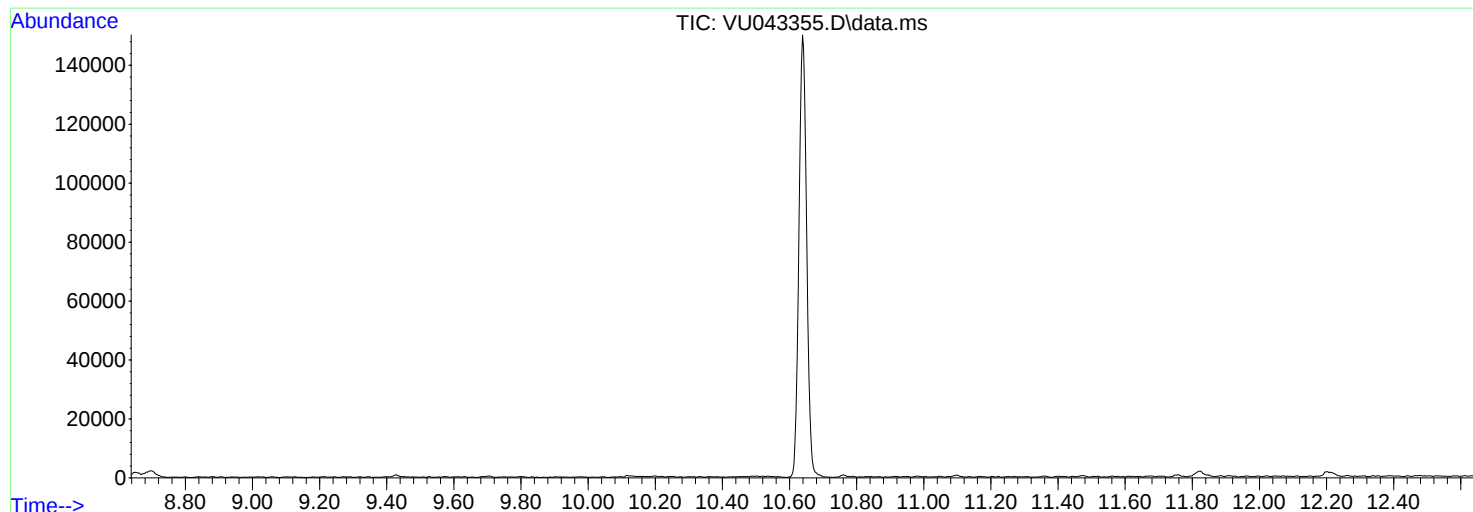

AutoFind: Scans 2891, 2892, 2893; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.2	6430	PASS
75	95	30	60	57.2	15193	PASS
95	95	100	100	100.0	26573	PASS
96	95	5	9	7.1	1874	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.9	23357	PASS
175	174	5	9	7.8	1826	PASS
176	174	95	101	95.6	22333	PASS
177	176	5	9	5.9	1309	PASS