
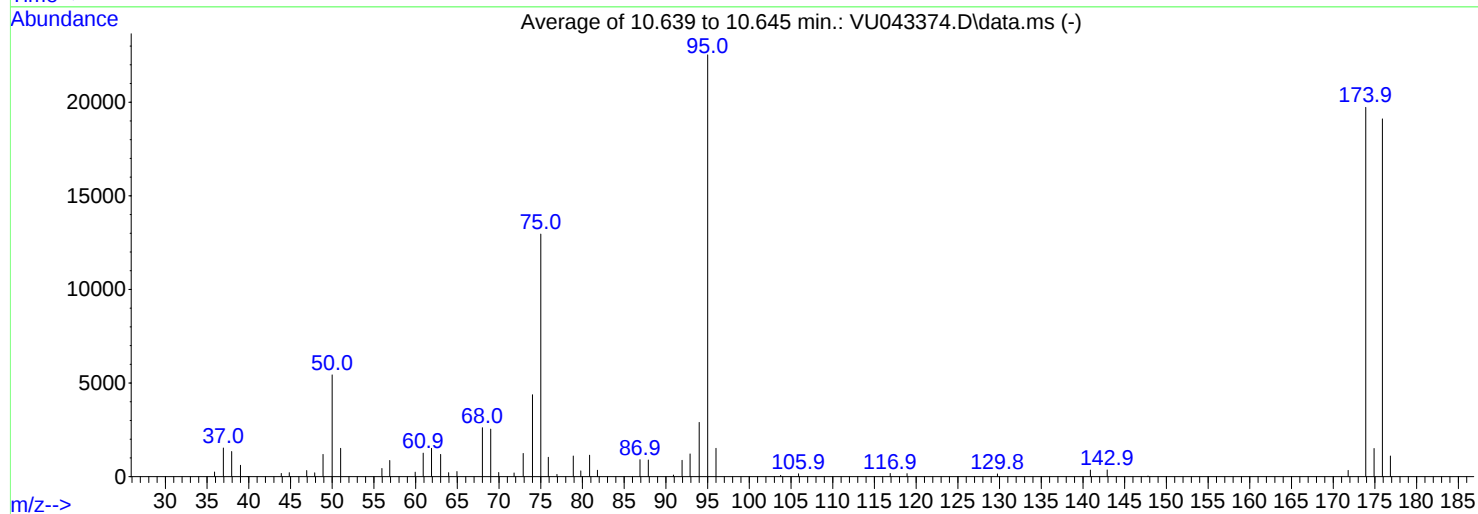


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042821\
Data File : VU043374.D
Acq On : 28 Apr 2021 09:38
Operator : SY/MD
Sample : BFB
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\82U041221W.M
Title : SW846 8260
Last Update : Mon Apr 12 13:17:29 2021

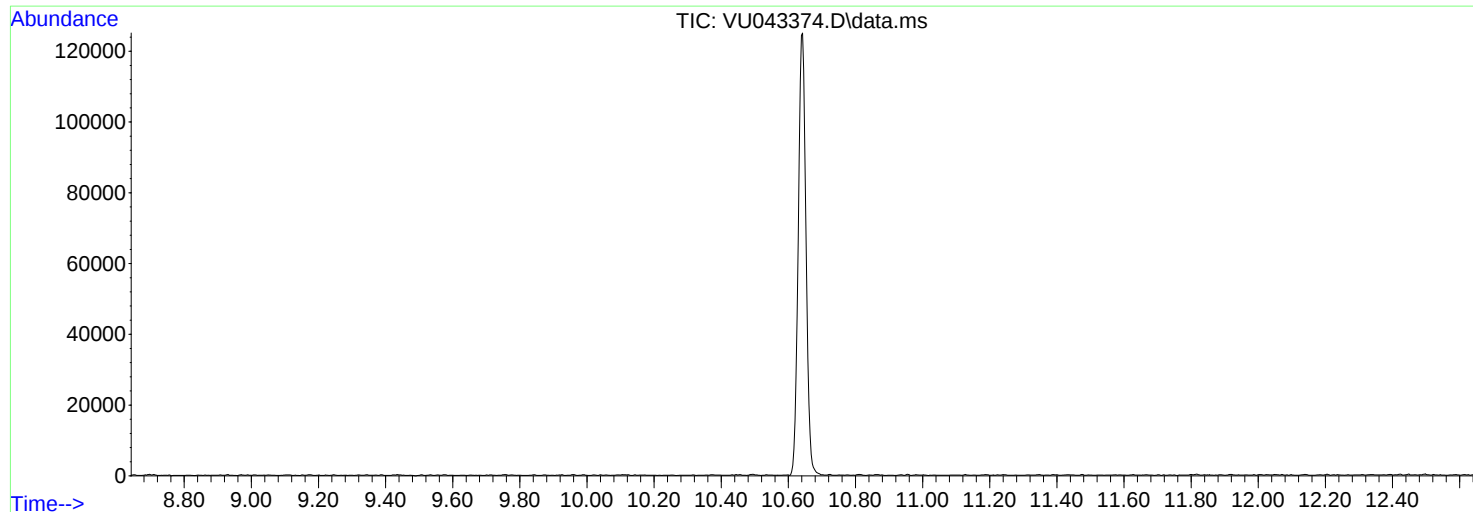

AutoFind: Scans 2892, 2893, 2894; Background Corrected with Scan 2879

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.1	5432	PASS
75	95	30	60	57.5	12961	PASS
95	95	100	100	100.0	22531	PASS
96	95	5	9	6.7	1517	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	87.6	19728	PASS
175	174	5	9	7.6	1503	PASS
176	174	95	101	96.9	19115	PASS
177	176	5	9	5.8	1107	PASS