

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042822\
 Data File : VU048331.D
 Acq On : 28 Apr 2022 11:19
 Operator : SY/MD
 Sample : VU0428WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK106

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M

Title : VOC Analysis

Signal : TIC: VU048331.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.485	40	45	49	rBV	4072	4689	0.28%	0.037%
2	1.600	73	81	101	rBV	173850	235663	13.99%	1.871%
3	1.903	167	175	199	rVB	139988	220586	13.09%	1.751%
4	2.491	356	358	360	rVB2	525	206	0.01%	0.002%
5	2.565	369	381	398	rBV	335562	554187	32.89%	4.399%
6	2.684	416	418	422	rVB3	681	391	0.02%	0.003%
7	2.793	446	452	460	rVB4	1233	1869	0.11%	0.015%
8	2.954	496	502	506	rBV4	652	846	0.05%	0.007%
9	3.054	525	533	540	rBV4	1586	2729	0.16%	0.022%
10	3.092	542	545	550	rBV2	377	275	0.02%	0.002%
11	3.186	562	574	575	rBV3	3017	3773	0.22%	0.030%
12	3.353	622	626	627	rBV2	553	432	0.03%	0.003%
13	3.362	627	629	636	rVB2	1124	1041	0.06%	0.008%
14	3.446	651	655	659	rBV2	249	235	0.01%	0.002%
15	3.700	727	734	736	rVV2	189	209	0.01%	0.002%
16	3.835	772	776	777	rBV	257	156	0.01%	0.001%
17	3.887	790	792	797	rVB2	246	173	0.01%	0.001%
18	3.960	812	815	818	rVB	246	154	0.01%	0.001%
19	3.980	818	821	825	rBV	297	275	0.02%	0.002%
20	4.086	850	854	859	rVB2	201	166	0.01%	0.001%
21	4.362	934	940	941	rBV	222	174	0.01%	0.001%
22	4.626	1008	1022	1053	rBV	181424	459314	27.26%	3.646%
23	4.919	1111	1113	1117	rVB2	287	184	0.01%	0.001%
24	4.977	1129	1131	1133	rVB	371	179	0.01%	0.001%
25	5.063	1142	1158	1180	rVV	297619	653252	38.77%	5.185%
26	5.224	1203	1208	1212	rBV2	420	449	0.03%	0.004%
27	5.292	1224	1229	1230	rBV2	591	510	0.03%	0.004%
28	5.382	1253	1257	1258	rBV	402	256	0.02%	0.002%
29	5.526	1293	1302	1303	rBV2	649	704	0.04%	0.006%
30	5.726	1341	1364	1397	rBV2	623546	1684930	100.00%	13.375%
31	5.980	1436	1443	1445	rBV5	498	578	0.03%	0.005%
32	6.112	1480	1484	1487	rBV2	277	265	0.02%	0.002%
33	6.250	1512	1527	1555	rBV	408382	776701	46.10%	6.165%
34	6.449	1585	1589	1592	rBV2	312	318	0.02%	0.003%
35	6.536	1607	1616	1627	rVB7	2144	4236	0.25%	0.034%
36	6.603	1634	1637	1641	rVB3	334	222	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042822\
 Data File : VU048331.D
 Acq On : 28 Apr 2022 11:19
 Operator : SY/MD
 Sample : VU0428WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK106

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.690	1649	1664	1683	rBV	385109	751477	44.60%	5.965%
38	7.105	1787	1793	1801	rVB4	794	1205	0.07%	0.010%
39	7.140	1801	1804	1806	rBV	261	157	0.01%	0.001%
40	7.185	1806	1818	1830	rBV4	3331	6790	0.40%	0.054%
41	7.565	1922	1936	1964	rBV	205643	368032	21.84%	2.921%
42	7.684	1969	1973	1975	rBV	780	688	0.04%	0.005%
43	7.796	1998	2008	2020	rVB6	2030	3635	0.22%	0.029%
44	7.899	2026	2040	2058	rBV	772529	1345936	79.88%	10.684%
45	8.179	2116	2127	2144	rBV	147945	247144	14.67%	1.962%
46	8.337	2174	2176	2181	rVB3	419	218	0.01%	0.002%
47	8.359	2181	2183	2190	rVB2	490	395	0.02%	0.003%
48	8.394	2190	2194	2195	rBV3	751	482	0.03%	0.004%
49	8.407	2195	2198	2205	rVB3	1076	849	0.05%	0.007%
50	8.472	2216	2218	2221	rBV2	322	205	0.01%	0.002%
51	8.555	2237	2244	2246	rBV3	1157	1270	0.08%	0.010%
52	8.639	2257	2270	2305	rBV	573667	1042258	61.86%	8.273%
53	8.912	2352	2355	2356	rBV	414	254	0.02%	0.002%
54	9.134	2422	2424	2428	rVB3	367	270	0.02%	0.002%
55	9.163	2428	2433	2437	rBV4	502	530	0.03%	0.004%
56	9.224	2449	2452	2455	rVV2	325	220	0.01%	0.002%
57	9.246	2457	2459	2463	rVB2	311	204	0.01%	0.002%
58	9.417	2497	2512	2541	rBV	581809	989757	58.74%	7.856%
59	9.574	2555	2561	2570	rVB2	1692	2527	0.15%	0.020%
60	9.616	2572	2574	2578	rVV	271	156	0.01%	0.001%
61	9.645	2578	2583	2588	rVB2	458	472	0.03%	0.004%
62	9.693	2589	2598	2611	rVB3	1786	2783	0.17%	0.022%
63	9.912	2663	2666	2670	rVB2	376	233	0.01%	0.002%
64	10.108	2718	2727	2733	rBV5	2033	3318	0.20%	0.026%
65	10.169	2743	2746	2748	rBV	289	187	0.01%	0.001%
66	10.285	2777	2782	2786	rBV3	308	317	0.02%	0.003%
67	10.417	2821	2823	2828	rVV2	253	207	0.01%	0.002%
68	10.449	2830	2833	2835	rVV2	293	185	0.01%	0.001%
69	10.491	2839	2846	2854	rVB2	999	1616	0.10%	0.013%
70	10.590	2875	2877	2882	rBV	247	202	0.01%	0.002%
71	10.639	2889	2892	2894	rBV4	426	344	0.02%	0.003%
72	10.674	2897	2903	2910	rVB4	2378	3248	0.19%	0.026%
73	10.758	2916	2929	2946	rBV	623247	1006290	59.72%	7.988%
74	10.883	2963	2968	2969	rBV2	908	665	0.04%	0.005%
75	10.983	2996	2999	3002	rBV	419	279	0.02%	0.002%
76	11.095	3028	3034	3037	rBV2	796	846	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042822\
 Data File : VU048331.D
 Acq On : 28 Apr 2022 11:19
 Operator : SY/MD
 Sample : VU0428WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK106

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	11.188	3059	3063	3065	rVV2	234	177	0.01%	0.001%
78	11.269	3085	3088	3092	rVB2	490	345	0.02%	0.003%
79	11.365	3116	3118	3123	rVB	490	276	0.02%	0.002%
80	11.394	3123	3127	3129	rBV2	417	376	0.02%	0.003%
81	11.455	3139	3146	3147	rBV3	2031	1851	0.11%	0.015%
82	11.468	3147	3150	3160	rVB4	3093	3180	0.19%	0.025%
83	11.578	3180	3184	3187	rBV3	333	304	0.02%	0.002%
84	11.693	3216	3220	3230	rVB3	1200	1406	0.08%	0.011%
85	11.748	3230	3237	3244	rBV5	2176	2984	0.18%	0.024%
86	11.812	3244	3257	3276	rBV	594732	940506	55.82%	7.465%
87	11.928	3287	3293	3294	rBV4	589	615	0.04%	0.005%
88	11.976	3303	3308	3317	rVB3	2158	2431	0.14%	0.019%
89	12.195	3362	3376	3392	rBV	766463	1226284	72.78%	9.734%
90	12.327	3415	3417	3425	rVB3	729	650	0.04%	0.005%
91	12.362	3425	3428	3430	rBV	437	285	0.02%	0.002%
92	12.635	3508	3513	3515	rBV3	397	402	0.02%	0.003%
93	12.774	3548	3556	3564	rBV2	1839	2857	0.17%	0.023%
94	12.867	3582	3585	3588	rBV2	251	198	0.01%	0.002%
95	13.147	3669	3672	3677	rBV5	320	352	0.02%	0.003%
96	13.227	3690	3697	3705	rVB2	1485	2131	0.13%	0.017%
97	13.848	3883	3890	3901	rBV5	2385	3435	0.20%	0.027%
98	14.089	3960	3965	3977	rVB3	4141	6322	0.38%	0.050%
99	14.333	4036	4041	4050	rVB5	2654	4096	0.24%	0.033%
100	14.458	4076	4080	4083	rBV2	443	409	0.02%	0.003%




Sum of corrected areas: 12598050

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042822\
Data File : VU048331.D
Acq On : 28 Apr 2022 11:19
Operator : SY/MD
Sample : VU0428WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK106

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

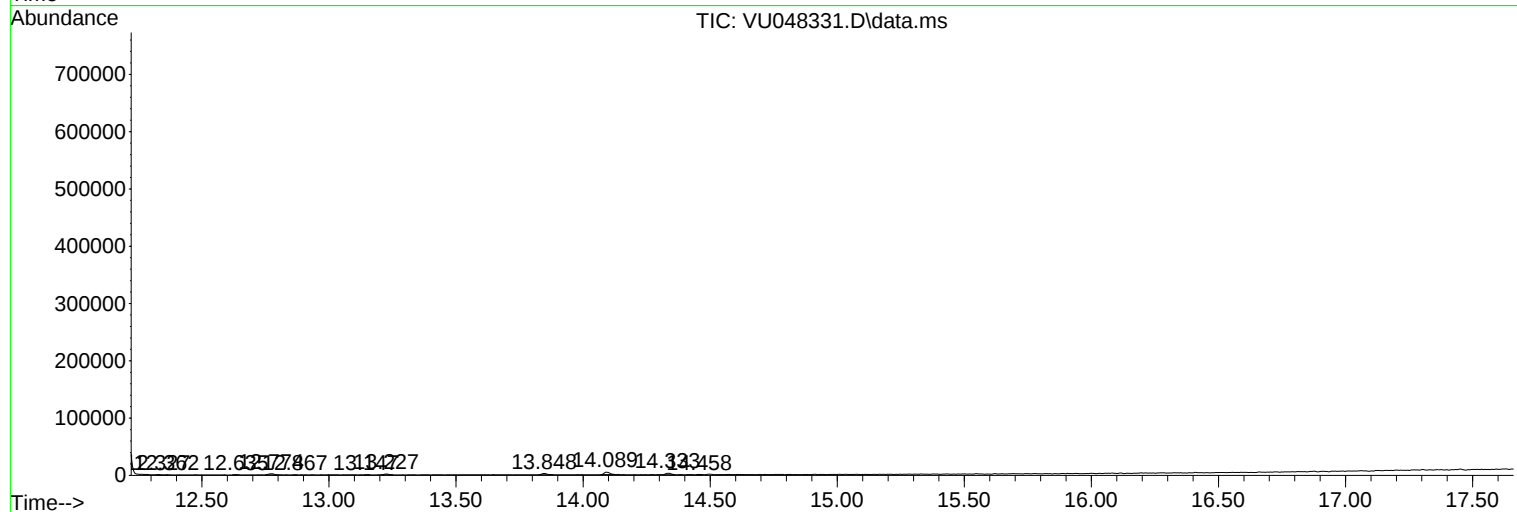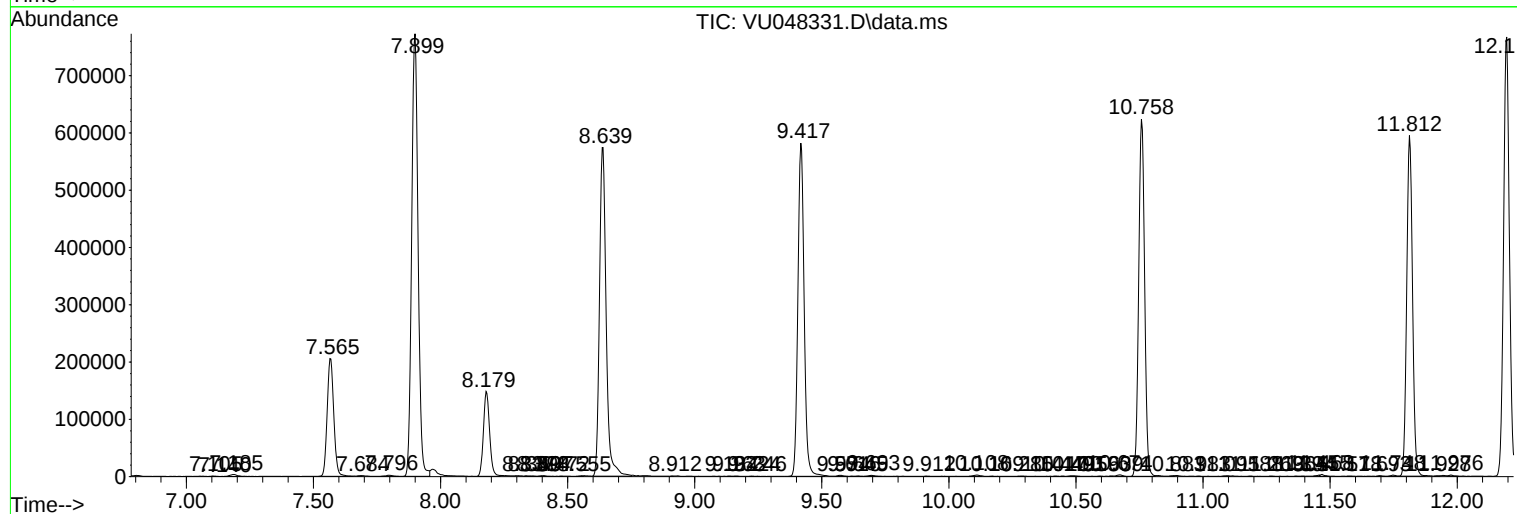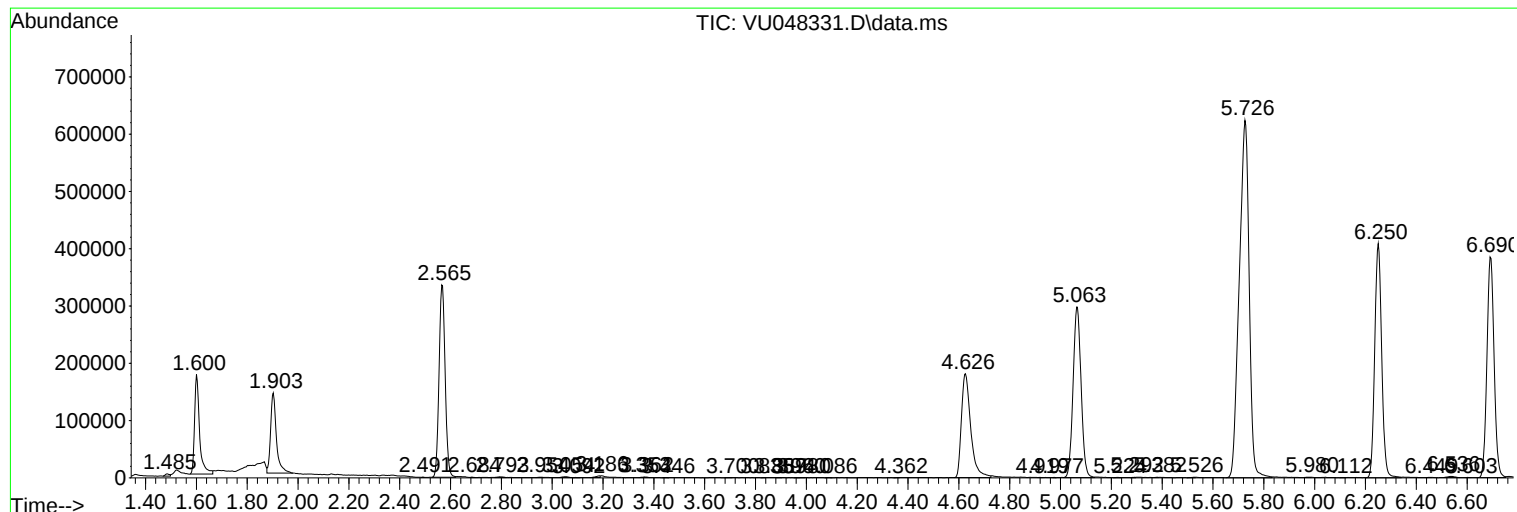

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042822\
Data File : VU048331.D
Acq On : 28 Apr 2022 11:19
Operator : SY/MD
Sample : VU0428WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK106

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042822\
Data File : VU048331.D
Acq On : 28 Apr 2022 11:19
Operator : SY/MD
Sample : VU0428WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK106

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------