

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042822\
 Data File : VU048339.D
 Acq On : 28 Apr 2022 14:28
 Operator : SY/MD
 Sample : VIBLK068
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK068

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

Signal : TIC: VU048339.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.356	3	5	15	rVB	15831	14546	0.91%	0.118%
2	1.488	39	46	52	rBV2	8345	12681	0.79%	0.103%
3	1.600	73	81	100	rBV	171582	227153	14.13%	1.839%
4	1.893	164	172	188	rVB	121209	179783	11.19%	1.456%
5	2.562	368	380	395	rBV	314744	513228	31.94%	4.155%
6	2.706	423	425	427	rBV2	320	202	0.01%	0.002%
7	2.729	427	432	433	rBV3	433	438	0.03%	0.004%
8	2.790	444	451	456	rBV	867	1117	0.07%	0.009%
9	2.829	460	463	466	rBV4	308	287	0.02%	0.002%
10	2.903	482	486	487	rBV	351	221	0.01%	0.002%
11	2.954	499	502	508	rVB4	548	630	0.04%	0.005%
12	3.044	522	530	541	rVB4	2156	4196	0.26%	0.034%
13	3.134	555	558	561	rVB2	332	232	0.01%	0.002%
14	3.182	561	573	591	rBV2	5369	13185	0.82%	0.107%
15	3.346	621	624	626	rBV2	336	235	0.01%	0.002%
16	3.507	671	674	678	rVB	328	261	0.02%	0.002%
17	3.587	695	699	703	rVB2	507	359	0.02%	0.003%
18	3.784	750	760	763	rBV	282	376	0.02%	0.003%
19	3.983	820	822	825	rVV	307	189	0.01%	0.002%
20	4.118	860	864	867	rVV2	225	179	0.01%	0.001%
21	4.160	871	877	879	rBV2	162	180	0.01%	0.001%
22	4.253	897	906	908	rVV2	261	230	0.01%	0.002%
23	4.620	1007	1020	1055	rBV	183558	446937	27.81%	3.618%
24	5.063	1141	1158	1184	rVV	292054	629200	39.15%	5.094%
25	5.192	1192	1198	1201	rBV2	454	572	0.04%	0.005%
26	5.279	1220	1225	1227	rBV3	472	519	0.03%	0.004%
27	5.340	1234	1244	1252	rVB3	1111	1893	0.12%	0.015%
28	5.398	1258	1262	1267	rBV3	339	333	0.02%	0.003%
29	5.423	1267	1270	1275	rVB2	314	221	0.01%	0.002%
30	5.481	1285	1288	1292	rBV	321	232	0.01%	0.002%
31	5.722	1342	1363	1397	rBV2	587695	1607095	100.00%	13.011%
32	5.883	1411	1413	1418	rVB3	632	410	0.03%	0.003%
33	5.960	1433	1437	1438	rBV2	394	238	0.01%	0.002%
34	6.044	1456	1463	1467	rBV3	458	633	0.04%	0.005%
35	6.250	1512	1527	1550	rBV	376538	723034	44.99%	5.854%
36	6.523	1607	1612	1622	rBV4	1589	2750	0.17%	0.022%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042822\
 Data File : VU048339.D
 Acq On : 28 Apr 2022 14:28
 Operator : SY/MD
 Sample : VIBLK068
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK068

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.690	1647	1664	1687	rBV	372463	720117	44.81%	5.830%
38	7.105	1791	1793	1803	rVB3	422	426	0.03%	0.003%
39	7.176	1803	1815	1831	rBV4	3226	8406	0.52%	0.068%
40	7.304	1850	1855	1858	rBV2	262	201	0.01%	0.002%
41	7.404	1884	1886	1890	rVB3	342	222	0.01%	0.002%
42	7.452	1896	1901	1904	rBV	369	321	0.02%	0.003%
43	7.494	1908	1914	1920	rVB6	1400	1938	0.12%	0.016%
44	7.520	1920	1922	1924	rBV	278	181	0.01%	0.001%
45	7.565	1924	1936	1956	rBV	204349	353741	22.01%	2.864%
46	7.681	1968	1972	1973	rBV3	780	564	0.04%	0.005%
47	7.793	1996	2007	2017	rVB6	1516	2815	0.18%	0.023%
48	7.838	2017	2021	2024	rBV	368	354	0.02%	0.003%
49	7.899	2024	2040	2057	rBV	731138	1277273	79.48%	10.341%
50	8.179	2115	2127	2145	rVV	145046	240329	14.95%	1.946%
51	8.359	2178	2183	2191	rVB6	1077	1652	0.10%	0.013%
52	8.468	2209	2217	2227	rBV3	872	1756	0.11%	0.014%
53	8.520	2231	2233	2236	rBV2	333	184	0.01%	0.001%
54	8.578	2240	2251	2257	rBV	8785	14830	0.92%	0.120%
55	8.636	2257	2269	2310	rVB	593611	1058981	65.89%	8.573%
56	8.906	2349	2353	2355	rBV2	367	218	0.01%	0.002%
57	9.105	2412	2415	2418	rBV2	256	216	0.01%	0.002%
58	9.163	2429	2433	2439	rVB4	649	742	0.05%	0.006%
59	9.253	2458	2461	2466	rVV2	237	180	0.01%	0.001%
60	9.417	2499	2512	2535	rBV	558153	955165	59.43%	7.733%
61	9.568	2553	2559	2560	rBV2	471	422	0.03%	0.003%
62	9.642	2579	2582	2588	rVB2	697	725	0.05%	0.006%
63	9.690	2591	2597	2601	rBV4	1089	1298	0.08%	0.011%
64	9.877	2650	2655	2659	rBV2	202	211	0.01%	0.002%
65	10.105	2719	2726	2736	rBV4	901	1522	0.09%	0.012%
66	10.410	2819	2821	2827	rVB2	358	229	0.01%	0.002%
67	10.443	2827	2831	2835	rBV2	285	324	0.02%	0.003%
68	10.484	2840	2844	2846	rBV2	720	643	0.04%	0.005%
69	10.561	2864	2868	2874	rVB2	280	340	0.02%	0.003%
70	10.677	2893	2904	2909	rVB5	1640	2819	0.18%	0.023%
71	10.758	2912	2929	2948	rBV	637441	1034049	64.34%	8.372%
72	10.870	2957	2964	2965	rBV3	719	791	0.05%	0.006%
73	10.893	2965	2971	2979	rVB4	2560	3953	0.25%	0.032%
74	10.967	2991	2994	2995	rBV	332	184	0.01%	0.001%
75	11.086	3024	3031	3032	rBV2	349	316	0.02%	0.003%
76	11.115	3037	3040	3046	rBV4	743	771	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042822\
 Data File : VU048339.D
 Acq On : 28 Apr 2022 14:28
 Operator : SY/MD
 Sample : VIBLK068
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK068

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	11.243	3078	3080	3083	rBV	267	192	0.01%	0.002%
78	11.282	3087	3092	3094	rBV	242	210	0.01%	0.002%
79	11.417	3132	3134	3136	rVB2	497	225	0.01%	0.002%
80	11.459	3138	3147	3148	rBV3	1562	1756	0.11%	0.014%
81	11.693	3215	3220	3229	rVB5	1084	1322	0.08%	0.011%
82	11.748	3229	3237	3244	rBV5	2118	3024	0.19%	0.024%
83	11.812	3244	3257	3282	rBV	587886	945078	58.81%	7.651%
84	11.950	3292	3300	3306	rBV8	2164	3715	0.23%	0.030%
85	12.195	3361	3376	3393	rBV	741055	1233155	76.73%	9.984%
86	12.359	3424	3427	3430	rVB2	338	195	0.01%	0.002%
87	12.481	3461	3465	3466	rBV2	267	205	0.01%	0.002%
88	12.629	3507	3511	3514	rBV4	530	393	0.02%	0.003%
89	12.700	3529	3533	3535	rBV2	291	256	0.02%	0.002%
90	12.774	3547	3556	3569	rBV3	3025	4780	0.30%	0.039%
91	12.973	3612	3618	3629	rVB3	2524	3917	0.24%	0.032%
92	13.217	3691	3694	3695	rBV	402	227	0.01%	0.002%
93	13.333	3728	3730	3734	rBV2	501	327	0.02%	0.003%
94	13.378	3738	3744	3755	rVB6	4518	6867	0.43%	0.056%
95	13.635	3822	3824	3828	rBV3	294	196	0.01%	0.002%
96	14.494	4083	4091	4102	rVB5	11406	18269	1.14%	0.148%
97	14.642	4135	4137	4141	rVB2	538	305	0.02%	0.002%
98	15.237	4319	4322	4324	rBV2	800	564	0.04%	0.005%
99	15.545	4408	4418	4432	rBV3	27735	42962	2.67%	0.348%
100	16.394	4675	4682	4690	rVB7	6787	10399	0.65%	0.084%


Sum of corrected areas: 12351923

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042822\
Data File : VU048339.D
Acq On : 28 Apr 2022 14:28
Operator : SY/MD
Sample : VIBLK068
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK068

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

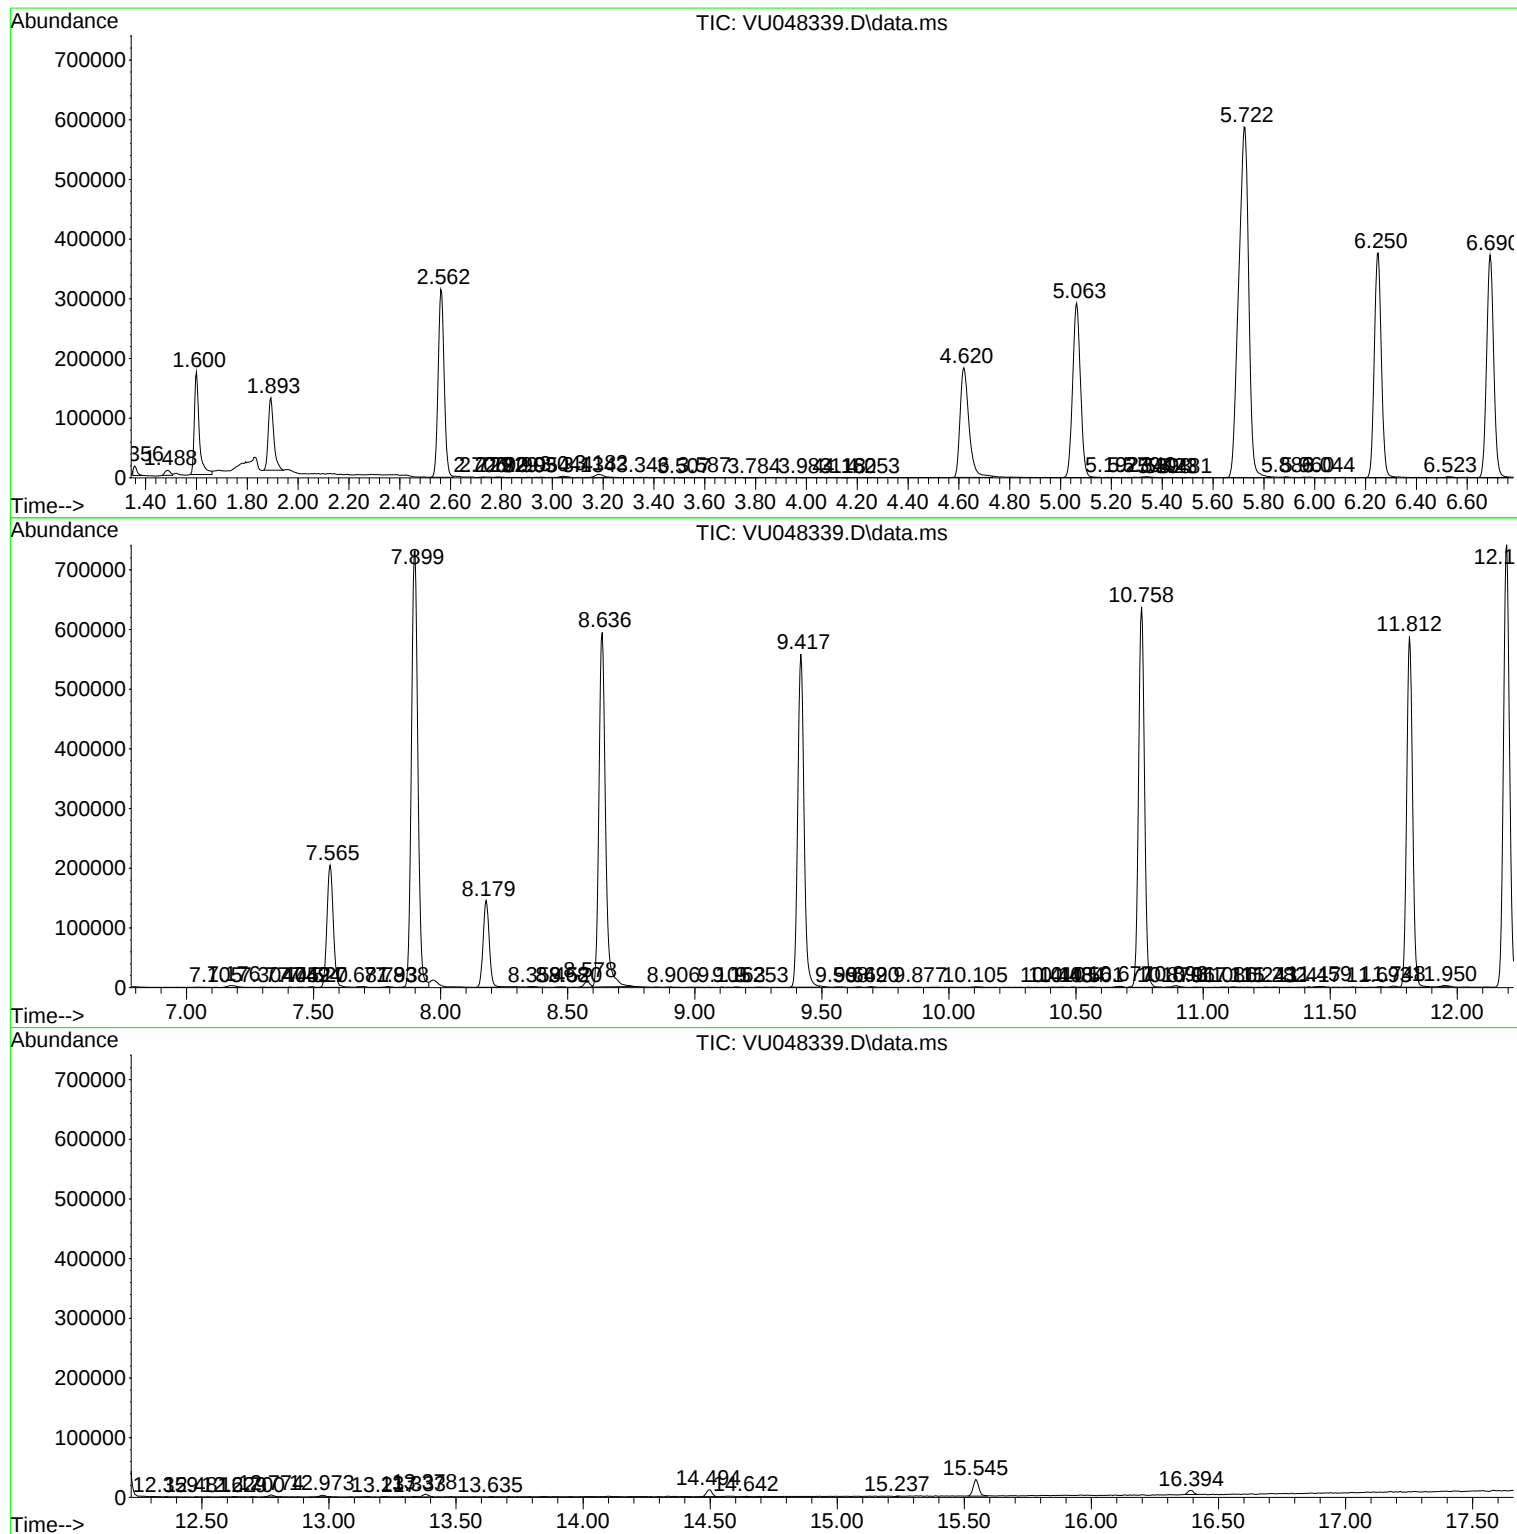

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042822\
Data File : VU048339.D
Acq On : 28 Apr 2022 14:28
Operator : SY/MD
Sample : VIBLK068
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK068

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042822\
Data File : VU048339.D
Acq On : 28 Apr 2022 14:28
Operator : SY/MD
Sample : VIBLK068
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK068

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------