

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042822\
 Data File : VU048345.D
 Acq On : 28 Apr 2022 16:48
 Operator : SY/MD
 Sample : N2587-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXET8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M

Title : VOC Analysis

Signal : TIC: VU048345.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.356	3	5	17	rVB	11526	10359	0.64%	0.079%
2	1.488	39	46	53	rBV2	7945	13902	0.86%	0.106%
3	1.601	73	81	100	rBV	165328	218249	13.53%	1.671%
4	1.890	164	171	190	rVB	122721	188415	11.68%	1.443%
5	2.562	367	380	398	rBV	311005	512123	31.74%	3.921%
6	2.787	446	450	452	rBV	487	442	0.03%	0.003%
7	2.867	472	475	478	rBV2	537	373	0.02%	0.003%
8	2.906	483	487	493	rVB2	527	549	0.03%	0.004%
9	2.954	498	502	505	rBV3	591	467	0.03%	0.004%
10	3.044	522	530	537	rBV4	1231	1764	0.11%	0.014%
11	3.112	547	551	556	rBV3	387	358	0.02%	0.003%
12	3.134	556	558	561	rBV2	424	233	0.01%	0.002%
13	3.189	561	575	584	rBV2	4845	11367	0.70%	0.087%
14	3.671	721	725	730	rBV2	485	432	0.03%	0.003%
15	3.957	812	814	816	rVV	395	218	0.01%	0.002%
16	4.031	831	837	839	rBV2	311	205	0.01%	0.002%
17	4.205	889	891	895	rBV2	291	253	0.02%	0.002%
18	4.298	912	920	923	rVB2	308	342	0.02%	0.003%
19	4.446	961	966	971	rBV2	210	259	0.02%	0.002%
20	4.485	976	978	983	rVB2	301	236	0.01%	0.002%
21	4.510	983	986	992	rBV2	209	208	0.01%	0.002%
22	4.620	1007	1020	1068	rBV	182678	457935	28.38%	3.506%
23	4.832	1083	1086	1089	rVB2	448	284	0.02%	0.002%
24	4.970	1126	1129	1134	rBV3	208	241	0.01%	0.002%
25	5.063	1139	1158	1181	rBV	307636	677394	41.98%	5.186%
26	5.215	1200	1205	1209	rBV3	295	258	0.02%	0.002%
27	5.285	1220	1227	1233	rBV5	797	1304	0.08%	0.010%
28	5.333	1239	1242	1244	rBV2	526	387	0.02%	0.003%
29	5.575	1314	1317	1323	rVB3	344	342	0.02%	0.003%
30	5.610	1323	1328	1332	rBV2	197	262	0.02%	0.002%
31	5.723	1341	1363	1390	rBV2	596468	1613628	100.00%	12.354%
32	5.960	1435	1437	1441	rBV4	430	377	0.02%	0.003%
33	6.105	1478	1482	1488	rBV3	275	318	0.02%	0.002%
34	6.250	1511	1527	1556	rBV	467350	899488	55.74%	6.887%
35	6.350	1556	1558	1564	rVB3	599	519	0.03%	0.004%
36	6.443	1584	1587	1591	rBV	257	236	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042822\
 Data File : VU048345.D
 Acq On : 28 Apr 2022 16:48
 Operator : SY/MD
 Sample : N2587-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXET8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

37	6.478	1595	1598	1601	rBV3	360	218	0.01%	0.002%
38	6.526	1608	1613	1619	rBV4	821	990	0.06%	0.008%
39	6.591	1627	1633	1637	rBV2	574	725	0.04%	0.006%
40	6.690	1649	1664	1682	rBV	381352	731796	45.35%	5.603%
41	6.886	1721	1725	1727	rBV2	275	276	0.02%	0.002%
42	6.928	1733	1738	1741	rBV3	255	247	0.02%	0.002%
43	6.989	1753	1757	1759	rBV3	373	280	0.02%	0.002%
44	7.176	1805	1815	1826	rVV6	3198	6927	0.43%	0.053%
45	7.285	1846	1849	1851	rBV	326	207	0.01%	0.002%
46	7.327	1860	1862	1869	rVB2	372	240	0.01%	0.002%
47	7.440	1894	1897	1901	rBV2	270	232	0.01%	0.002%
48	7.494	1907	1914	1923	rBV4	1008	1466	0.09%	0.011%
49	7.565	1923	1936	1954	rBV	203630	353444	21.90%	2.706%
50	7.671	1966	1969	1970	rBV2	431	235	0.01%	0.002%
51	7.687	1970	1974	1977	rVV3	890	846	0.05%	0.006%
52	7.780	2001	2003	2007	rVB3	405	242	0.01%	0.002%
53	7.806	2007	2011	2017	rBV2	266	289	0.02%	0.002%
54	7.899	2025	2040	2056	rBV	740093	1278483	79.23%	9.788%
55	8.179	2115	2127	2145	rBV	142769	240183	14.88%	1.839%
56	8.433	2202	2206	2207	rBV	326	239	0.01%	0.002%
57	8.468	2209	2217	2226	rVV3	3508	6012	0.37%	0.046%
58	8.575	2242	2250	2258	rBV2	10781	17663	1.09%	0.135%
59	8.636	2258	2269	2305	rVB	591558	1090291	67.57%	8.348%
60	8.899	2350	2351	2356	rVB	439	223	0.01%	0.002%
61	9.166	2425	2434	2435	rBV3	529	580	0.04%	0.004%
62	9.256	2459	2462	2467	rVB2	319	227	0.01%	0.002%
63	9.304	2474	2477	2480	rBV	322	204	0.01%	0.002%
64	9.417	2498	2512	2550	rVB	694100	1168215	72.40%	8.944%
65	9.552	2551	2554	2560	rBV3	292	314	0.02%	0.002%
66	9.581	2561	2563	2566	rVB2	487	229	0.01%	0.002%
67	9.642	2577	2582	2583	rBV	424	263	0.02%	0.002%
68	9.693	2594	2598	2607	rVB3	686	909	0.06%	0.007%
69	9.758	2613	2618	2622	rBV3	364	403	0.02%	0.003%
70	9.828	2637	2640	2646	rBV2	388	336	0.02%	0.003%
71	9.870	2648	2653	2658	rBV3	300	363	0.02%	0.003%
72	10.153	2738	2741	2745	rVV2	260	215	0.01%	0.002%
73	10.214	2754	2760	2762	rBV2	252	282	0.02%	0.002%
74	10.417	2820	2823	2827	rBV3	337	236	0.01%	0.002%
75	10.674	2896	2903	2908	rVB3	1540	1842	0.11%	0.014%
76	10.758	2915	2929	2948	rBV	665760	1069208	66.26%	8.186%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042822\
 Data File : VU048345.D
 Acq On : 28 Apr 2022 16:48
 Operator : SY/MD
 Sample : N2587-12
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 EXET8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
 Title : VOC Analysis

77	10.864	2959	2962	2963	rBV	502	267	0.02%	0.002%
78	10.893	2963	2971	2983	rVB2	5968	10232	0.63%	0.078%
79	11.111	3036	3039	3044	rVB2	772	568	0.04%	0.004%
80	11.147	3044	3050	3053	rBV2	337	442	0.03%	0.003%
81	11.417	3129	3134	3137	rBV3	682	619	0.04%	0.005%
82	11.455	3139	3146	3150	rBV2	1303	1736	0.11%	0.013%
83	11.697	3217	3221	3227	rVB2	656	605	0.04%	0.005%
84	11.751	3231	3238	3244	rBV5	1643	2315	0.14%	0.018%
85	11.812	3244	3257	3274	rBV	716185	1125462	69.75%	8.617%
86	11.925	3289	3292	3294	rVB2	458	234	0.01%	0.002%
87	11.954	3295	3301	3304	rBV7	1382	1611	0.10%	0.012%
88	12.047	3325	3330	3334	rBV4	364	397	0.02%	0.003%
89	12.070	3334	3337	3339	rBV	595	344	0.02%	0.003%
90	12.095	3343	3345	3349	rVB2	376	270	0.02%	0.002%
91	12.195	3362	3376	3396	rBV	755657	1245041	77.16%	9.532%
92	12.327	3415	3417	3418	rBV	428	218	0.01%	0.002%
93	12.770	3548	3555	3564	rBV4	1631	2768	0.17%	0.021%
94	12.976	3611	3619	3628	rVB3	3741	6400	0.40%	0.049%
95	13.095	3653	3656	3660	rBV	397	297	0.02%	0.002%
96	13.214	3689	3693	3694	rBV2	365	239	0.01%	0.002%
97	13.336	3727	3731	3737	rBV4	649	857	0.05%	0.007%
98	13.378	3737	3744	3754	rVB6	5724	8572	0.53%	0.066%
99	14.497	4083	4092	4103	rVB5	11659	18388	1.14%	0.141%
100	15.545	4409	4418	4430	rBV3	28159	43899	2.72%	0.336%




Sum of corrected areas: 13061088

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042822\
Data File : VU048345.D
Acq On : 28 Apr 2022 16:48
Operator : SY/MD
Sample : N2587-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXET8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

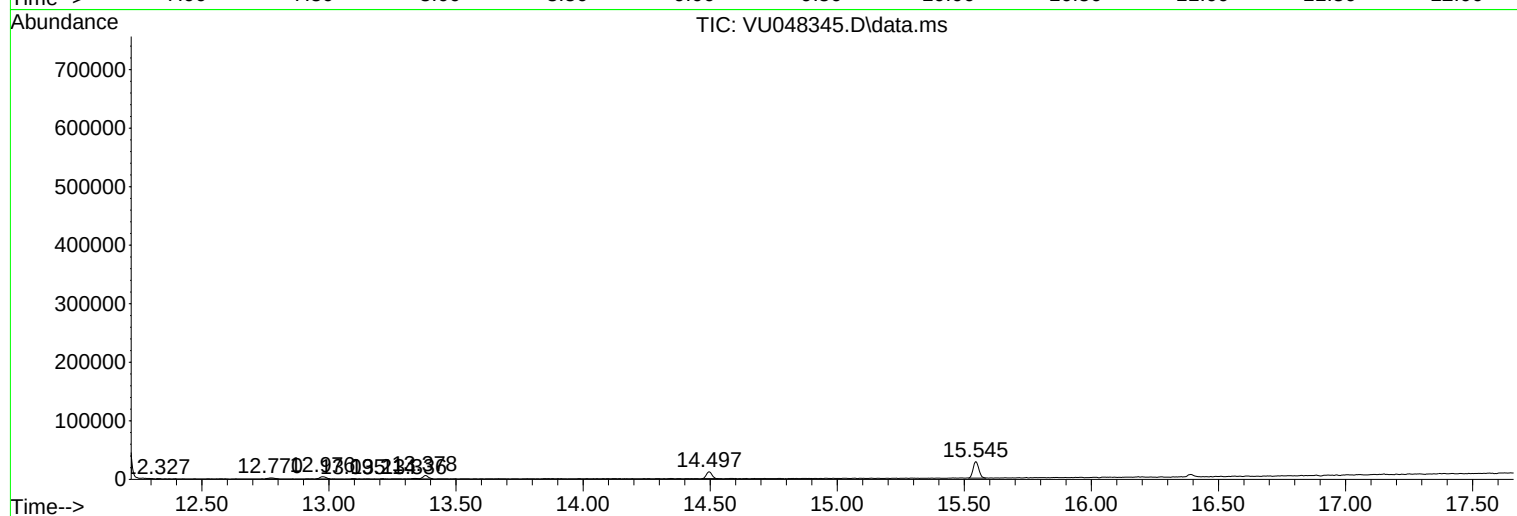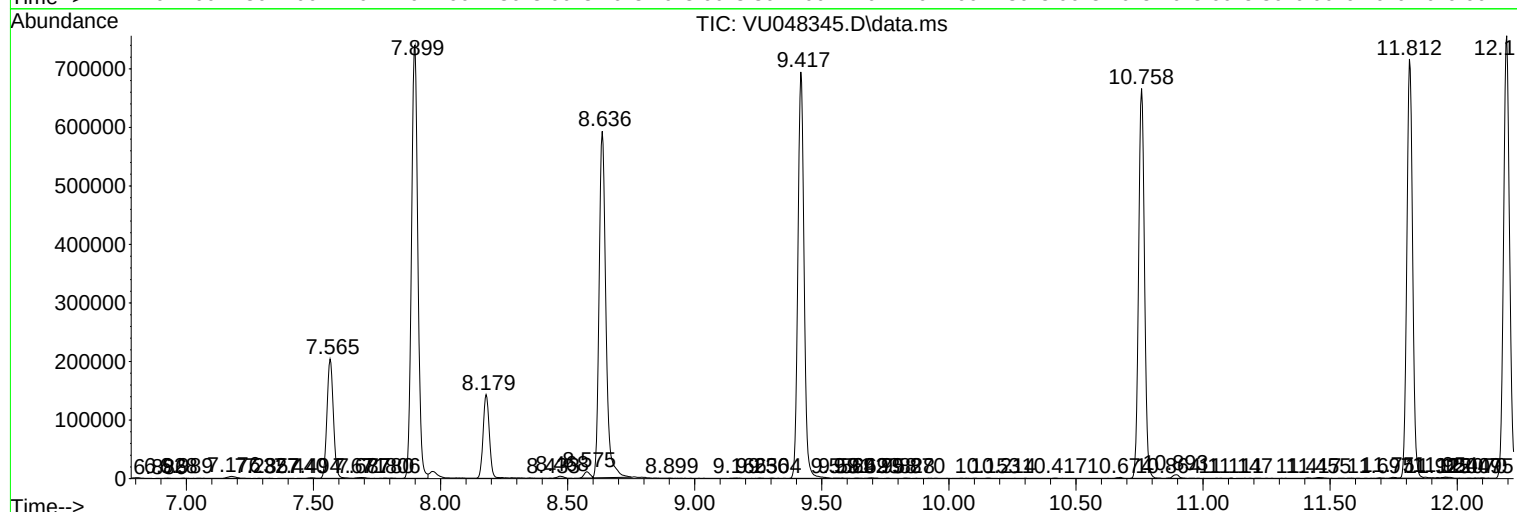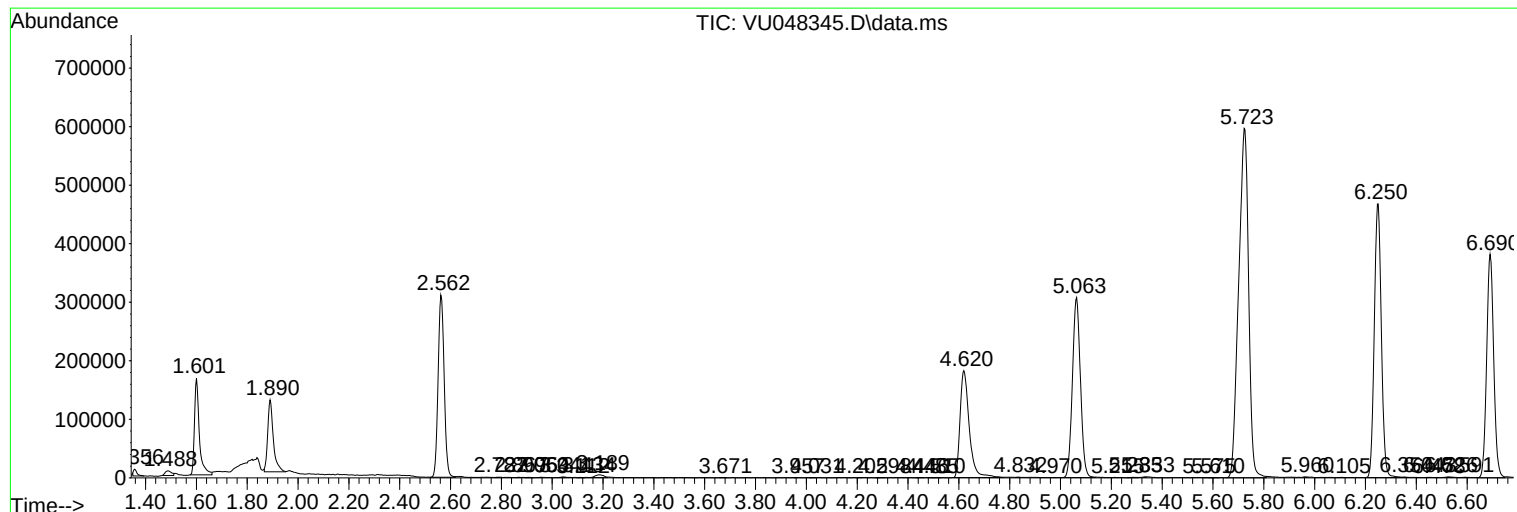

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042822\
Data File : VU048345.D
Acq On : 28 Apr 2022 16:48
Operator : SY/MD
Sample : N2587-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXET8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042822\
Data File : VU048345.D
Acq On : 28 Apr 2022 16:48
Operator : SY/MD
Sample : N2587-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
EXET8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------