


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042822\
Data File : VU048328.D
Acq On : 28 Apr 2022 08:50
Operator : SY/MD
Sample : BFB075
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB075

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM042522WMA.M
Title : VOC Analysis
Last Update : Fri Apr 29 04:27:14 2022

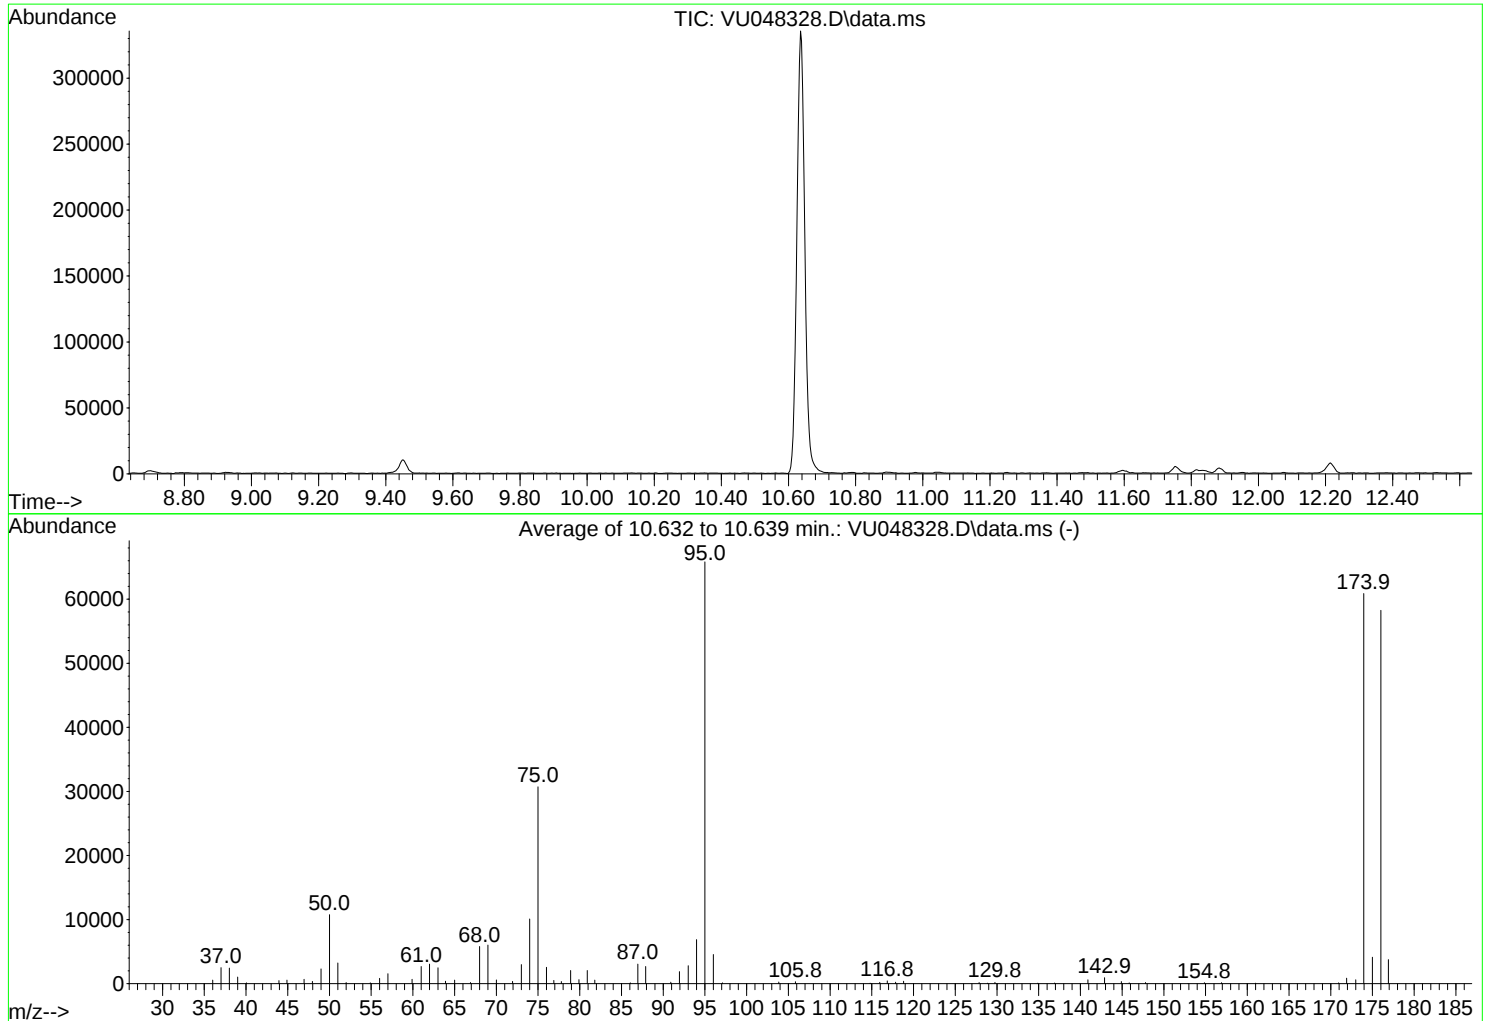

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.3	10761	PASS
75	95	30	80	46.7	30717	PASS
95	95	100	100	100.0	65832	PASS
96	95	5	9	6.9	4557	PASS
173	174	0.00	2	1.0	606	PASS
174	95	50	120	92.5	60880	PASS
175	174	5	9	6.8	4131	PASS
176	174	95	101	95.7	58256	PASS
177	176	5	9	6.4	3757	PASS

m/z	Abundance
39.80	107.0
43.90	310.0

Instrument :
MSVOA_U
ClientSampleId :
BFB075

m/z	Abundance
36.00	498.0
37.00	2539.0
38.00	2295.0
39.00	943.0
40.10	179.0
44.00	831.0
44.90	524.0
47.00	587.0
48.00	367.0
49.00	2244.0
50.00	10723.0
51.00	3167.0
52.00	166.0
54.90	129.0
56.00	808.0
57.00	1643.0
59.90	701.0
61.00	2641.0
62.00	3007.0
63.00	2612.0
63.80	322.0
65.00	553.0
66.90	196.0
68.00	5831.0
69.00	6044.0
70.00	568.0
71.90	349.0
73.00	3055.0
74.00	9909.0
75.00	30672.0
76.00	2481.0
76.90	464.0
77.80	308.0
78.90	2071.0
79.90	592.0
80.90	2054.0
81.80	588.0
86.00	113.0
87.00	3111.0
87.90	2755.0
90.90	237.0
92.00	1864.0
93.00	2747.0
94.00	6814.0
95.00	65744.0
96.00	4350.0
97.10	129.0
103.90	247.0
105.80	328.0
114.80	103.0
115.90	191.0
116.80	429.0
117.90	211.0
118.80	406.0
127.80	219.0
128.90	128.0
129.70	232.0
134.90	119.0
136.90	112.0
140.90	587.0
142.90	923.0
144.90	320.0
145.80	141.0
147.80	183.0
152.90	101.0
154.80	155.0
156.90	149.0
161.00	126.0
171.00	103.0
171.90	798.0
173.00	532.0
173.90	62832.0
175.00	4109.0
176.00	59856.0
176.90	3920.0

Instrument :
MSVOA_U
ClientSampleId :
BFB075

m/z	Abundance
36.00	583.0
37.00	2585.0
38.00	2533.0
39.00	1079.0
40.00	168.0
44.00	805.0
44.90	564.0
47.00	685.0
47.90	366.0
49.00	2406.0
50.00	11120.0
51.00	3329.0
52.00	183.0
54.90	135.0
56.00	881.0
57.00	1583.0
59.90	713.0
61.00	2768.0
62.00	3189.0
63.00	2582.0
63.90	379.0
65.00	551.0
66.90	196.0
68.00	5952.0
69.00	6214.0
70.00	616.0
71.90	378.0
73.00	3054.0
74.00	10371.0
75.00	31736.0
76.00	2641.0
76.90	513.0
77.80	336.0
78.90	2138.0
79.90	644.0
80.90	2090.0
81.80	560.0
86.10	125.0
86.90	3127.0
87.90	2745.0
90.90	244.0
92.00	1923.0
93.00	2882.0
94.00	6975.0
95.00	68024.0
96.00	4816.0
97.10	130.0
103.80	242.0
105.80	325.0
114.80	118.0
116.00	224.0
116.90	442.0
117.80	231.0
118.80	416.0
127.80	192.0
128.80	117.0
129.70	208.0
134.90	122.0
136.90	120.0
140.90	608.0
142.90	965.0
144.90	339.0
145.90	120.0
147.80	188.0
154.90	163.0
156.90	156.0
161.00	101.0
171.00	118.0
171.90	878.0
173.00	601.0
174.00	62880.0
175.00	4243.0
176.00	60072.0
176.90	3886.0

Instrument :
MSVOA_U
ClientSampleId :
BFB075

m/z	Abundance
36.00	575.0
37.00	2408.0
38.00	2439.0
39.00	1077.0
39.80	179.0
44.00	716.0
44.90	555.0
46.90	748.0
47.90	322.0
49.00	2245.0
50.00	10441.0
51.00	3202.0
52.00	176.0
54.90	130.0
56.00	793.0
57.00	1410.0
59.90	607.0
61.00	2635.0
62.00	2938.0
63.00	2260.0
64.00	431.0
65.00	526.0
66.90	171.0
68.00	5577.0
69.00	5772.0
70.00	569.0
72.00	355.0
73.00	2796.0
74.00	10020.0
75.00	29744.0
76.00	2502.0
76.90	537.0
77.80	307.0
78.90	1959.0
79.90	651.0
80.90	2034.0
81.80	503.0
86.10	131.0
86.90	2931.0
87.90	2551.0
90.90	233.0
91.90	1855.0
93.00	2774.0
94.00	6780.0
95.00	63728.0
96.00	4506.0
97.10	119.0
103.80	243.0
105.90	283.0
115.90	213.0
116.80	445.0
117.80	217.0
118.80	335.0
127.90	151.0
129.90	180.0
136.90	105.0
140.90	620.0
142.90	866.0
144.90	342.0
145.90	111.0
147.80	180.0
154.90	151.0
156.90	138.0
170.90	133.0
171.90	894.0
173.00	684.0
174.00	56928.0
175.00	4041.0
176.00	54840.0
176.90	3465.0

Instrument :
MSVOA_U
ClientSampleId :
BFB075