

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042823\
 Data File : VU053942.D
 Acq On : 27 Apr 2023 18:02
 Operator : JC/MD
 Sample : 02488-06
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE62

Quant Time: Apr 28 07:20:40 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 27 05:52:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	145435	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	137263	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.809	152	65631	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.600	65	29286	3.306	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	66.200%
7) Chloroethane-d5	1.916	69	27835	3.744	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	74.800%
11) 1,1-Dichloroethene-d2	2.565	65	13739	3.769	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	75.400%
20) 2-Butanone-d5	4.636	46	78365	48.300	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.600%
24) Chloroform-d	5.060	84	72520	4.344	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.800%
26) 1,2-Dichloroethane-d4	5.700	65	34781	4.509	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.200%
32) Benzene-d6	5.722	84	141472	4.375	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.600%
36) 1,2-Dichloropropane-d6	6.687	67	44999	4.600	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.000%
41) Toluene-d8	7.893	98	124490	4.125	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.600%
43) trans-1,3-Dichloroprop...	8.179	79	15669	4.073	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.400%
46) 2-Hexanone-d5	8.629	63	65378	48.017	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	96.040%
56) 1,1,2,2-Tetrachloroeth...	10.751	84	35055	4.434	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.600%
66) 1,2-Dichlorobenzene-d4	12.188	152	45850	4.356	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	87.200%
Target Compounds						Qvalue
12) 1,1-Dichloroethene	2.581	96	3776	0.413	ug/L #	1
17) Methyl tert-butyl Ether	3.359	73	6075	0.307	ug/L #	85
19) 1,1-Dichloroethane	3.867	63	2757	0.165	ug/L #	87
22) cis-1,2-Dichloroethene	4.665	96	16452	1.578	ug/L	95
25) Chloroform	5.086	83	11361	0.625	ug/L	99
31) Carbon tetrachloride	5.520	117	7526	0.561	ug/L	100
34) Trichloroethene	6.539	95	108212	10.264	ug/L	98
47) Tetrachloroethene	8.552	164	22842	2.733	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042823\
Data File : VU053942.D
Acq On : 27 Apr 2023 18:02
Operator : JC/MD
Sample : 02488-06
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE62

Quant Time: Apr 28 07:20:40 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 27 05:52:18 2023
Response via : Initial Calibration

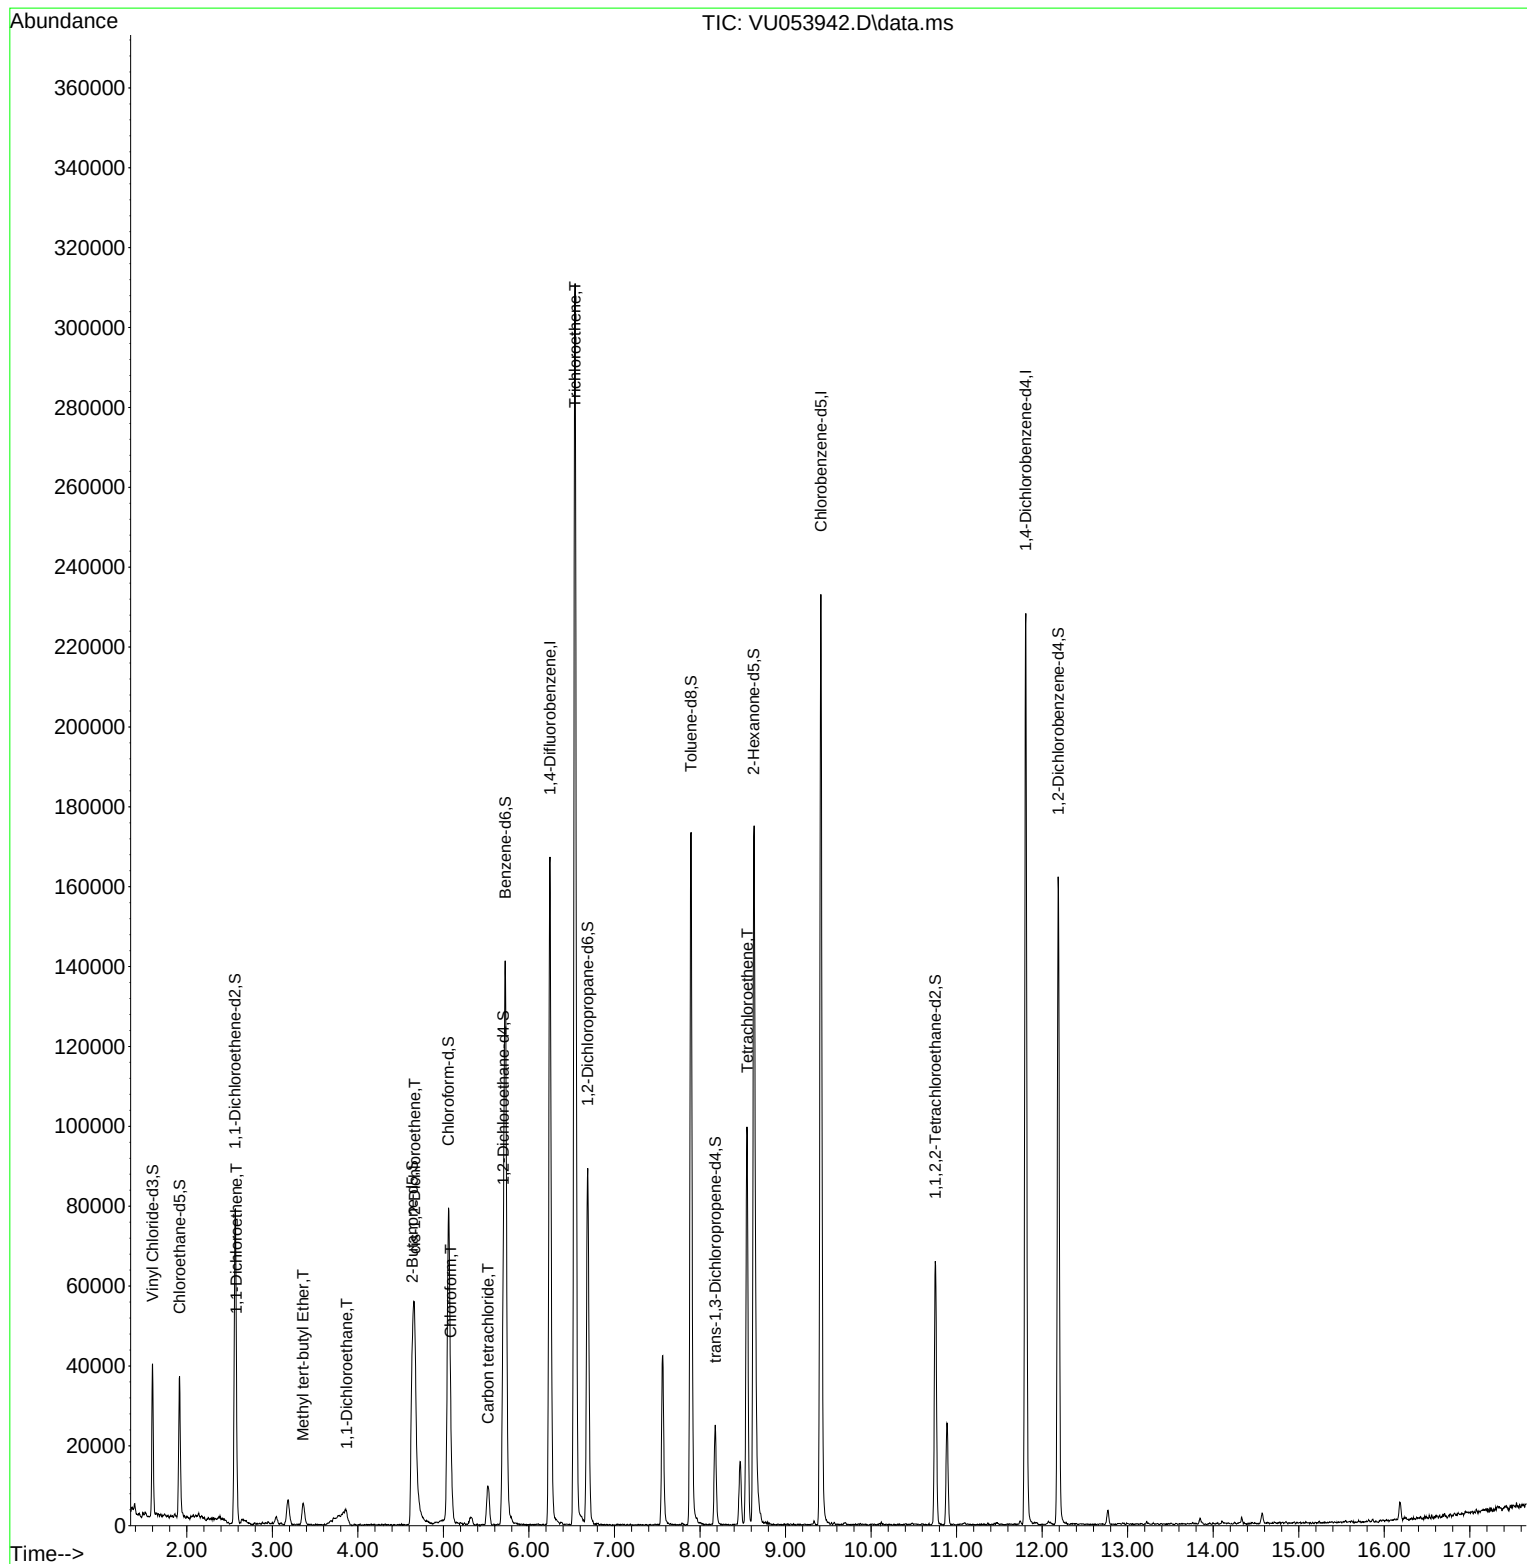

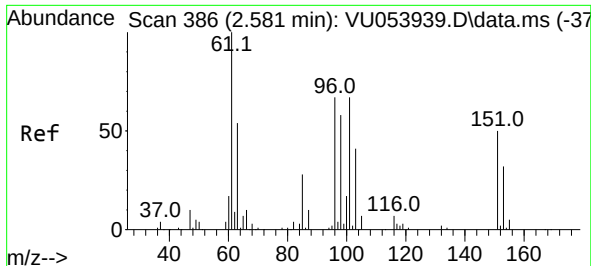

#12

1,1-Dichloroethene

Concen: 0.413 ug/L

RT: 2.581 min Scan# 386

Delta R.T. 0.003 min

Lab File: VU053942.D

Acq: 27 Apr 2023 18:02

Instrument :

MSVOA_U

ClientSampleId :

BHE62





Tgt Ion: 96 Resp: 3776

Ion Ratio Lower Upper

96 100

61 176.9 111.5 207.1

63 476.0 68.7 127.7#

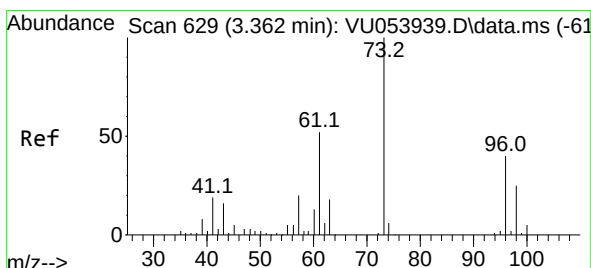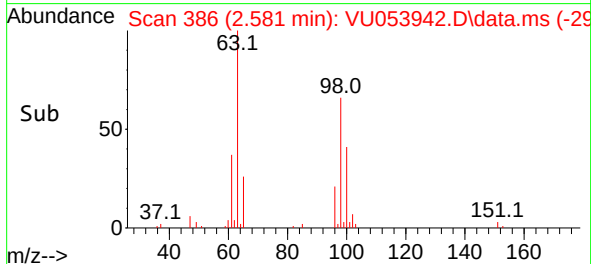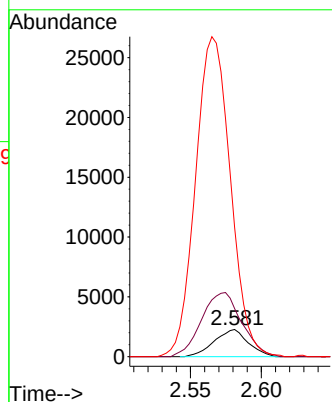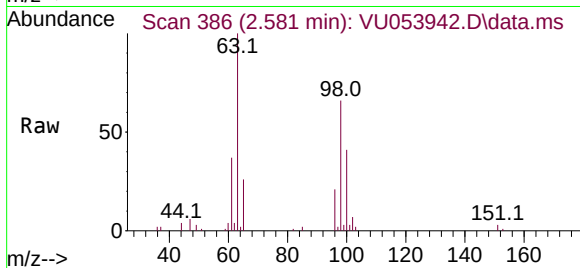

#17

Methyl tert-butyl Ether

Concen: 0.307 ug/L

RT: 3.359 min Scan# 628

Delta R.T. -0.003 min

Lab File: VU053942.D

Acq: 27 Apr 2023 18:02




Tgt Ion: 73 Resp: 6075


Ion Ratio Lower Upper

73 100

43 18.8 13.4 20.2

57 10.9 17.2 25.8#


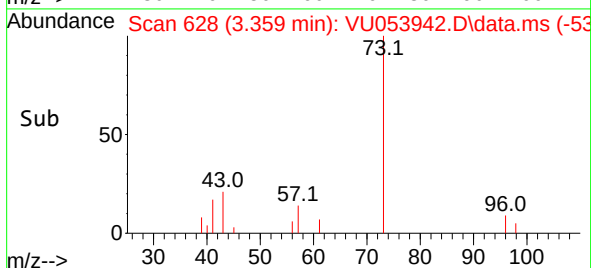
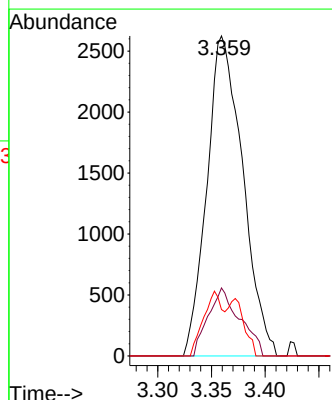
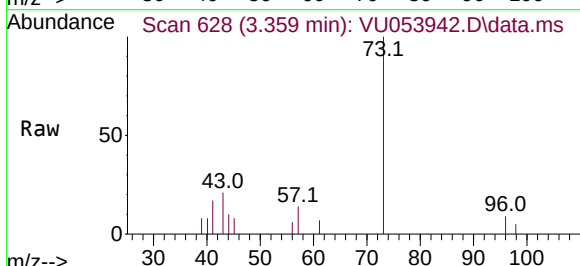


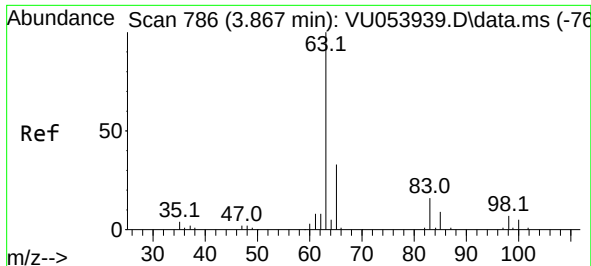

#19
1,1-Dichloroethane
Concen: 0.165 ug/L
RT: 3.867 min Scan# 71
Delta R.T. 0.003 min
Lab File: VU053942.D
Acq: 27 Apr 2023 18:02




Instrument :
MSVOA_U
ClientSampleId :
BHE62


Tgt Ion:	63	Resp:	2757
Ion	Ratio	Lower	Upper
63	100		
65	38.3	22.0	40.8
83	8.8	10.3	19.1#

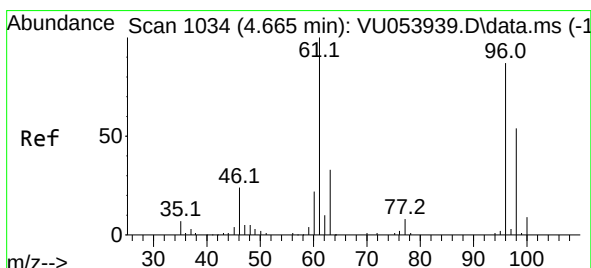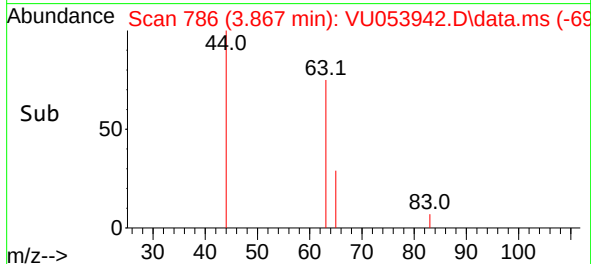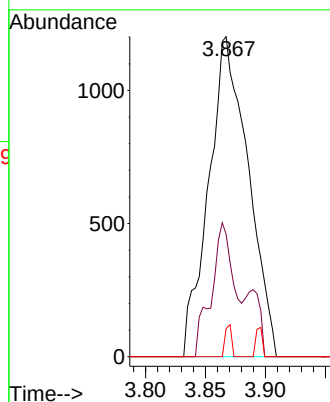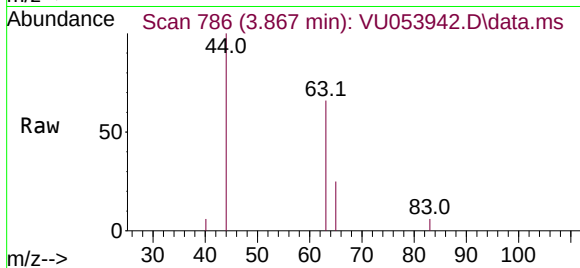

#22
cis-1,2-Dichloroethene
Concen: 1.578 ug/L
RT: 4.665 min Scan# 1034
Delta R.T. 0.003 min
Lab File: VU053942.D
Acq: 27 Apr 2023 18:02

Tgt Ion:	96	Resp:	16452
Ion	Ratio	Lower	Upper
96	100		
61	113.4	84.3	156.5
98	67.8	46.4	86.2

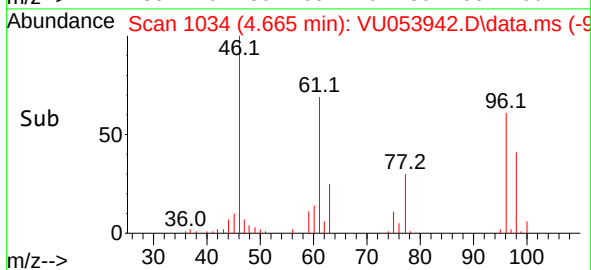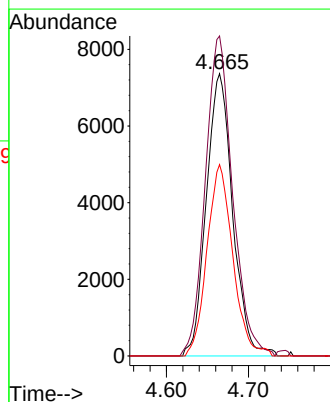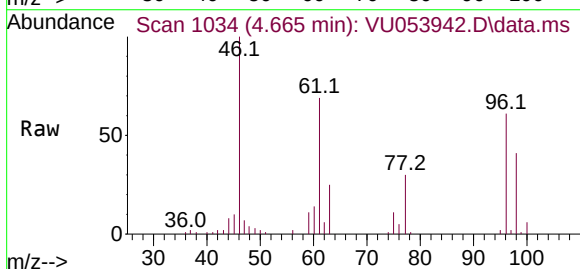

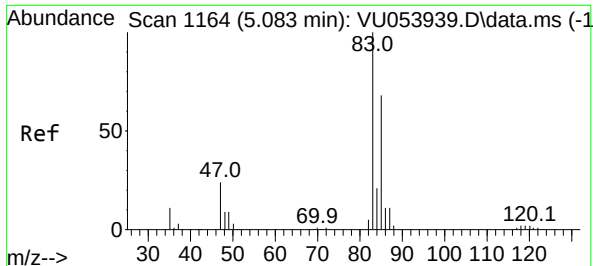

#25

Chloroform

Concen: 0.625 ug/L

RT: 5.086 min Scan# 1164

Delta R.T. 0.000 min

Lab File: VU053942.D

Acq: 27 Apr 2023 18:02

Instrument :

MSVOA_U

ClientSampleId :





BHE62

Tgt Ion: 83 Resp: 11361

Ion Ratio Lower Upper

83 100

85 66.0 45.6 84.8

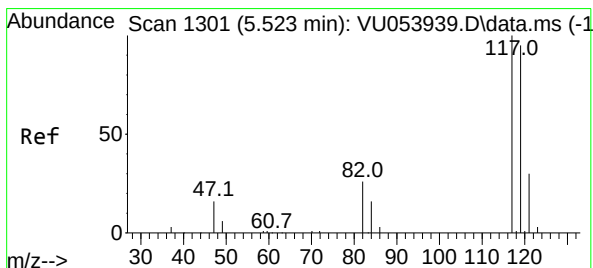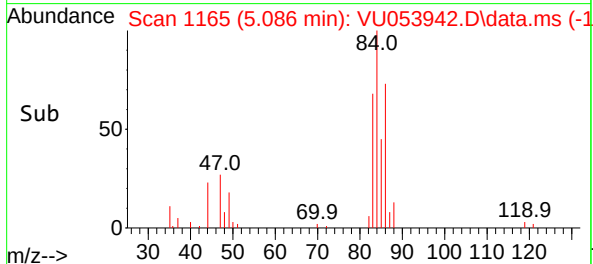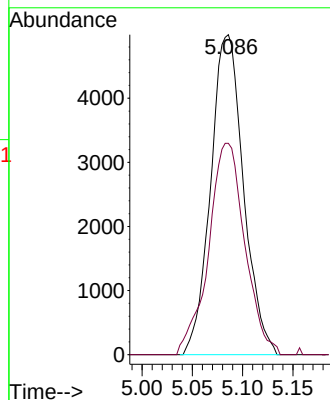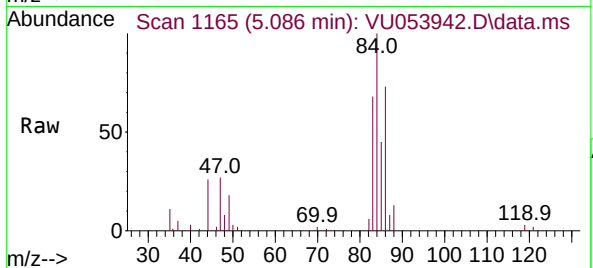

#31

Carbon tetrachloride

Concen: 0.561 ug/L

RT: 5.520 min Scan# 1300

Delta R.T. 0.000 min

Lab File: VU053942.D




Acq: 27 Apr 2023 18:02


Tgt Ion: 117 Resp: 7526

Ion Ratio Lower Upper

117 100

119 94.0 75.0 112.6


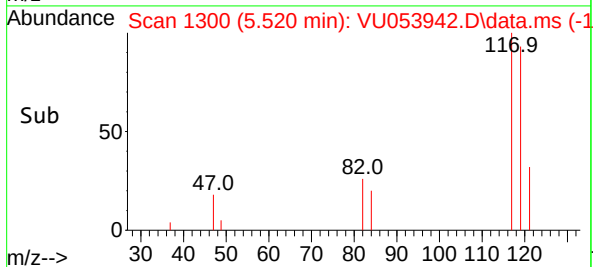
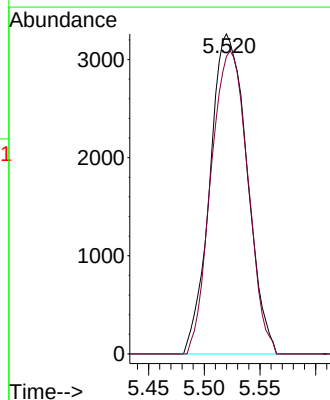
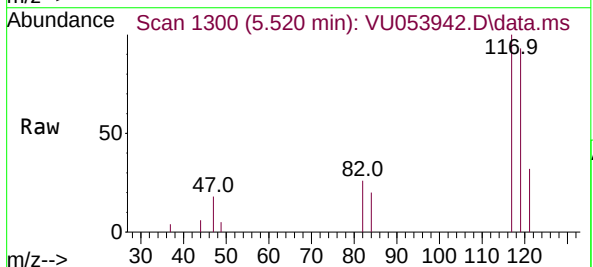


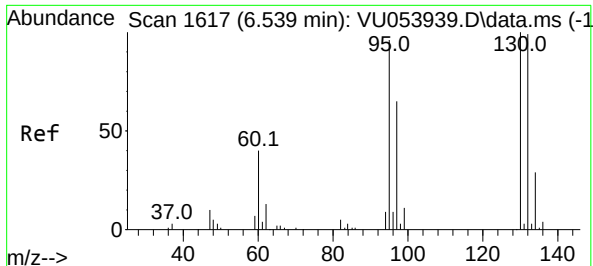

#34
Trichloroethene
Concen: 10.264 ug/L
RT: 6.539 min Scan# 1
Delta R.T. 0.000 min
Lab File: VU053942.D
Acq: 27 Apr 2023 18:02

Instrument :
MSVOA_U
ClientSampleId :
BHE62

Tgt Ion: 95 Resp: 108212
Ion Ratio Lower Upper
95 100
97 62.7 45.1 83.9
132 96.3 69.9 129.9
130 101.9 71.3 132.3

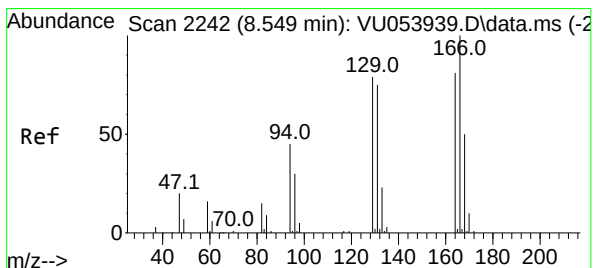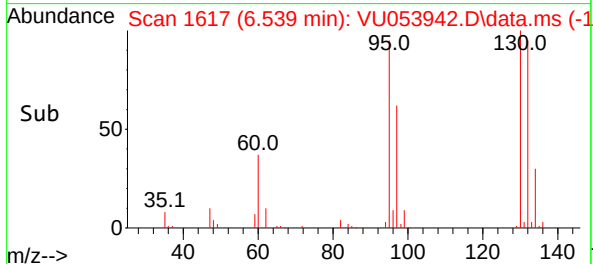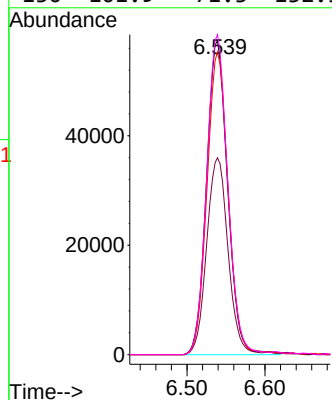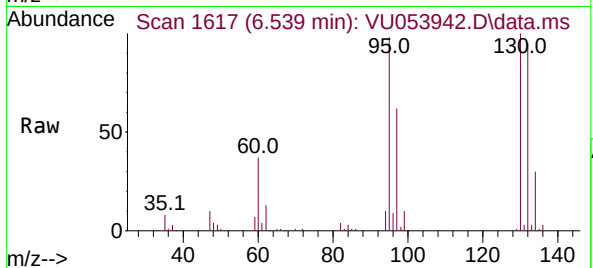

#47
Tetrachloroethene
Concen: 2.733 ug/L
RT: 8.552 min Scan# 2243
Delta R.T. 0.003 min
Lab File: VU053942.D
Acq: 27 Apr 2023 18:02

Tgt Ion:164 Resp: 22842
Ion Ratio Lower Upper
164 100
129 89.8 68.3 126.8
131 89.3 64.4 119.6
166 120.4 88.3 163.9

