

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042823\
 Data File : VU053959.D
 Acq On : 28 Apr 2023 00:54
 Operator : JC/MD
 Sample : 02528-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 HOA39

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 05/01/2023
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 28 07:22:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 27 05:52:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.247	114	140511	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.414	117	133427	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.806	152	65076	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.597	65	27615	3.226	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	64.600%	
7) Chloroethane-d5	1.912	69	25981	3.617	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	72.400%	
11) 1,1-Dichloroethene-d2	2.565	65	13314	3.780	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	75.600%	
20) 2-Butanone-d5	4.645	46	69775	44.512	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	89.020%	
24) Chloroform-d	5.060	84	82591	5.121	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	102.400%	
26) 1,2-Dichloroethane-d4	5.697	65	31338	4.205	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	84.000%	
32) Benzene-d6	5.723	84	129332	4.115	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	82.200%	
36) 1,2-Dichloropropane-d6	6.687	67	41741	4.390	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	87.800%	
41) Toluene-d8	7.896	98	114110	3.890	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	77.800%	
43) trans-1,3-Dichloroprop...	8.176	79	14587	3.901	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	78.000%	
46) 2-Hexanone-d5	8.632	63	64062	48.404	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	96.800%	
56) 1,1,2,2-Tetrachloroeth...	10.751	84	33494	4.359	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	87.200%	
66) 1,2-Dichlorobenzene-d4	12.189	152	42477	4.070	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	81.400%	
Target Compounds						
					Qvalue	
3) Chloromethane	1.520	50	2485	0.245	ug/L	99
6) Bromomethane	1.858	94	2866	0.377	ug/L	91
12) 1,1-Dichloroethene	2.578	96	250307	28.322	ug/L #	79
13) Acetone	2.678	43	21079m	16.582	ug/L	
14) Carbon disulfide	2.790	76	4112	0.170	ug/L	97
16) Methylene chloride	3.044	84	6991	0.580	ug/L	91
18) trans-1,2-Dichloroethene	3.346	96	2749	0.308	ug/L	87
19) 1,1-Dichloroethane	3.864	63	162326	10.043	ug/L	96
22) cis-1,2-Dichloroethene	4.662	96	54126	5.372	ug/L	97
25) Chloroform	5.083	83	404916	23.068	ug/L	100
27) 1,2-Dichloroethane	5.800	62	4282	0.426	ug/L #	92
29) 1,1,1-Trichloroethane	5.311	97	446183	29.747	ug/L	98
31) Carbon tetrachloride	5.520	117	6937	0.532	ug/L	90
33) Benzene	5.774	78	13876	0.369	ug/L	100
34) Trichloroethene	6.536	95	2179831	212.695	ug/L	99
38) Bromodichloromethane	7.105	83	3138	0.269	ug/L #	84
45) 1,1,2-Trichloroethane	8.398	97	5581	0.798	ug/L	95
47) Tetrachloroethene	8.562	164	12769294	1571.992	ug/L	94
54) o-Xylene	10.102	106	3487	0.215	ug/L	97

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042823\
 Data File : VU053959.D
 Acq On : 28 Apr 2023 00:54
 Operator : JC/MD
 Sample : 02528-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 HOA39

Manual Integrations
 APPROVED

Reviewed By :Krupa Patel 05/01/2023
 Supervised By :Mahesh Dadoda 05/01/2023

Quant Time: Apr 28 07:22:44 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Apr 27 05:52:18 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
57) 1,1,2,2-Tetrachloroethane	10.777	83	2555	0.306	ug/L	85
64) 1,3-Dichlorobenzene	11.742	146	18809	0.962	ug/L	94
65) 1,4-Dichlorobenzene	11.832	146	34429	1.742	ug/L	96
67) 1,2-Dichlorobenzene	12.208	146	145447	8.054	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042823\
Data File : VU053959.D
Acq On : 28 Apr 2023 00:54
Operator : JC/MD
Sample : 02528-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1


Instrument :
MSVOA_U
ClientSampleId :
HOA39

Manual Integrations
APPROVED

Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023


Quant Time: Apr 28 07:22:44 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Apr 27 05:52:18 2023
Response via : Initial Calibration

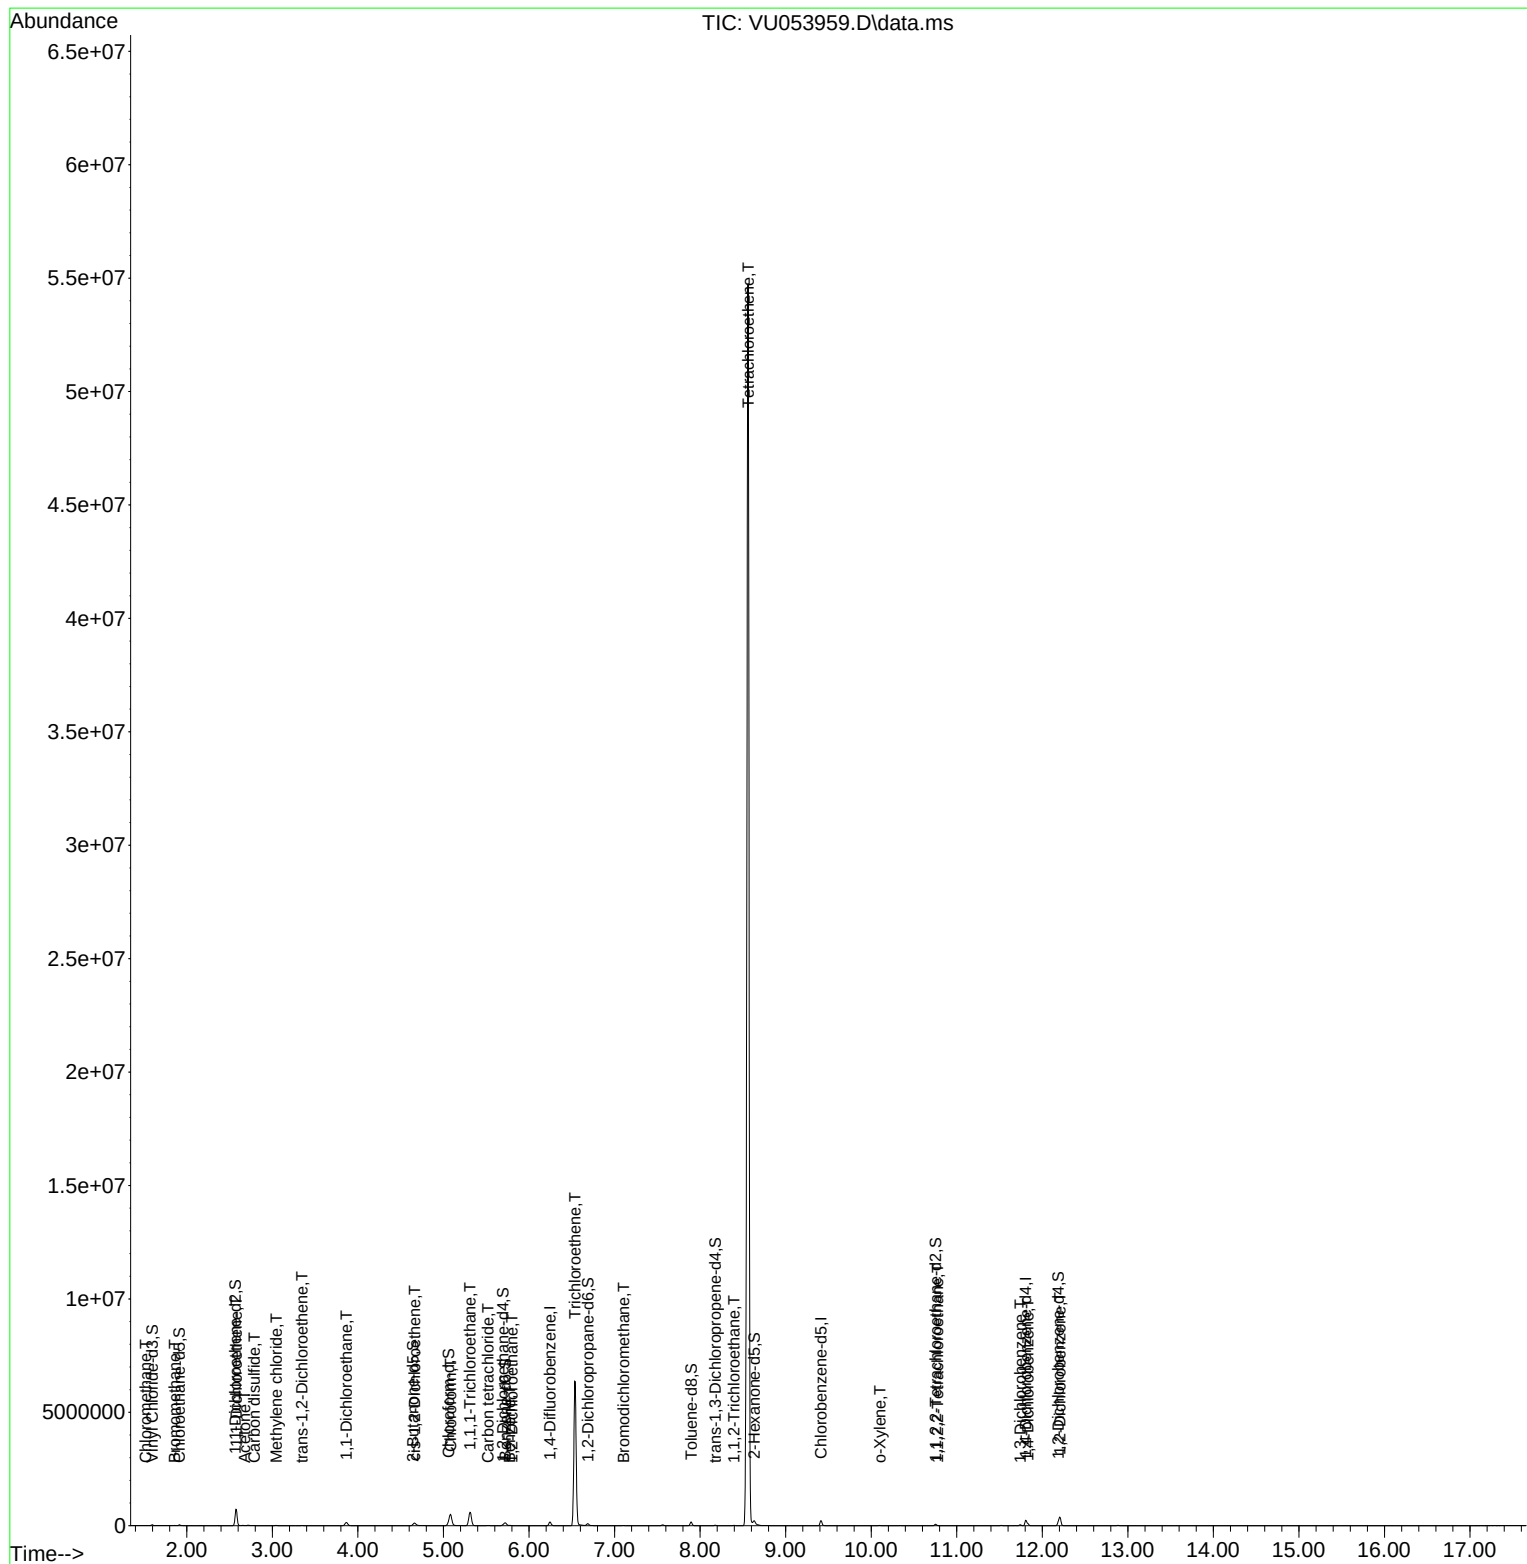

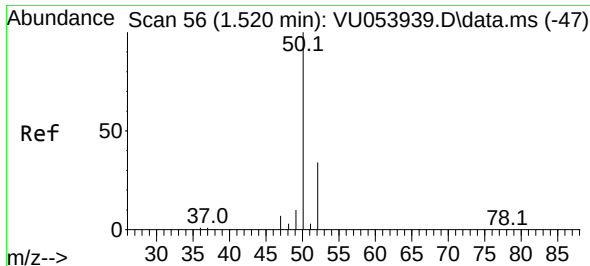

#3
Chloromethane
Concen: 0.245 ug/L
RT: 1.520 min Scan# 50
Delta R.T. 0.000 min
Lab File: VU053959.D
Acq: 28 Apr 2023 00:54




Instrument :
MSVOA_U
ClientSampleId :
HOA39

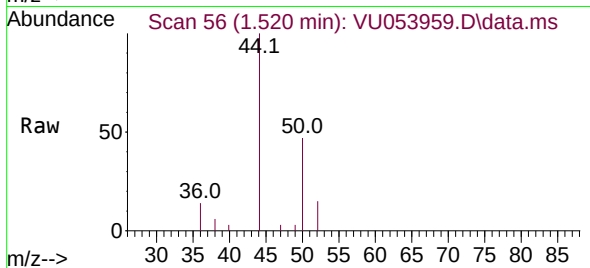


Tgt Ion: 50 Resp: 248
Ion Ratio Lower Upper
50 100
52 32.9 23.4 43.6

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

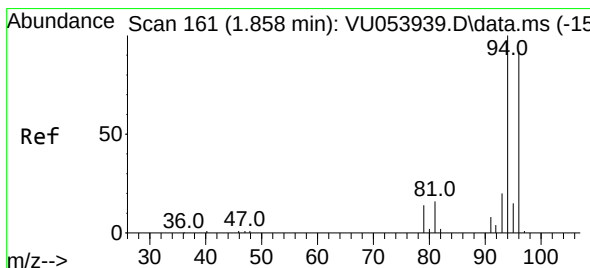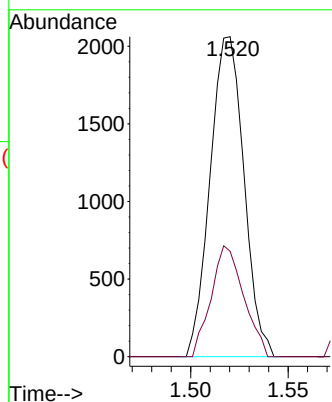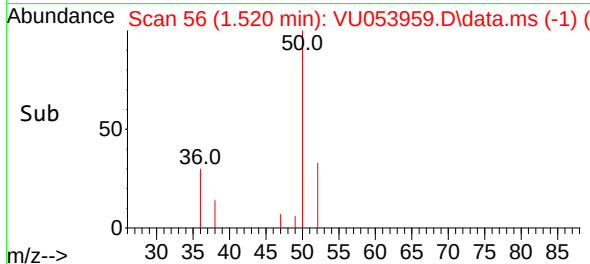


#6
Bromomethane
Concen: 0.377 ug/L
RT: 1.858 min Scan# 161
Delta R.T. -0.003 min
Lab File: VU053959.D
Acq: 28 Apr 2023 00:54

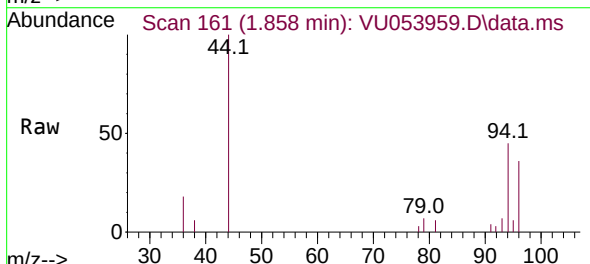

Tgt Ion: 94 Resp: 2866
Ion Ratio Lower Upper
94 100
96 80.3 61.9 114.9

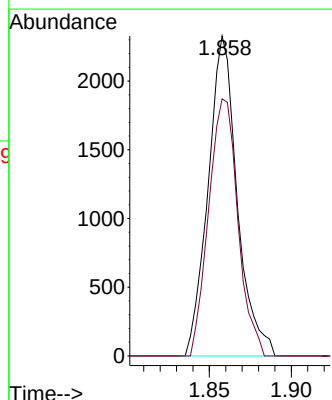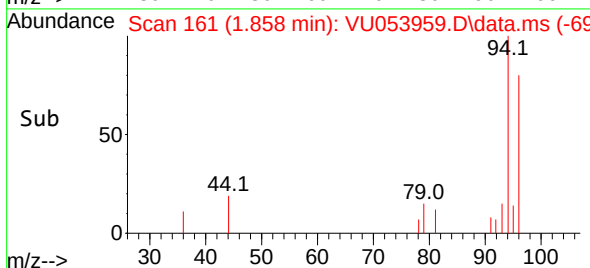

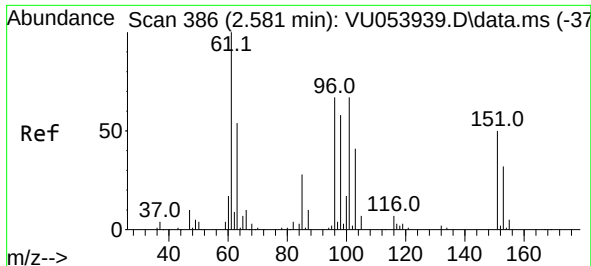

#12

1,1-Dichloroethene

Concen: 28.322 ug/L

RT: 2.578 min Scan# 386

Delta R.T. 0.000 min

Lab File: VU053959.D

Acq: 28 Apr 2023 00:54

Instrument :

MSVOA_U

ClientSampleId :

HOA39

Tgt Ion: 96 Resp: 25030

Ion Ratio Lower Upper

96 100

61 149.7 111.5 207.1





63 54.7 68.7 127.7

Manual Integrations

APPROVED

Reviewed By :Krupa Patel 05/01/2023

Supervised By :Mahesh Dadoda 05/01/2023

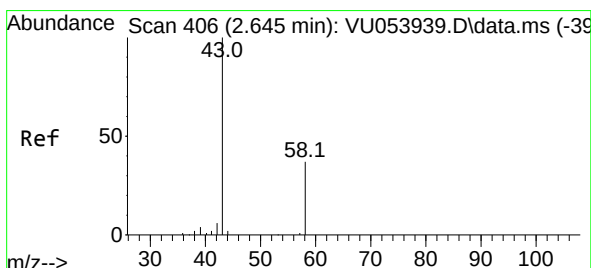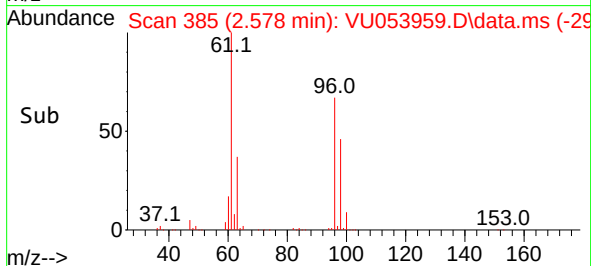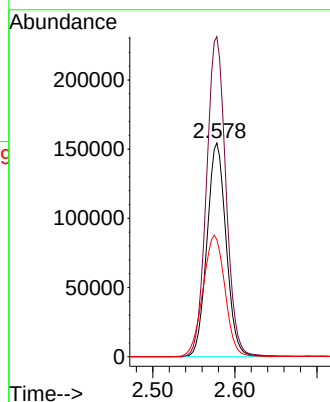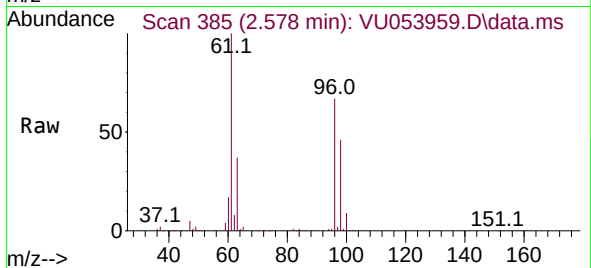

#13

Acetone

Concen: 16.582 ug/L m

RT: 2.678 min Scan# 416

Delta R.T. 0.016 min

Lab File: VU053959.D




Acq: 28 Apr 2023 00:54


Tgt Ion: 43 Resp: 21079

Ion Ratio Lower Upper

43 100

58 31.3 0.0 76.2

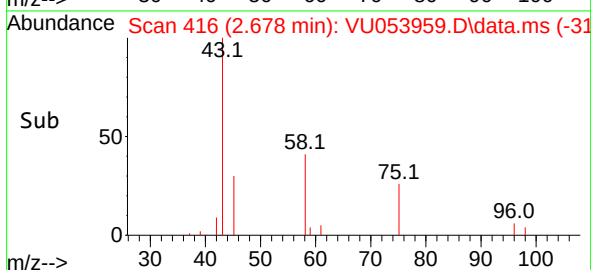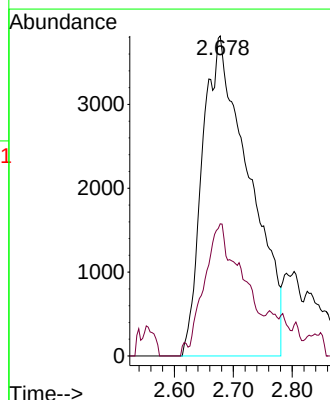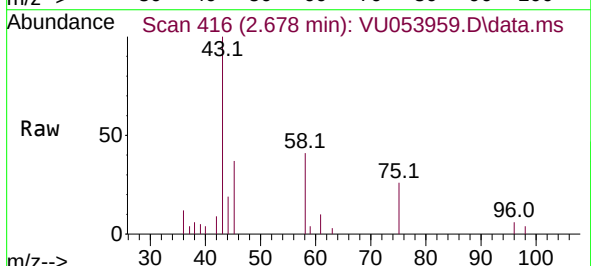

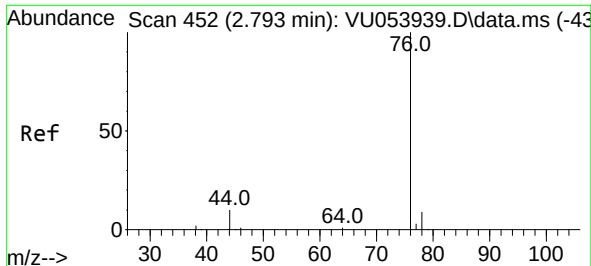





#14
Carbon disulfide
Concen: 0.170 ug/L
RT: 2.790 min Scan# 411
Delta R.T. -0.003 min
Lab File: VU053959.D
Acq: 28 Apr 2023 00:54

Instrument :
MSVOA_U
ClientSampleId :
HOA39

Tgt Ion: 76 Resp: 411
Ion Ratio Lower Upper
76 100
78 7.9 7.3 10.9




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

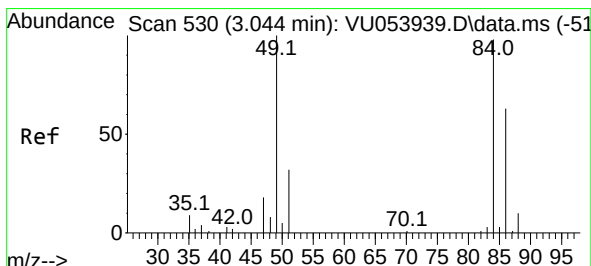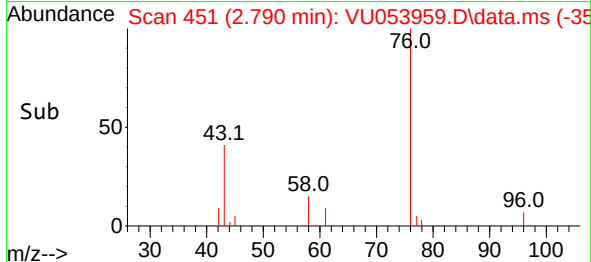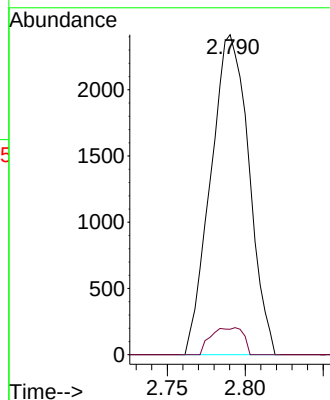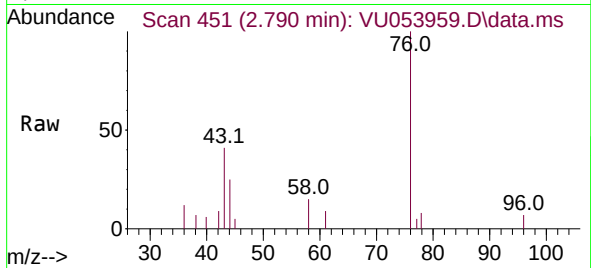

#16
Methylene chloride
Concen: 0.580 ug/L
RT: 3.044 min Scan# 530
Delta R.T. 0.000 min
Lab File: VU053959.D
Acq: 28 Apr 2023 00:54


Tgt Ion: 84 Resp: 6991
Ion Ratio Lower Upper
84 100
86 54.3 45.0 83.6
49 99.1 74.8 138.8

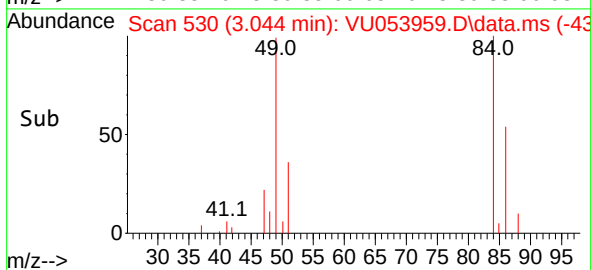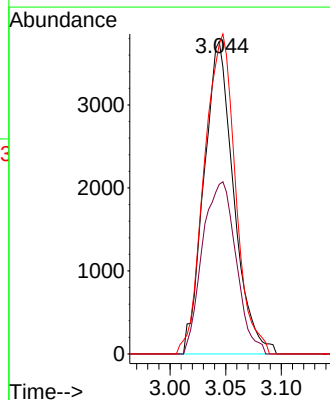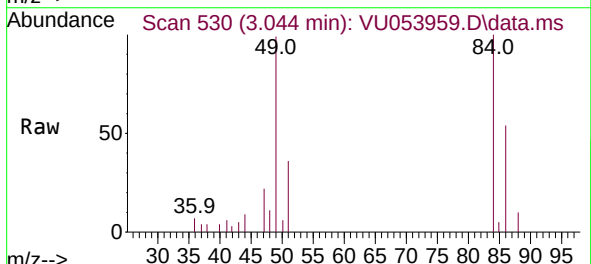

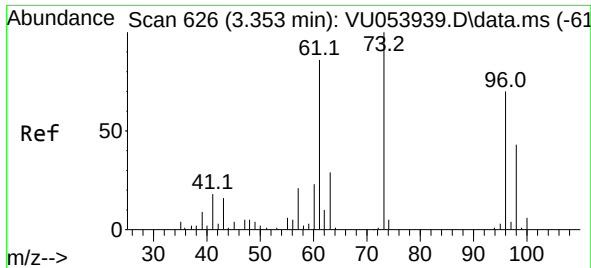

#18
trans-1,2-Dichloroethene
Concen: 0.308 ug/L
RT: 3.346 min Scan# 611
Delta R.T. -0.006 min
Lab File: VU053959.D
Acq: 28 Apr 2023 00:54




Instrument :
MSVOA_U
ClientSampleId :
HOA39

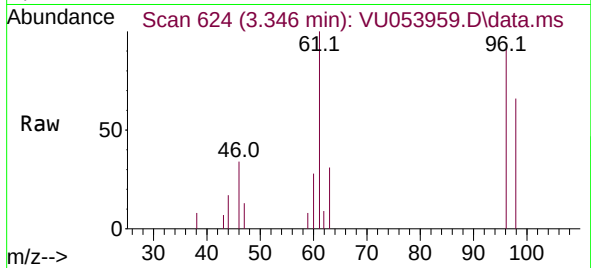


Tgt Ion: 96 Resp: 2749
Ion Ratio Lower Upper
96 100
61 110.0 86.2 160.0
98 72.5 42.8 79.4

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

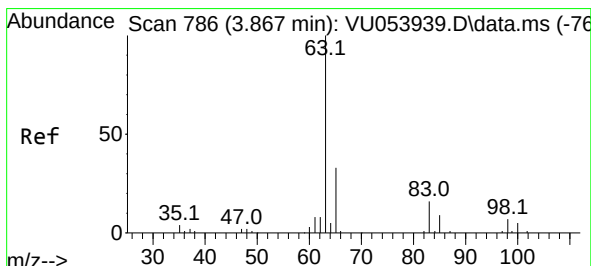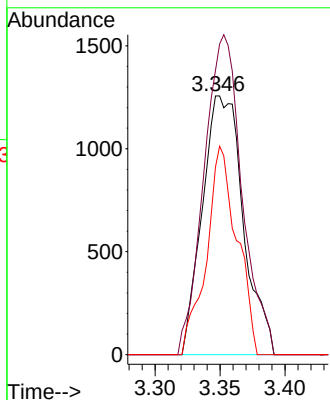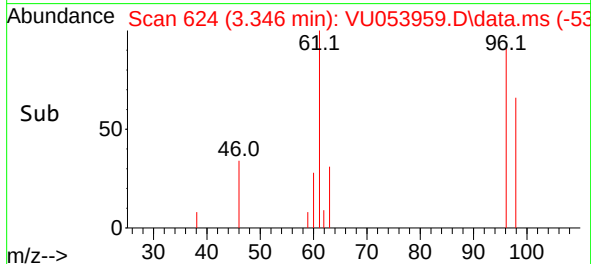


#19
1,1-Dichloroethane
Concen: 10.043 ug/L
RT: 3.864 min Scan# 785
Delta R.T. 0.000 min
Lab File: VU053959.D
Acq: 28 Apr 2023 00:54

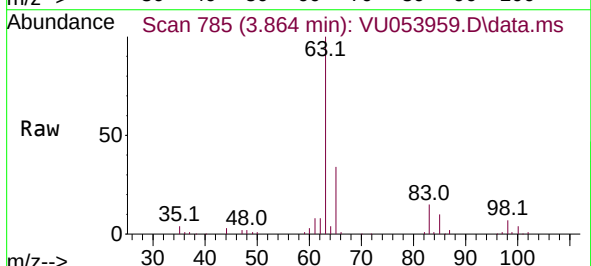

Tgt Ion: 63 Resp: 162326
Ion Ratio Lower Upper
63 100
65 34.4 22.0 40.8
83 14.9 10.3 19.1

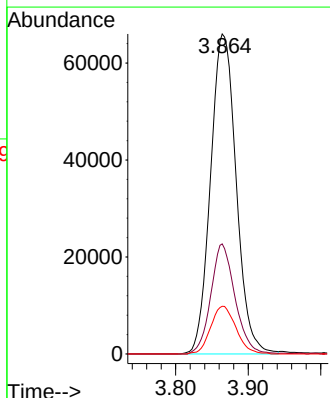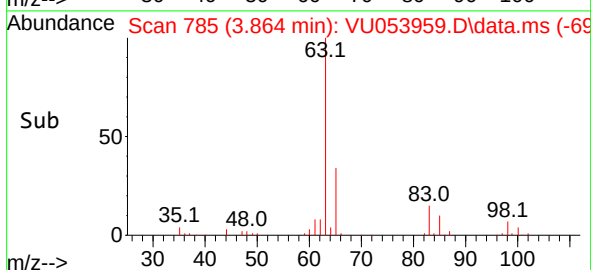







#22
cis-1,2-Dichloroethene
Concen: 5.372 ug/L
RT: 4.662 min Scan# 1033
Delta R.T. 0.000 min
Lab File: VU053959.D
Acq: 28 Apr 2023 00:54

Instrument :
MSVOA_U
ClientSampleId :
HOA39

Tgt Ion: 96 Resp: 54120
Ion Ratio Lower Upper
96 100
61 115.0 84.3 156.5
98 66.4 46.4 86.2




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

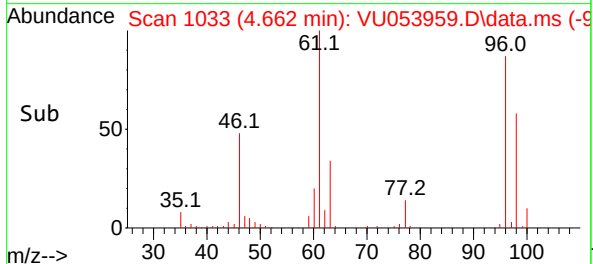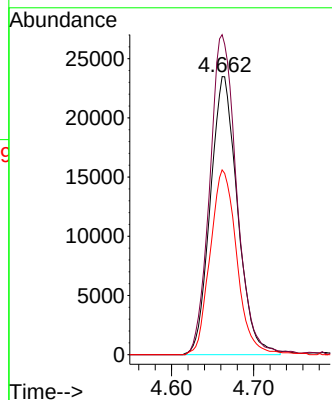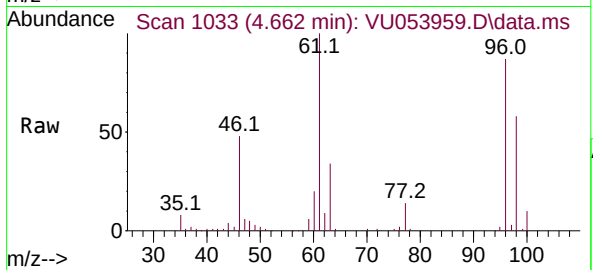

#25
Chloroform
Concen: 23.068 ug/L
RT: 5.083 min Scan# 1164
Delta R.T. -0.003 min
Lab File: VU053959.D
Acq: 28 Apr 2023 00:54

Tgt Ion: 83 Resp: 404916
Ion Ratio Lower Upper
83 100
85 65.3 45.6 84.8

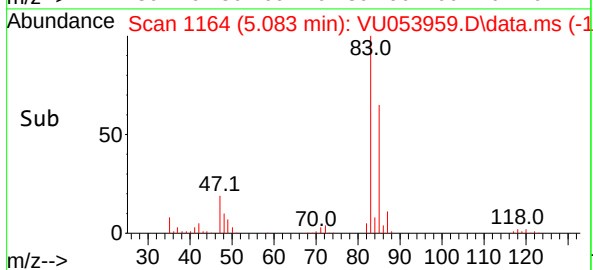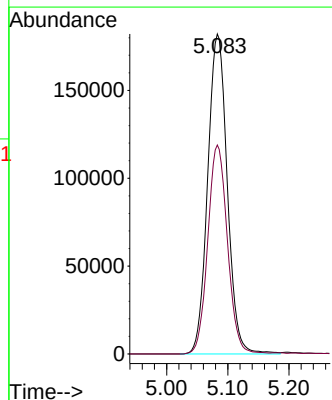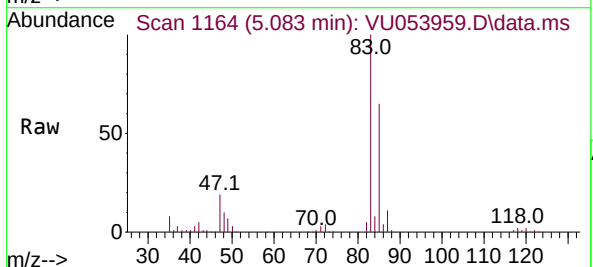

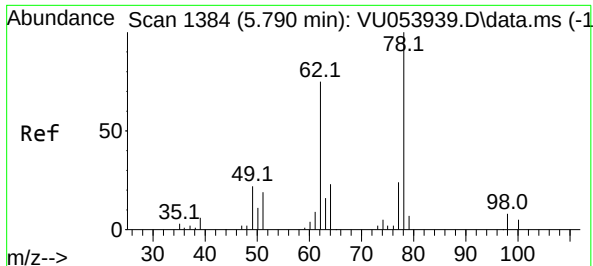





#27
 1,2-Dichloroethane
 Concen: 0.426 ug/L
 RT: 5.800 min Scan# 11
 Delta R.T. 0.010 min
 Lab File: VU053959.D
 Acq: 28 Apr 2023 00:54

Instrument :
 MSVOA_U
 ClientSampleId :
 HOA39

Tgt Ion: 62 Resp: 428
 Ion Ratio Lower Upper
 62 100
 98 7.7 8.7 13.1




Manual Integrations
 APPROVED


Reviewed By :Krupa Patel 05/01/2023
 Supervised By :Mahesh Dadoda 05/01/2023

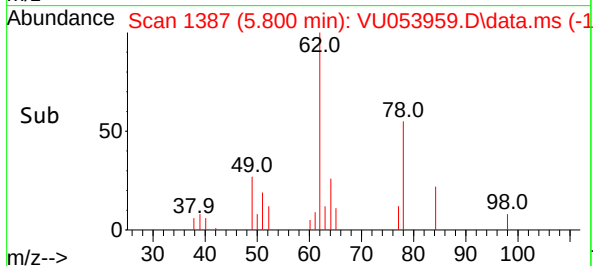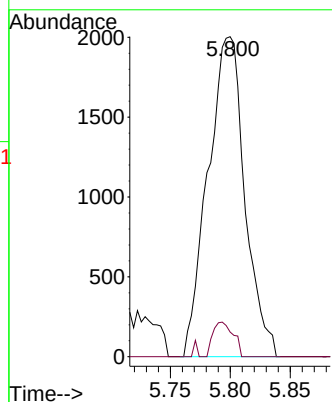

#29
 1,1,1-Trichloroethane
 Concen: 29.747 ug/L
 RT: 5.311 min Scan# 1235
 Delta R.T. -0.003 min
 Lab File: VU053959.D
 Acq: 28 Apr 2023 00:54

Tgt Ion: 97 Resp: 446183
 Ion Ratio Lower Upper
 97 100
 99 65.2 52.9 79.3
 61 40.7 33.8 50.8

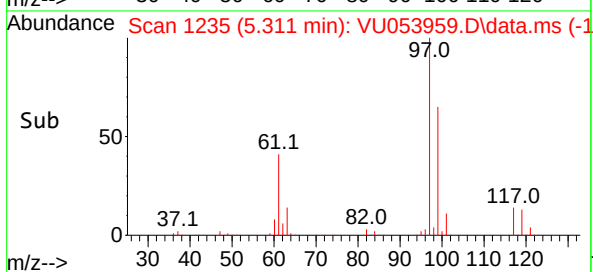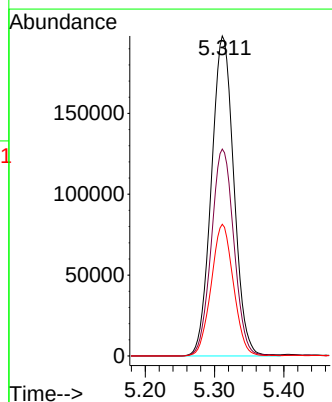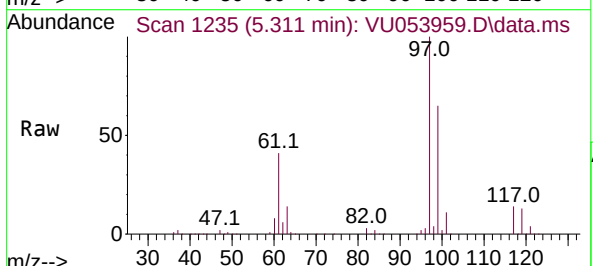







#31
Carbon tetrachloride
Concen: 0.532 ug/L
RT: 5.520 min Scan# 117
Delta R.T. 0.000 min
Lab File: VU053959.D
Acq: 28 Apr 2023 00:54

Instrument :
MSVOA_U
ClientSampleId :
HOA39

Tgt Ion:117 Resp: 693
Ion Ratio Lower Upper
117 100
119 103.1 75.0 112.6




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

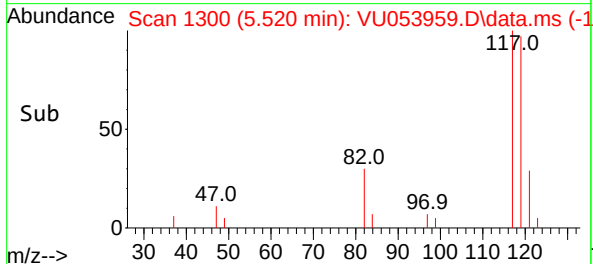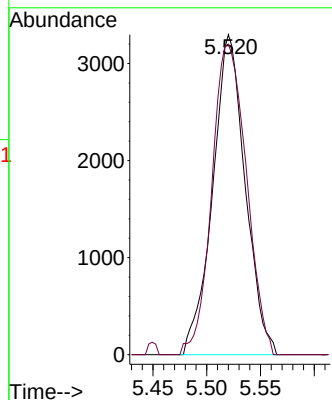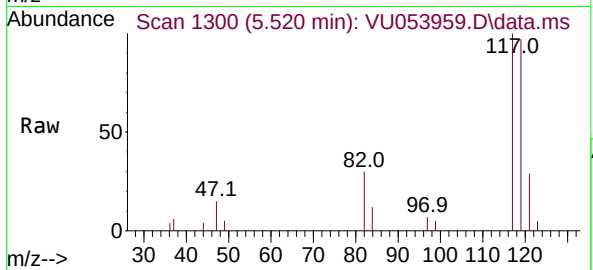

#33
Benzene
Concen: 0.369 ug/L
RT: 5.774 min Scan# 1379
Delta R.T. 0.003 min
Lab File: VU053959.D
Acq: 28 Apr 2023 00:54

Tgt Ion: 78 Resp: 13876

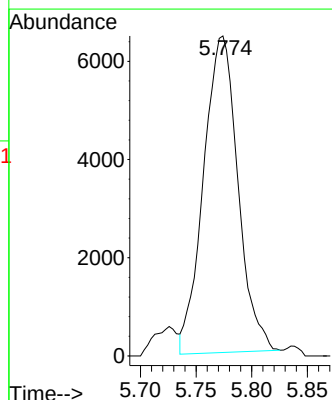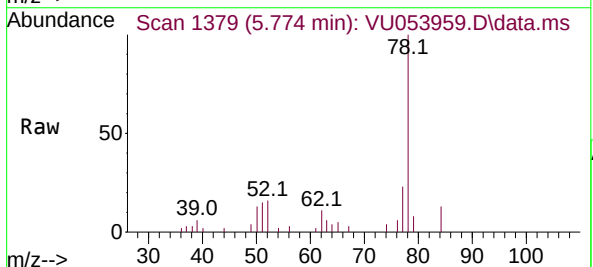



#34

Trichloroethene

Concen: 212.695 ug/L

RT: 6.536 min Scan# 1

Delta R.T. -0.003 min

Lab File: VU053959.D


Acq: 28 Apr 2023 00:54

Instrument :

MSVOA_U

ClientSampleId :

HOA39



Tgt Ion: 95 Resp: 217983

Ion Ratio Lower Upper

95 100

97 64.5 45.1 83.9

132 97.6 69.9 129.9




130 101.5 71.3 132.3

Manual Integrations

APPROVED

Reviewed By :Krupa Patel 05/01/2023

Supervised By :Mahesh Dadoda 05/01/2023

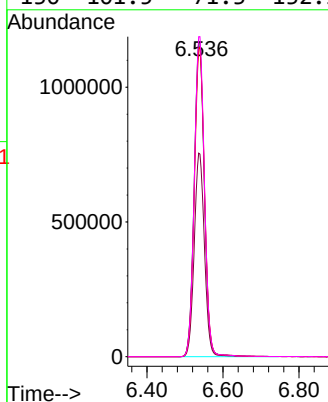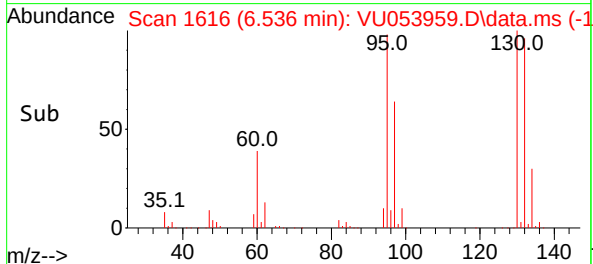

#38

Bromodichloromethane

Concen: 0.269 ug/L

RT: 7.105 min Scan# 1793

Delta R.T. 0.003 min

Lab File: VU053959.D

Acq: 28 Apr 2023 00:54




Tgt Ion: 83 Resp: 3138


Ion Ratio Lower Upper

83 100

85 51.0 45.2 84.0


127 6.1 7.3 10.9#

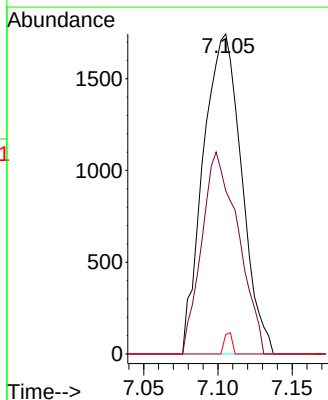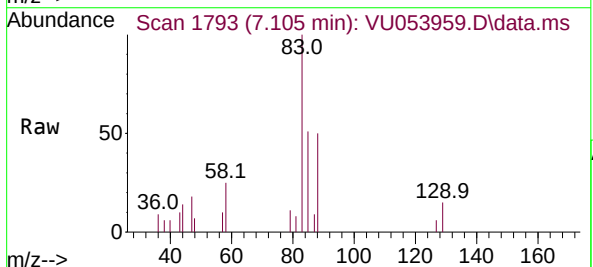

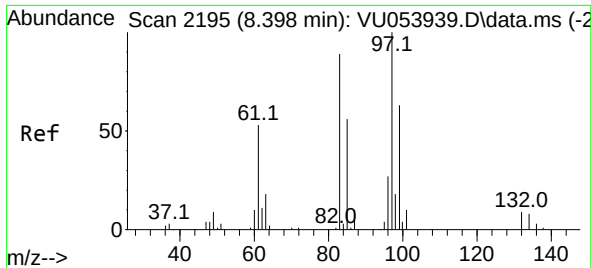

#45
1,1,2-Trichloroethane
Concen: 0.798 ug/L
RT: 8.398 min Scan# 2195
Delta R.T. 0.003 min
Lab File: VU053959.D
Acq: 28 Apr 2023 00:54




Instrument :
MSVOA_U
ClientSampleId :
HOA39

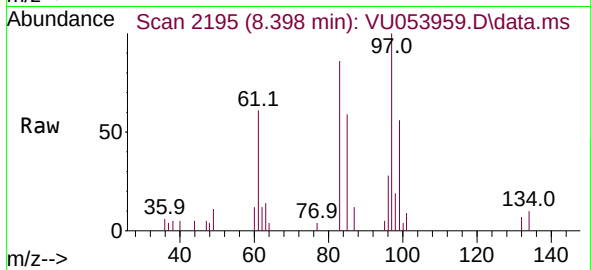

Tgt Ion	Ratio	Lower	Upper
97	100		
99	55.6	44.7	83.1
83	86.1	59.8	111.1
85	59.2	39.5	73.3




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

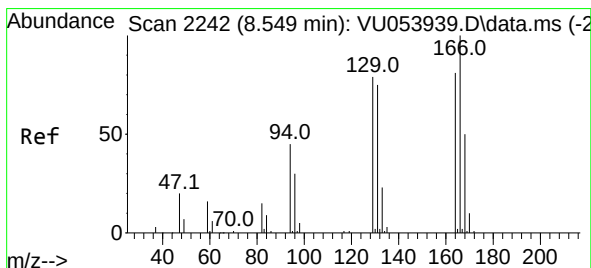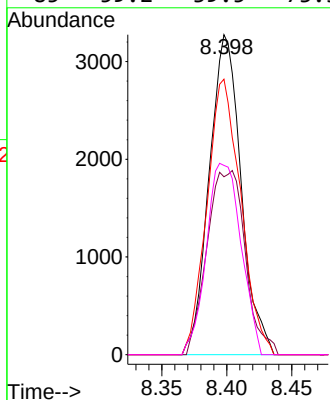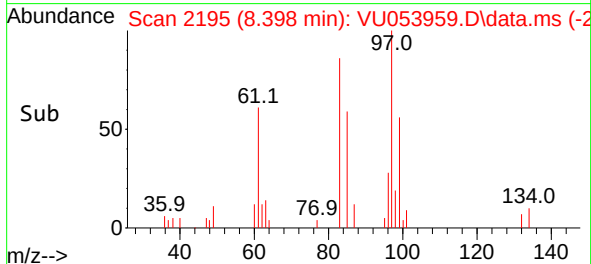

#47
Tetrachloroethene
Concen: 1571.992 ug/L
RT: 8.562 min Scan# 2246
Delta R.T. 0.013 min
Lab File: VU053959.D
Acq: 28 Apr 2023 00:54

Tgt Ion	Ratio	Lower	Upper
164	100		
129	100.5	68.3	126.8
131	97.8	64.4	119.6
166	116.2	88.3	163.9

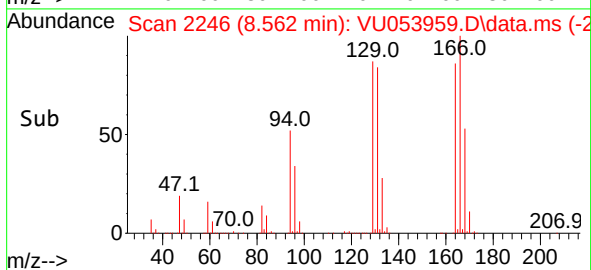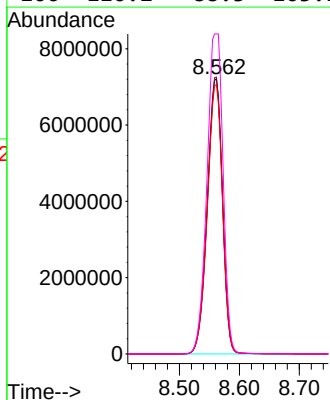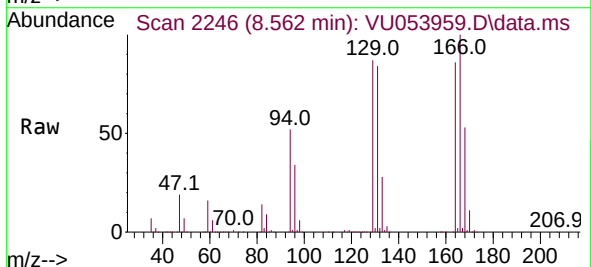

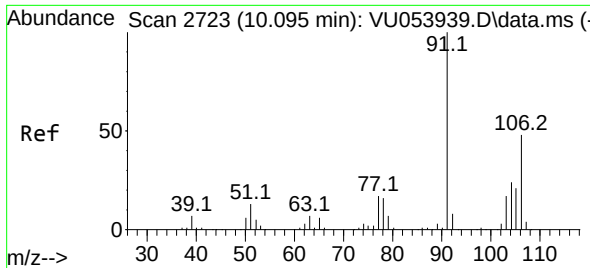





#54
o-Xylene
Concen: 0.215 ug/L
RT: 10.102 min Scan# 2106
Delta R.T. 0.007 min
Lab File: VU053959.D
Acq: 28 Apr 2023 00:54

Instrument :
MSVOA_U
ClientSampleId :
HOA39

Tgt Ion:106 Resp: 348
Ion Ratio Lower Upper
106 100
91 202.7 145.5 270.1




Manual Integrations
APPROVED


Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

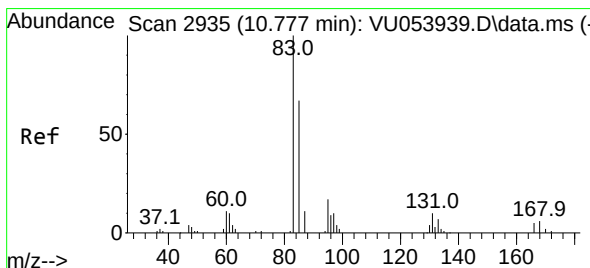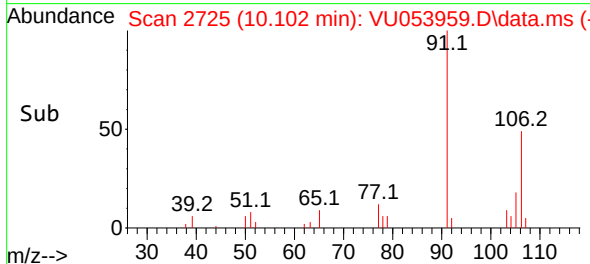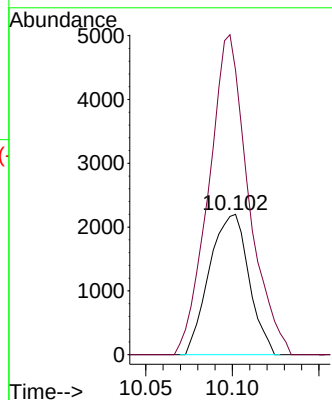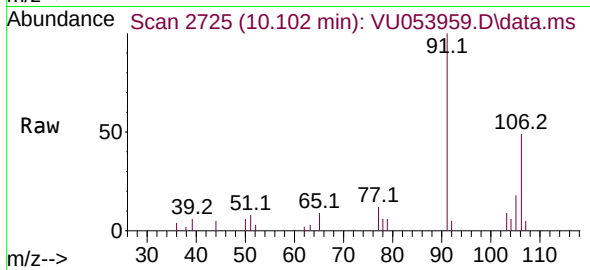

#57
1,1,2,2-Tetrachloroethane
Concen: 0.306 ug/L
RT: 10.777 min Scan# 2935
Delta R.T. 0.000 min
Lab File: VU053959.D
Acq: 28 Apr 2023 00:54


Tgt Ion: 83 Resp: 2555
Ion Ratio Lower Upper
83 100
85 75.3 43.5 80.9
131 11.1 7.8 11.6

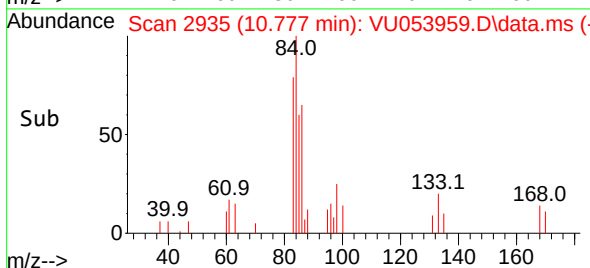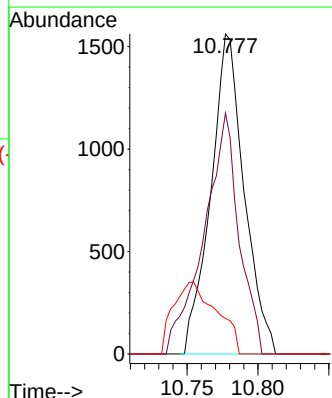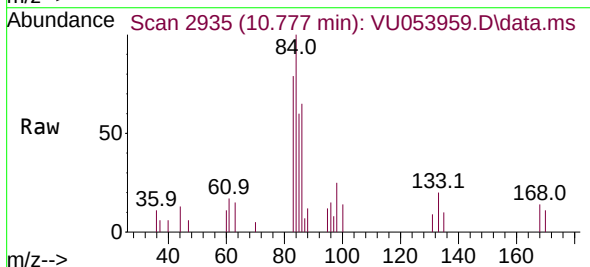

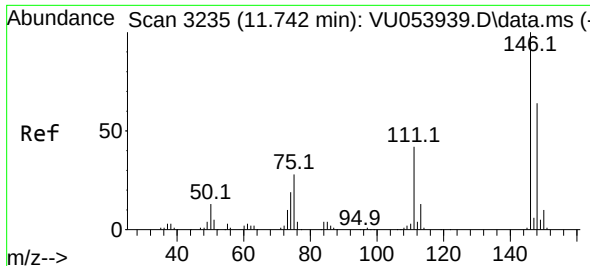

#64
1,3-Dichlorobenzene
Concen: 0.962 ug/L
RT: 11.742 min Scan# 3235
Delta R.T. 0.000 min
Lab File: VU053959.D
Acq: 28 Apr 2023 00:54




Instrument :
MSVOA_U
ClientSampleId :
HOA39

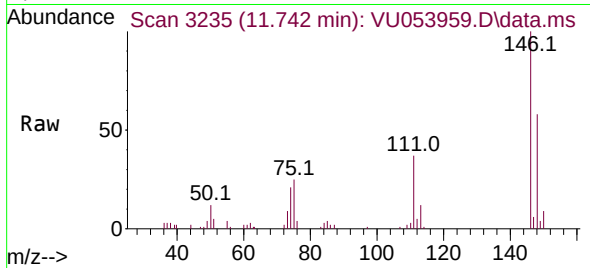


Tgt Ion:146 Resp: 18809
Ion Ratio Lower Upper
146 100
111 37.0 27.9 51.9
148 57.8 43.7 81.1

Manual Integrations
APPROVED



Reviewed By :Krupa Patel 05/01/2023
Supervised By :Mahesh Dadoda 05/01/2023

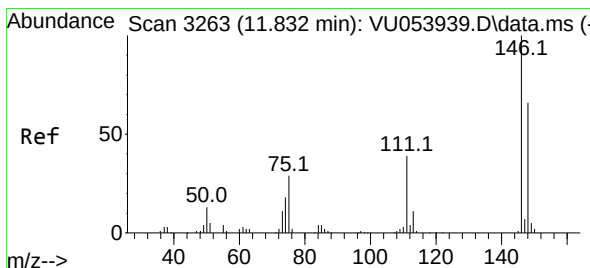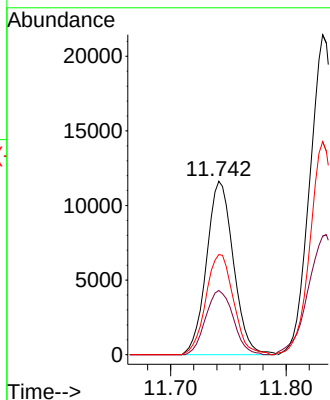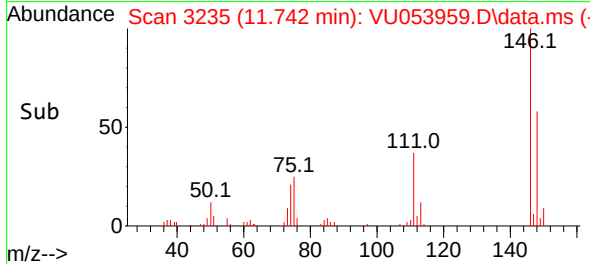


#65
1,4-Dichlorobenzene
Concen: 1.742 ug/L
RT: 11.832 min Scan# 3263
Delta R.T. 0.000 min
Lab File: VU053959.D
Acq: 28 Apr 2023 00:54

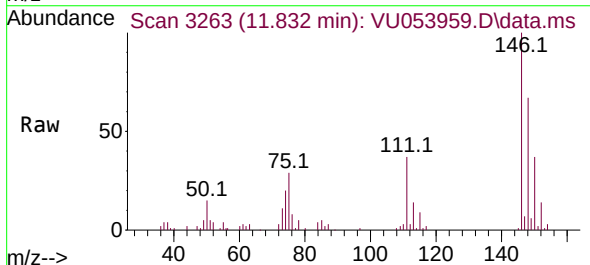

Tgt Ion:146 Resp: 34429
Ion Ratio Lower Upper
146 100
111 37.0 28.3 52.7
148 66.6 45.4 84.2

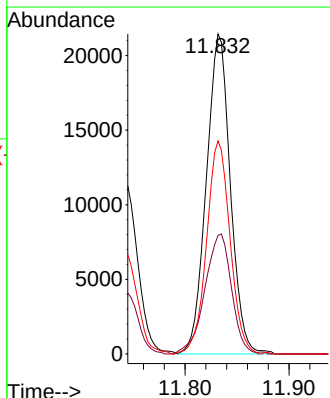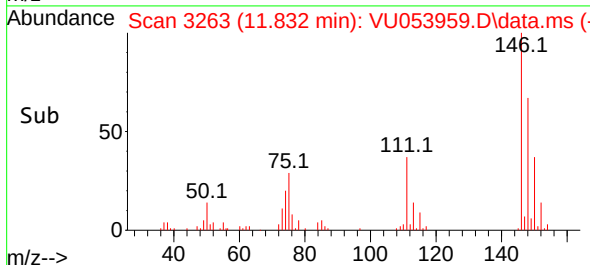

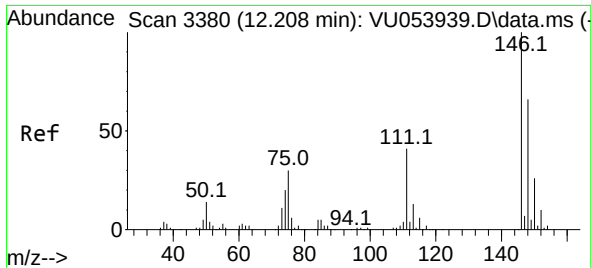

#67

1,2-Dichlorobenzene

Concen: 8.054 ug/L

RT: 12.208 min Scan# 31

Delta R.T. 0.000 min

Lab File: VU053959.D

Acq: 28 Apr 2023 00:54

Instrument :

MSVOA_U

ClientSampleId :

HOA39

Tgt Ion:146 Resp: 14544

Ion Ratio Lower Upper

146 100

111 42.3 32.6 49.0

148 65.3 51.0 76.4

Manual Integrations

APPROVED

Reviewed By :Krupa Patel 05/01/2023

Supervised By :Mahesh Dadoda 05/01/2023

