

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042823\
 Data File : VU053940.D
 Acq On : 27 Apr 2023 17:09
 Operator : JC/MD
 Sample : VU0428WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK191

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU053940.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	92	rVB	40104	45103	12.32%	1.405%
2	1.916	170	179	195	rBV	37047	52906	14.45%	1.648%
3	2.565	370	381	399	rVB	75828	124709	34.05%	3.886%
4	3.044	519	530	543	rBV2	8449	14959	4.08%	0.466%
5	4.633	1012	1024	1049	rBV2	46911	130944	35.76%	4.080%
6	5.060	1141	1157	1174	rBV2	77404	169968	46.41%	5.296%
7	5.723	1342	1363	1389	rBV2	142274	366200	100.00%	11.410%
8	6.243	1506	1525	1550	rBV	153334	294659	80.46%	9.181%
9	6.684	1647	1662	1681	rBV	89222	175017	47.79%	5.453%
10	7.562	1922	1935	1951	rBV2	42474	76870	20.99%	2.395%
11	7.893	2021	2038	2055	rBV	171980	303061	82.76%	9.443%
12	8.176	2116	2126	2144	rBV2	25404	42978	11.74%	1.339%
13	8.629	2256	2267	2298	rBV	180524	336965	92.02%	10.499%
14	9.414	2498	2511	2534	rBV	206788	349775	95.51%	10.899%
15	10.751	2915	2927	2944	rBV	69633	113805	31.08%	3.546%
16	11.806	3244	3255	3276	rVV	204078	330578	90.27%	10.300%
17	12.189	3358	3374	3395	rBV	159534	263680	72.00%	8.216%
18	13.841	3875	3888	3900	rBV6	4063	6743	1.84%	0.210%
19	14.095	3957	3967	3976	rBV4	2426	3909	1.07%	0.122%
20	14.330	4031	4040	4049	rBV4	4228	6547	1.79%	0.204%




Sum of corrected areas: 3209376

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042823\
Data File : VU053940.D
Acq On : 27 Apr 2023 17:09
Operator : JC/MD
Sample : VU0428WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK191

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

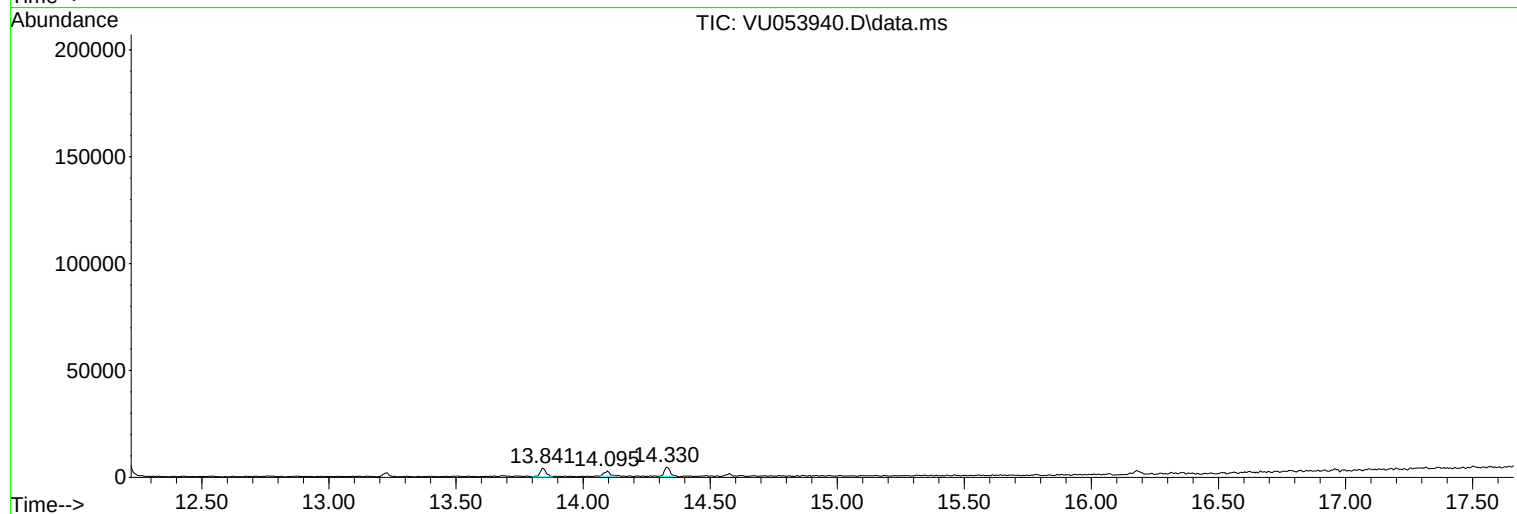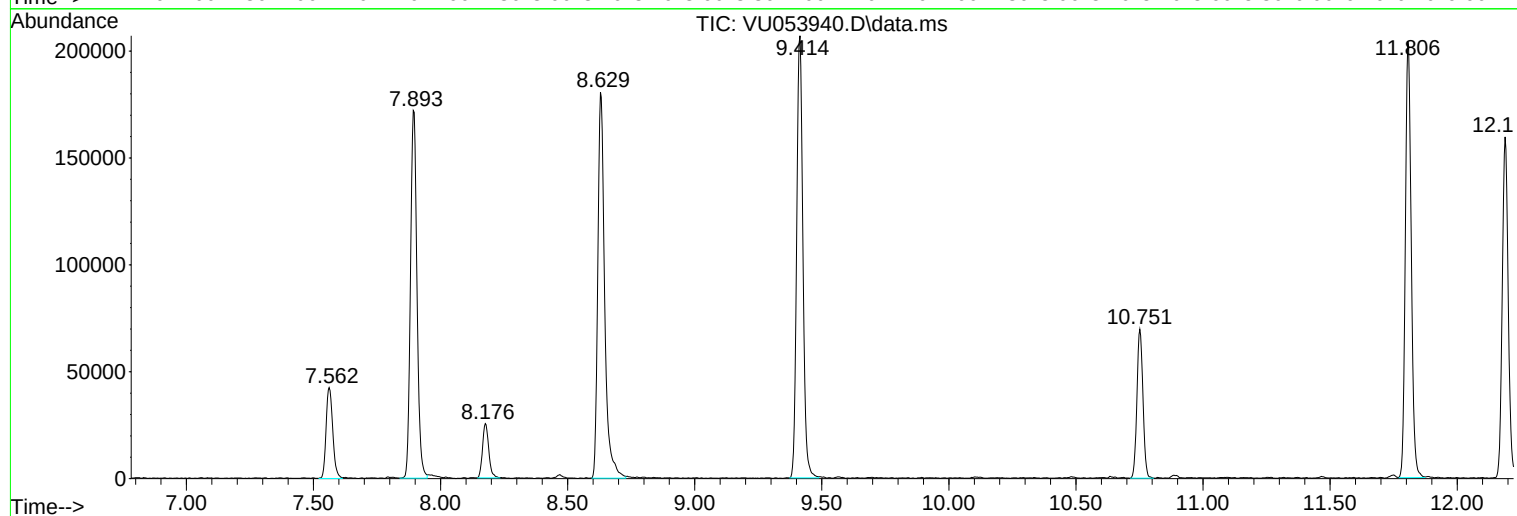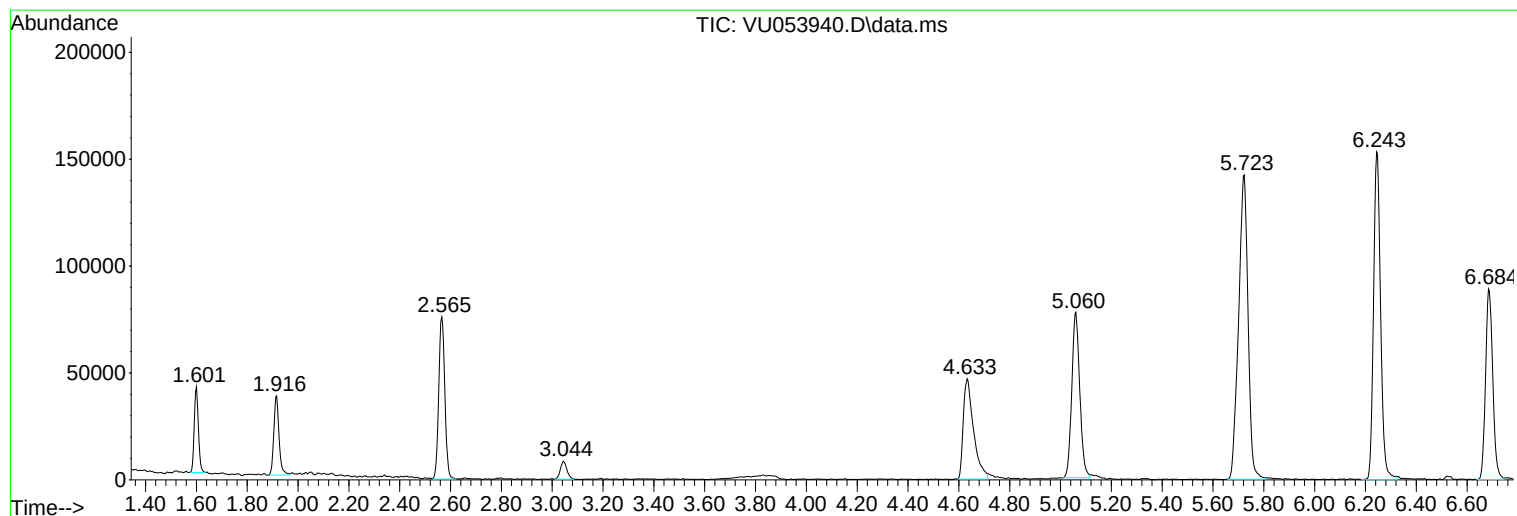

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042823\
Data File : VU053940.D
Acq On : 27 Apr 2023 17:09
Operator : JC/MD
Sample : VU0428WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK191










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.562	1.30 ug/L	76870	1,4-Difluorobenzene	6.247

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1,3-Cyclohexadiene	80	C6H8	000592-57-4	38
2			Methane, oxybis[chloro-	114	C2H4Cl2O	000542-88-1	28
3			2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	28
4			2-Propanol, 1,3-dichloro-	128	C3H6Cl2O	000096-23-1	28
5			Methanesulfonyl chloride	114	CH3ClO2S	000124-63-0	9

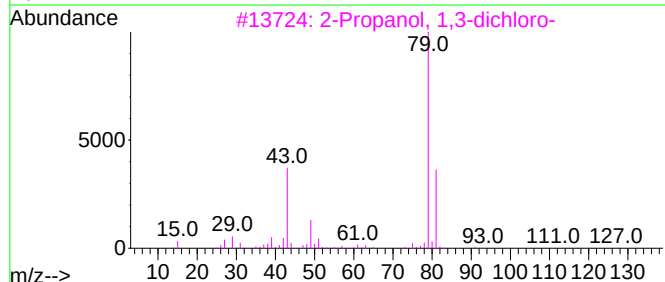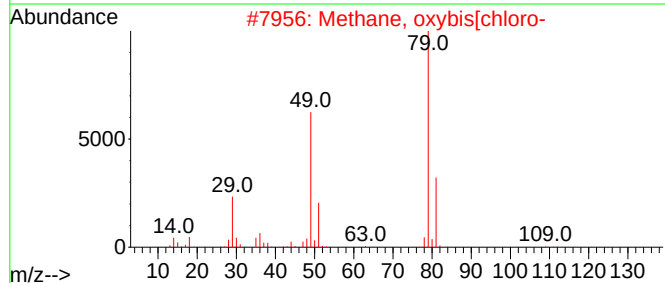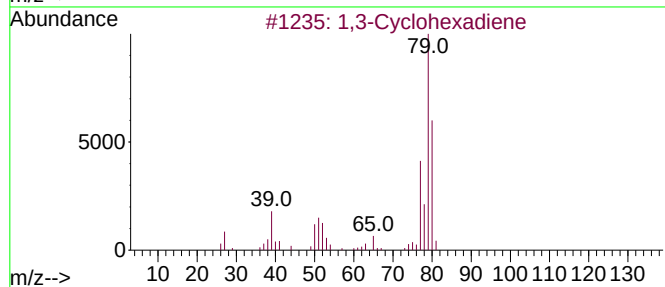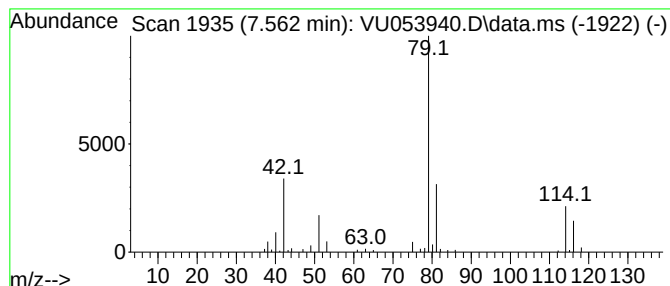

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042823\
Data File : VU053940.D
Acq On : 27 Apr 2023 17:09
Operator : JC/MD
Sample : VU0428WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK191

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	7.562	1.3	ug/L	76870	1	6.247	294659	5.0