

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042823\
 Data File : VU053945.D
 Acq On : 27 Apr 2023 19:15
 Operator : JC/MD
 Sample : 02488-16
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE71

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU053945.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	93	rBV	39008	46095	12.64%	1.381%
2	1.916	170	179	189	rBV	36070	48522	13.30%	1.454%
3	2.565	368	381	397	rBV	73580	120032	32.91%	3.597%
4	3.044	522	530	539	rVB3	2350	4070	1.12%	0.122%
5	3.179	559	572	586	rBV2	3815	7700	2.11%	0.231%
6	4.636	1011	1025	1064	rBV	44712	141703	38.85%	4.246%
7	5.057	1138	1156	1186	rBV	78123	177955	48.79%	5.332%
8	5.723	1342	1363	1384	rBV2	138280	355863	97.57%	10.663%
9	6.247	1512	1526	1547	rBV	156896	306204	83.95%	9.175%
10	6.687	1649	1663	1688	rBV	84797	170537	46.76%	5.110%
11	7.562	1923	1935	1954	rBV	43869	75454	20.69%	2.261%
12	7.896	2025	2039	2055	rBV	166264	296578	81.32%	8.887%
13	7.967	2055	2061	2071	rVB3	4518	7351	2.02%	0.220%
14	8.176	2115	2126	2140	rBV2	24535	42696	11.71%	1.279%
15	8.468	2205	2217	2228	rBV2	14181	24780	6.79%	0.743%
16	8.632	2256	2268	2298	rBV	171741	333021	91.31%	9.979%
17	9.414	2499	2511	2532	rBV	215528	364726	100.00%	10.929%
18	10.083	2709	2719	2729	rBV4	3263	6142	1.68%	0.184%
19	10.751	2916	2927	2942	rBV2	69580	110647	30.34%	3.315%
20	10.890	2956	2970	2984	rVB4	17480	29426	8.07%	0.882%
21	11.806	3243	3255	3274	rBV	224796	360570	98.86%	10.804%
22	12.189	3361	3374	3388	rBV	164207	266804	73.15%	7.995%
23	12.767	3544	3554	3562	rBV4	2684	4138	1.13%	0.124%
24	12.883	3582	3590	3603	rBV3	12432	18293	5.02%	0.548%
25	13.208	3684	3691	3704	rVB7	2154	3741	1.03%	0.112%
26	14.574	4105	4116	4123	rVB3	2333	3947	1.08%	0.118%
27	16.182	4600	4616	4628	rBV3	5645	10296	2.82%	0.309%




Sum of corrected areas: 3337291

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042823\
Data File : VU053945.D
Acq On : 27 Apr 2023 19:15
Operator : JC/MD
Sample : 02488-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

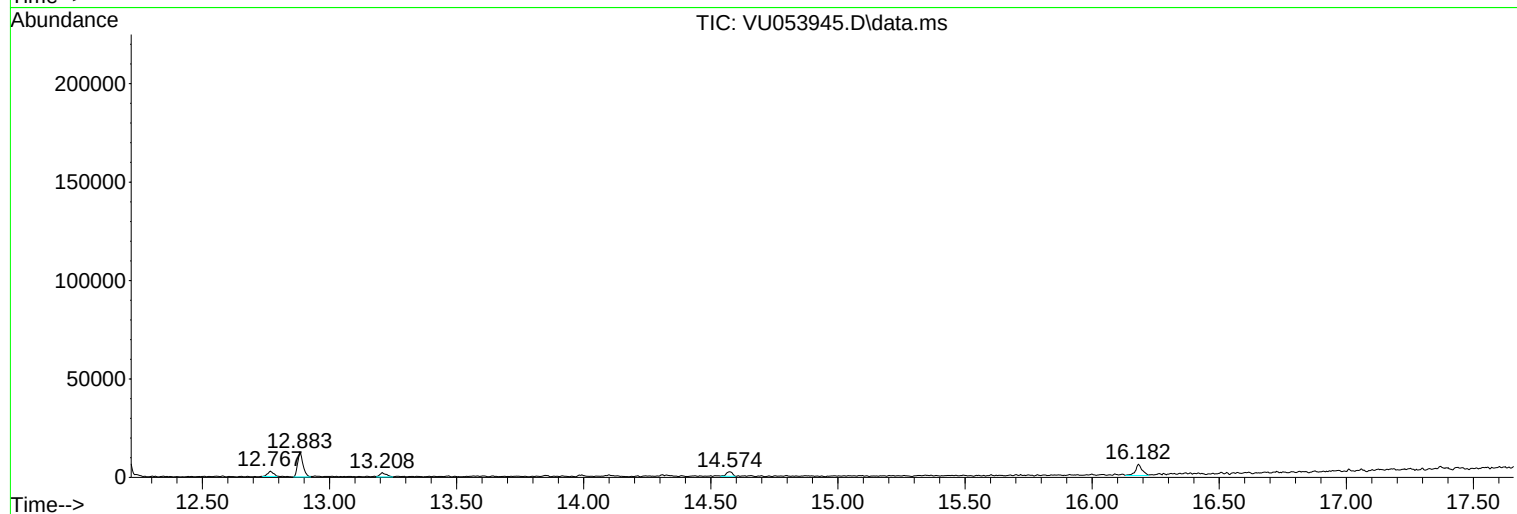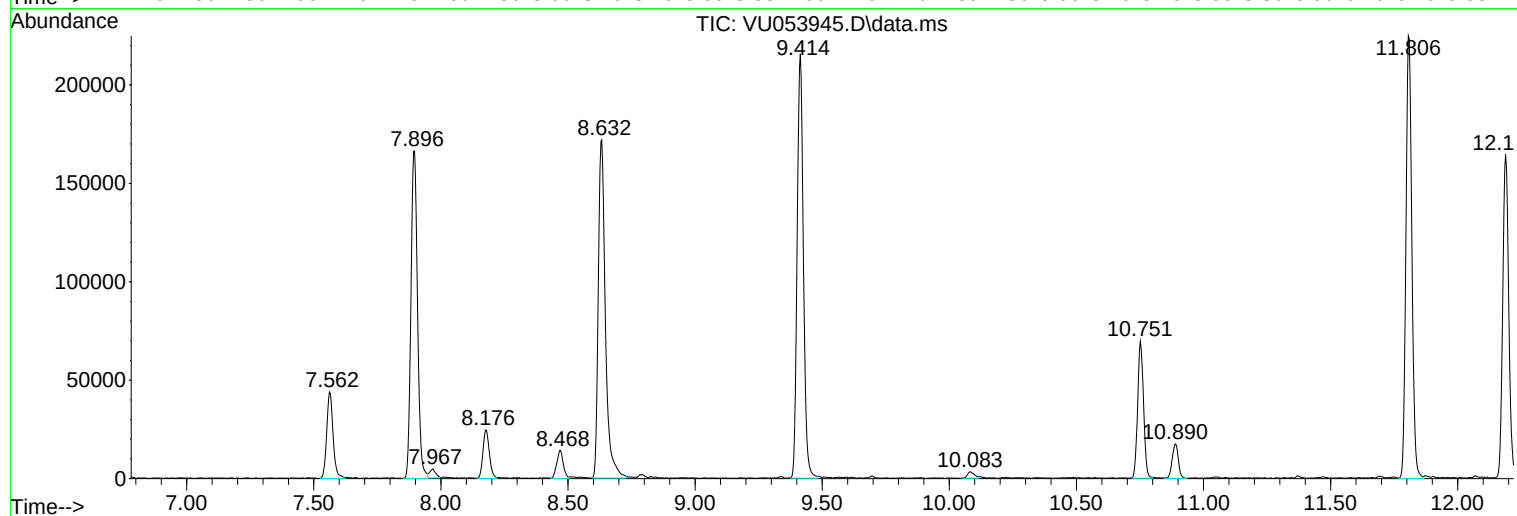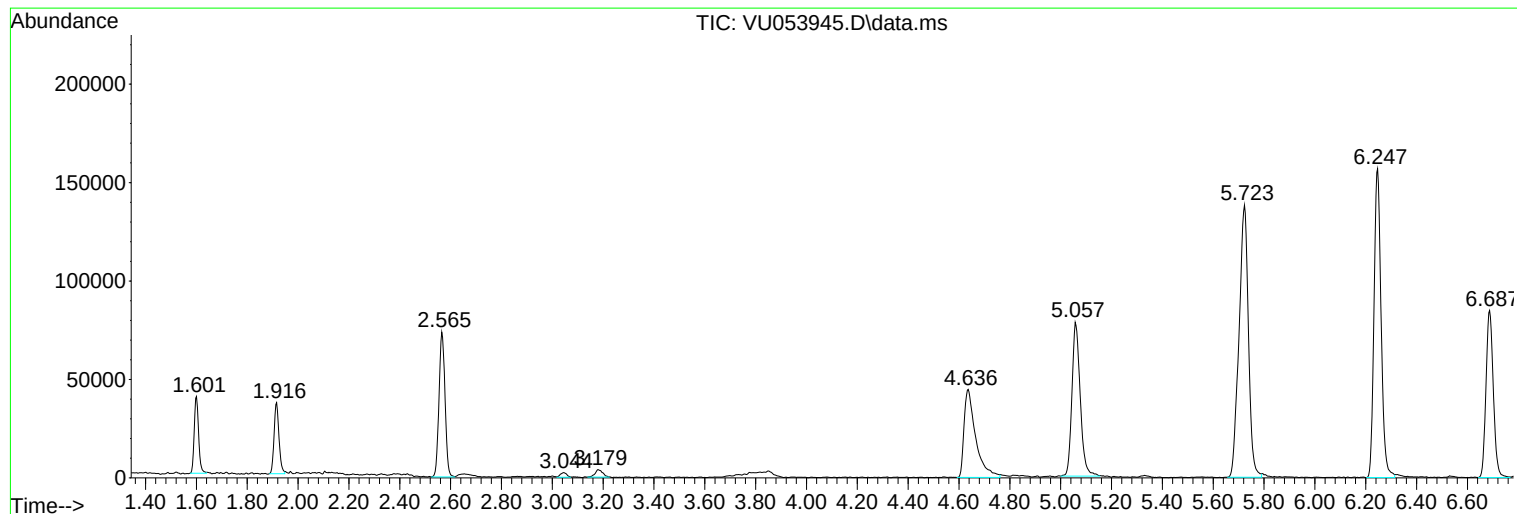

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042823\
Data File : VU053945.D
Acq On : 27 Apr 2023 19:15
Operator : JC/MD
Sample : 02488-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042823\
Data File : VU053945.D
Acq On : 27 Apr 2023 19:15
Operator : JC/MD
Sample : 02488-16
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE71

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------