

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042823\
 Data File : VU053951.D
 Acq On : 27 Apr 2023 21:41
 Operator : JC/MD
 Sample : 02488-19 50X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BHE74

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU053951.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.597	72	80	93	rBV	51420	61611	13.26%	1.584%
2	1.912	170	178	195	rVB	46077	63832	13.74%	1.641%
3	2.565	368	381	399	rVB	99239	163994	35.30%	4.217%
4	3.041	519	529	541	rBV2	7314	13387	2.88%	0.344%
5	4.636	1013	1025	1059	rBV	53848	174389	37.53%	4.485%
6	5.060	1142	1157	1182	rVB	99609	221626	47.70%	5.699%
7	5.723	1343	1363	1389	rBV2	179666	464625	100.00%	11.948%
8	6.247	1513	1526	1544	rBV2	150809	287777	61.94%	7.400%
9	6.542	1602	1618	1631	rBV2	14473	27924	6.01%	0.718%
10	6.687	1647	1663	1683	rBV	115471	224668	48.35%	5.777%
11	7.562	1924	1935	1955	rBV2	53443	97152	20.91%	2.498%
12	7.893	2026	2038	2056	rBV	224354	390140	83.97%	10.033%
13	8.176	2116	2126	2145	rBV2	32212	54668	11.77%	1.406%
14	8.468	2207	2217	2230	rBV4	5151	8874	1.91%	0.228%
15	8.552	2230	2243	2251	rBV3	6971	10924	2.35%	0.281%
16	8.632	2255	2268	2299	rBV	230315	440806	94.87%	11.336%
17	9.414	2499	2511	2533	rBV	207340	350275	75.39%	9.008%
18	10.751	2916	2927	2944	rBV	90386	146921	31.62%	3.778%
19	10.890	2961	2970	2984	rBV2	6421	10177	2.19%	0.262%
20	11.809	3244	3256	3270	rBV	205132	332964	71.66%	8.562%
21	12.189	3362	3374	3390	rBV	209898	341949	73.60%	8.793%




Sum of corrected areas: 3888683

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042823\
Data File : VU053951.D
Acq On : 27 Apr 2023 21:41
Operator : JC/MD
Sample : 02488-19 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE74

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

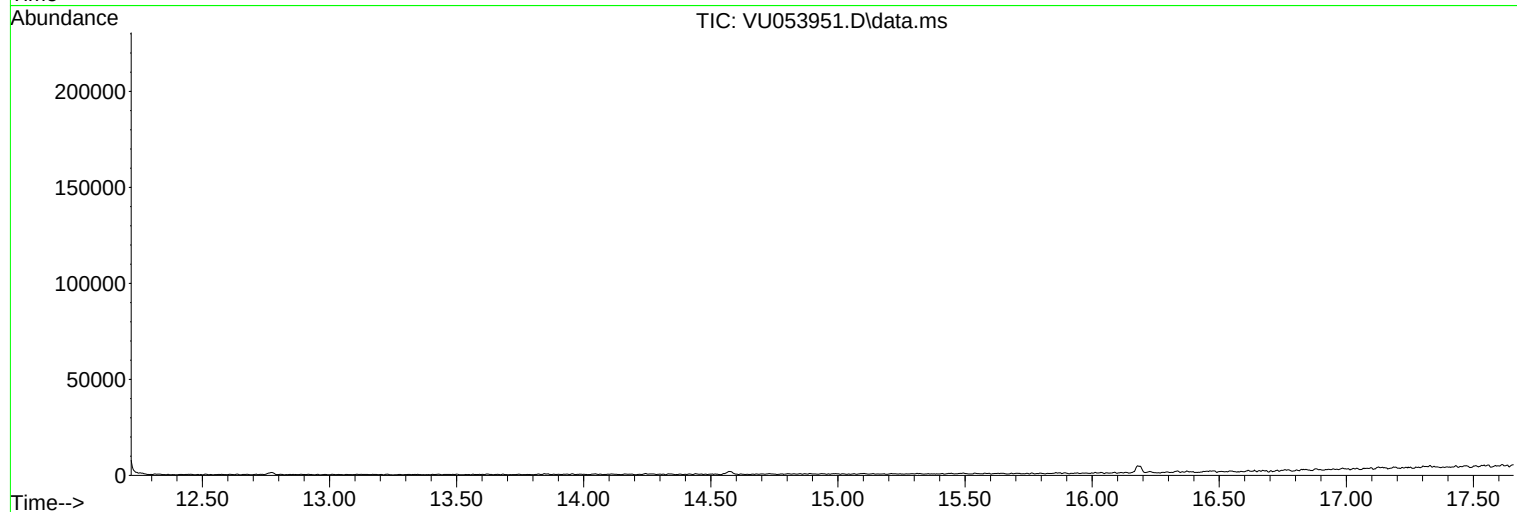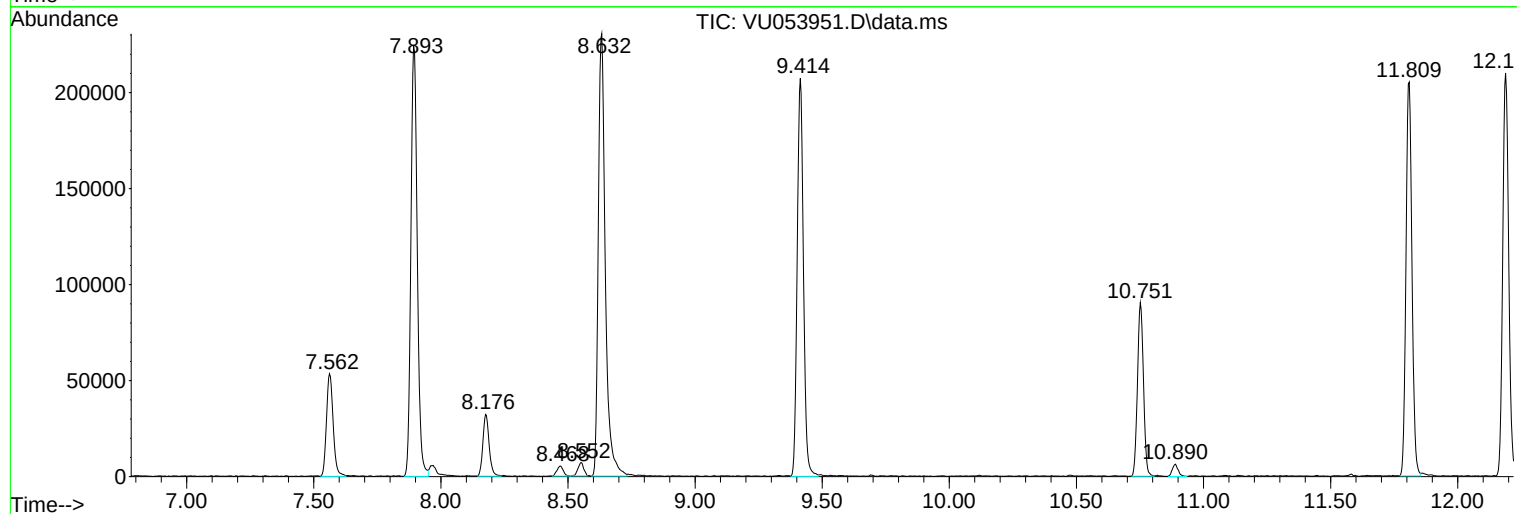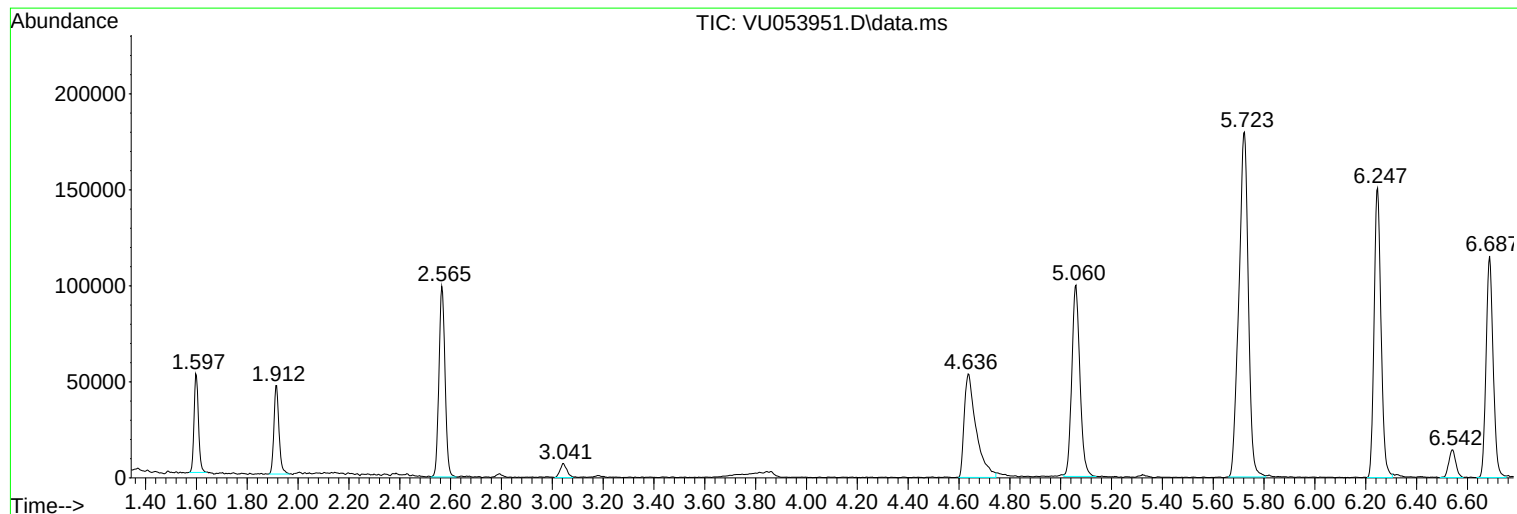

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042823\
Data File : VU053951.D
Acq On : 27 Apr 2023 21:41
Operator : JC/MD
Sample : 02488-19 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE74

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042823\
Data File : VU053951.D
Acq On : 27 Apr 2023 21:41
Operator : JC/MD
Sample : 02488-19 50X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BHE74

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------