


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042823\
Data File : VU053938.D
Acq On : 27 Apr 2023 15:17
Operator : JC/MD
Sample : BFB010
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB010

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR042423WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Apr 27 05:52:18 2023

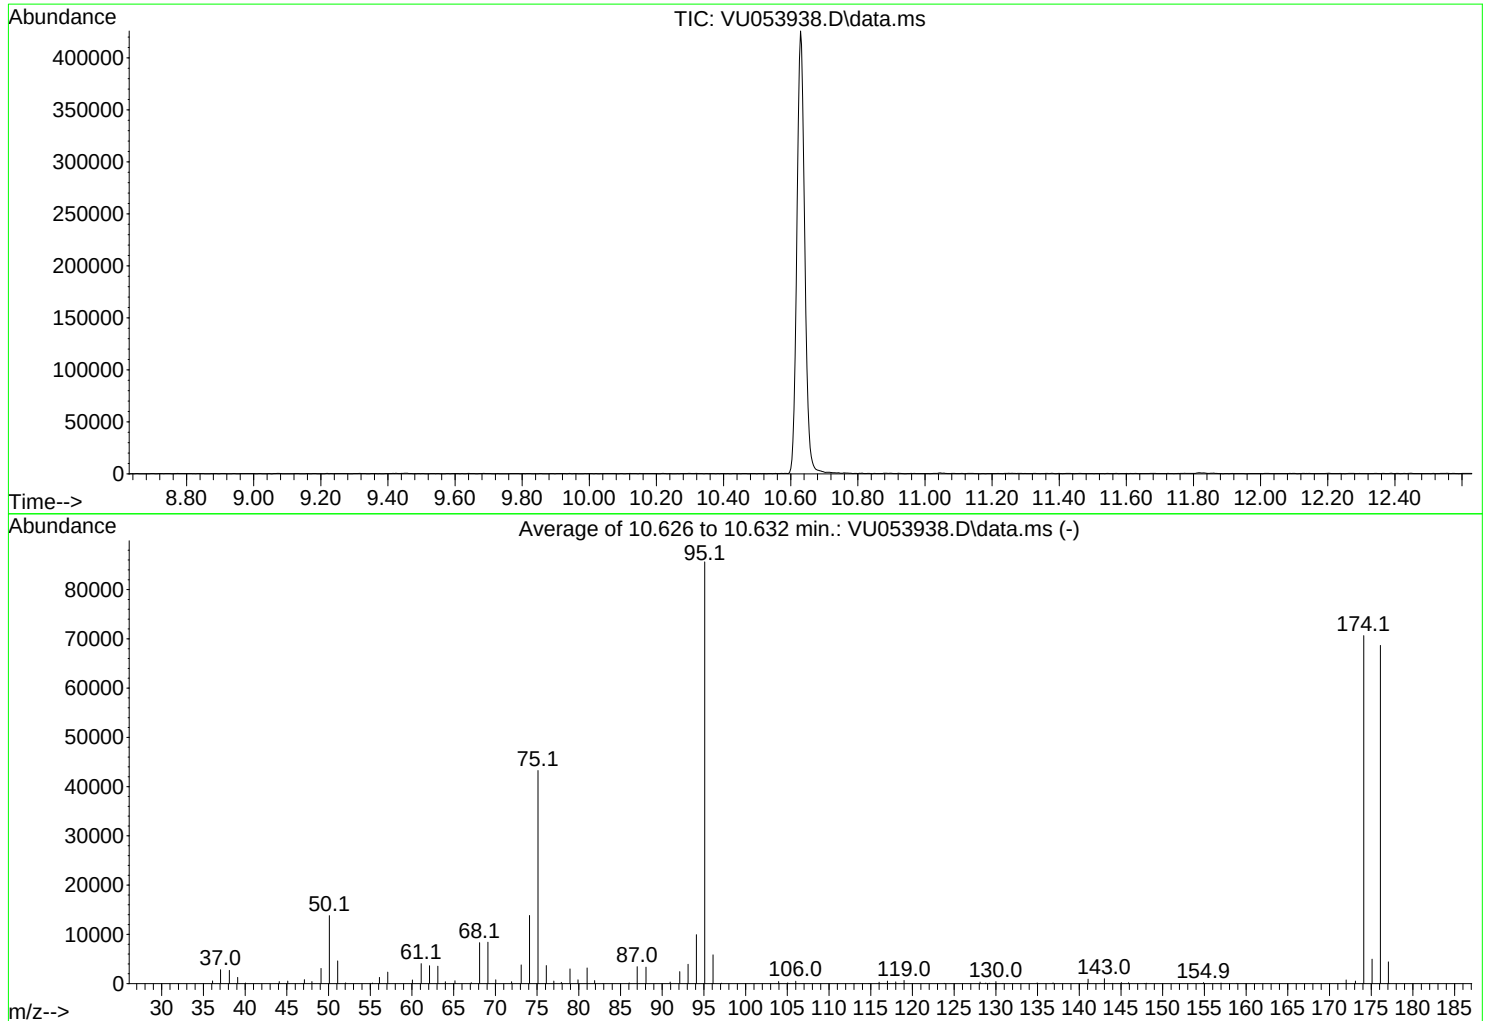

AutoFind: Scans 2888, 2889, 2890; Background Corrected with Scan 2875

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.1	13807	PASS
75	95	30	80	50.5	43272	PASS
95	95	100	100	100.0	85632	PASS
96	95	5	9	6.9	5866	PASS
173	174	0.00	2	0.7	518	PASS
174	95	50	120	82.5	70656	PASS
175	174	5	9	7.0	4963	PASS
176	174	95	101	97.2	68664	PASS
177	176	5	9	6.4	4405	PASS

m/z	Abundance
39.80	142.0
44.10	298.0

Instrument :
MSVOA_U
ClientSampleId :
BFB010

m/z	Abundance
36.10	602.0
37.10	2792.0
38.10	2641.0
39.10	1351.0
40.00	105.0
44.10	734.0
45.10	555.0
47.10	833.0
48.00	477.0
49.10	2944.0
50.10	13626.0
51.10	4774.0
52.10	201.0
55.00	164.0
56.10	1296.0
57.10	2122.0
60.10	758.0
61.10	4122.0
62.10	3694.0
63.10	3510.0
64.00	344.0
65.20	458.0
67.10	201.0
68.10	8385.0
69.10	8437.0
70.10	714.0
72.00	360.0
73.10	3568.0
74.10	13446.0
75.10	41864.0
76.10	3647.0
77.00	507.0
77.90	255.0
78.90	2905.0
79.90	723.0
81.00	3129.0
81.90	616.0
82.90	113.0
86.10	128.0
87.00	3520.0
88.10	3318.0
91.00	284.0
92.10	2295.0
93.10	3948.0
94.10	9649.0
95.10	83288.0
96.10	5869.0
103.90	380.0
105.00	169.0
106.00	502.0
116.00	324.0
117.00	552.0
118.00	363.0
119.00	676.0
128.10	340.0
128.80	123.0
129.20	125.0
130.00	413.0
130.80	135.0
134.90	178.0
136.90	130.0
141.10	771.0
143.00	908.0
145.10	208.0
145.90	151.0
147.80	124.0
154.90	245.0
157.10	127.0
172.00	709.0
173.10	497.0
174.10	66360.0
175.10	4585.0
176.10	65016.0
177.10	4579.0

Instrument :
MSVOA_U
ClientSampleId :
BFB010

m/z	Abundance
36.10	585.0
37.00	2955.0
38.10	2817.0
39.10	1330.0
40.00	133.0
44.10	761.0
45.10	519.0
47.10	828.0
48.00	424.0
49.10	3229.0
50.10	14354.0
51.10	4733.0
52.00	163.0
55.20	197.0
56.10	1369.0
57.10	2463.0
60.10	771.0
61.10	4190.0
62.10	3704.0
63.10	3731.0
64.00	415.0
65.20	595.0
67.10	190.0
68.10	8544.0
69.10	8658.0
70.00	815.0
71.90	415.0
73.10	3892.0
74.10	14360.0
75.10	44848.0
76.10	3774.0
77.00	555.0
77.90	259.0
79.00	3077.0
79.90	807.0
81.00	3344.0
81.90	628.0
86.10	173.0
87.00	3573.0
88.00	3506.0
90.90	334.0
92.10	2506.0
93.10	4138.0
94.10	10253.0
95.10	88616.0
96.10	6060.0
97.10	130.0
104.00	433.0
105.00	154.0
106.00	541.0
116.00	293.0
117.00	528.0
118.00	363.0
119.00	680.0
123.80	110.0
128.10	344.0
128.80	136.0
129.20	130.0
130.00	441.0
130.90	112.0
134.90	180.0
136.80	180.0
141.00	949.0
143.00	1055.0
143.90	108.0
145.10	227.0
145.90	220.0
148.00	115.0
154.90	247.0
157.00	124.0
158.90	124.0
172.00	797.0
173.10	546.0
174.10	72744.0
175.10	5142.0
176.10	70560.0
177.10	4505.0

Instrument :
MSVOA_U
ClientSampleId :
BFB010

m/z	Abundance
36.10	483.0
37.00	2689.0
38.10	2666.0
39.10	1160.0
40.10	133.0
44.10	685.0
45.10	501.0
47.10	763.0
48.00	360.0
49.10	3117.0
50.10	13442.0
51.10	4348.0
52.00	160.0
55.30	194.0
56.10	1181.0
57.10	2455.0
60.00	741.0
61.10	3836.0
62.10	3493.0
63.10	3407.0
64.00	393.0
65.10	664.0
67.10	220.0
68.10	7985.0
69.10	8121.0
70.10	776.0
71.90	399.0
73.10	3965.0
74.10	13733.0
75.10	43104.0
76.10	3569.0
77.00	482.0
77.90	266.0
79.00	2969.0
79.90	793.0
81.00	3133.0
81.90	582.0
86.00	171.0
87.00	3257.0
88.00	3250.0
90.90	361.0
92.10	2494.0
93.10	3672.0
94.10	9923.0
95.10	84992.0
96.10	5669.0
97.10	139.0
104.00	463.0
105.10	141.0
106.00	459.0
106.90	129.0
111.00	111.0
113.00	113.0
114.80	140.0
116.00	282.0
117.00	469.0
118.00	364.0
119.00	574.0
123.80	116.0
128.10	290.0
128.80	131.0
130.00	395.0
135.00	157.0
136.80	204.0
141.00	1010.0
143.00	1050.0
144.00	110.0
145.00	215.0
145.90	200.0
148.10	164.0
154.90	197.0
156.90	124.0
158.90	124.0
172.00	793.0
173.10	511.0
174.10	72864.0
175.10	5161.0
176.10	70416.0
177.00	4130.0

Instrument :
MSVOA_U
ClientSampleId :
BFB010