
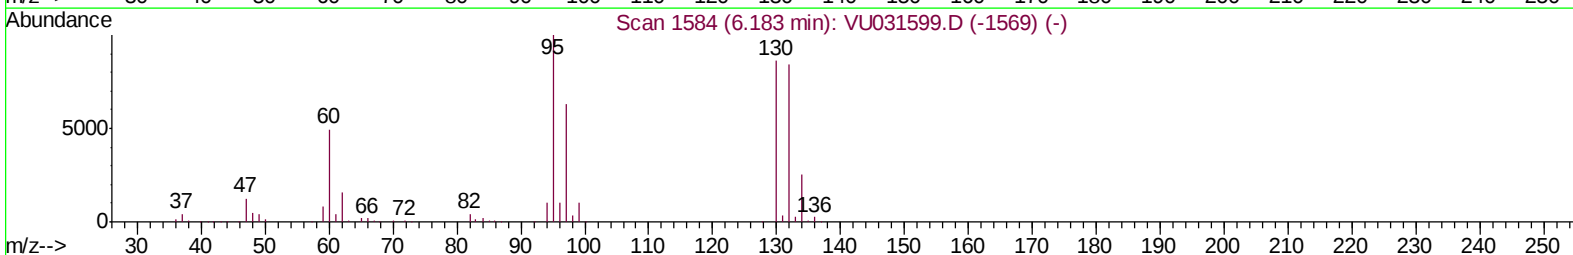
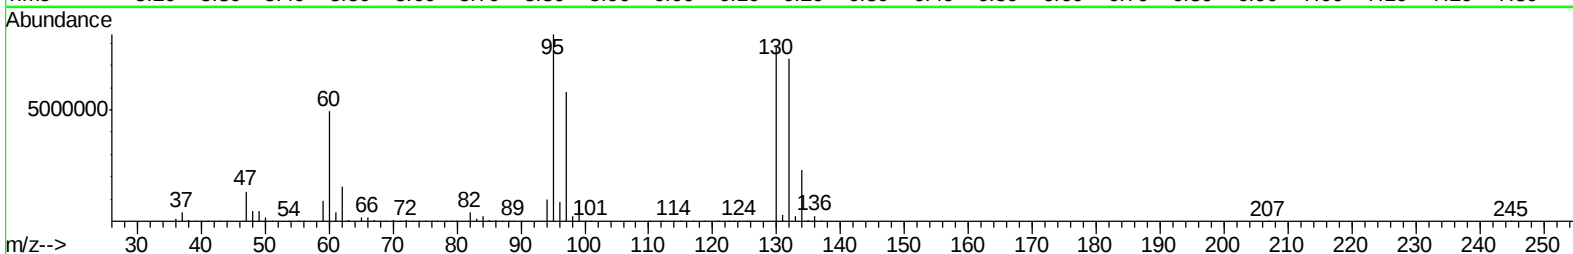


Data File : VU031622.D
Acq On : 30 Apr 2019 05:51
Operator : JC/SP
Sample : K2593-11 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 55 Sample Multiplier: 1

Quant Time: Apr 30 08:03:10 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 30 04:50:11 2019
Response via : Initial Calibration

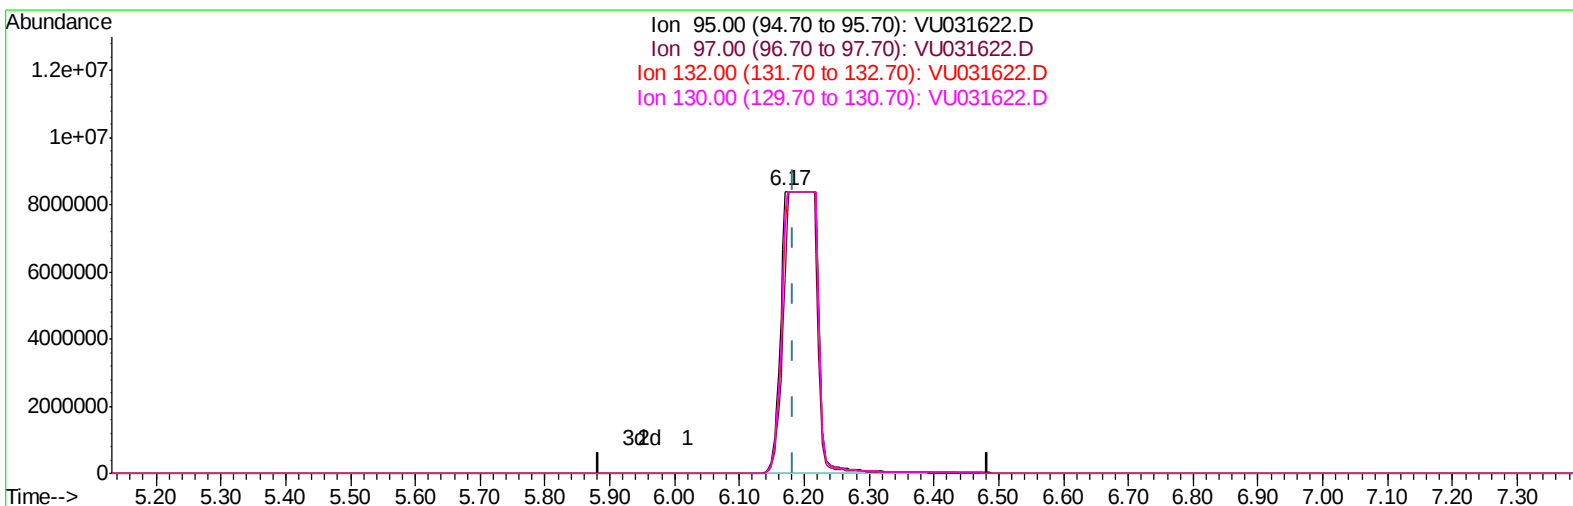

TIC: VU031622.D

(34) Trichloroethene (T)

6.170min (-0.013) 5544.42ug/L m

response 32260797

Ion	Exp%	Act%
95.00	100	100
97.00	64.00	69.24
132.00	90.10	86.85
130.00	95.00	93.40