

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031597.D
 Acq On : 29 Apr 2019 19:24
 Operator : JC/SP
 Sample : K2536-21
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X09

Quant Time: Apr 30 04:35:52 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Apr 30 01:54:25 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.88	114	650503	50.00	ug/L	0.00
28) Chlorobenzene-d5	9.09	117	638275	50.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.48	152	242398	50.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.40	65	291876	53.61	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	107.22%
7) Chloroethane-d5	1.68	69	239364	56.89	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	113.78%
11) 1,1-Dichloroethene-d2	2.27	63	447936	41.32	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.64%
21) 2-Butanone-d5	4.19	46	606957	123.05	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	123.05%
24) Chloroform-d	4.64	84	538412	54.00	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	108.00%
26) 1,2-Dichloroethane-d4	5.31	65	373376	57.32	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	114.64%
32) Benzene-d6	5.34	84	1049912	53.57	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	107.14%
36) 1,2-Dichloropropane-d6	6.33	67	378215	54.85	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	109.70%
41) Toluene-d8	7.56	98	854804	50.07	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	100.14%
43) trans-1,3-Dichloropropene-	7.85	79	145935	49.30	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	98.60%
47) 2-Hexanone-d5	8.31	63	332686	111.47	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	111.47%
57) 1,1,2,2-Tetrachloroethane-	10.43	84	476678	51.51	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	103.02%
64) 1,2-Dichlorobenzene-d4	11.85	152	275916	54.13	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	108.26%

Target Compounds


					Ovalue
9) Trichlorofluoromethane	1.88	101	101080	10.958	ug/L 96
13) Acetone	2.34	43	59295	10.672	ug/L 99
20) cis-1,2-Dichloroethene	4.22	96	28137	4.960	ug/L 98
34) Trichloroethene	6.18	95	2057295	361.663	ug/L 95
46) Tetrachloroethene	8.22	164	95160	24.538	ug/L 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042919\
Data File : VU031597.D
Acq On : 29 Apr 2019 19:24
Operator : JC/SP
Sample : K2536-21
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X09

Quant Time: Apr 30 04:35:52 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Apr 30 01:54:25 2019
Response via : Initial Calibration

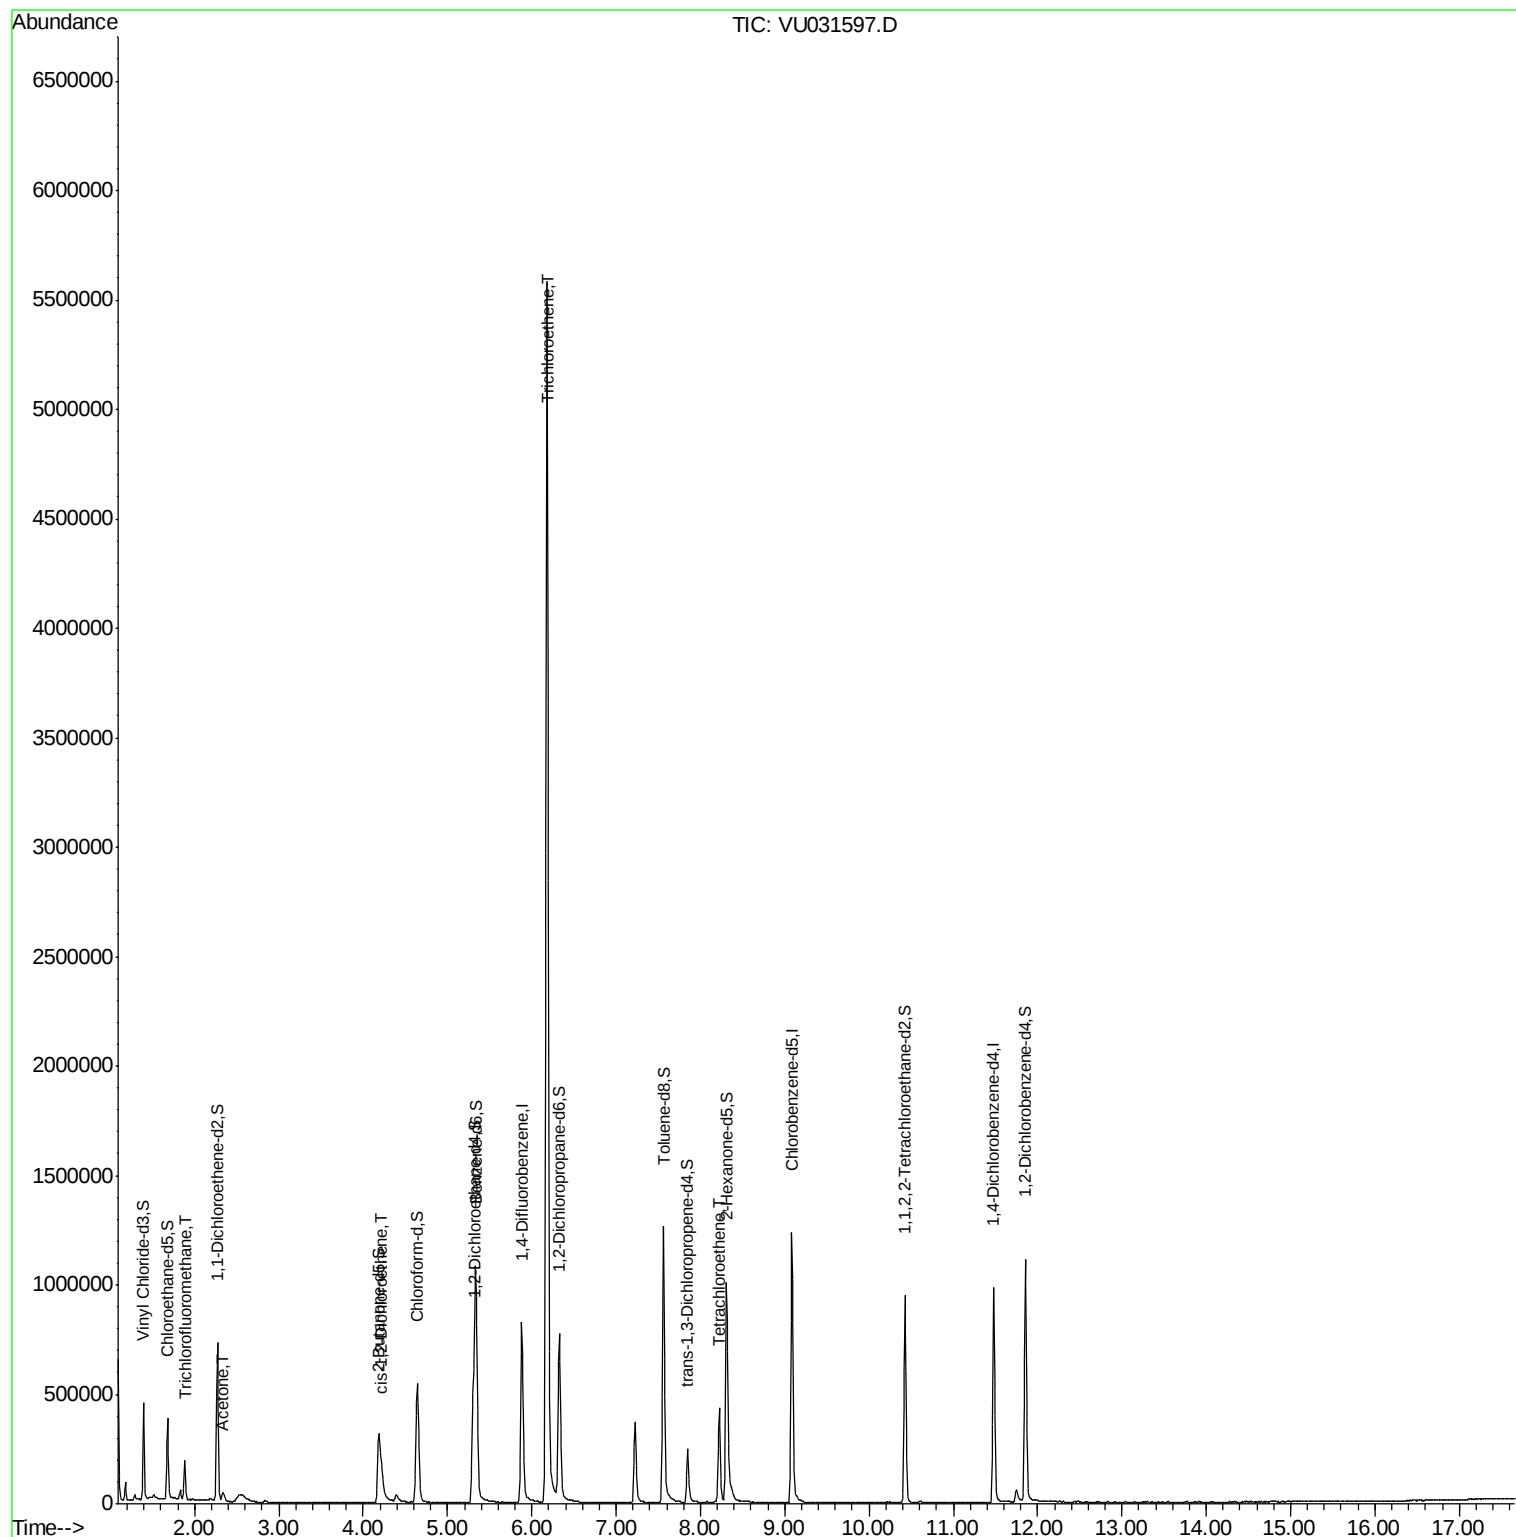




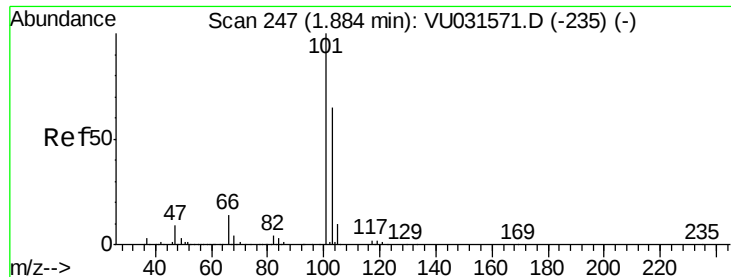


#9

Trichlorofluoromethane
 Concen: 10.958 ug/L
 RT: 1.88 min Scan# 246
 Delta R.T. -0.00 min
 Lab File: VU031597.D
 Acq: 29 Apr 2019 19:24

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X09




Tot Ion:101 Resp: 101080
 Ion Ratio Lower Upper
 101 100
 103 66.6 50.8 76.2

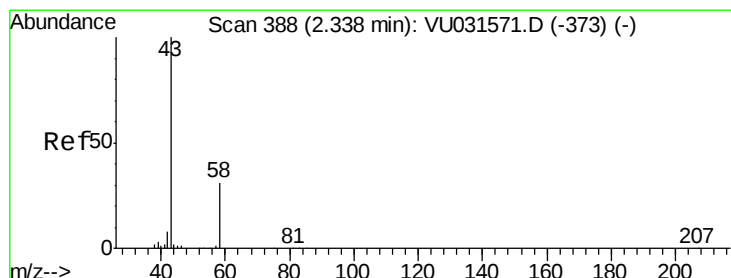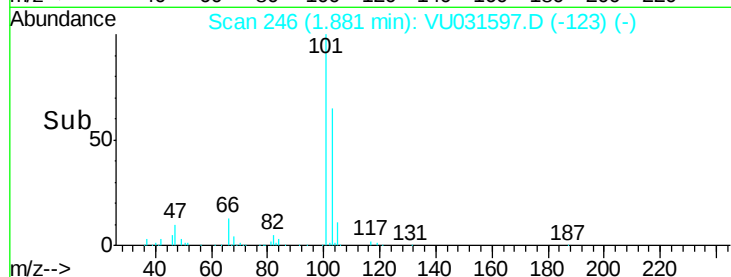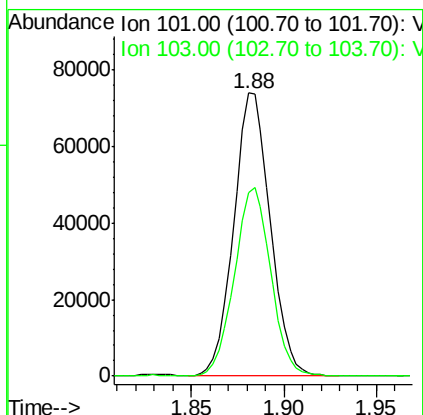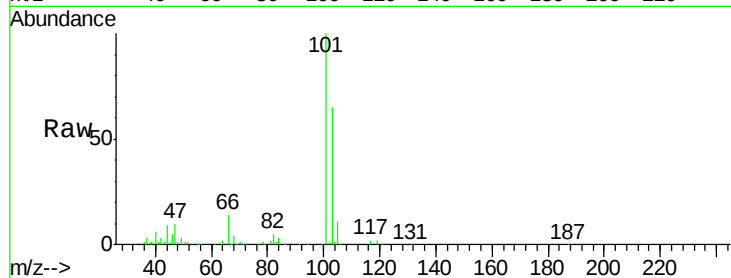


#13

Acetone
 Concen: 10.672 ug/L
 RT: 2.34 min Scan# 388
 Delta R.T. -0.00 min
 Lab File: VU031597.D
 Acq: 29 Apr 2019 19:24

Tgt Ion: 43 Resp: 59295
 Ion Ratio Lower Upper
 43 100
 58 31.4 0.0 64.4

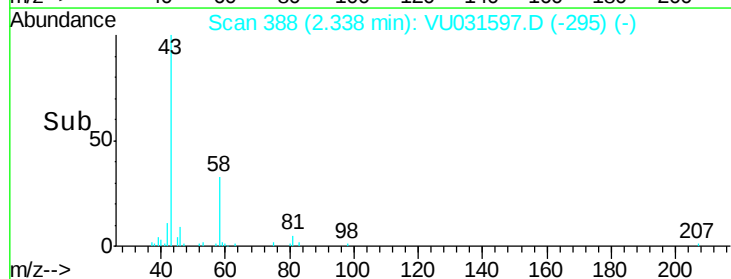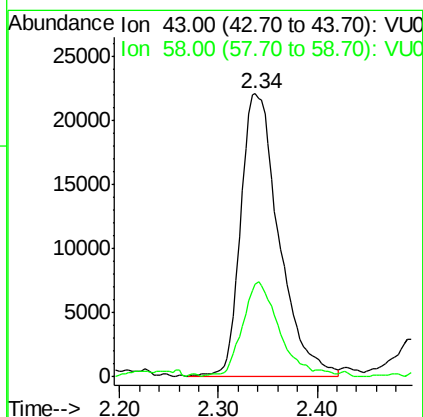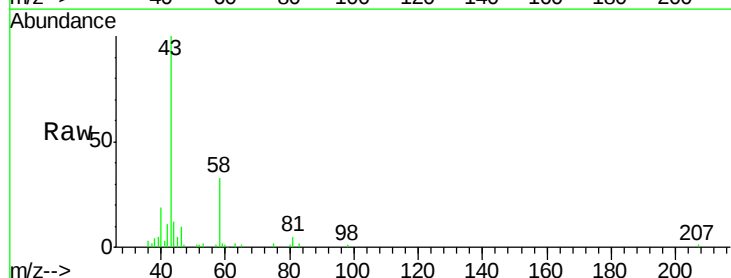




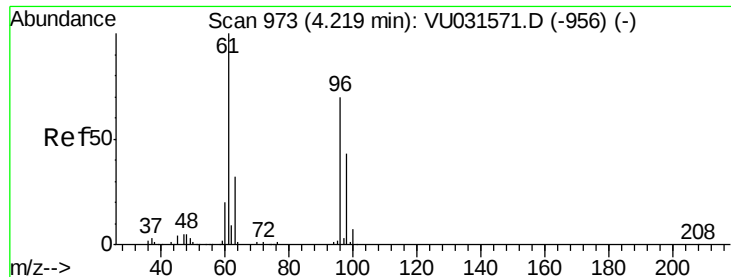


#20

cis-1,2-Dichloroethene
 Concen: 4.960 ug/L
 RT: 4.22 min Scan# 973
 Delta R.T. -0.00 min
 Lab File: VU031597.D
 Acq: 29 Apr 2019 19:24

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X09




Tot Ion	Ratio	Lower	Upper
96	100		
61	144.5	99.5	184.7
68	0.0	0.0	0.0

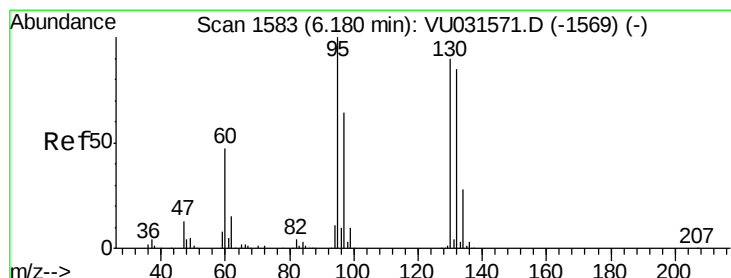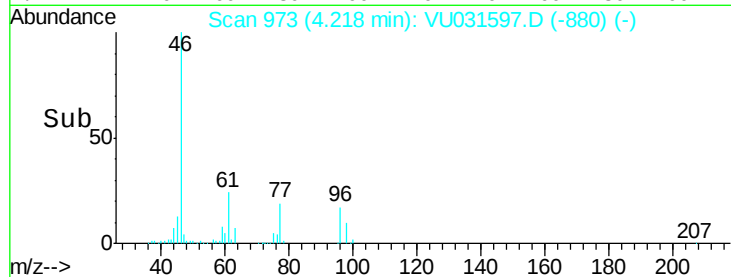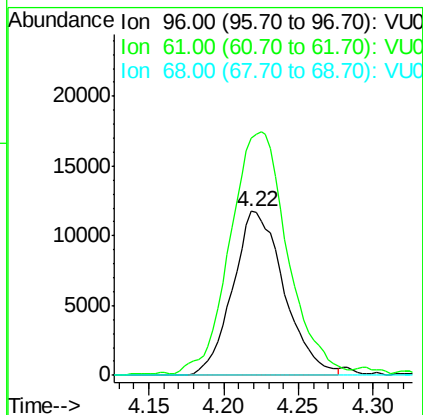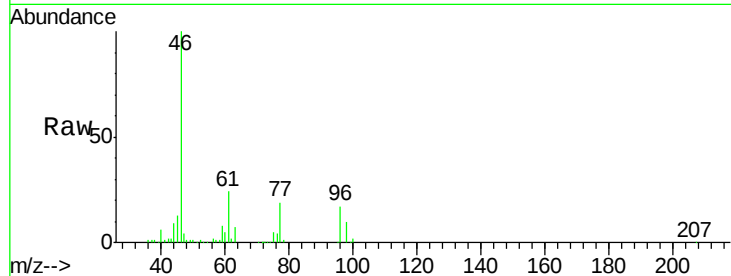


#34

Trichloroethene
 Concen: 361.663 ug/L
 RT: 6.18 min Scan# 1583
 Delta R.T. -0.00 min
 Lab File: VU031597.D
 Acq: 29 Apr 2019 19:24

Tgt Ion	Ratio	Lower	Upper
95	100		
97	64.8	44.8	83.2
132	84.2	63.1	117.1
130	89.0	66.5	123.5

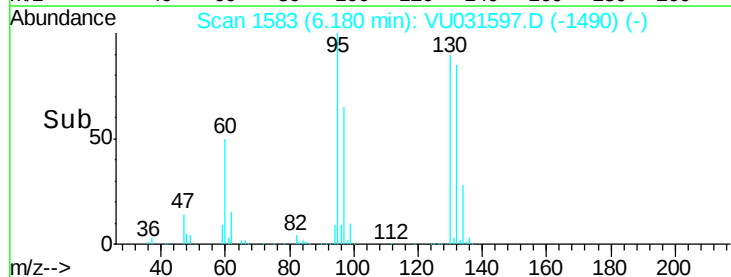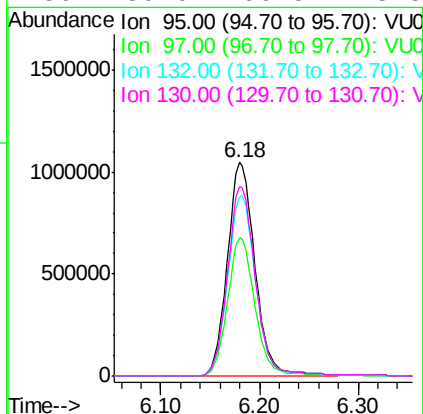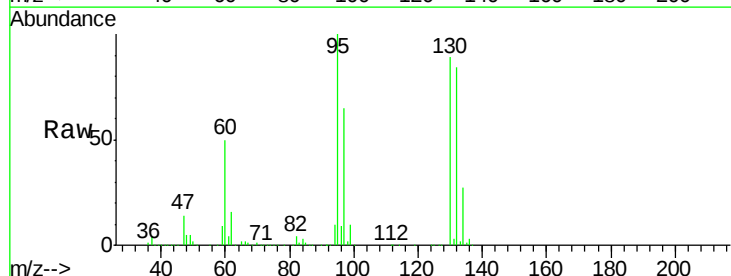

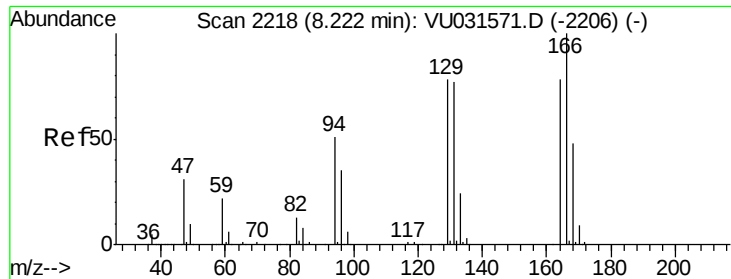

#46

Tetrachloroethene

Concen: 24.538 ug/L

RT: 8.22 min Scan# 2219

Delta R.T. 0.00 min

Lab File: VU031597.D


Acq: 29 Apr 2019 19:24

Instrument :

MSVOA_U

ClientSampleId :

C0X09

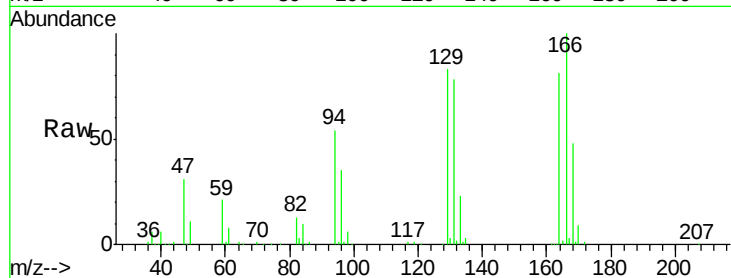

Tot Ion:164 Resp: 95160

Ion Ratio Lower Upper

164 100

129 101.7 71.5 132.9

131 95.4 69.0 128.2

166 122.8 93.7 173.9

Abundance Ion 164.00 (163.70 to 164.70): V

Ion 129.00 (128.70 to 129.70): V

Ion 131.00 (130.70 to 131.70): V

Ion 166.00 (165.70 to 166.70): V

