

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031580.D
 Acq On : 29 Apr 2019 12:49
 Operator : JC/SP
 Sample : K2536-18 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	34	rVB3	22470	20218	0.59%	0.072%
2	1.286	56	61	70	rBV4	19671	25603	0.75%	0.091%
3	1.396	88	95	108	rVB	475348	502884	14.67%	1.785%
4	1.678	176	183	199	rBV	358886	449327	13.11%	1.595%
5	1.881	242	246	260	rVB2	32235	43056	1.26%	0.153%
6	2.270	356	367	380	rVB	766520	1171191	34.17%	4.158%
7	2.473	428	430	436	rVB5	2042	1275	0.04%	0.005%
8	2.694	490	499	511	rVB8	5589	10695	0.31%	0.038%
9	2.746	511	515	517	rBV3	801	715	0.02%	0.003%
10	2.820	535	538	540	rBV4	1450	861	0.03%	0.003%
11	2.891	557	560	566	rVB4	1238	960	0.03%	0.003%
12	2.955	576	580	582	rVV2	1423	1222	0.04%	0.004%
13	2.981	585	588	593	rVV5	1935	2029	0.06%	0.007%
14	3.003	593	595	600	rVV3	1176	923	0.03%	0.003%
15	3.032	600	604	608	rVB3	1222	902	0.03%	0.003%
16	3.071	613	616	619	rBV3	1123	696	0.02%	0.002%
17	3.129	630	634	636	rBV3	1070	876	0.03%	0.003%
18	3.164	642	645	652	rVB5	1633	1335	0.04%	0.005%
19	3.238	666	668	677	rVB4	1895	2214	0.06%	0.008%
20	3.283	677	682	685	rBV3	1783	1908	0.06%	0.007%
21	3.309	685	690	696	rVV4	1418	1559	0.05%	0.006%
22	3.418	721	724	727	rBV2	1096	795	0.02%	0.003%
23	3.534	756	760	763	rBV3	1312	1092	0.03%	0.004%
24	3.579	769	774	777	rBV3	876	806	0.02%	0.003%
25	3.630	787	790	793	rVB2	1317	775	0.02%	0.003%
26	3.649	793	796	799	rBV2	1552	784	0.02%	0.003%
27	3.669	799	802	806	rVB	1075	776	0.02%	0.003%
28	3.707	810	814	819	rVB4	1221	920	0.03%	0.003%
29	3.858	859	861	866	rVV6	1233	1002	0.03%	0.004%
30	3.897	870	873	881	rVB5	1637	1640	0.05%	0.006%
31	3.942	881	887	891	rBV2	1100	1235	0.04%	0.004%
32	3.984	897	900	908	rVB3	1812	2009	0.06%	0.007%
33	4.125	939	944	948	rBV3	822	800	0.02%	0.003%
34	4.186	949	963	992	rBV	325350	1043810	30.46%	3.706%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031580.D
 Acq On : 29 Apr 2019 12:49
 Operator : JC/SP
 Sample : K2536-18 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	4.534	1068	1071	1073	rBV4	1488	915	0.03%	0.003%
36	4.582	1083	1086	1088	rBV2	1164	749	0.02%	0.003%
37	4.643	1088	1105	1136	rVV2	557696	1330717	38.83%	4.725%
38	4.874	1173	1177	1179	rBV3	1881	1544	0.05%	0.005%
39	5.151	1261	1263	1267	rVB4	1459	905	0.03%	0.003%
40	5.247	1289	1293	1296	rBV3	848	774	0.02%	0.003%
41	5.337	1296	1321	1353	rBV2	1116009	3427296	100.00%	12.168%
42	5.646	1413	1417	1418	rBV3	2318	1602	0.05%	0.006%
43	5.884	1477	1491	1532	rBV	849449	1806815	52.72%	6.415%
44	6.183	1569	1584	1615	rBV	1549384	3172043	92.55%	11.262%
45	6.328	1617	1629	1649	rVB	757362	1552489	45.30%	5.512%
46	6.694	1740	1743	1747	rBV2	1303	943	0.03%	0.003%
47	6.752	1756	1761	1764	rBV3	2190	2086	0.06%	0.007%
48	6.952	1820	1823	1825	rBV4	1298	757	0.02%	0.003%
49	7.035	1846	1849	1852	rBV	1008	744	0.02%	0.003%
50	7.225	1895	1908	1934	rBV	393685	744900	21.73%	2.645%
51	7.521	1997	2000	2001	rBV2	1256	698	0.02%	0.002%
52	7.562	2001	2013	2057	rVV	1357655	2526721	73.72%	8.971%
53	7.849	2090	2102	2127	rBV	273616	499805	14.58%	1.775%
54	8.132	2187	2190	2192	rBV3	1392	1041	0.03%	0.004%
55	8.167	2195	2201	2204	rBV6	2382	2937	0.09%	0.010%
56	8.225	2209	2219	2234	rVV2	58980	105602	3.08%	0.375%
57	8.312	2234	2246	2291	rBV	1063802	2156947	62.93%	7.658%
58	8.681	2358	2361	2363	rBV4	1586	1149	0.03%	0.004%
59	8.813	2397	2402	2404	rBV5	1320	1369	0.04%	0.005%
60	9.006	2459	2462	2465	rVB3	1729	1109	0.03%	0.004%
61	9.086	2475	2487	2526	rBV	1265859	2223575	64.88%	7.895%
62	9.312	2554	2557	2561	rVB2	2203	1495	0.04%	0.005%
63	9.350	2566	2569	2573	rVB5	2191	1664	0.05%	0.006%
64	9.382	2573	2579	2581	rBV4	1835	1949	0.06%	0.007%
65	9.418	2586	2590	2593	rBV4	2460	2067	0.06%	0.007%
66	9.527	2621	2624	2627	rVB3	1438	846	0.02%	0.003%
67	9.746	2688	2692	2694	rBV3	916	756	0.02%	0.003%
68	9.762	2694	2697	2701	rVB	1008	754	0.02%	0.003%
69	9.855	2723	2726	2729	rBV4	999	853	0.02%	0.003%
70	9.874	2729	2732	2739	rVB3	1374	1517	0.04%	0.005%
71	9.903	2739	2741	2748	rBV3	1559	1796	0.05%	0.006%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031580.D
 Acq On : 29 Apr 2019 12:49
 Operator : JC/SP
 Sample : K2536-18 20X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X06

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.041	2780	2784	2787	rBV3	923	877	0.03%	0.003%
73	10.115	2804	2807	2811	rBV2	1524	1359	0.04%	0.005%
74	10.176	2823	2826	2833	rVB4	1669	1771	0.05%	0.006%
75	10.257	2846	2851	2852	rBV2	1006	890	0.03%	0.003%
76	10.279	2855	2858	2861	rBV3	1098	828	0.02%	0.003%
77	10.340	2871	2877	2879	rBV4	1464	1391	0.04%	0.005%
78	10.427	2892	2904	2928	rBV	990132	1612944	47.06%	5.727%
79	10.877	3041	3044	3046	rBV4	1742	1171	0.03%	0.004%
80	10.922	3056	3058	3061	rVB2	1585	696	0.02%	0.002%
81	11.029	3087	3091	3095	rBV3	1573	1455	0.04%	0.005%
82	11.054	3096	3099	3100	rBV	1297	712	0.02%	0.003%
83	11.196	3140	3143	3148	rBV3	1206	1106	0.03%	0.004%
84	11.385	3197	3202	3203	rBV2	1282	1180	0.03%	0.004%
85	11.479	3217	3231	3251	rBV	1037461	1700491	49.62%	6.037%
86	11.736	3309	3311	3315	rVB3	1577	726	0.02%	0.003%
87	11.855	3336	3348	3375	rBV	1157752	1944982	56.75%	6.906%
88	12.273	3474	3478	3481	rBV4	1907	1513	0.04%	0.005%
89	12.630	3587	3589	3592	rBV2	1134	774	0.02%	0.003%
90	12.691	3603	3608	3611	rBV5	1165	1287	0.04%	0.005%
91	12.816	3644	3647	3650	rBV3	1532	1066	0.03%	0.004%
92	12.877	3663	3666	3669	rBV	1453	833	0.02%	0.003%
93	13.180	3757	3760	3765	rBV5	1892	1966	0.06%	0.007%
94	13.244	3778	3780	3783	rBV2	1273	791	0.02%	0.003%
95	13.295	3793	3796	3800	rBV3	1489	1439	0.04%	0.005%
96	13.501	3857	3860	3861	rBV2	1124	700	0.02%	0.002%
97	13.546	3871	3874	3877	rVB3	1786	1056	0.03%	0.004%
98	13.694	3917	3920	3923	rVB	1714	1108	0.03%	0.004%
99	14.128	4052	4055	4058	rBV3	1881	1349	0.04%	0.005%
100	14.819	4267	4270	4278	rBV6	1819	2284	0.07%	0.008%


Sum of corrected areas: 28165567

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042919\
Data File : VU031580.D
Acq On : 29 Apr 2019 12:49
Operator : JC/SP
Sample : K2536-18 20X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X06

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

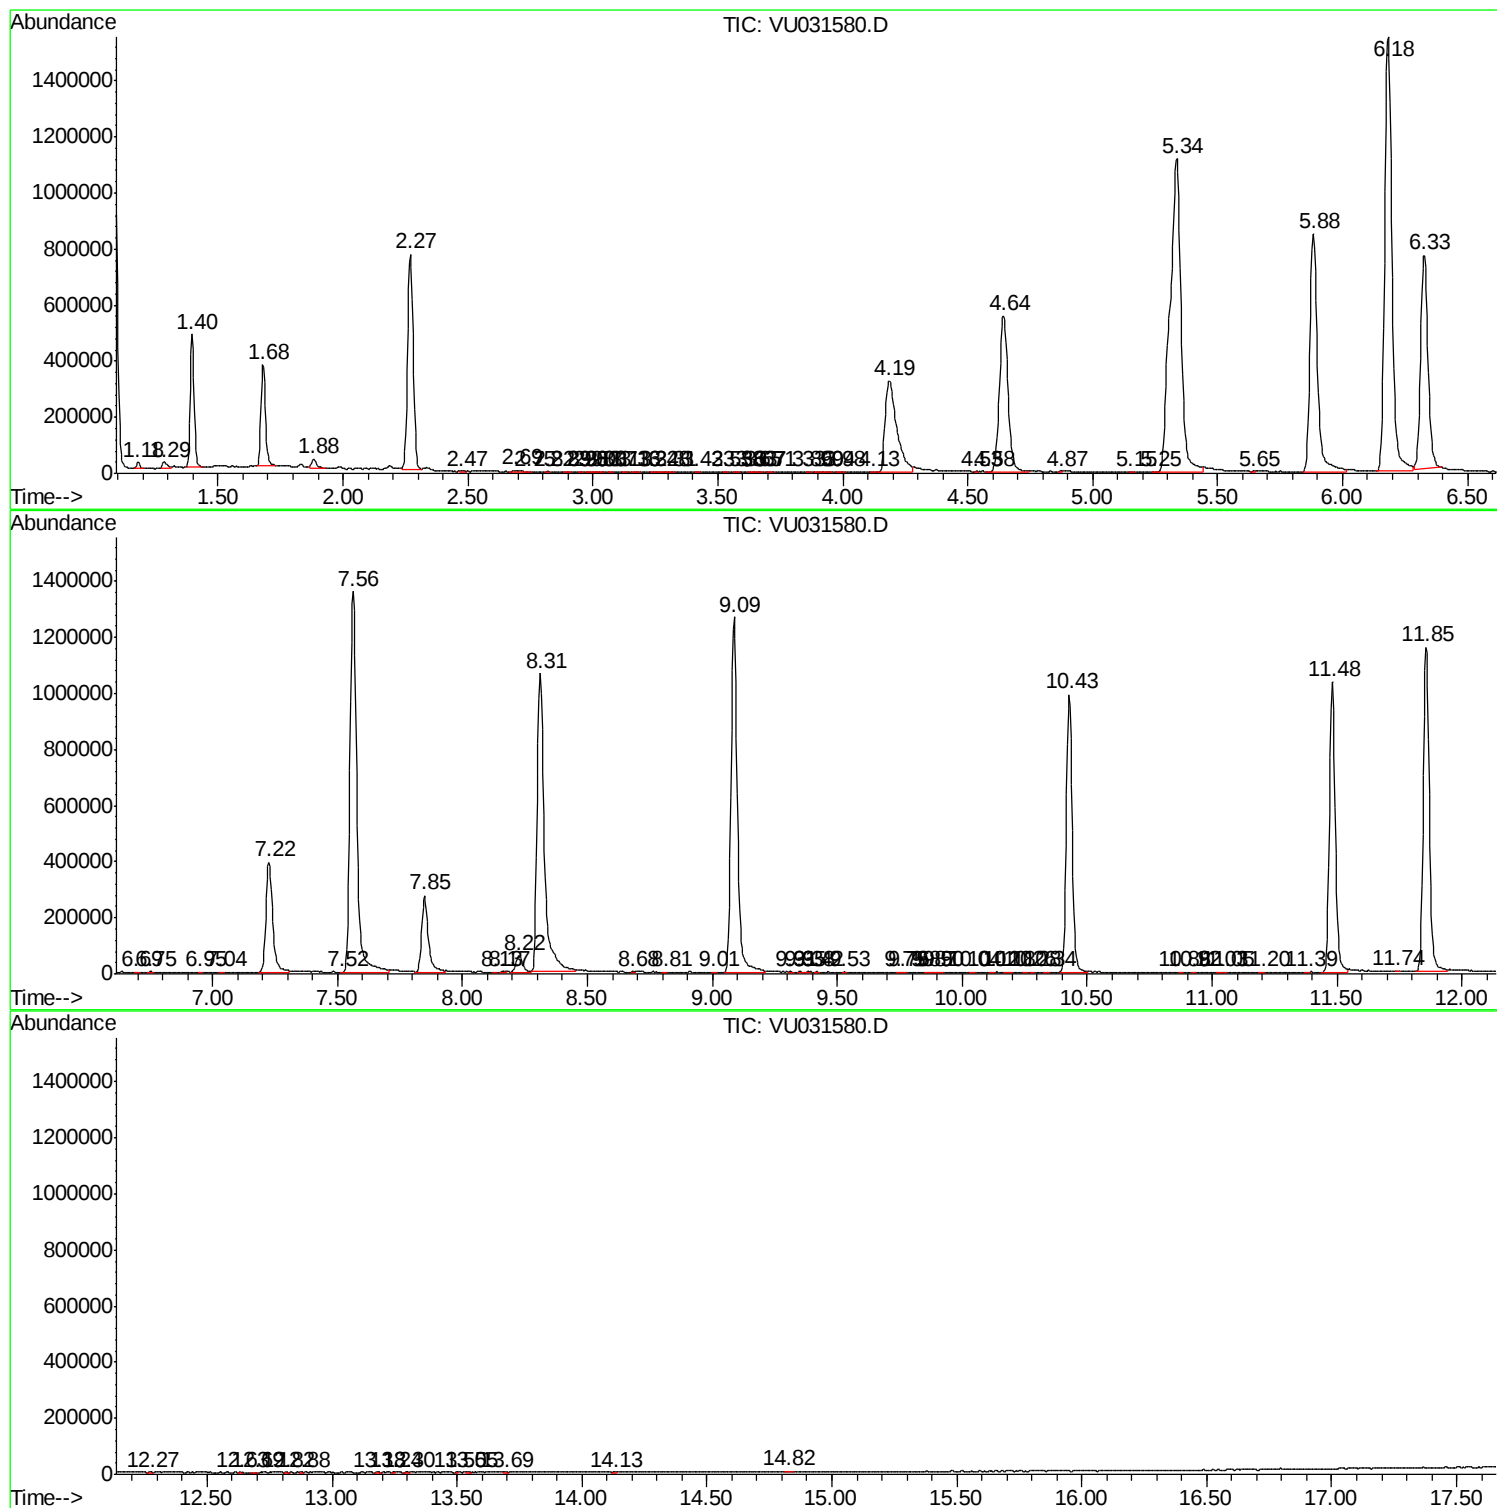

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042919\
Data File : VU031580.D
Acq On : 29 Apr 2019 12:49
Operator : JC/SP
Sample : K2536-18 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X06

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042919\
Data File : VU031580.D
Acq On : 29 Apr 2019 12:49
Operator : JC/SP
Sample : K2536-18 20X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X06

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc