

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031587.D
 Acq On : 29 Apr 2019 15:32
 Operator : JC/SP
 Sample : K2586-20DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X66DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	36	rVB4	22125	22318	0.66%	0.087%
2	1.396	88	95	109	rVB	436150	478629	14.11%	1.856%
3	1.679	176	183	195	rBV	366541	441313	13.01%	1.711%
4	2.270	356	367	380	rVB	737787	1129826	33.31%	4.382%
5	2.775	521	524	528	rBV4	773	689	0.02%	0.003%
6	2.839	533	544	549	rBV3	6054	11251	0.33%	0.044%
7	2.994	587	592	595	rBV3	1335	1073	0.03%	0.004%
8	3.129	628	634	637	rBV3	1705	1737	0.05%	0.007%
9	3.232	664	666	671	rVB2	998	866	0.03%	0.003%
10	3.283	679	682	684	rBV2	1298	832	0.02%	0.003%
11	3.338	695	699	706	rBV3	1711	2256	0.07%	0.009%
12	3.389	710	715	718	rBV3	1060	1093	0.03%	0.004%
13	3.514	752	754	758	rVB3	1581	944	0.03%	0.004%
14	3.537	758	761	768	rBV3	2026	1624	0.05%	0.006%
15	3.727	818	820	827	rVV2	812	855	0.03%	0.003%
16	3.778	832	836	839	rBV4	636	598	0.02%	0.002%
17	3.826	848	851	856	rVB3	938	980	0.03%	0.004%
18	3.916	875	879	884	rBV5	715	783	0.02%	0.003%
19	3.974	893	897	901	rBV2	1784	1667	0.05%	0.006%
20	4.016	907	910	912	rBV	898	686	0.02%	0.003%
21	4.045	916	919	923	rVB2	821	602	0.02%	0.002%
22	4.106	935	938	940	rBV2	1103	682	0.02%	0.003%
23	4.186	949	963	1001	rBV	317601	1014042	29.89%	3.933%
24	4.643	1089	1105	1134	rBV	540138	1282466	37.81%	4.974%
25	4.842	1160	1167	1171	rBV3	2504	3373	0.10%	0.013%
26	4.945	1196	1199	1201	rBV3	932	747	0.02%	0.003%
27	5.016	1218	1221	1225	rVB3	1121	914	0.03%	0.004%
28	5.231	1283	1288	1290	rVB3	1042	806	0.02%	0.003%
29	5.257	1290	1296	1297	rBV2	1029	818	0.02%	0.003%
30	5.334	1297	1320	1368	rBV2	1102453	3392183	100.00%	13.155%
31	5.784	1457	1460	1463	rBV3	1490	1099	0.03%	0.004%
32	5.881	1475	1490	1521	rBV	850368	1760263	51.89%	6.826%
33	6.183	1570	1584	1612	rBV	780937	1590352	46.88%	6.168%
34	6.325	1616	1628	1651	rVB	744573	1511152	44.55%	5.860%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031587.D
 Acq On : 29 Apr 2019 15:32
 Operator : JC/SP
 Sample : K2586-20DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X66DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	6.765	1761	1765	1771	rBV6	833	1060	0.03%	0.004%
36	6.823	1780	1783	1787	rBV3	739	631	0.02%	0.002%
37	6.997	1834	1837	1843	rBV6	1058	1133	0.03%	0.004%
38	7.122	1873	1876	1882	rVB5	1303	1092	0.03%	0.004%
39	7.154	1882	1886	1888	rBV	1116	839	0.02%	0.003%
40	7.225	1894	1908	1930	rBV	373211	709058	20.90%	2.750%
41	7.373	1951	1954	1955	rBV3	1502	805	0.02%	0.003%
42	7.418	1965	1968	1969	rBV3	1218	731	0.02%	0.003%
43	7.498	1990	1993	1997	rVB4	2086	1587	0.05%	0.006%
44	7.563	1997	2013	2050	rBV	1288105	2438383	71.88%	9.456%
45	7.849	2091	2102	2135	rBV	256314	475284	14.01%	1.843%
46	7.981	2141	2143	2147	rBV3	1471	987	0.03%	0.004%
47	8.128	2184	2189	2192	rBV5	1392	1609	0.05%	0.006%
48	8.225	2211	2219	2230	rBV8	12043	20696	0.61%	0.080%
49	8.312	2235	2246	2297	rBV	1042232	2133358	62.89%	8.273%
50	8.826	2403	2406	2412	rBV7	978	784	0.02%	0.003%
51	8.987	2451	2456	2460	rBV5	1277	1410	0.04%	0.005%
52	9.016	2460	2465	2470	rBV6	1154	1067	0.03%	0.004%
53	9.087	2474	2487	2523	rBV	1229385	2194726	64.70%	8.511%
54	9.389	2576	2581	2584	rBV6	1692	1721	0.05%	0.007%
55	9.447	2597	2599	2603	rVB4	1693	974	0.03%	0.004%
56	9.556	2630	2633	2638	rBV4	1074	848	0.02%	0.003%
57	9.591	2642	2644	2647	rBV2	1272	891	0.03%	0.003%
58	9.607	2647	2649	2652	rVB2	1253	726	0.02%	0.003%
59	9.624	2652	2654	2657	rVB2	1355	651	0.02%	0.003%
60	9.646	2657	2661	2662	rBV3	1458	981	0.03%	0.004%
61	9.704	2676	2679	2683	rBV2	1008	738	0.02%	0.003%
62	9.791	2703	2706	2711	rVV3	1178	932	0.03%	0.004%
63	9.878	2730	2733	2738	rVB5	1267	1000	0.03%	0.004%
64	9.958	2756	2758	2762	rVB	925	636	0.02%	0.002%
65	9.990	2764	2768	2771	rBV3	859	781	0.02%	0.003%
66	10.038	2780	2783	2787	rBV2	1233	762	0.02%	0.003%
67	10.067	2787	2792	2798	rBV5	1299	1658	0.05%	0.006%
68	10.183	2825	2828	2833	rVB4	1156	1025	0.03%	0.004%
69	10.209	2833	2836	2842	rBV6	1303	1514	0.04%	0.006%
70	10.238	2842	2845	2847	rVV2	1014	694	0.02%	0.003%
71	10.267	2851	2854	2859	rVB4	1263	1017	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031587.D
 Acq On : 29 Apr 2019 15:32
 Operator : JC/SP
 Sample : K2586-20DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X66DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.315	2866	2869	2871	rBV3	982	615	0.02%	0.002%
73	10.379	2885	2889	2891	rVB3	895	641	0.02%	0.002%
74	10.427	2891	2904	2925	rBV	968430	1568581	46.24%	6.083%
75	10.572	2946	2949	2951	rBV3	1456	772	0.02%	0.003%
76	10.604	2953	2959	2967	rVV4	3654	5641	0.17%	0.022%
77	10.652	2972	2974	2978	rBV2	1319	905	0.03%	0.004%
78	10.733	2997	2999	3003	rVB2	1351	798	0.02%	0.003%
79	10.807	3019	3022	3024	rBV4	1233	809	0.02%	0.003%
80	10.849	3032	3035	3038	rBV3	1031	751	0.02%	0.003%
81	10.996	3078	3081	3086	rBV2	1168	1290	0.04%	0.005%
82	11.022	3086	3089	3092	rVV2	954	735	0.02%	0.003%
83	11.077	3101	3106	3107	rBV3	1162	1040	0.03%	0.004%
84	11.132	3120	3123	3128	rVB3	1501	1113	0.03%	0.004%
85	11.283	3166	3170	3178	rVB3	1485	2020	0.06%	0.008%
86	11.479	3215	3231	3264	rBV	999650	1664986	49.08%	6.457%
87	11.855	3334	3348	3370	rBV	1113052	1854711	54.68%	7.193%
88	12.318	3490	3492	3497	rVB5	1815	1156	0.03%	0.004%
89	12.762	3627	3630	3632	rBV3	1241	918	0.03%	0.004%
90	12.778	3632	3635	3638	rVV2	1607	1073	0.03%	0.004%
91	12.848	3651	3657	3665	rBV8	2732	4534	0.13%	0.018%
92	13.041	3714	3717	3719	rBV3	1274	783	0.02%	0.003%
93	13.160	3751	3754	3757	rBV2	1695	1199	0.04%	0.005%
94	13.315	3796	3802	3805	rBV6	1444	1435	0.04%	0.006%
95	13.482	3851	3854	3860	rBV5	1692	1549	0.05%	0.006%
96	13.601	3889	3891	3895	rBV2	1347	826	0.02%	0.003%
97	13.662	3908	3910	3914	rBV3	1151	789	0.02%	0.003%
98	13.720	3925	3928	3931	rBV3	1185	858	0.03%	0.003%
99	13.762	3939	3941	3944	rBV2	1466	953	0.03%	0.004%
100	14.633	4208	4212	4216	rBV4	2027	1982	0.06%	0.008%


Sum of corrected areas: 25785771

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042919\
Data File : VU031587.D
Acq On : 29 Apr 2019 15:32
Operator : JC/SP
Sample : K2586-20DL 5X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X66DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

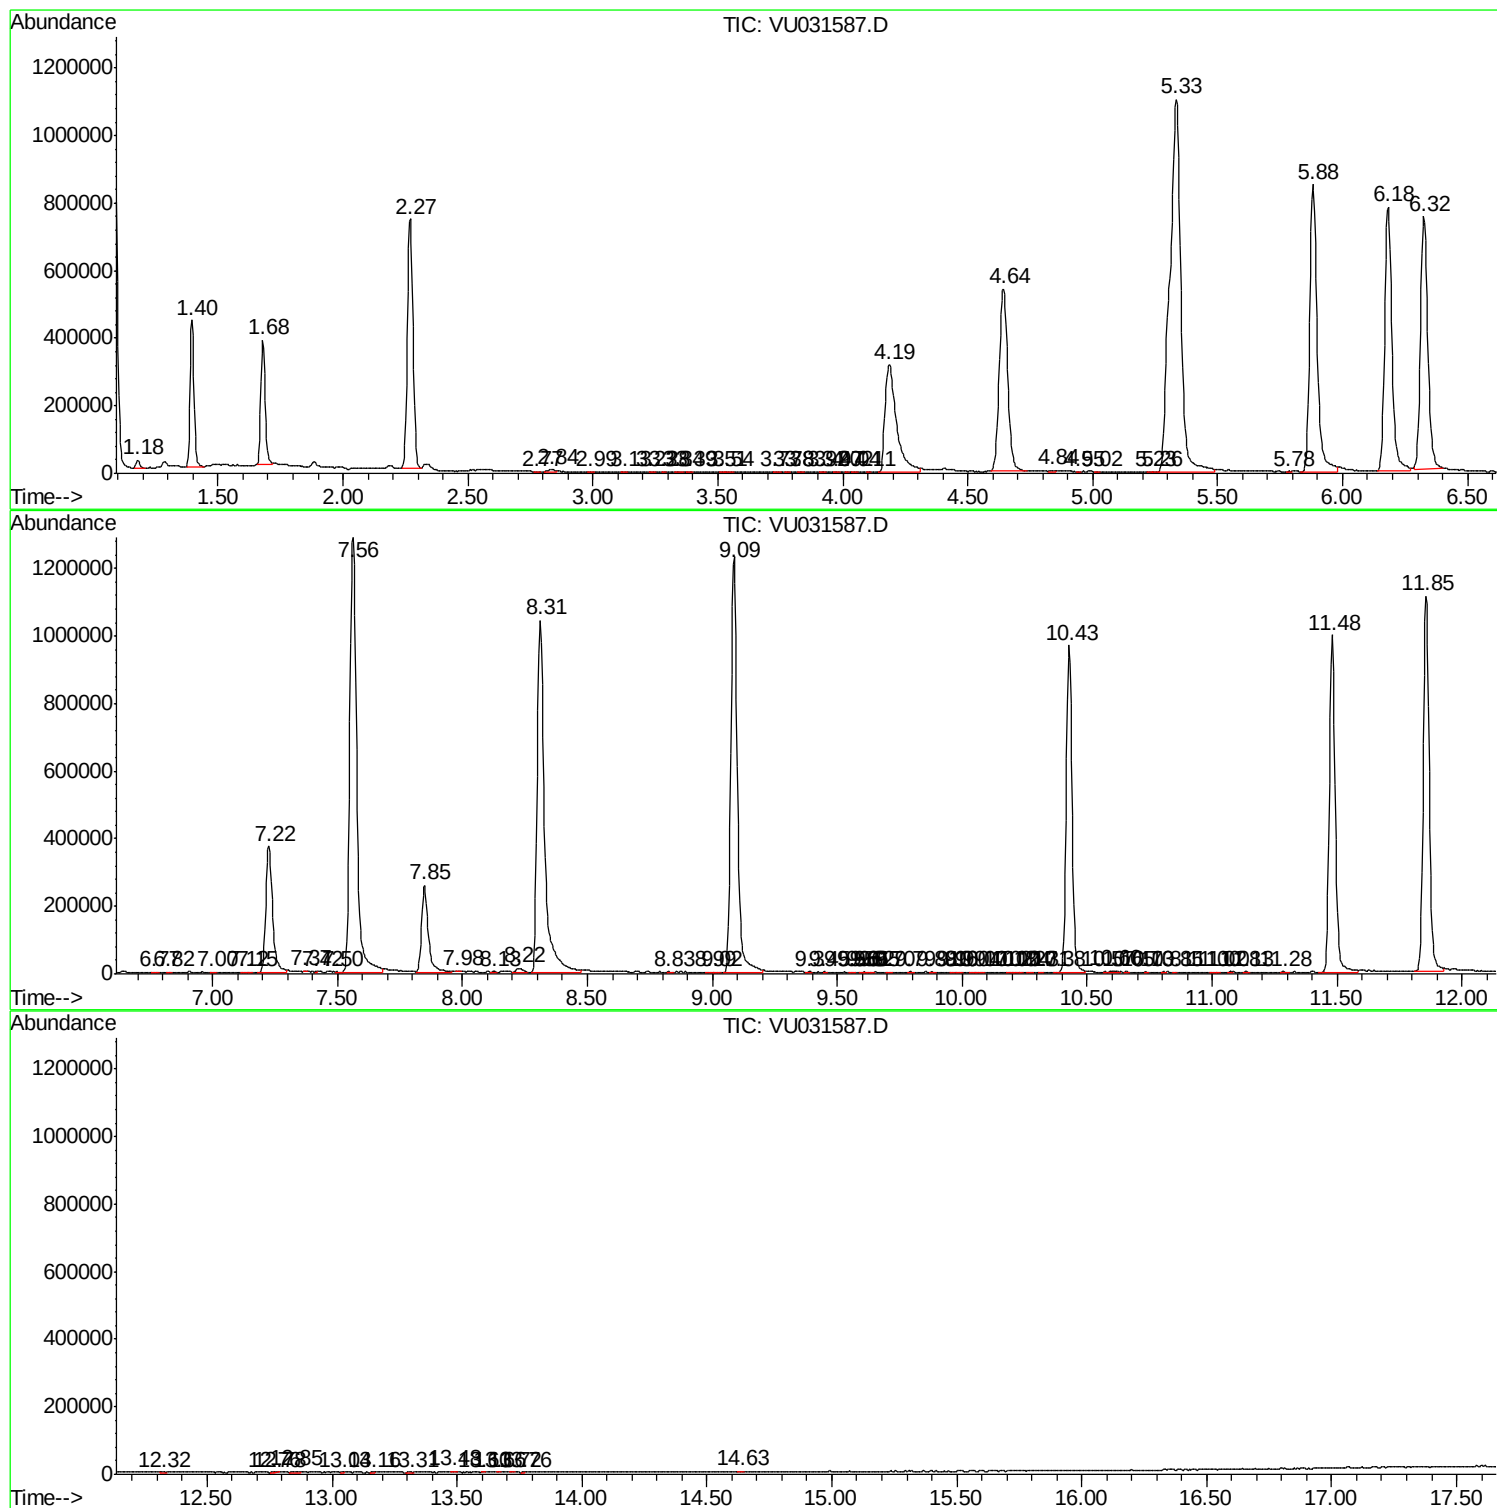

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042919\
Data File : VU031587.D
Acq On : 29 Apr 2019 15:32
Operator : JC/SP
Sample : K2586-20DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X66DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042919\
Data File : VU031587.D
Acq On : 29 Apr 2019 15:32
Operator : JC/SP
Sample : K2586-20DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X66DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc