

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031588.D
 Acq On : 29 Apr 2019 15:55
 Operator : JC/SP
 Sample : K2590-13DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XB9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	38	rVB2	20381	20921	0.63%	0.078%
2	1.396	88	95	108	rBV	432749	472510	14.19%	1.762%
3	1.678	176	183	196	rBV	344906	427859	12.85%	1.596%
4	1.881	238	246	258	rVB	163750	227026	6.82%	0.847%
5	2.270	356	367	381	rVB	737653	1124761	33.78%	4.194%
6	2.579	459	463	467	rBV5	2153	1841	0.06%	0.007%
7	2.762	516	520	523	rBV3	1301	1096	0.03%	0.004%
8	2.817	532	537	539	rBV2	3111	2636	0.08%	0.010%
9	2.887	557	559	564	rBV2	1094	842	0.03%	0.003%
10	2.932	568	573	576	rBV4	894	862	0.03%	0.003%
11	3.125	630	633	636	rVB3	970	669	0.02%	0.002%
12	3.254	670	673	678	rVB6	1575	1152	0.03%	0.004%
13	3.283	678	682	686	rBV2	1000	916	0.03%	0.003%
14	3.309	686	690	692	rBV2	1064	736	0.02%	0.003%
15	3.383	707	713	716	rVV6	1001	898	0.03%	0.003%
16	3.399	716	718	721	rVV3	1200	711	0.02%	0.003%
17	3.476	739	742	748	rVB3	1331	1180	0.04%	0.004%
18	3.550	763	765	771	rVB4	1082	958	0.03%	0.004%
19	3.620	783	787	791	rVB3	774	738	0.02%	0.003%
20	3.823	844	850	855	rVV4	994	1140	0.03%	0.004%
21	3.926	877	882	883	rBV2	909	669	0.02%	0.002%
22	3.997	899	904	907	rVB2	1343	1119	0.03%	0.004%
23	4.026	907	913	916	rBV3	885	1088	0.03%	0.004%
24	4.042	916	918	922	rVB3	1234	773	0.02%	0.003%
25	4.186	950	963	1001	rBV	312567	978552	29.39%	3.649%
26	4.559	1076	1079	1082	rBV3	1319	797	0.02%	0.003%
27	4.643	1088	1105	1131	rBV	548941	1301813	39.09%	4.855%
28	4.987	1206	1212	1217	rBV7	2033	2437	0.07%	0.009%
29	5.103	1242	1248	1249	rBV3	1944	1788	0.05%	0.007%
30	5.138	1249	1259	1266	rVB7	3226	6015	0.18%	0.022%
31	5.212	1277	1282	1288	rBV3	1118	1238	0.04%	0.005%
32	5.334	1294	1320	1351	rBV2	1091157	3329927	100.00%	12.418%
33	5.611	1403	1406	1410	rBV4	1715	1667	0.05%	0.006%
34	5.784	1458	1460	1463	rBV3	1136	704	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031588.D
 Acq On : 29 Apr 2019 15:55
 Operator : JC/SP
 Sample : K2590-13DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XB9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.881	1477	1490	1517	rBV	832253	1728503	51.91%	6.446%
36	6.183	1570	1584	1609	rBV	292633	621802	18.67%	2.319%
37	6.325	1615	1628	1661	rVB	746479	1522480	45.72%	5.677%
38	6.566	1700	1703	1706	rBV5	1064	853	0.03%	0.003%
39	6.633	1721	1724	1729	rVB4	2046	1403	0.04%	0.005%
40	6.739	1753	1757	1759	rBV4	952	763	0.02%	0.003%
41	6.765	1762	1765	1767	rBV3	1381	881	0.03%	0.003%
42	6.836	1783	1787	1789	rBV3	1010	773	0.02%	0.003%
43	6.881	1797	1801	1802	rBV3	1239	737	0.02%	0.003%
44	6.890	1802	1804	1811	rVB5	2085	1677	0.05%	0.006%
45	6.923	1811	1814	1817	rBV3	1513	1239	0.04%	0.005%
46	7.016	1840	1843	1845	rBV3	1104	774	0.02%	0.003%
47	7.080	1859	1863	1866	rBV3	1061	968	0.03%	0.004%
48	7.099	1866	1869	1872	rVB	1437	907	0.03%	0.003%
49	7.148	1881	1884	1888	rVB3	1878	1298	0.04%	0.005%
50	7.225	1893	1908	1940	rBV	375231	717188	21.54%	2.674%
51	7.562	2000	2013	2052	rBV	1265852	2407438	72.30%	8.977%
52	7.849	2090	2102	2124	rBV2	243808	461456	13.86%	1.721%
53	8.080	2172	2174	2177	rBV3	1539	1057	0.03%	0.004%
54	8.125	2186	2188	2191	rBV4	1069	657	0.02%	0.002%
55	8.164	2195	2200	2201	rBV4	2895	2426	0.07%	0.009%
56	8.222	2206	2218	2235	rVV	1165159	2060967	61.89%	7.685%
57	8.312	2236	2246	2293	rVB	1030834	2106878	63.27%	7.857%
58	8.582	2325	2330	2331	rBV4	1744	1461	0.04%	0.005%
59	8.627	2341	2344	2347	rBV5	1243	1139	0.03%	0.004%
60	8.662	2352	2355	2358	rVB4	1484	981	0.03%	0.004%
61	8.704	2364	2368	2371	rVB3	2356	1839	0.06%	0.007%
62	8.726	2371	2375	2379	rBV5	1313	1047	0.03%	0.004%
63	8.755	2379	2384	2387	rBV5	1432	1727	0.05%	0.006%
64	8.852	2411	2414	2421	rBV5	1588	1846	0.06%	0.007%
65	9.003	2458	2461	2465	rBV2	1540	1068	0.03%	0.004%
66	9.087	2474	2487	2516	rBV	1241099	2167850	65.10%	8.084%
67	9.273	2543	2545	2551	rVB6	2069	1597	0.05%	0.006%
68	9.366	2571	2574	2577	rVB5	1198	796	0.02%	0.003%
69	9.382	2577	2579	2583	rBV4	1117	732	0.02%	0.003%
70	9.466	2603	2605	2608	rBV3	1138	834	0.03%	0.003%
71	9.556	2630	2633	2637	rBV3	1174	918	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031588.D
 Acq On : 29 Apr 2019 15:55
 Operator : JC/SP
 Sample : K2590-13DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XB9DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	9.739	2686	2690	2692	rVV3	1428	1207	0.04%	0.005%
73	9.765	2696	2698	2701	rVB3	1833	1001	0.03%	0.004%
74	9.849	2721	2724	2730	rVB4	1106	999	0.03%	0.004%
75	9.884	2730	2735	2740	rBV5	1258	1374	0.04%	0.005%
76	10.003	2766	2772	2776	rBV5	1645	1428	0.04%	0.005%
77	10.119	2803	2808	2810	rBV2	956	837	0.03%	0.003%
78	10.154	2814	2819	2823	rVB3	1247	1298	0.04%	0.005%
79	10.183	2823	2828	2833	rBV3	1409	2041	0.06%	0.008%
80	10.225	2838	2841	2844	rBV3	1114	770	0.02%	0.003%
81	10.334	2873	2875	2881	rVB3	1169	793	0.02%	0.003%
82	10.369	2881	2886	2888	rBV3	1671	1187	0.04%	0.004%
83	10.427	2892	2904	2926	rBV	968348	1555481	46.71%	5.800%
84	10.604	2956	2959	2970	rVB7	4338	5699	0.17%	0.021%
85	10.855	3032	3037	3041	rBV5	1283	1528	0.05%	0.006%
86	10.903	3047	3052	3054	rBV4	1626	1384	0.04%	0.005%
87	11.003	3078	3083	3085	rBV2	1424	1159	0.03%	0.004%
88	11.148	3123	3128	3129	rBV	1293	1004	0.03%	0.004%
89	11.286	3168	3171	3174	rBV3	1346	826	0.02%	0.003%
90	11.308	3174	3178	3180	rBV3	903	830	0.02%	0.003%
91	11.402	3203	3207	3210	rBV4	1644	1413	0.04%	0.005%
92	11.482	3219	3232	3250	rBV	991885	1631787	49.00%	6.085%
93	11.855	3336	3348	3373	rBV	1104968	1848737	55.52%	6.894%
94	12.900	3670	3673	3675	rBV3	1155	725	0.02%	0.003%
95	12.945	3682	3687	3689	rBV3	1716	1553	0.05%	0.006%
96	13.035	3713	3715	3719	rVB3	1836	1116	0.03%	0.004%
97	13.057	3719	3722	3726	rBV4	1424	1230	0.04%	0.005%
98	13.106	3735	3737	3739	rBV	1146	758	0.02%	0.003%
99	13.212	3765	3770	3772	rBV2	1824	1911	0.06%	0.007%
100	13.498	3857	3859	3863	rBV3	1518	1307	0.04%	0.005%


Sum of corrected areas: 26816382

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042919\
Data File : VU031588.D
Acq On : 29 Apr 2019 15:55
Operator : JC/SP
Sample : K2590-13DL 5X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XB9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

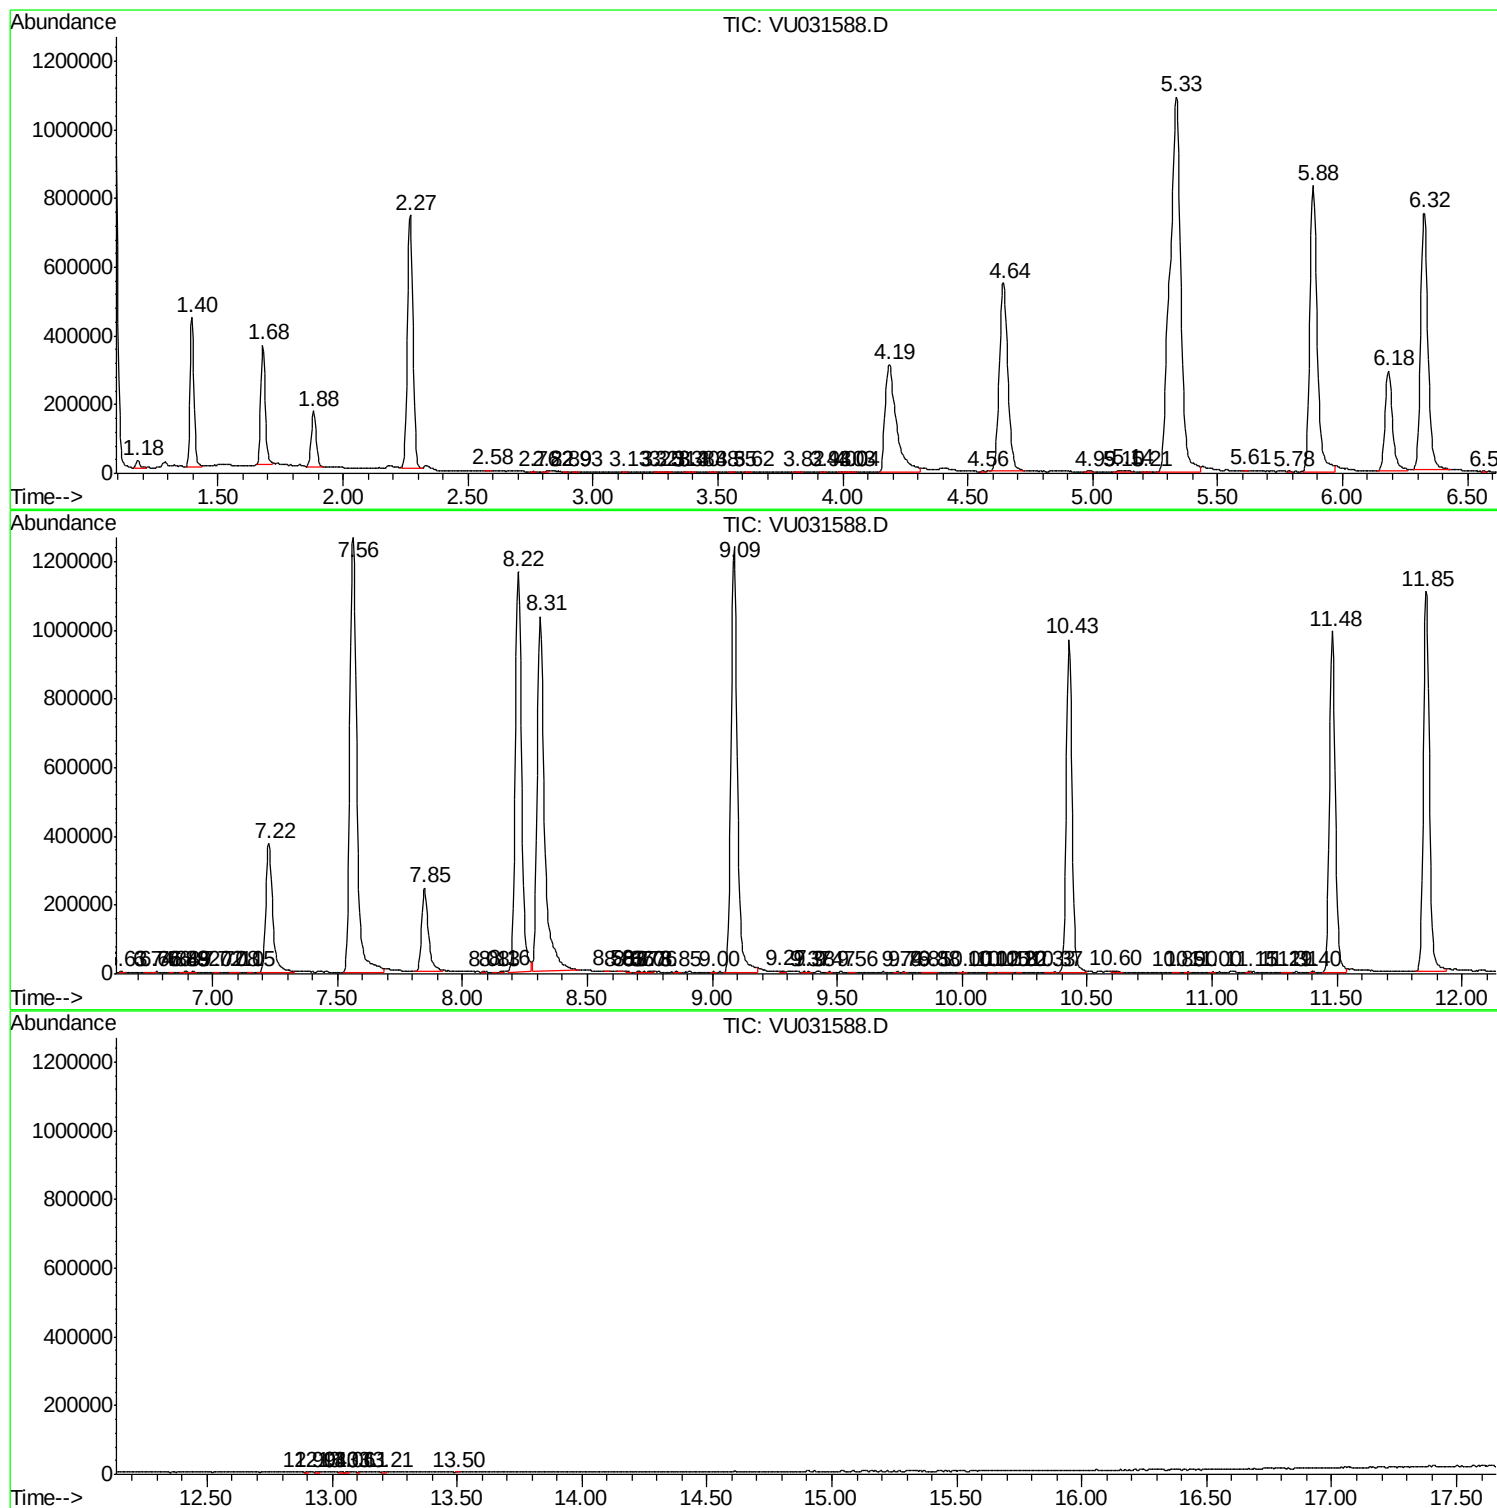

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042919\
Data File : VU031588.D
Acq On : 29 Apr 2019 15:55
Operator : JC/SP
Sample : K2590-13DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XB9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU042919\
Data File : VU031588.D
Acq On : 29 Apr 2019 15:55
Operator : JC/SP
Sample : K2590-13DL 5X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
C0XB9DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc