

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031589.D
 Acq On : 29 Apr 2019 16:18
 Operator : JC/SP
 Sample : K2536-21DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X09DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	34	rBV2	26843	24696	0.72%	0.093%
2	1.396	87	95	106	rBV	437252	479858	14.09%	1.810%
3	1.679	176	183	201	rVB	361800	450434	13.22%	1.699%
4	1.884	240	247	259	rVB2	42814	59248	1.74%	0.223%
5	2.270	356	367	380	rVB	733395	1128492	33.13%	4.257%
6	2.466	423	428	432	rBV6	1981	1863	0.05%	0.007%
7	2.518	441	444	446	rBV4	2220	1778	0.05%	0.007%
8	2.978	581	587	591	rBV7	1324	1467	0.04%	0.006%
9	3.125	629	633	636	rVB4	1217	916	0.03%	0.003%
10	3.174	644	648	650	rBV4	1077	823	0.02%	0.003%
11	3.238	666	668	672	rVB3	1508	874	0.03%	0.003%
12	3.286	677	683	685	rBV2	885	920	0.03%	0.003%
13	3.328	693	696	699	rVB2	1482	999	0.03%	0.004%
14	3.351	699	703	705	rBV	1713	1235	0.04%	0.005%
15	3.399	715	718	724	rVB3	1396	1120	0.03%	0.004%
16	3.428	724	727	729	rBV2	1395	819	0.02%	0.003%
17	3.540	758	762	765	rBV3	966	992	0.03%	0.004%
18	3.608	778	783	789	rVB5	1735	1885	0.06%	0.007%
19	3.688	801	808	812	rVB4	1607	1596	0.05%	0.006%
20	3.736	818	823	826	rVB2	1548	1162	0.03%	0.004%
21	3.839	852	855	860	rVB3	1376	1207	0.04%	0.005%
22	3.875	860	866	870	rBV3	983	1209	0.04%	0.005%
23	4.103	931	937	939	rBV3	995	1011	0.03%	0.004%
24	4.190	950	964	1012	rBV2	296465	1037350	30.45%	3.913%
25	4.547	1070	1075	1078	rBV6	1063	1116	0.03%	0.004%
26	4.643	1089	1105	1135	rBV	539317	1315819	38.62%	4.964%
27	4.868	1172	1175	1179	rBV3	1946	1796	0.05%	0.007%
28	4.949	1196	1200	1203	rVB4	1294	958	0.03%	0.004%
29	4.968	1203	1206	1208	rBV3	1766	1193	0.04%	0.005%
30	4.984	1208	1211	1215	rVV3	1413	1451	0.04%	0.005%
31	5.122	1249	1254	1256	rBV4	998	945	0.03%	0.004%
32	5.334	1296	1320	1356	rBV2	1116318	3406707	100.00%	12.851%
33	5.653	1417	1419	1421	rBV3	1563	830	0.02%	0.003%
34	5.778	1455	1458	1466	rVB5	2312	2775	0.08%	0.010%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031589.D
 Acq On : 29 Apr 2019 16:18
 Operator : JC/SP
 Sample : K2536-21DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X09DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.823	1466	1472	1476	rBV4	1459	1984	0.06%	0.007%
36	5.881	1477	1490	1518	rBV	838844	1765098	51.81%	6.658%
37	6.129	1565	1567	1569	rBV3	1565	985	0.03%	0.004%
38	6.180	1570	1583	1610	rVV	1022927	2065579	60.63%	7.792%
39	6.325	1616	1628	1652	rVB	760214	1531690	44.96%	5.778%
40	6.678	1733	1738	1744	rVB6	1751	1849	0.05%	0.007%
41	6.717	1745	1750	1752	rBV4	868	872	0.03%	0.003%
42	6.765	1761	1765	1772	rVB5	934	968	0.03%	0.004%
43	7.083	1860	1864	1868	rBV5	801	870	0.03%	0.003%
44	7.225	1894	1908	1941	rBV	374070	716689	21.04%	2.703%
45	7.456	1979	1980	1984	rVB2	1958	871	0.03%	0.003%
46	7.508	1993	1996	1999	rBV3	1494	852	0.03%	0.003%
47	7.563	1999	2013	2058	rBV	1289165	2440555	71.64%	9.206%
48	7.849	2092	2102	2130	rBV	247612	458199	13.45%	1.728%
49	8.042	2160	2162	2169	rVB6	1903	1526	0.04%	0.006%
50	8.173	2193	2203	2207	rBV5	4902	7631	0.22%	0.029%
51	8.225	2209	2219	2231	rVV2	80888	144517	4.24%	0.545%
52	8.312	2235	2246	2298	rVV	1014333	2095818	61.52%	7.906%
53	8.698	2364	2366	2369	rVV2	1713	944	0.03%	0.004%
54	8.849	2410	2413	2416	rBV3	1726	1182	0.03%	0.004%
55	8.932	2436	2439	2442	rVB2	1360	853	0.03%	0.003%
56	8.952	2442	2445	2450	rBV5	1274	1023	0.03%	0.004%
57	9.087	2474	2487	2520	rBV	1229290	2171787	63.75%	8.192%
58	9.337	2561	2565	2567	rBV4	1288	1110	0.03%	0.004%
59	9.472	2604	2607	2614	rVB3	1951	2315	0.07%	0.009%
60	9.514	2615	2620	2624	rBV5	1522	1526	0.04%	0.006%
61	9.601	2644	2647	2653	rVB5	1530	1127	0.03%	0.004%
62	9.784	2700	2704	2709	rBV7	1599	1303	0.04%	0.005%
63	9.836	2716	2720	2724	rBV4	753	885	0.03%	0.003%
64	10.096	2797	2801	2803	rVV3	1242	1120	0.03%	0.004%
65	10.215	2835	2838	2844	rBV5	1110	878	0.03%	0.003%
66	10.267	2851	2854	2857	rBV3	1286	861	0.03%	0.003%
67	10.289	2857	2861	2864	rVB3	1486	1167	0.03%	0.004%
68	10.337	2873	2876	2879	rVB3	1222	879	0.03%	0.003%
69	10.427	2891	2904	2929	rBV	957157	1570321	46.09%	5.924%
70	10.598	2953	2957	2962	rBV6	3085	3396	0.10%	0.013%
71	10.749	2998	3004	3008	rBV4	1144	1241	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031589.D
 Acq On : 29 Apr 2019 16:18
 Operator : JC/SP
 Sample : K2536-21DL 5X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X09DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.939	3061	3063	3067	rVB3	1321	822	0.02%	0.003%
73	10.964	3067	3071	3072	rBV	1265	778	0.02%	0.003%
74	11.038	3089	3094	3097	rVV4	1870	1350	0.04%	0.005%
75	11.225	3150	3152	3156	rVV2	1119	814	0.02%	0.003%
76	11.279	3166	3169	3174	rVB3	1902	1556	0.05%	0.006%
77	11.312	3174	3179	3181	rBV4	1107	1145	0.03%	0.004%
78	11.328	3181	3184	3187	rVB3	1524	911	0.03%	0.003%
79	11.366	3192	3196	3204	rVB2	1181	1411	0.04%	0.005%
80	11.408	3204	3209	3211	rBV3	1576	1406	0.04%	0.005%
81	11.479	3219	3231	3258	rBV	1008639	1652189	48.50%	6.232%
82	11.797	3327	3330	3334	rBV5	2162	1807	0.05%	0.007%
83	11.855	3335	3348	3376	rBV	1117392	1884775	55.33%	7.110%
84	12.218	3457	3461	3463	rBV3	2418	1934	0.06%	0.007%
85	12.469	3534	3539	3544	rBV6	2142	2789	0.08%	0.011%
86	12.530	3555	3558	3560	rBV2	1283	859	0.03%	0.003%
87	12.627	3584	3588	3590	rBV3	1095	996	0.03%	0.004%
88	12.701	3608	3611	3615	rBV2	1423	1314	0.04%	0.005%
89	12.845	3652	3656	3658	rBV3	1548	1291	0.04%	0.005%
90	12.996	3700	3703	3709	rBV5	1592	1305	0.04%	0.005%
91	13.167	3752	3756	3760	rBV3	1187	1303	0.04%	0.005%
92	13.234	3775	3777	3783	rBV4	1348	933	0.03%	0.004%
93	13.318	3800	3803	3807	rBV4	1464	1106	0.03%	0.004%
94	13.382	3817	3823	3825	rBV3	2467	2726	0.08%	0.010%
95	13.440	3838	3841	3845	rVB2	1767	1045	0.03%	0.004%
96	13.508	3859	3862	3866	rBV2	1905	1909	0.06%	0.007%
97	13.800	3950	3953	3958	rVB4	1835	1439	0.04%	0.005%
98	14.054	4029	4032	4035	rBV2	1822	1565	0.05%	0.006%
99	14.106	4046	4048	4051	rVB2	1803	988	0.03%	0.004%
100	15.459	4467	4469	4472	rBV2	2020	1197	0.04%	0.005%


Sum of corrected areas: 26509678

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042919\
Data File : VU031589.D
Acq On : 29 Apr 2019 16:18
Operator : JC/SP
Sample : K2536-21DL 5X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X09DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

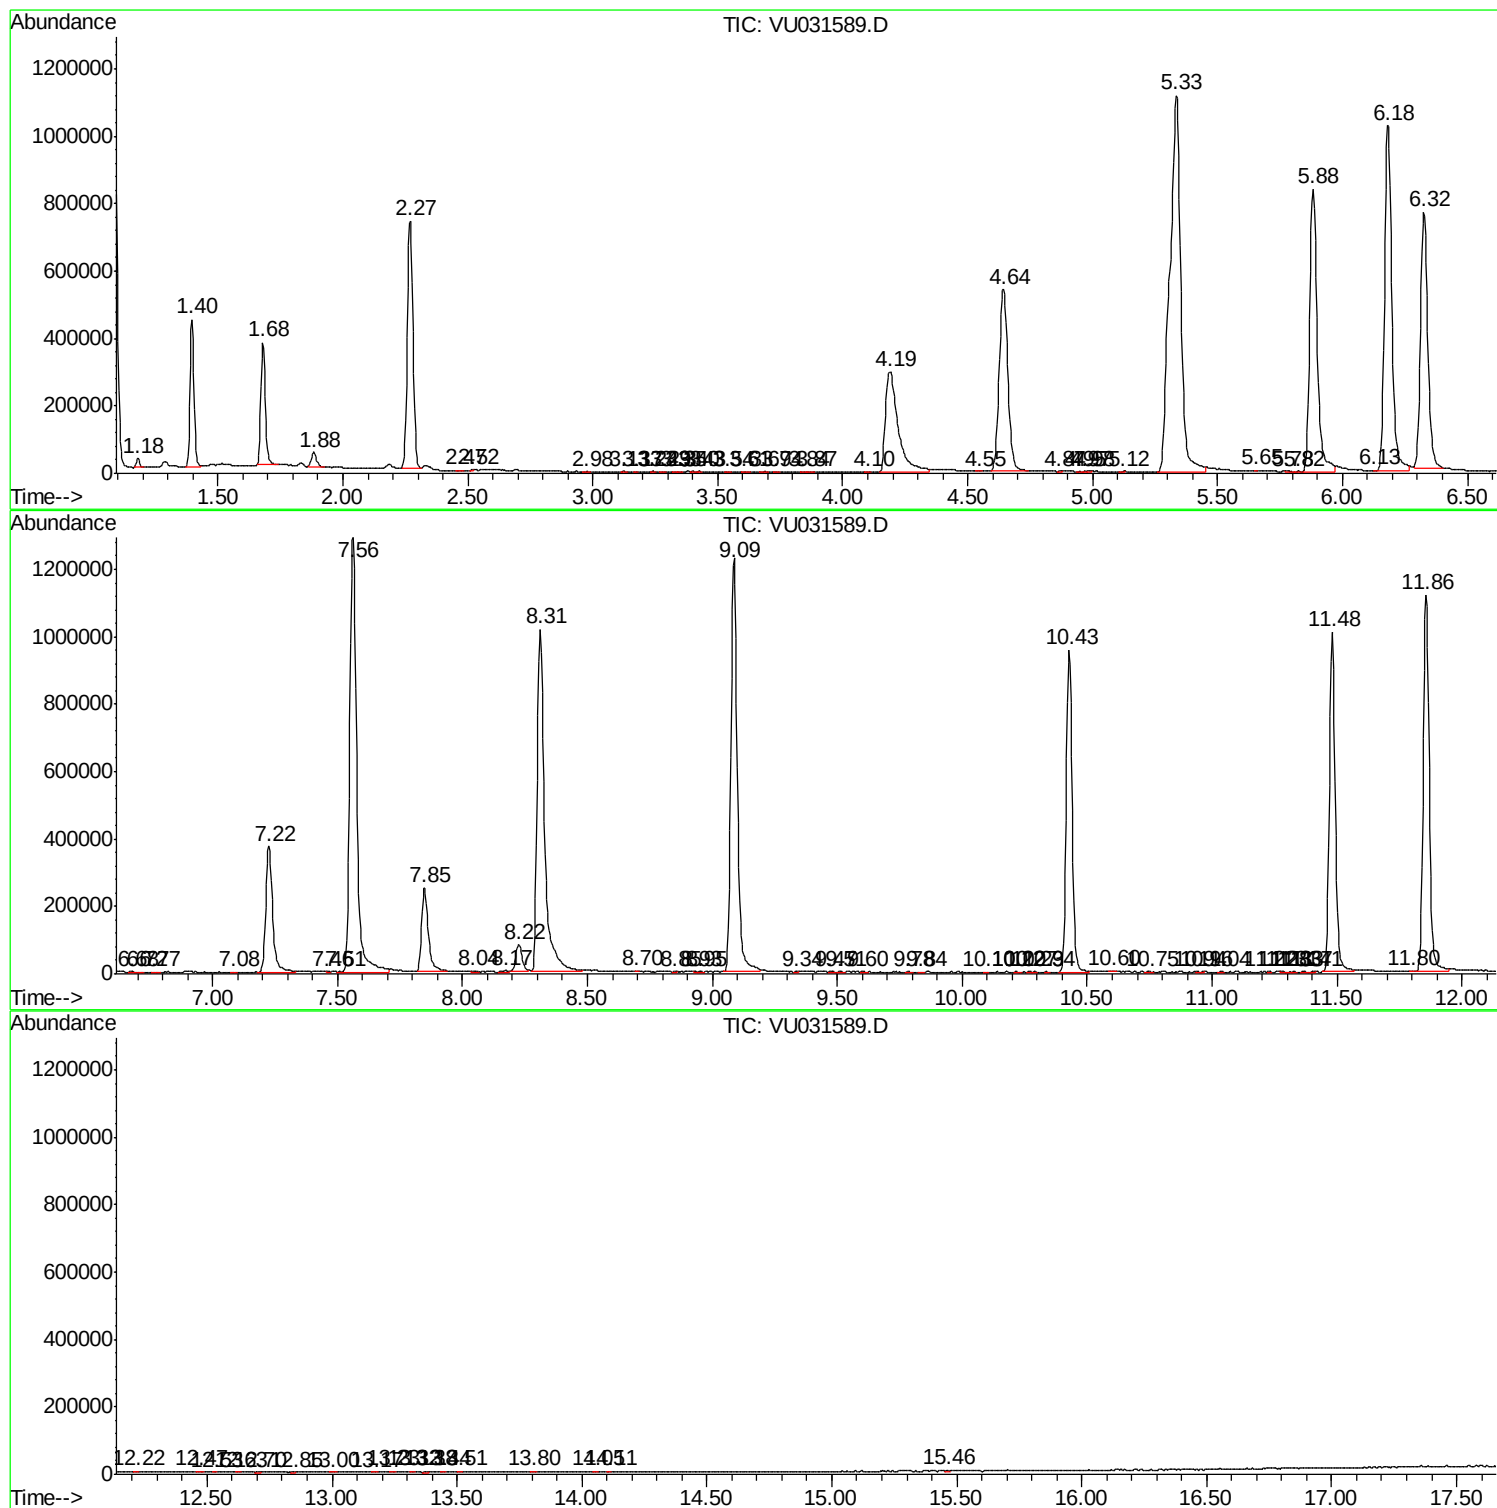

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042919\
Data File : VU031589.D
Acq On : 29 Apr 2019 16:18
Operator : JC/SP
Sample : K2536-21DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X09DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042919\
Data File : VU031589.D
Acq On : 29 Apr 2019 16:18
Operator : JC/SP
Sample : K2536-21DL 5X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X09DL

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc