

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031590.D
 Acq On : 29 Apr 2019 16:41
 Operator : JC/SP
 Sample : K2536-22DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X10DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	23	28	35	rBV4	19990	20393	0.63%	0.081%
2	1.286	56	61	68	rBV3	20950	23930	0.73%	0.095%
3	1.395	88	95	109	rVB	422911	460658	14.15%	1.821%
4	1.678	176	183	196	rBV	348958	433359	13.31%	1.713%
5	1.881	241	246	254	rVB	39773	49191	1.51%	0.194%
6	2.267	356	366	379	rVB	713969	1097945	33.72%	4.340%
7	2.469	427	429	431	rBV3	1305	747	0.02%	0.003%
8	2.550	452	454	459	rBV4	1456	1034	0.03%	0.004%
9	2.701	492	501	510	rBV5	4746	7940	0.24%	0.031%
10	2.778	520	525	527	rVB5	1023	821	0.03%	0.003%
11	2.794	527	530	532	rBV2	1091	716	0.02%	0.003%
12	2.807	532	534	536	rVV3	1425	1035	0.03%	0.004%
13	2.836	536	543	553	rVB6	3739	7117	0.22%	0.028%
14	3.080	616	619	620	rBV2	1084	742	0.02%	0.003%
15	3.167	640	646	647	rBV4	917	845	0.03%	0.003%
16	3.180	647	650	652	rVV4	1444	853	0.03%	0.003%
17	3.251	668	672	673	rBV2	1114	715	0.02%	0.003%
18	3.292	678	685	686	rBV2	1263	1485	0.05%	0.006%
19	3.341	697	700	705	rVB3	1151	885	0.03%	0.003%
20	3.382	708	713	716	rBV4	1440	1538	0.05%	0.006%
21	3.640	790	793	797	rBV3	1136	917	0.03%	0.004%
22	3.759	826	830	833	rBV3	1141	1151	0.04%	0.005%
23	3.845	853	857	861	rVB2	1504	972	0.03%	0.004%
24	4.112	935	940	943	rVB	1341	1078	0.03%	0.004%
25	4.189	951	964	996	rBV2	281176	928639	28.52%	3.671%
26	4.643	1087	1105	1128	rVV	533830	1271208	39.04%	5.025%
27	4.820	1156	1160	1163	rBV4	1606	1584	0.05%	0.006%
28	4.871	1172	1176	1178	rBV3	1701	1494	0.05%	0.006%
29	4.987	1204	1212	1215	rBV7	2386	3484	0.11%	0.014%
30	5.096	1244	1246	1250	rBV2	1131	813	0.02%	0.003%
31	5.125	1253	1255	1259	rVB3	1188	770	0.02%	0.003%
32	5.160	1264	1266	1274	rVB5	1533	1806	0.06%	0.007%
33	5.199	1274	1278	1280	rBV3	1079	841	0.03%	0.003%
34	5.254	1292	1295	1297	rBV2	1034	743	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031590.D
 Acq On : 29 Apr 2019 16:41
 Operator : JC/SP
 Sample : K2536-22DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X10DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.334	1297	1320	1350	rBV2	1071356	3256395	100.00%	12.873%
36	5.881	1477	1490	1517	rBV	817410	1704492	52.34%	6.738%
37	6.183	1569	1584	1615	rBV	832274	1726944	53.03%	6.827%
38	6.324	1615	1628	1652	rVV	727915	1499858	46.06%	5.929%
39	6.617	1716	1719	1725	rVB4	968	873	0.03%	0.003%
40	6.717	1748	1750	1753	rVB3	1662	944	0.03%	0.004%
41	6.800	1774	1776	1784	rVB2	1285	1052	0.03%	0.004%
42	6.890	1798	1804	1806	rBV5	1645	1604	0.05%	0.006%
43	7.041	1845	1851	1856	rBV4	1892	2457	0.08%	0.010%
44	7.151	1882	1885	1891	rVB3	1197	1090	0.03%	0.004%
45	7.176	1891	1893	1896	rBV3	1270	948	0.03%	0.004%
46	7.225	1896	1908	1938	rBV	360875	691654	21.24%	2.734%
47	7.562	1999	2013	2041	rBV	1260352	2329947	71.55%	9.211%
48	7.848	2092	2102	2129	rBV2	240465	455240	13.98%	1.800%
49	8.080	2171	2174	2178	rBV5	1311	1135	0.03%	0.004%
50	8.170	2194	2202	2208	rBV6	4619	7144	0.22%	0.028%
51	8.225	2208	2219	2235	rVV	134544	235365	7.23%	0.930%
52	8.312	2235	2246	2281	rBV2	981439	1978526	60.76%	7.821%
53	8.758	2381	2385	2388	rBV3	1636	1465	0.04%	0.006%
54	8.775	2388	2390	2393	rVB4	1597	794	0.02%	0.003%
55	8.797	2394	2397	2400	rVV3	1464	786	0.02%	0.003%
56	8.836	2406	2409	2411	rBV3	1111	784	0.02%	0.003%
57	8.906	2427	2431	2435	rVV6	1370	1214	0.04%	0.005%
58	9.086	2474	2487	2514	rBV	1194311	2124169	65.23%	8.397%
59	9.360	2570	2572	2575	rVB3	1603	776	0.02%	0.003%
60	9.649	2658	2662	2664	rBV3	2009	1398	0.04%	0.006%
61	9.662	2664	2666	2672	rVV5	1504	1488	0.05%	0.006%
62	9.910	2740	2743	2748	rVB4	884	765	0.02%	0.003%
63	9.938	2748	2752	2759	rBV3	1468	1588	0.05%	0.006%
64	9.971	2759	2762	2766	rBV3	1231	951	0.03%	0.004%
65	10.218	2835	2839	2846	rBV7	976	1423	0.04%	0.006%
66	10.257	2849	2851	2858	rVB3	1701	1317	0.04%	0.005%
67	10.427	2887	2904	2927	rBV	937992	1525567	46.85%	6.031%
68	10.594	2949	2956	2957	rBV5	2856	2825	0.09%	0.011%
69	10.643	2968	2971	2975	rBV3	1332	729	0.02%	0.003%
70	10.713	2991	2993	2999	rVB5	1014	930	0.03%	0.004%
71	10.742	2999	3002	3004	rBV2	1331	830	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031590.D
 Acq On : 29 Apr 2019 16:41
 Operator : JC/SP
 Sample : K2536-22DL 10X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X10DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.810	3019	3023	3024	rBV3	1582	1135	0.03%	0.004%
73	10.868	3034	3041	3044	rBV3	1447	1767	0.05%	0.007%
74	10.887	3044	3047	3050	rBV4	999	929	0.03%	0.004%
75	10.951	3065	3067	3072	rVB2	1241	789	0.02%	0.003%
76	10.977	3072	3075	3077	rBV2	1324	890	0.03%	0.004%
77	11.080	3101	3107	3109	rBV3	1446	1234	0.04%	0.005%
78	11.154	3126	3130	3133	rBV2	1145	1065	0.03%	0.004%
79	11.231	3150	3154	3158	rVB4	1355	1130	0.03%	0.004%
80	11.254	3158	3161	3164	rBV3	1780	1187	0.04%	0.005%
81	11.295	3172	3174	3179	rVB3	1329	1009	0.03%	0.004%
82	11.347	3186	3190	3195	rBV3	1028	929	0.03%	0.004%
83	11.482	3218	3232	3255	rBV	954229	1589399	48.81%	6.283%
84	11.855	3336	3348	3371	rBV	1066984	1783459	54.77%	7.050%
85	12.112	3426	3428	3431	rVB4	1762	874	0.03%	0.003%
86	12.308	3486	3489	3490	rBV3	1238	747	0.02%	0.003%
87	12.440	3527	3530	3533	rVB4	1209	784	0.02%	0.003%
88	12.462	3534	3537	3539	rBV2	1771	1325	0.04%	0.005%
89	12.514	3550	3553	3556	rBV3	1165	1031	0.03%	0.004%
90	12.630	3585	3589	3592	rBV4	1680	1544	0.05%	0.006%
91	12.704	3608	3612	3615	rBV3	1668	1588	0.05%	0.006%
92	12.794	3636	3640	3645	rVB3	1982	1865	0.06%	0.007%
93	13.286	3790	3793	3796	rBV2	1281	1063	0.03%	0.004%
94	13.382	3820	3823	3826	rBV2	1564	965	0.03%	0.004%
95	13.501	3857	3860	3863	rBV2	1625	1093	0.03%	0.004%
96	13.778	3942	3946	3948	rBV3	1480	1280	0.04%	0.005%
97	13.835	3961	3964	3966	rBV2	1200	776	0.02%	0.003%
98	14.105	4045	4048	4055	rBV5	1403	1321	0.04%	0.005%
99	14.212	4077	4081	4085	rBV3	1804	1779	0.05%	0.007%
100	14.925	4301	4303	4304	rBV2	1654	719	0.02%	0.003%


Sum of corrected areas: 25296592

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042919\
Data File : VU031590.D
Acq On : 29 Apr 2019 16:41
Operator : JC/SP
Sample : K2536-22DL 10X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X10DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

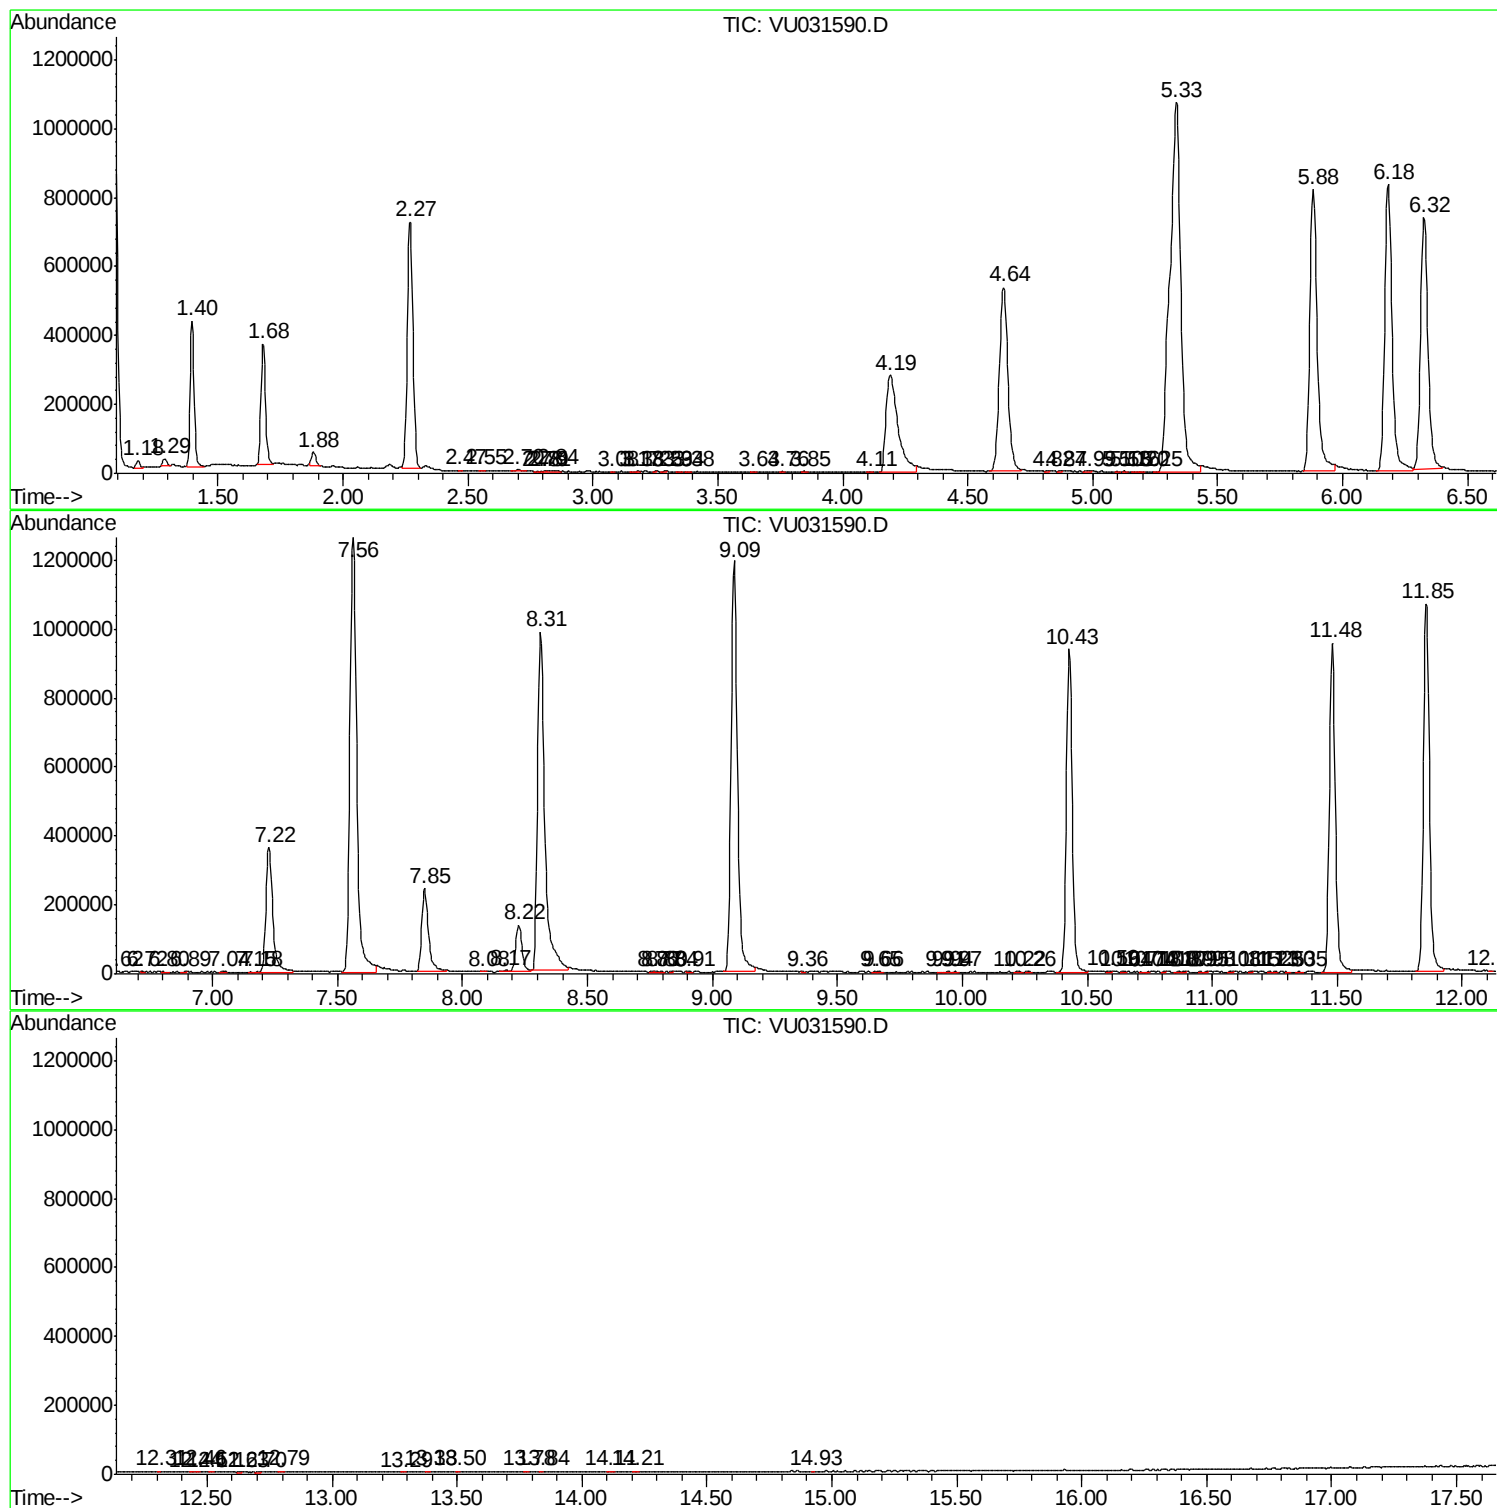

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042919\
Data File : VU031590.D
Acq On : 29 Apr 2019 16:41
Operator : JC/SP
Sample : K2536-22DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X10DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042919\
Data File : VU031590.D
Acq On : 29 Apr 2019 16:41
Operator : JC/SP
Sample : K2536-22DL 10X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X10DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc