

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031592.D
 Acq On : 29 Apr 2019 17:28
 Operator : JC/SP
 Sample : K2592-05 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0WZ6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	38	rVB2	17022	16061	0.53%	0.070%
2	1.395	88	95	109	rBV	373909	409496	13.49%	1.788%
3	1.678	176	183	196	rVB	334804	406967	13.41%	1.777%
4	2.267	356	366	381	rVB	649694	991077	32.65%	4.327%
5	2.466	426	428	431	rBV2	1260	847	0.03%	0.004%
6	2.559	454	457	465	rBV8	1807	2336	0.08%	0.010%
7	2.698	495	500	501	rBV3	3132	2658	0.09%	0.012%
8	2.762	517	520	523	rBV3	1177	842	0.03%	0.004%
9	2.794	527	530	535	rVV4	1044	891	0.03%	0.004%
10	2.932	570	573	576	rBV2	1035	801	0.03%	0.003%
11	3.617	784	786	790	rVV2	1021	800	0.03%	0.003%
12	3.665	798	801	806	rVB3	1305	1080	0.04%	0.005%
13	3.714	813	816	818	rBV2	1169	773	0.03%	0.003%
14	3.778	834	836	840	rVB	1130	751	0.02%	0.003%
15	3.813	843	847	854	rBV5	1286	1306	0.04%	0.006%
16	3.849	854	858	861	rBV2	1080	793	0.03%	0.003%
17	3.884	865	869	870	rBV2	1718	1195	0.04%	0.005%
18	3.919	877	880	883	rBV2	940	743	0.02%	0.003%
19	3.968	892	895	897	rBV2	1310	888	0.03%	0.004%
20	4.045	914	919	921	rBV2	1328	1138	0.04%	0.005%
21	4.190	951	964	1005	rBV	286727	956523	31.51%	4.177%
22	4.643	1086	1105	1128	rBV	500772	1206205	39.73%	5.267%
23	4.813	1154	1158	1162	rBV4	944	923	0.03%	0.004%
24	4.977	1207	1209	1213	rBV3	970	748	0.02%	0.003%
25	5.042	1226	1229	1233	rBV4	1085	788	0.03%	0.003%
26	5.199	1274	1278	1280	rBV2	917	793	0.03%	0.003%
27	5.334	1295	1320	1348	rBV2	996908	3035657	100.00%	13.255%
28	5.543	1383	1385	1388	rBV3	1656	1067	0.04%	0.005%
29	5.759	1446	1452	1455	rBV5	1418	1529	0.05%	0.007%
30	5.784	1457	1460	1463	rBV3	2023	1504	0.05%	0.007%
31	5.881	1477	1490	1528	rBV	820839	1722023	56.73%	7.519%
32	6.071	1547	1549	1556	rVB7	2395	2381	0.08%	0.010%
33	6.183	1571	1584	1614	rBV2	275732	584178	19.24%	2.551%
34	6.325	1615	1628	1651	rVV	677592	1393121	45.89%	6.083%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031592.D
 Acq On : 29 Apr 2019 17:28
 Operator : JC/SP
 Sample : K2592-05 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0WZ6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	6.678	1735	1738	1741	rBV3	1621	825	0.03%	0.004%
36	6.736	1751	1756	1758	rBV3	1313	976	0.03%	0.004%
37	6.765	1763	1765	1771	rBV3	1190	1173	0.04%	0.005%
38	6.884	1796	1802	1804	rBV6	1335	1439	0.05%	0.006%
39	6.968	1826	1828	1832	rBV	1208	840	0.03%	0.004%
40	7.051	1850	1854	1859	rVB5	2036	1762	0.06%	0.008%
41	7.074	1859	1861	1866	rBV3	1411	927	0.03%	0.004%
42	7.103	1866	1870	1876	rBV4	819	1000	0.03%	0.004%
43	7.180	1889	1894	1896	rBV3	1119	875	0.03%	0.004%
44	7.225	1896	1908	1941	rVV	340308	646128	21.28%	2.821%
45	7.424	1965	1970	1971	rBV3	1145	1102	0.04%	0.005%
46	7.562	1996	2013	2044	rBV	1144491	2135701	70.35%	9.325%
47	7.849	2090	2102	2127	rBV	227444	431188	14.20%	1.883%
48	7.971	2137	2140	2142	rBV3	2040	1114	0.04%	0.005%
49	8.096	2174	2179	2182	rBV4	744	788	0.03%	0.003%
50	8.177	2196	2204	2206	rBV6	3713	4272	0.14%	0.019%
51	8.228	2210	2220	2232	rBV4	20969	38540	1.27%	0.168%
52	8.312	2235	2246	2285	rBV2	971749	1997751	65.81%	8.723%
53	8.768	2384	2388	2394	rVB6	1673	1716	0.06%	0.007%
54	9.086	2474	2487	2511	rBV	1209289	2110801	69.53%	9.217%
55	9.286	2546	2549	2552	rBV4	921	757	0.02%	0.003%
56	9.476	2606	2608	2610	rVV2	1720	936	0.03%	0.004%
57	9.508	2614	2618	2623	rBV5	1535	1558	0.05%	0.007%
58	9.556	2628	2633	2637	rBV8	1492	1670	0.06%	0.007%
59	9.582	2637	2641	2643	rBV2	1370	1052	0.03%	0.005%
60	9.595	2643	2645	2649	rVB4	1524	1164	0.04%	0.005%
61	9.623	2649	2654	2659	rBV7	1372	1224	0.04%	0.005%
62	9.643	2659	2660	2664	rVB3	1722	995	0.03%	0.004%
63	9.668	2664	2668	2671	rBV3	1510	1469	0.05%	0.006%
64	9.691	2673	2675	2679	rBV2	960	891	0.03%	0.004%
65	9.813	2709	2713	2714	rBV	1693	1170	0.04%	0.005%
66	9.871	2728	2731	2737	rVB5	1622	1248	0.04%	0.005%
67	9.951	2753	2756	2758	rBV2	1407	863	0.03%	0.004%
68	9.977	2762	2764	2768	rVB3	1241	750	0.02%	0.003%
69	10.022	2771	2778	2781	rBV4	1574	1814	0.06%	0.008%
70	10.109	2802	2805	2810	rBV4	1110	814	0.03%	0.004%
71	10.160	2816	2821	2826	rBV4	1380	1181	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031592.D
 Acq On : 29 Apr 2019 17:28
 Operator : JC/SP
 Sample : K2592-05 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0WZ6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.199	2829	2833	2836	rBV4	878	765	0.03%	0.003%
73	10.334	2871	2875	2878	rBV3	1417	1075	0.04%	0.005%
74	10.427	2890	2904	2924	rBV	905173	1468079	48.36%	6.410%
75	10.585	2949	2953	2957	rBV5	2018	2053	0.07%	0.009%
76	10.604	2957	2959	2964	rVB3	1925	1628	0.05%	0.007%
77	11.016	3084	3087	3093	rVB4	1571	1462	0.05%	0.006%
78	11.051	3094	3098	3104	rBV5	1674	1940	0.06%	0.008%
79	11.160	3130	3132	3137	rVB3	1308	1069	0.04%	0.005%
80	11.199	3137	3144	3147	rVB3	1287	1429	0.05%	0.006%
81	11.228	3147	3153	3154	rBV2	1111	1039	0.03%	0.005%
82	11.344	3185	3189	3192	rBV3	1597	1405	0.05%	0.006%
83	11.479	3219	3231	3255	rBV	945311	1584470	52.20%	6.918%
84	11.855	3336	3348	3370	rBV	986228	1669267	54.99%	7.289%
85	12.221	3459	3462	3464	rBV4	1863	1232	0.04%	0.005%
86	12.469	3537	3539	3540	rBV2	2367	1129	0.04%	0.005%
87	12.527	3553	3557	3559	rVB3	1071	740	0.02%	0.003%
88	12.588	3573	3576	3587	rBV5	1704	2257	0.07%	0.010%
89	12.713	3612	3615	3618	rBV3	1779	1299	0.04%	0.006%
90	12.832	3650	3652	3656	rVB2	1537	810	0.03%	0.004%
91	12.906	3672	3675	3679	rVB5	1469	1030	0.03%	0.004%
92	13.057	3720	3722	3726	rVB2	1371	926	0.03%	0.004%
93	13.154	3748	3752	3755	rBV2	1939	1633	0.05%	0.007%
94	13.273	3786	3789	3793	rBV3	1665	1259	0.04%	0.005%
95	13.305	3796	3799	3803	rBV3	1723	1396	0.05%	0.006%
96	13.450	3840	3844	3846	rVB2	2274	1331	0.04%	0.006%
97	13.717	3925	3927	3929	rBV2	1571	903	0.03%	0.004%
98	13.755	3936	3939	3942	rVB2	1715	1082	0.04%	0.005%
99	14.189	4072	4074	4080	rVB2	1567	1316	0.04%	0.006%
100	14.221	4082	4084	4088	rVV2	1445	919	0.03%	0.004%


Sum of corrected areas: 22902300

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042919\
Data File : VU031592.D
Acq On : 29 Apr 2019 17:28
Operator : JC/SP
Sample : K2592-05 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
COWZ6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

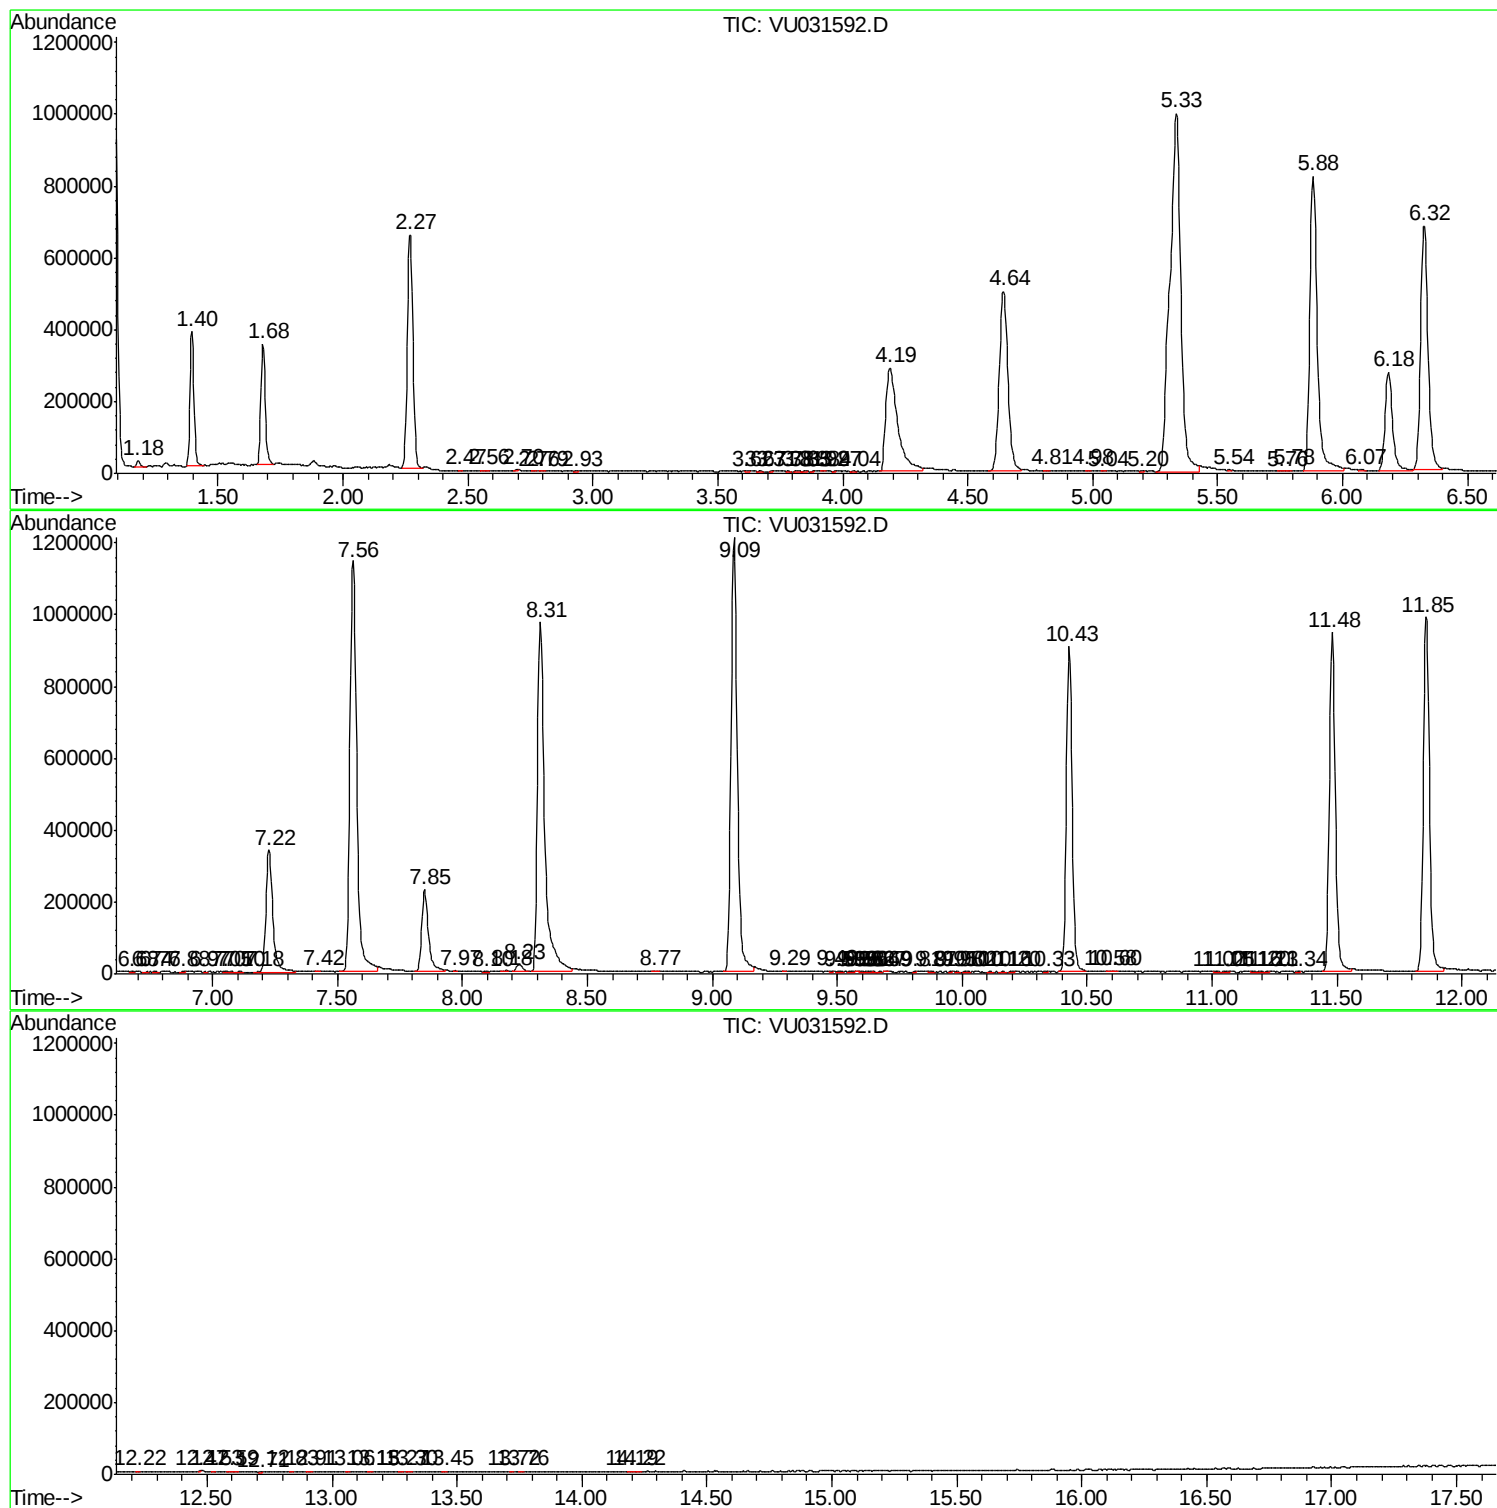

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042919\
Data File : VU031592.D
Acq On : 29 Apr 2019 17:28
Operator : JC/SP
Sample : K2592-05 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0WZ6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042919\
Data File : VU031592.D
Acq On : 29 Apr 2019 17:28
Operator : JC/SP
Sample : K2592-05 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0WZ6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc