

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031593.D
 Acq On : 29 Apr 2019 17:51
 Operator : JC/SP
 Sample : K2592-14DL 2500X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X77DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	40	rVB	15766	15724	0.51%	0.063%
2	1.289	59	62	67	rBV2	11783	9745	0.32%	0.039%
3	1.395	88	95	112	rVB	387928	415628	13.55%	1.677%
4	1.678	176	183	200	rVB	336873	412138	13.43%	1.663%
5	2.270	356	367	380	rVB	649381	999511	32.58%	4.034%
6	2.415	410	412	419	rVB4	2301	2110	0.07%	0.009%
7	2.698	496	500	511	rVV10	3940	6059	0.20%	0.024%
8	2.743	512	514	518	rVB3	1120	725	0.02%	0.003%
9	2.775	520	524	527	rBV2	1173	785	0.03%	0.003%
10	2.968	581	584	588	rVB2	1002	739	0.02%	0.003%
11	2.993	588	592	595	rBV3	971	1143	0.04%	0.005%
12	3.013	595	598	601	rVB4	1540	1073	0.03%	0.004%
13	3.209	655	659	662	rBV3	634	682	0.02%	0.003%
14	3.228	662	665	668	rVB	1714	935	0.03%	0.004%
15	3.251	668	672	679	rBV4	1092	1409	0.05%	0.006%
16	3.299	685	687	690	rVB3	1041	642	0.02%	0.003%
17	3.379	707	712	715	rBV6	973	1049	0.03%	0.004%
18	3.421	721	725	726	rBV3	1024	670	0.02%	0.003%
19	3.489	742	746	753	rBV3	1339	1237	0.04%	0.005%
20	3.524	753	757	764	rBV4	1069	1347	0.04%	0.005%
21	3.620	782	787	792	rVB3	889	747	0.02%	0.003%
22	3.720	812	818	821	rBV4	1249	1502	0.05%	0.006%
23	3.736	821	823	826	rVB2	1125	667	0.02%	0.003%
24	3.752	826	828	832	rVB4	1109	779	0.03%	0.003%
25	3.775	832	835	838	rBV2	1927	1481	0.05%	0.006%
26	3.820	846	849	853	rVB2	1121	869	0.03%	0.004%
27	3.842	853	856	860	rVB2	1178	652	0.02%	0.003%
28	3.865	860	863	865	rBV4	1339	813	0.03%	0.003%
29	3.884	866	869	872	rBV2	1217	810	0.03%	0.003%
30	3.916	876	879	884	rBV3	953	885	0.03%	0.004%
31	3.958	887	892	893	rBV2	1033	918	0.03%	0.004%
32	4.000	902	905	907	rBV	1150	692	0.02%	0.003%
33	4.186	950	963	996	rBV	307412	955515	31.14%	3.856%
34	4.530	1067	1070	1076	rBV5	1166	1243	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\U042919\
 Data File : VU031593.D
 Acq On : 29 Apr 2019 17:51
 Operator : JC/SP
 Sample : K2592-14DL 2500X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X77DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	4.643	1088	1105	1135	rBV	508603	1218784	39.73%	4.919%
36	4.929	1191	1194	1198	rVB3	1511	1407	0.05%	0.006%
37	5.096	1243	1246	1249	rVB3	1013	704	0.02%	0.003%
38	5.167	1263	1268	1270	rBV3	1005	860	0.03%	0.003%
39	5.186	1270	1274	1276	rBV3	1104	907	0.03%	0.004%
40	5.334	1297	1320	1344	rBV2	1015936	3068038	100.00%	12.382%
41	5.749	1447	1449	1453	rBV6	1298	1161	0.04%	0.005%
42	5.884	1476	1491	1525	rBV	814076	1716122	55.94%	6.926%
43	6.183	1570	1584	1611	rBV	1049792	2112042	68.84%	8.524%
44	6.328	1616	1629	1652	rVB	694340	1433769	46.73%	5.787%
45	6.640	1723	1726	1730	rBV4	934	804	0.03%	0.003%
46	6.887	1799	1803	1806	rBV3	1257	1137	0.04%	0.005%
47	6.910	1806	1810	1812	rVV5	1369	1041	0.03%	0.004%
48	7.054	1853	1855	1861	rVB5	1554	943	0.03%	0.004%
49	7.225	1896	1908	1931	rBV	342063	651345	21.23%	2.629%
50	7.562	2000	2013	2048	rBV	1171467	2178925	71.02%	8.794%
51	7.848	2092	2102	2125	rBV	230282	425229	13.86%	1.716%
52	8.032	2157	2159	2167	rVB7	2334	1887	0.06%	0.008%
53	8.170	2200	2202	2206	rBV4	1468	989	0.03%	0.004%
54	8.228	2211	2220	2234	rVB3	34459	60716	1.98%	0.245%
55	8.312	2234	2246	2290	rBV	1018232	2042961	66.59%	8.245%
56	8.729	2373	2376	2378	rBV2	1002	734	0.02%	0.003%
57	8.794	2393	2396	2399	rBV3	1472	1217	0.04%	0.005%
58	8.832	2405	2408	2410	rBV2	1128	729	0.02%	0.003%
59	9.086	2472	2487	2530	rBV	1212256	2135363	69.60%	8.618%
60	9.356	2569	2571	2575	rBV3	800	676	0.02%	0.003%
61	9.398	2581	2584	2588	rBV6	1514	1120	0.04%	0.005%
62	9.447	2596	2599	2601	rBV3	1203	732	0.02%	0.003%
63	9.537	2625	2627	2632	rBV2	942	766	0.02%	0.003%
64	9.601	2645	2647	2652	rVB5	1275	980	0.03%	0.004%
65	9.639	2652	2659	2661	rBV4	1484	1397	0.05%	0.006%
66	9.694	2673	2676	2681	rBV8	795	846	0.03%	0.003%
67	9.758	2692	2696	2698	rBV2	769	690	0.02%	0.003%
68	9.903	2735	2741	2743	rBV3	1024	1183	0.04%	0.005%
69	9.993	2765	2769	2773	rVB5	1910	1539	0.05%	0.006%
70	10.019	2773	2777	2780	rBV4	1603	1447	0.05%	0.006%
71	10.070	2790	2793	2796	rBV2	1129	921	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031593.D
 Acq On : 29 Apr 2019 17:51
 Operator : JC/SP
 Sample : K2592-14DL 2500X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X77DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.128	2807	2811	2816	rBV4	1779	1983	0.06%	0.008%
73	10.292	2858	2862	2864	rBV2	1052	804	0.03%	0.003%
74	10.363	2881	2884	2889	rVB3	1322	1129	0.04%	0.005%
75	10.427	2889	2904	2934	rBV	936173	1529917	49.87%	6.175%
76	10.643	2968	2971	2973	rBV3	1322	903	0.03%	0.004%
77	10.729	2995	2998	3000	rBV2	1569	880	0.03%	0.004%
78	10.746	3001	3003	3009	rVB4	1287	1141	0.04%	0.005%
79	11.003	3079	3083	3085	rBV3	1480	1242	0.04%	0.005%
80	11.154	3127	3130	3134	rVB4	1052	918	0.03%	0.004%
81	11.286	3167	3171	3172	rBV	1468	1079	0.04%	0.004%
82	11.401	3204	3207	3210	rBV2	929	659	0.02%	0.003%
83	11.482	3218	3232	3252	rBV	958732	1586091	51.70%	6.401%
84	11.768	3319	3321	3323	rBV2	1537	919	0.03%	0.004%
85	11.855	3336	3348	3368	rBV	1004133	1716142	55.94%	6.926%
86	12.266	3474	3476	3480	rBV3	1275	882	0.03%	0.004%
87	12.434	3522	3528	3530	rBV5	1240	1228	0.04%	0.005%
88	12.688	3605	3607	3612	rVV4	1476	1130	0.04%	0.005%
89	12.739	3618	3623	3624	rBV4	1343	1143	0.04%	0.005%
90	12.778	3631	3635	3640	rBV6	1359	1800	0.06%	0.007%
91	12.964	3690	3693	3694	rBV2	1949	1084	0.04%	0.004%
92	13.073	3723	3727	3730	rBV2	1387	1334	0.04%	0.005%
93	13.430	3834	3838	3840	rBV3	1415	1373	0.04%	0.006%
94	13.462	3845	3848	3855	rVV2	2534	2857	0.09%	0.012%
95	13.594	3887	3889	3892	rBV	1558	1078	0.04%	0.004%
96	13.842	3961	3966	3968	rBV3	2442	2151	0.07%	0.009%
97	14.340	4116	4121	4123	rBV3	2055	2197	0.07%	0.009%
98	14.662	4219	4221	4229	rBV4	2004	1990	0.06%	0.008%
99	14.861	4280	4283	4285	rBV	1600	1019	0.03%	0.004%
100	14.919	4299	4301	4306	rBV3	1587	1267	0.04%	0.005%


Sum of corrected areas: 24777375

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042919\
Data File : VU031593.D
Acq On : 29 Apr 2019 17:51
Operator : JC/SP
Sample : K2592-14DL 2500X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X77DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

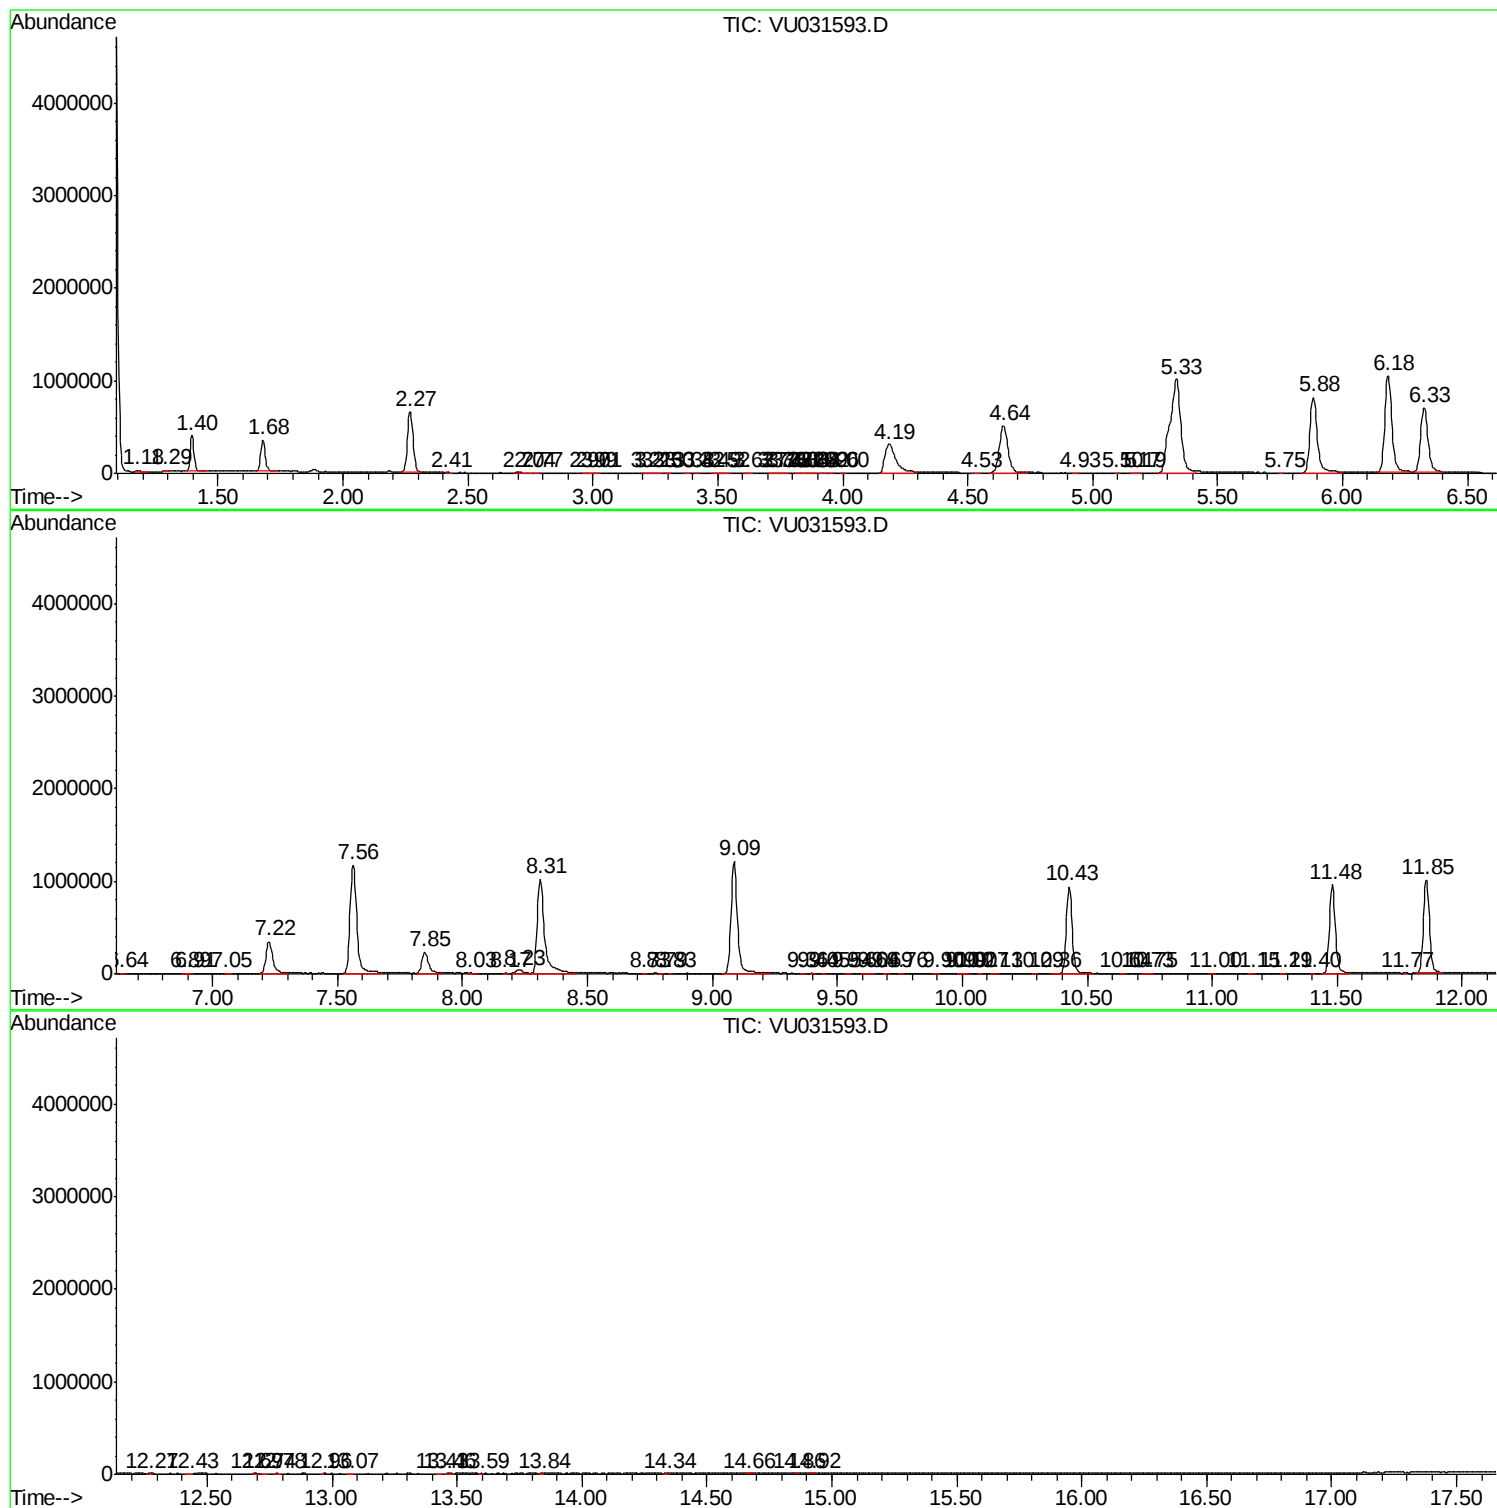

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042919\
Data File : VU031593.D
Acq On : 29 Apr 2019 17:51
Operator : JC/SP
Sample : K2592-14DL 2500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X77DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU042919\
Data File : VU031593.D
Acq On : 29 Apr 2019 17:51
Operator : JC/SP
Sample : K2592-14DL 2500X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
C0X77DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc