

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031606.D
 Acq On : 29 Apr 2019 23:40
 Operator : JC/SP
 Sample : K2592-09DL 250X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X02DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	34	rVB2	16229	14409	0.46%	0.060%
2	1.395	88	95	110	rBV	491273	532120	16.85%	2.218%
3	1.678	176	183	202	rVB	369472	457840	14.50%	1.908%
4	2.270	356	367	381	rVB	764938	1167306	36.96%	4.866%
5	2.469	425	429	432	rBV5	2375	2181	0.07%	0.009%
6	2.608	469	472	477	rBV6	1125	1026	0.03%	0.004%
7	2.694	492	499	513	rVB7	3931	6799	0.22%	0.028%
8	3.000	591	594	598	rVB4	1747	1206	0.04%	0.005%
9	3.071	613	616	622	rVB4	1244	1121	0.04%	0.005%
10	3.141	634	638	644	rBV2	1519	1416	0.04%	0.006%
11	3.186	649	652	654	rBV	1291	872	0.03%	0.004%
12	3.244	667	670	673	rVB3	1487	869	0.03%	0.004%
13	3.421	719	725	727	rBV3	1037	1009	0.03%	0.004%
14	3.469	737	740	744	rVB2	1327	843	0.03%	0.004%
15	3.553	762	766	769	rBV	955	867	0.03%	0.004%
16	3.588	773	777	782	rVB4	1477	1469	0.05%	0.006%
17	3.640	790	793	797	rBV	1029	896	0.03%	0.004%
18	3.694	804	810	813	rBV4	1198	1488	0.05%	0.006%
19	3.891	865	871	878	rBV4	1073	1850	0.06%	0.008%
20	3.977	894	898	902	rVB3	1536	1140	0.04%	0.005%
21	4.119	939	942	945	rBV	1209	916	0.03%	0.004%
22	4.183	950	962	996	rBV	281994	843773	26.72%	3.517%
23	4.643	1087	1105	1135	rVV	502480	1212463	38.39%	5.054%
24	4.881	1174	1179	1182	rBV5	1919	2320	0.07%	0.010%
25	4.945	1196	1199	1203	rVB2	1474	1124	0.04%	0.005%
26	4.987	1206	1212	1216	rBV5	2610	2733	0.09%	0.011%
27	5.035	1222	1227	1230	rBV3	1490	1491	0.05%	0.006%
28	5.334	1297	1320	1355	rBV2	1033969	3158415	100.00%	13.165%
29	5.588	1396	1399	1402	rVB4	2137	1237	0.04%	0.005%
30	5.688	1428	1430	1434	rVB3	2345	1644	0.05%	0.007%
31	5.881	1476	1490	1524	rBV	777727	1654990	52.40%	6.898%
32	6.183	1569	1584	1605	rBV2	801261	1618283	51.24%	6.745%
33	6.325	1616	1628	1653	rVB	697566	1423396	45.07%	5.933%
34	6.579	1704	1707	1712	rBV4	1760	1257	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031606.D
 Acq On : 29 Apr 2019 23:40
 Operator : JC/SP
 Sample : K2592-09DL 250X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X02DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	6.617	1716	1719	1720	rBV3	1400	830	0.03%	0.003%
36	6.646	1725	1728	1734	rVB4	1202	1293	0.04%	0.005%
37	6.691	1739	1742	1748	rBV6	1128	904	0.03%	0.004%
38	6.807	1774	1778	1780	rBV2	1102	889	0.03%	0.004%
39	6.887	1800	1803	1808	rVB3	1456	983	0.03%	0.004%
40	6.964	1822	1827	1830	rBV4	1121	1233	0.04%	0.005%
41	6.980	1830	1832	1836	rVB3	1334	1010	0.03%	0.004%
42	7.003	1836	1839	1844	rBV4	829	940	0.03%	0.004%
43	7.058	1854	1856	1859	rBV3	1229	950	0.03%	0.004%
44	7.173	1884	1892	1895	rBV4	1463	1354	0.04%	0.006%
45	7.225	1895	1908	1935	rBV	337648	641480	20.31%	2.674%
46	7.505	1992	1995	1997	rVB2	1346	832	0.03%	0.003%
47	7.562	1997	2013	2048	rBV	1207975	2257904	71.49%	9.411%
48	7.849	2091	2102	2125	rBV	226548	427090	13.52%	1.780%
49	8.058	2164	2167	2168	rBV3	1372	834	0.03%	0.003%
50	8.093	2173	2178	2182	rBV4	2004	1868	0.06%	0.008%
51	8.170	2199	2202	2207	rBV2	1530	1391	0.04%	0.006%
52	8.228	2210	2220	2231	rBV4	32179	55277	1.75%	0.230%
53	8.312	2235	2246	2292	rBV	903335	1842496	58.34%	7.680%
54	8.553	2318	2321	2325	rBV3	1985	1528	0.05%	0.006%
55	8.607	2335	2338	2345	rBV8	1277	1570	0.05%	0.007%
56	8.662	2353	2355	2361	rVB4	1632	1355	0.04%	0.006%
57	8.713	2368	2371	2374	rBV3	1312	1081	0.03%	0.005%
58	8.775	2388	2390	2395	rBV2	1047	977	0.03%	0.004%
59	8.800	2395	2398	2404	rVB4	1945	1638	0.05%	0.007%
60	8.845	2409	2412	2417	rBV6	1912	1480	0.05%	0.006%
61	8.874	2417	2421	2423	rBV2	1078	871	0.03%	0.004%
62	9.086	2473	2487	2515	rBV	1181237	2041725	64.64%	8.510%
63	9.283	2544	2548	2549	rBV3	1768	1221	0.04%	0.005%
64	9.566	2633	2636	2641	rVB4	1633	1229	0.04%	0.005%
65	9.623	2651	2654	2660	rVB5	1767	1720	0.05%	0.007%
66	9.704	2676	2679	2684	rVB4	1323	904	0.03%	0.004%
67	9.874	2726	2732	2736	rVB3	904	947	0.03%	0.004%
68	9.897	2736	2739	2741	rBV	1407	851	0.03%	0.004%
69	10.128	2808	2811	2813	rBV2	1455	869	0.03%	0.004%
70	10.148	2813	2817	2821	rVV3	1815	1404	0.04%	0.006%
71	10.228	2837	2842	2845	rBV4	1559	1278	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031606.D
 Acq On : 29 Apr 2019 23:40
 Operator : JC/SP
 Sample : K2592-09DL 250X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X02DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.305	2863	2866	2872	rVB4	1900	1392	0.04%	0.006%
73	10.340	2872	2877	2881	rBV4	1940	2003	0.06%	0.008%
74	10.427	2892	2904	2931	rBV	858794	1402601	44.41%	5.846%
75	10.601	2954	2958	2960	rBV4	2160	1693	0.05%	0.007%
76	10.681	2980	2983	2986	rBV2	1457	934	0.03%	0.004%
77	10.697	2986	2988	2992	rVB3	1677	1000	0.03%	0.004%
78	10.742	2999	3002	3006	rBV3	1432	1084	0.03%	0.005%
79	10.781	3010	3014	3015	rBV2	1251	848	0.03%	0.004%
80	10.852	3033	3036	3040	rVV3	1824	1189	0.04%	0.005%
81	10.893	3044	3049	3052	rBV5	1208	1190	0.04%	0.005%
82	11.048	3092	3097	3100	rBV4	1665	1980	0.06%	0.008%
83	11.077	3100	3106	3108	rBV3	1500	1622	0.05%	0.007%
84	11.170	3131	3135	3140	rBV3	1333	1369	0.04%	0.006%
85	11.360	3191	3194	3198	rBV	2381	1882	0.06%	0.008%
86	11.479	3220	3231	3251	rBV	902417	1483924	46.98%	6.185%
87	11.855	3336	3348	3375	rBV	952331	1644763	52.08%	6.856%
88	12.556	3564	3566	3568	rBV2	1851	968	0.03%	0.004%
89	12.636	3588	3591	3597	rVB4	1657	1712	0.05%	0.007%
90	12.845	3654	3656	3660	rBV2	1355	883	0.03%	0.004%
91	12.903	3669	3674	3677	rBV4	1780	1972	0.06%	0.008%
92	12.945	3683	3687	3691	rBV4	1717	1687	0.05%	0.007%
93	13.221	3770	3773	3776	rBV2	1483	1089	0.03%	0.005%
94	13.337	3806	3809	3814	rBV4	1418	1406	0.04%	0.006%
95	13.527	3865	3868	3875	rVB2	1796	1734	0.05%	0.007%
96	13.636	3899	3902	3904	rBV2	1352	903	0.03%	0.004%
97	14.305	4108	4110	4113	rBV2	1333	822	0.03%	0.003%
98	14.417	4141	4145	4151	rBV4	2264	2642	0.08%	0.011%
99	14.524	4175	4178	4180	rBV3	1780	1218	0.04%	0.005%
100	14.688	4225	4229	4231	rBV3	1983	1639	0.05%	0.007%


Sum of corrected areas: 23991124

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042919\
Data File : VU031606.D
Acq On : 29 Apr 2019 23:40
Operator : JC/SP
Sample : K2592-09DL 250X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X02DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

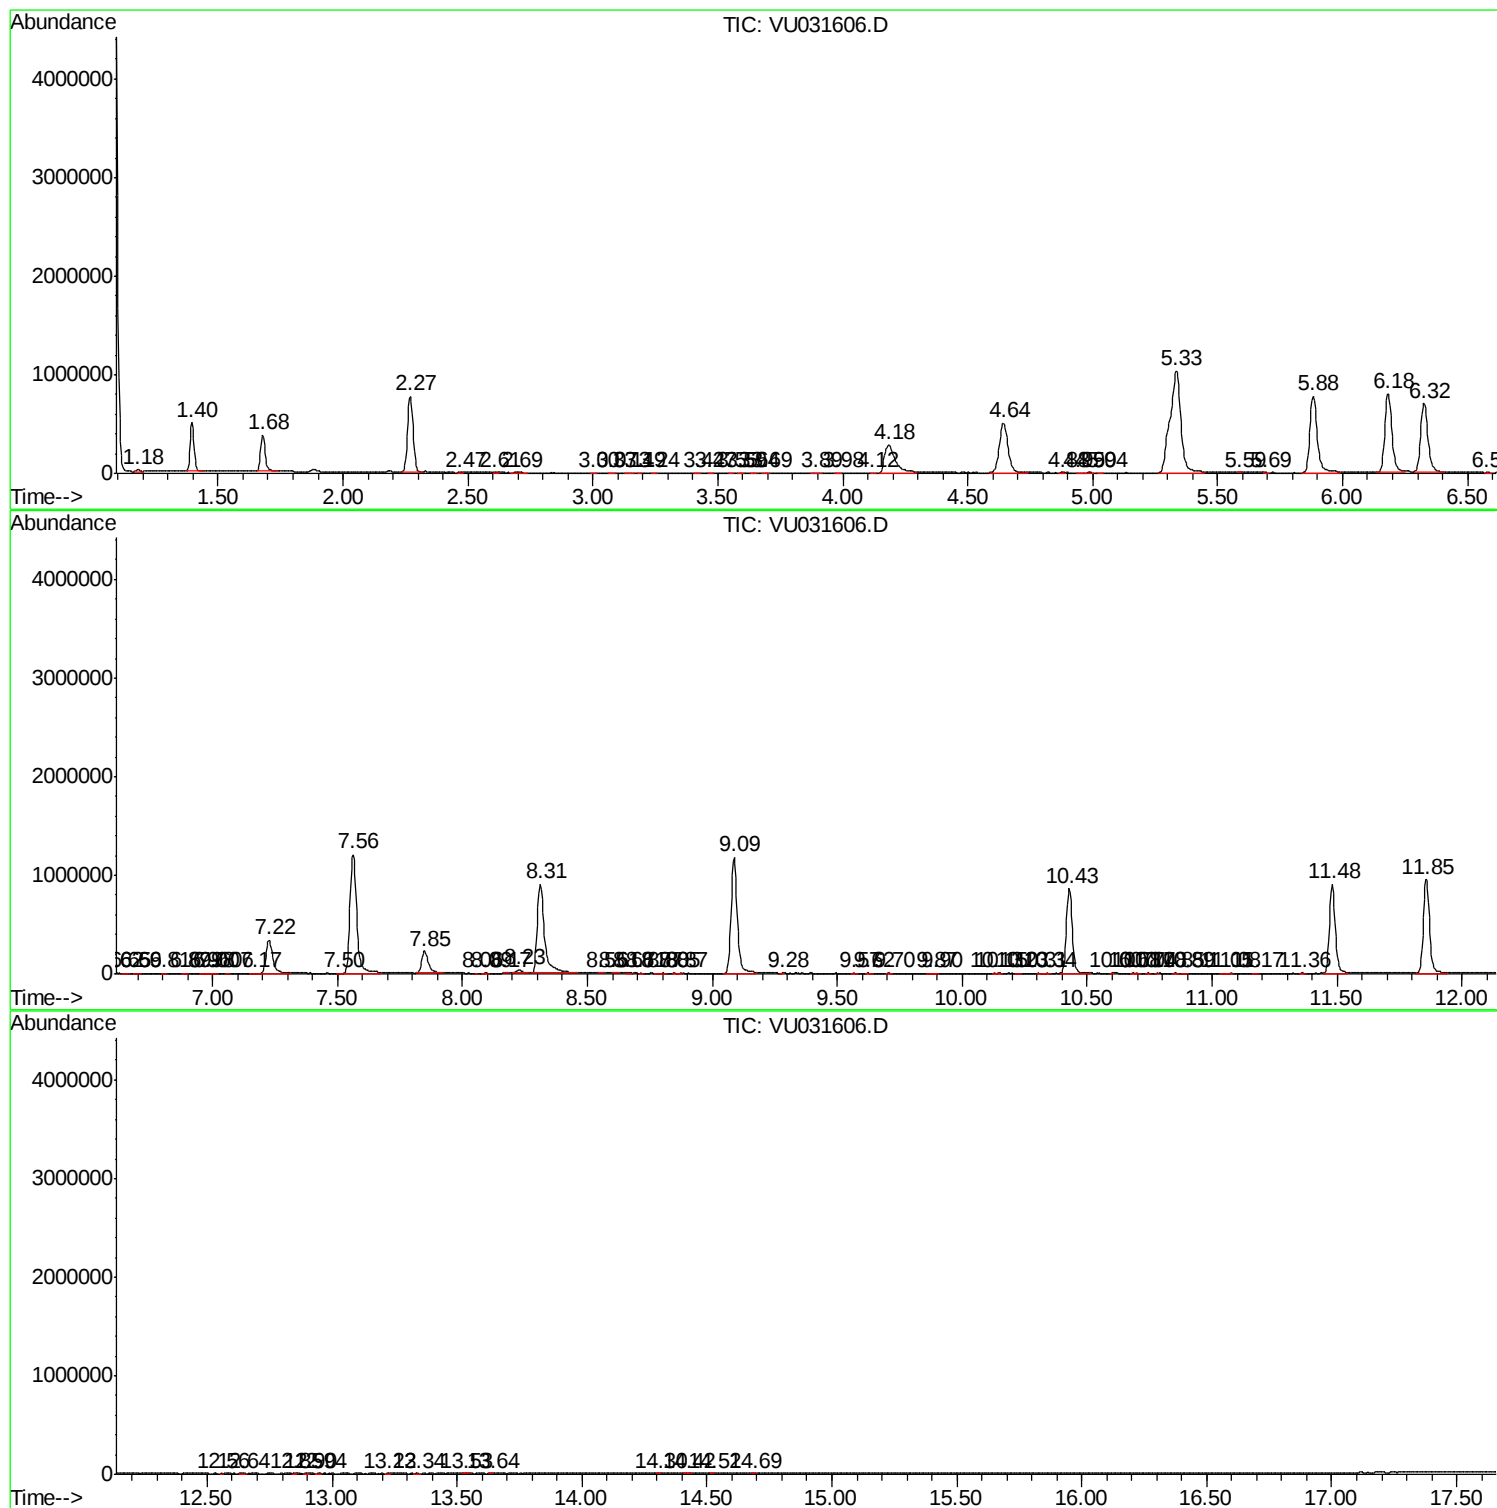

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042919\
Data File : VU031606.D
Acq On : 29 Apr 2019 23:40
Operator : JC/SP
Sample : K2592-09DL 250X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X02DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU042919\
Data File : VU031606.D
Acq On : 29 Apr 2019 23:40
Operator : JC/SP
Sample : K2592-09DL 250X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
C0X02DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc