

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031608.D
 Acq On : 30 Apr 2019 00:27
 Operator : JC/SP
 Sample : K2592-11DL 250X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X04DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	35	rBV3	15280	14041	0.44%	0.058%
2	1.396	88	95	108	rBV	493235	532987	16.79%	2.208%
3	1.678	176	183	200	rVB	361369	455185	14.34%	1.885%
4	2.270	356	367	381	rBV	759845	1162056	36.61%	4.813%
5	2.611	471	473	475	rBV2	1391	730	0.02%	0.003%
6	2.669	488	491	493	rBV3	1221	710	0.02%	0.003%
7	2.701	494	501	508	rVB8	2860	3997	0.13%	0.017%
8	2.778	523	525	530	rVB3	1313	941	0.03%	0.004%
9	2.904	562	564	568	rBV2	921	802	0.03%	0.003%
10	3.026	598	602	609	rBV5	1536	1957	0.06%	0.008%
11	3.093	619	623	629	rVB	1491	1576	0.05%	0.007%
12	3.186	647	652	659	rVB3	1558	2231	0.07%	0.009%
13	3.235	659	667	669	rBV	1936	2474	0.08%	0.010%
14	3.289	682	684	688	rVB2	1585	862	0.03%	0.004%
15	3.315	688	692	697	rVB3	1482	1040	0.03%	0.004%
16	3.347	697	702	704	rBV	824	746	0.02%	0.003%
17	3.379	710	712	717	rVB3	1127	759	0.02%	0.003%
18	3.453	733	735	739	rVB2	1105	675	0.02%	0.003%
19	3.505	745	751	756	rVB4	1185	1370	0.04%	0.006%
20	3.550	762	765	767	rBV2	1393	963	0.03%	0.004%
21	3.624	785	788	791	rBV	1287	775	0.02%	0.003%
22	3.788	833	839	844	rBV4	1280	1368	0.04%	0.006%
23	3.820	844	849	854	rBV4	987	1330	0.04%	0.006%
24	3.936	882	885	889	rVV3	923	725	0.02%	0.003%
25	3.977	896	898	902	rVB3	1024	735	0.02%	0.003%
26	4.000	902	905	910	rVB	1281	1008	0.03%	0.004%
27	4.084	924	931	934	rBV4	1028	1511	0.05%	0.006%
28	4.183	950	962	1004	rBV	275077	872618	27.49%	3.615%
29	4.563	1077	1080	1082	rVB4	1691	843	0.03%	0.003%
30	4.643	1082	1105	1138	rBV	507862	1235146	38.91%	5.116%
31	4.804	1153	1155	1160	rBV4	1258	1056	0.03%	0.004%
32	4.868	1171	1175	1177	rBV3	1819	1335	0.04%	0.006%
33	4.974	1206	1208	1211	rBV3	1058	739	0.02%	0.003%
34	5.222	1279	1285	1290	rBV4	1655	2084	0.07%	0.009%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031608.D
 Acq On : 30 Apr 2019 00:27
 Operator : JC/SP
 Sample : K2592-11DL 250X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X04DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.334	1297	1320	1350	rBV2	1037736	3174122	100.00%	13.148%
36	5.797	1460	1464	1469	rVB6	1662	1472	0.05%	0.006%
37	5.826	1469	1473	1476	rBV3	1380	1252	0.04%	0.005%
38	5.881	1477	1490	1531	rBV	785755	1673588	52.73%	6.932%
39	6.183	1570	1584	1610	rBV2	784081	1613074	50.82%	6.682%
40	6.325	1616	1628	1654	rVB	699075	1410868	44.45%	5.844%
41	6.614	1716	1718	1721	rVB3	1489	774	0.02%	0.003%
42	6.749	1757	1760	1767	rVV7	1084	1264	0.04%	0.005%
43	6.842	1785	1789	1792	rBV2	1037	793	0.02%	0.003%
44	6.884	1797	1802	1804	rBV4	1461	1262	0.04%	0.005%
45	6.997	1833	1837	1842	rVV4	1352	1019	0.03%	0.004%
46	7.087	1863	1865	1873	rVB5	965	1091	0.03%	0.005%
47	7.225	1896	1908	1933	rBV	343855	638837	20.13%	2.646%
48	7.386	1954	1958	1962	rBV5	1608	1463	0.05%	0.006%
49	7.418	1965	1968	1971	rBV3	1323	922	0.03%	0.004%
50	7.495	1989	1992	1995	rBV4	2171	1894	0.06%	0.008%
51	7.563	2000	2013	2047	rBV	1215077	2280257	71.84%	9.445%
52	7.849	2091	2102	2120	rBV	229652	424266	13.37%	1.757%
53	8.054	2163	2166	2171	rVB4	2423	1914	0.06%	0.008%
54	8.080	2171	2174	2176	rBV3	1258	685	0.02%	0.003%
55	8.148	2192	2195	2198	rBV2	954	725	0.02%	0.003%
56	8.228	2210	2220	2230	rBV3	23469	43462	1.37%	0.180%
57	8.312	2234	2246	2278	rBV2	896640	1835635	57.83%	7.604%
58	8.958	2444	2447	2451	rVB3	1512	1142	0.04%	0.005%
59	9.025	2466	2468	2474	rVB5	934	724	0.02%	0.003%
60	9.087	2474	2487	2532	rBV	1184146	2068820	65.18%	8.569%
61	9.498	2611	2615	2619	rBV6	1853	1745	0.05%	0.007%
62	9.521	2619	2622	2630	rVB6	1670	2026	0.06%	0.008%
63	9.649	2657	2662	2666	rBV6	1047	1325	0.04%	0.005%
64	9.672	2666	2669	2676	rVB5	1044	1231	0.04%	0.005%
65	9.704	2676	2679	2683	rBV3	1436	1060	0.03%	0.004%
66	9.906	2740	2742	2745	rVB	1529	720	0.02%	0.003%
67	9.932	2745	2750	2755	rVB3	1470	1327	0.04%	0.005%
68	9.984	2763	2766	2770	rVB3	1416	1148	0.04%	0.005%
69	10.006	2770	2773	2777	rBV2	1396	802	0.03%	0.003%
70	10.029	2777	2780	2781	rBV	1466	919	0.03%	0.004%
71	10.096	2794	2801	2804	rBV6	1348	1763	0.06%	0.007%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031608.D
 Acq On : 30 Apr 2019 00:27
 Operator : JC/SP
 Sample : K2592-11DL 250X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X04DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.186	2826	2829	2832	rBV2	1582	1190	0.04%	0.005%
73	10.238	2843	2845	2851	rVB2	1084	827	0.03%	0.003%
74	10.331	2871	2874	2878	rVB3	1483	971	0.03%	0.004%
75	10.427	2890	2904	2925	rBV	865482	1416927	44.64%	5.869%
76	10.717	2992	2994	2998	rVB	1704	1022	0.03%	0.004%
77	10.755	3004	3006	3008	rBV	1345	783	0.02%	0.003%
78	10.784	3012	3015	3017	rBV2	1741	973	0.03%	0.004%
79	10.894	3047	3049	3052	rBV3	1084	791	0.02%	0.003%
80	11.000	3080	3082	3086	rVB3	1141	688	0.02%	0.003%
81	11.022	3086	3089	3095	rBV5	1627	1974	0.06%	0.008%
82	11.386	3198	3202	3204	rBV2	1364	1052	0.03%	0.004%
83	11.405	3205	3208	3212	rVB3	1705	1199	0.04%	0.005%
84	11.482	3219	3232	3256	rBV	915637	1508547	47.53%	6.249%
85	11.855	3335	3348	3374	rBV	977791	1679036	52.90%	6.955%
86	12.427	3523	3526	3529	rBV3	1539	1198	0.04%	0.005%
87	12.447	3529	3532	3537	rVV6	1647	1820	0.06%	0.008%
88	12.659	3595	3598	3602	rBV4	1146	868	0.03%	0.004%
89	12.713	3613	3615	3618	rBV2	1229	748	0.02%	0.003%
90	12.848	3654	3657	3660	rBV2	1713	1447	0.05%	0.006%
91	12.887	3666	3669	3672	rBV3	1281	963	0.03%	0.004%
92	12.987	3695	3700	3703	rBV3	1742	1816	0.06%	0.008%
93	13.189	3759	3763	3768	rBV5	1528	1443	0.05%	0.006%
94	13.254	3780	3783	3787	rBV2	1533	1563	0.05%	0.006%
95	13.556	3874	3877	3881	rBV3	2120	1933	0.06%	0.008%
96	13.771	3940	3944	3948	rVB3	1569	1349	0.04%	0.006%
97	13.797	3950	3952	3958	rVB3	1985	1506	0.05%	0.006%
98	13.826	3958	3961	3964	rBV2	1696	1423	0.04%	0.006%
99	14.392	4134	4137	4143	rBV5	2334	2292	0.07%	0.009%
100	14.729	4238	4242	4248	rBV5	1946	2618	0.08%	0.011%


Sum of corrected areas: 24141733

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042919\
Data File : VU031608.D
Acq On : 30 Apr 2019 00:27
Operator : JC/SP
Sample : K2592-11DL 250X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X04DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

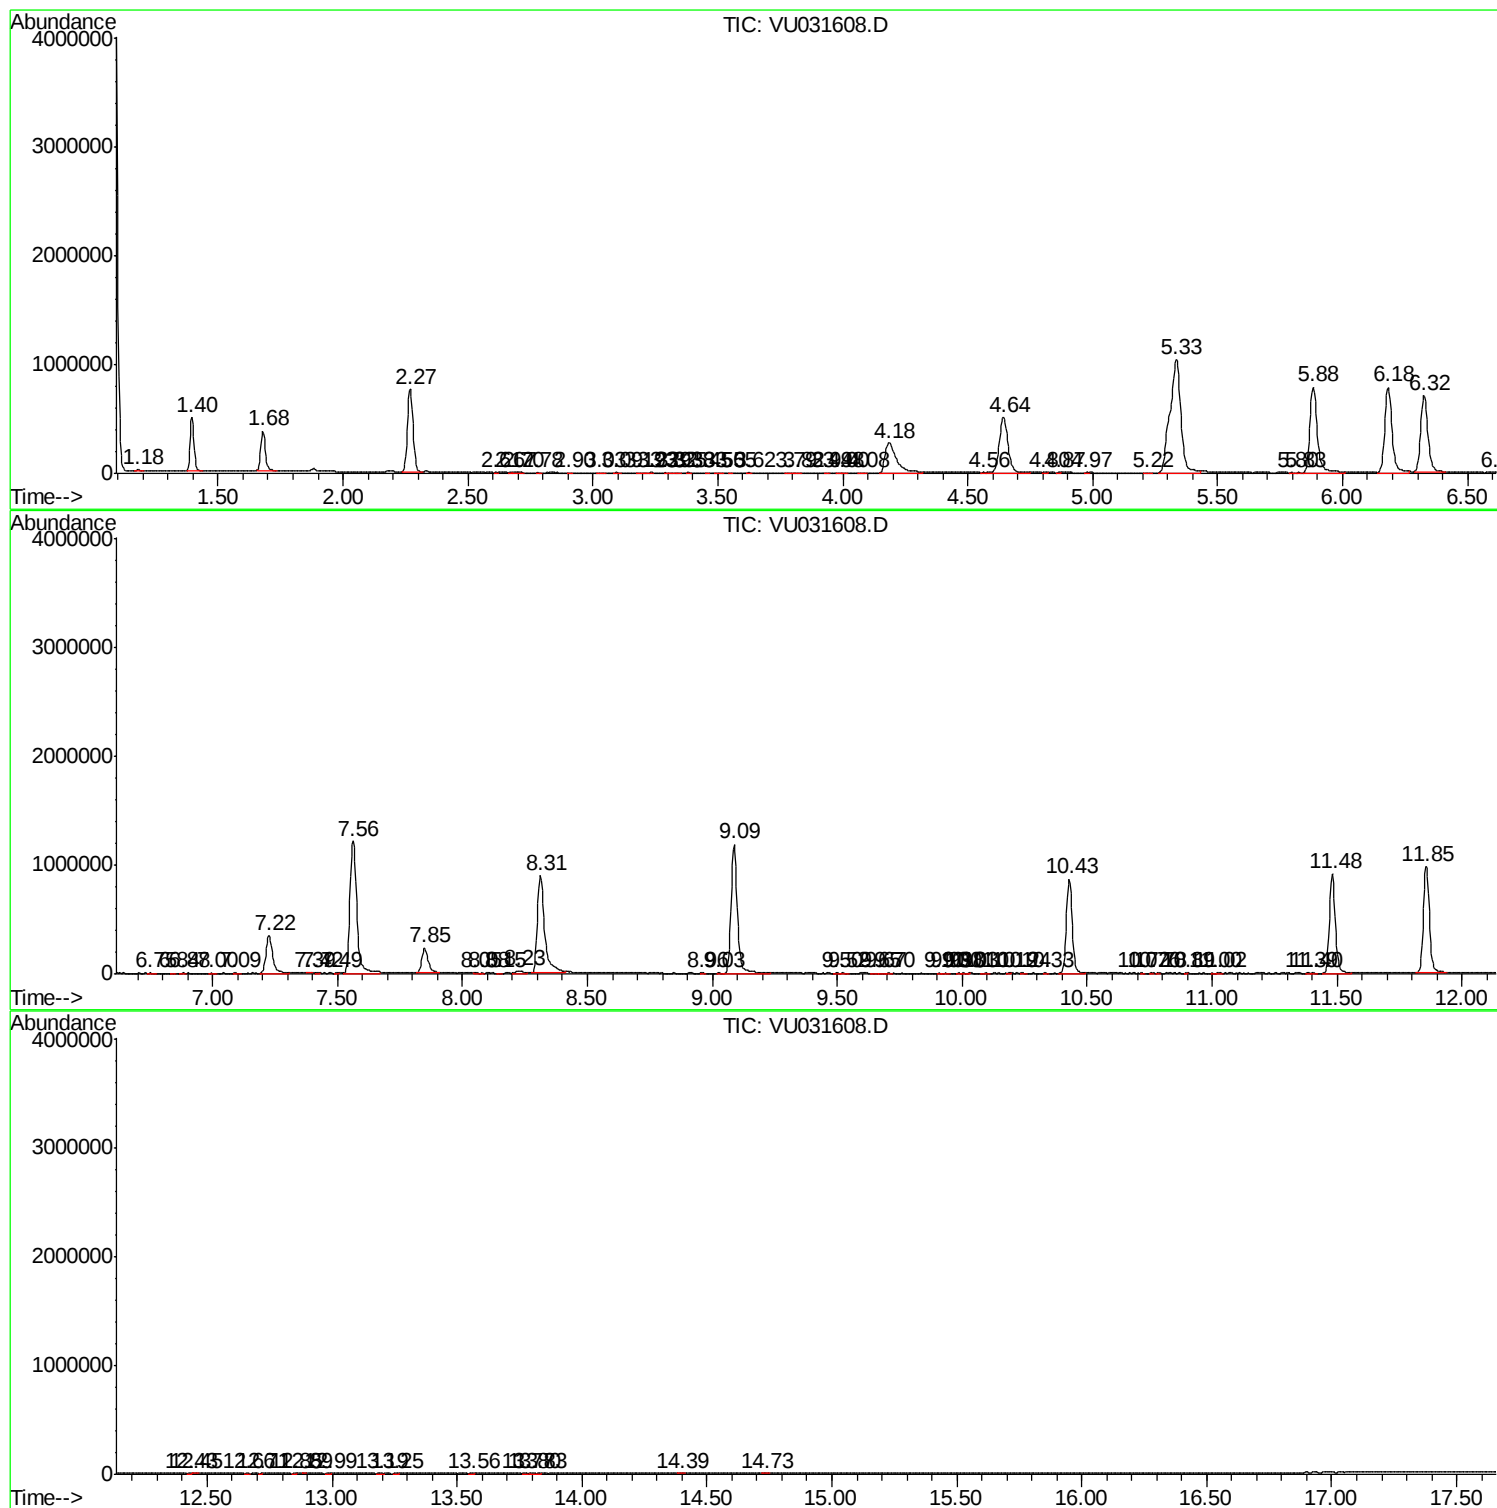

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042919\
Data File : VU031608.D
Acq On : 30 Apr 2019 00:27
Operator : JC/SP
Sample : K2592-11DL 250X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X04DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU042919\
Data File : VU031608.D
Acq On : 30 Apr 2019 00:27
Operator : JC/SP
Sample : K2592-11DL 250X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
C0X04DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc