

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031610.D
 Acq On : 30 Apr 2019 01:13
 Operator : JC/SP
 Sample : K2592-20DL 250X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X87DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	33	rBV2	15089	12419	0.40%	0.051%
2	1.395	88	95	107	rVB	480386	516018	16.68%	2.135%
3	1.678	176	183	197	rBV	371424	451920	14.60%	1.870%
4	2.270	356	367	381	rBV	753608	1151553	37.21%	4.765%
5	2.530	441	448	454	rBV6	2172	3791	0.12%	0.016%
6	2.694	494	499	503	rBV6	3661	4318	0.14%	0.018%
7	2.855	542	549	552	rBV6	974	1265	0.04%	0.005%
8	2.871	552	554	557	rVB2	1698	862	0.03%	0.004%
9	2.891	557	560	562	rBV4	1543	1176	0.04%	0.005%
10	2.961	579	582	586	rBV2	1152	847	0.03%	0.004%
11	3.013	596	598	602	rBV2	1063	722	0.02%	0.003%
12	3.125	630	633	637	rVB2	1264	996	0.03%	0.004%
13	3.151	637	641	645	rBV4	1380	1284	0.04%	0.005%
14	3.170	645	647	650	rVV3	1102	758	0.02%	0.003%
15	3.186	650	652	657	rVV3	1316	977	0.03%	0.004%
16	3.225	660	664	669	rBV2	1055	1244	0.04%	0.005%
17	3.289	679	684	686	rBV3	1262	990	0.03%	0.004%
18	3.337	694	699	701	rBV2	1296	1233	0.04%	0.005%
19	3.473	739	741	748	rVB4	921	850	0.03%	0.004%
20	3.508	748	752	754	rBV2	1161	926	0.03%	0.004%
21	3.534	757	760	765	rVV4	910	883	0.03%	0.004%
22	3.569	768	771	775	rVB3	1360	982	0.03%	0.004%
23	3.759	826	830	835	rBV5	850	898	0.03%	0.004%
24	3.855	858	860	867	rVB4	1358	1183	0.04%	0.005%
25	3.910	873	877	883	rBV3	1256	1064	0.03%	0.004%
26	3.942	883	887	890	rBV2	990	764	0.02%	0.003%
27	3.997	900	904	909	rBV2	1252	890	0.03%	0.004%
28	4.186	951	963	1004	rBV	271328	860932	27.82%	3.563%
29	4.643	1088	1105	1132	rBV	500936	1212134	39.17%	5.016%
30	4.913	1186	1189	1194	rVB4	1524	1515	0.05%	0.006%
31	4.971	1204	1207	1211	rBV4	1621	1490	0.05%	0.006%
32	5.206	1275	1280	1281	rBV3	1013	798	0.03%	0.003%
33	5.334	1297	1320	1346	rBV2	1027149	3094408	100.00%	12.805%
34	5.669	1421	1424	1426	rBV3	1480	1029	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031610.D
 Acq On : 30 Apr 2019 01:13
 Operator : JC/SP
 Sample : K2592-20DL 250X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X87DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.765	1451	1454	1457	rVV5	1623	1061	0.03%	0.004%
36	5.884	1476	1491	1526	rBV	769604	1629384	52.66%	6.743%
37	6.183	1569	1584	1610	rBV	1038847	2099508	67.85%	8.688%
38	6.324	1616	1628	1652	rVB	690355	1392533	45.00%	5.763%
39	6.527	1689	1691	1695	rBV4	1416	1118	0.04%	0.005%
40	6.662	1731	1733	1736	rBV	1161	720	0.02%	0.003%
41	6.726	1750	1753	1758	rVB3	1769	1372	0.04%	0.006%
42	6.759	1758	1763	1768	rBV4	1439	1480	0.05%	0.006%
43	6.784	1768	1771	1777	rBV3	1096	988	0.03%	0.004%
44	6.839	1785	1788	1791	rBV2	1542	1193	0.04%	0.005%
45	6.858	1791	1794	1798	rVB3	1474	1026	0.03%	0.004%
46	6.900	1802	1807	1811	rBB7	1231	1083	0.03%	0.004%
47	7.048	1849	1853	1856	rBV2	1415	1393	0.05%	0.006%
48	7.225	1895	1908	1936	rBV	331018	633954	20.49%	2.623%
49	7.373	1952	1954	1957	rBV3	1878	1068	0.03%	0.004%
50	7.562	2000	2013	2038	rBV	1195377	2197053	71.00%	9.092%
51	7.849	2091	2102	2126	rBV	221531	422017	13.64%	1.746%
52	8.048	2160	2164	2168	rBV5	1008	1046	0.03%	0.004%
53	8.093	2175	2178	2180	rBV3	1701	826	0.03%	0.003%
54	8.106	2180	2182	2185	rBV3	1820	1263	0.04%	0.005%
55	8.154	2194	2197	2200	rBV2	1138	943	0.03%	0.004%
56	8.228	2210	2220	2231	rBV3	24628	43439	1.40%	0.180%
57	8.312	2235	2246	2287	rBV	904449	1836188	59.34%	7.599%
58	8.646	2348	2350	2354	rBV4	1210	931	0.03%	0.004%
59	8.749	2378	2382	2386	rVB3	1922	1383	0.04%	0.006%
60	8.781	2386	2392	2395	rBV4	1639	2129	0.07%	0.009%
61	8.823	2402	2405	2408	rBV2	1106	740	0.02%	0.003%
62	8.865	2415	2418	2420	rVB3	1571	710	0.02%	0.003%
63	8.893	2423	2427	2429	rBV3	1097	851	0.03%	0.004%
64	8.955	2444	2446	2448	rBV3	1242	726	0.02%	0.003%
65	9.086	2474	2487	2523	rBV	1152047	2020196	65.29%	8.360%
66	9.254	2537	2539	2544	rVB5	1909	1482	0.05%	0.006%
67	9.418	2586	2590	2592	rBV4	1167	827	0.03%	0.003%
68	9.569	2634	2637	2642	rBV5	1260	995	0.03%	0.004%
69	9.594	2642	2645	2648	rVB3	1362	850	0.03%	0.004%
70	9.643	2656	2660	2663	rBV3	1364	863	0.03%	0.004%
71	9.726	2683	2686	2689	rBV3	1281	1053	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031610.D
 Acq On : 30 Apr 2019 01:13
 Operator : JC/SP
 Sample : K2592-20DL 250X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X87DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	9.784	2702	2704	2707	rBV2	1101	705	0.02%	0.003%
73	9.906	2738	2742	2745	rVB2	1222	815	0.03%	0.003%
74	9.926	2745	2748	2753	rBV4	1268	1290	0.04%	0.005%
75	10.054	2783	2788	2792	rVB3	1539	1254	0.04%	0.005%
76	10.093	2795	2800	2804	rBV2	1640	1476	0.05%	0.006%
77	10.141	2811	2815	2819	rBV3	748	857	0.03%	0.004%
78	10.427	2892	2904	2931	rBV	848189	1386218	44.80%	5.736%
79	10.819	3023	3026	3028	rBV2	1246	804	0.03%	0.003%
80	10.858	3033	3038	3039	rBV4	1752	1448	0.05%	0.006%
81	11.077	3102	3106	3112	rVB6	1880	2049	0.07%	0.008%
82	11.112	3112	3117	3121	rBV5	1540	1696	0.05%	0.007%
83	11.215	3146	3149	3152	rBV2	1075	698	0.02%	0.003%
84	11.234	3152	3155	3157	rVV	1127	735	0.02%	0.003%
85	11.266	3161	3165	3169	rBV2	1677	1354	0.04%	0.006%
86	11.373	3195	3198	3204	rBV4	1221	1260	0.04%	0.005%
87	11.482	3220	3232	3253	rBV	895352	1479235	47.80%	6.121%
88	11.630	3276	3278	3283	rVB4	2681	1672	0.05%	0.007%
89	11.855	3336	3348	3372	rBV	978224	1630171	52.68%	6.746%
90	12.276	3473	3479	3482	rBV5	1857	1711	0.06%	0.007%
91	12.382	3509	3512	3513	rBV	1374	793	0.03%	0.003%
92	12.543	3560	3562	3564	rBV3	1170	742	0.02%	0.003%
93	12.649	3592	3595	3599	rBV2	2408	2089	0.07%	0.009%
94	13.041	3714	3717	3722	rBV4	1747	1252	0.04%	0.005%
95	13.096	3732	3734	3738	rBV2	1221	856	0.03%	0.004%
96	13.157	3751	3753	3757	rVB2	1509	907	0.03%	0.004%
97	13.983	4005	4010	4011	rBV3	1456	1198	0.04%	0.005%
98	14.064	4032	4035	4039	rBV2	1553	1249	0.04%	0.005%
99	14.540	4180	4183	4187	rBV5	1491	1422	0.05%	0.006%
100	15.218	4391	4394	4397	rBV4	2317	1569	0.05%	0.006%


Sum of corrected areas: 24165036

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042919\
Data File : VU031610.D
Acq On : 30 Apr 2019 01:13
Operator : JC/SP
Sample : K2592-20DL 250X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X87DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

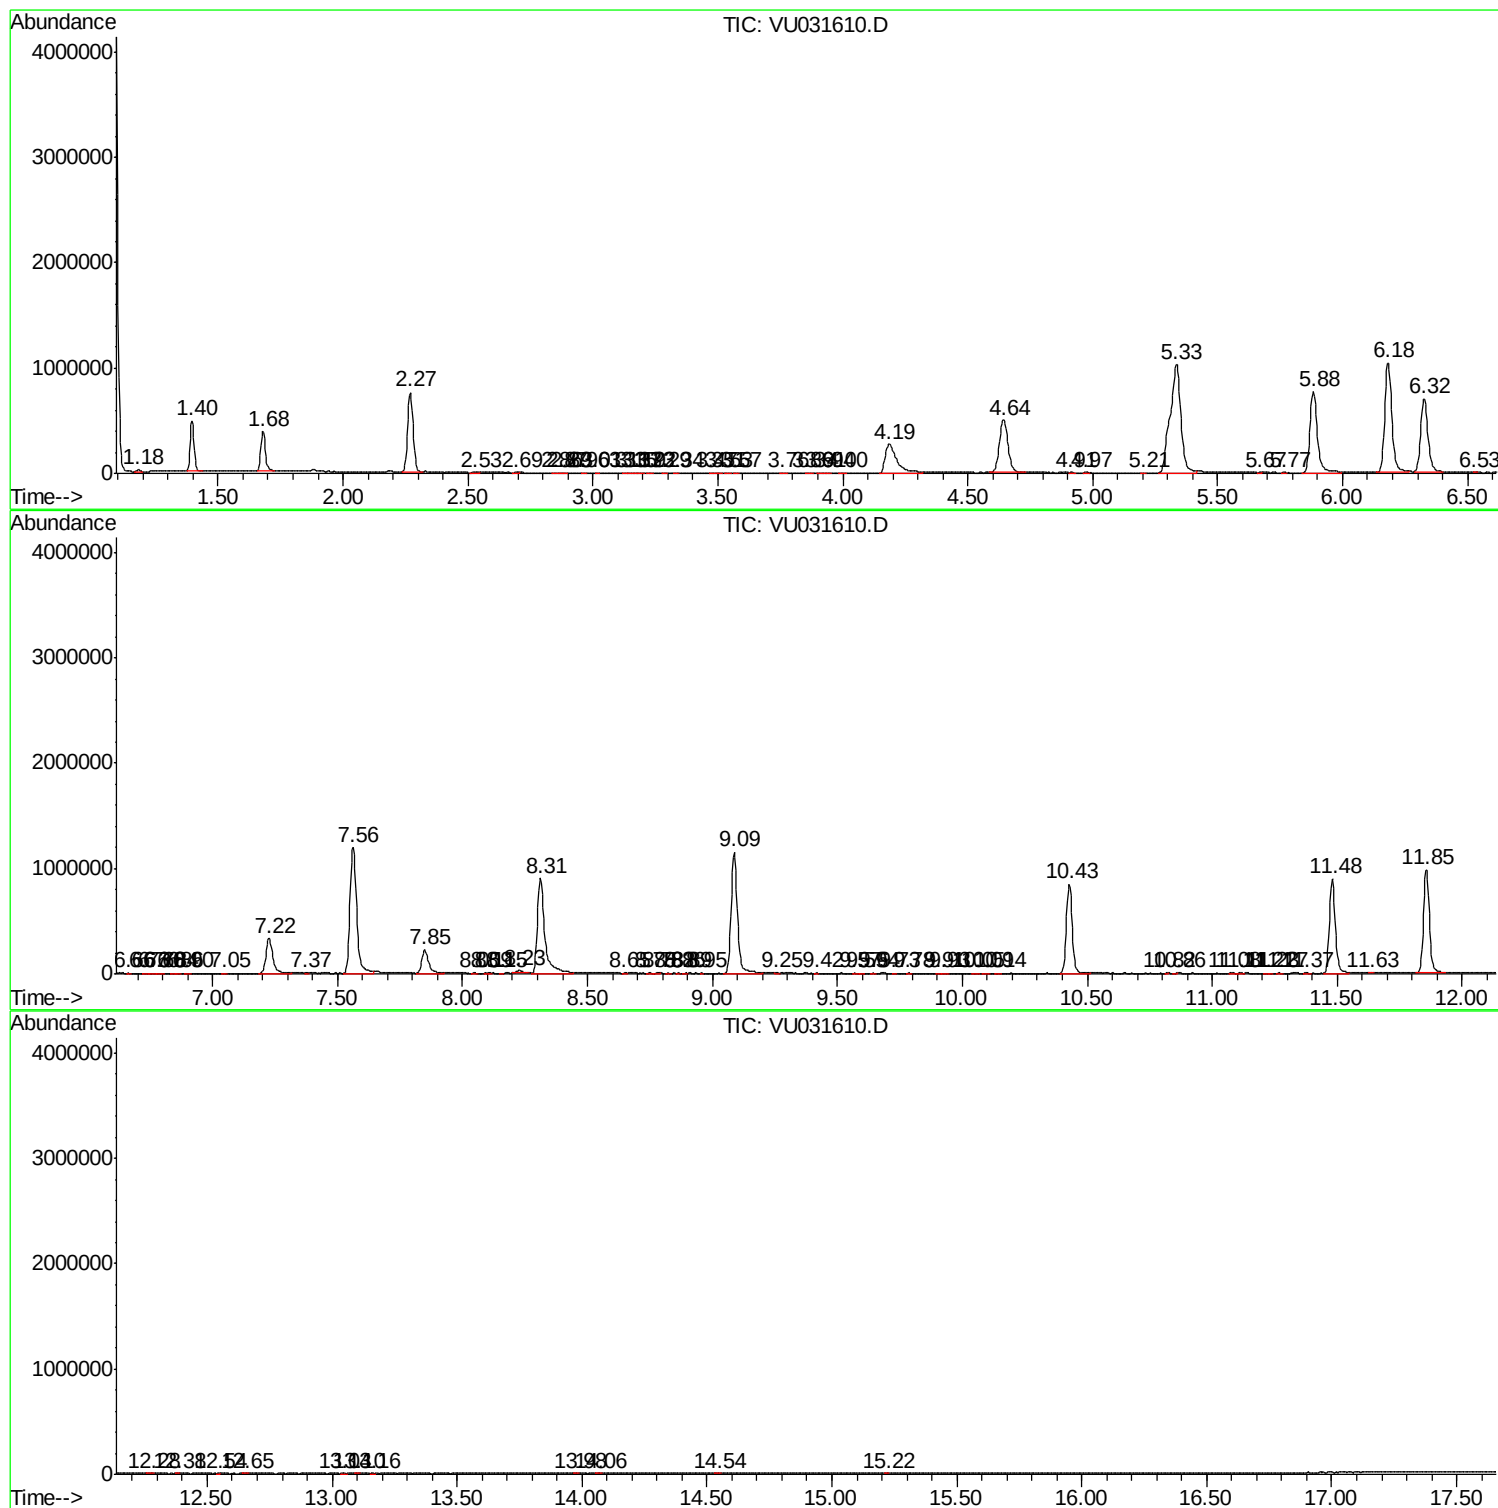

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042919\
Data File : VU031610.D
Acq On : 30 Apr 2019 01:13
Operator : JC/SP
Sample : K2592-20DL 250X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X87DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU042919\
Data File : VU031610.D
Acq On : 30 Apr 2019 01:13
Operator : JC/SP
Sample : K2592-20DL 250X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
C0X87DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc