

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031611.D
 Acq On : 30 Apr 2019 01:36
 Operator : JC/SP
 Sample : K2593-01DL 500X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XB2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	35	rVB2	15886	15641	0.49%	0.065%
2	1.396	88	95	107	rVB	512841	539590	16.94%	2.259%
3	1.679	176	183	198	rVB	382955	459655	14.43%	1.925%
4	2.270	357	367	380	rVB	771945	1176353	36.94%	4.926%
5	2.518	442	444	446	rBV3	1110	691	0.02%	0.003%
6	2.563	456	458	462	rVB2	1185	760	0.02%	0.003%
7	2.662	486	489	492	rVB3	1611	842	0.03%	0.004%
8	2.695	493	499	500	rBV4	2485	2188	0.07%	0.009%
9	2.842	543	545	549	rVB3	2229	1296	0.04%	0.005%
10	2.868	549	553	558	rBV3	1395	1531	0.05%	0.006%
11	2.926	569	571	574	rBV	1325	811	0.03%	0.003%
12	2.961	577	582	584	rBV2	903	737	0.02%	0.003%
13	2.978	584	587	590	rBV4	1978	1253	0.04%	0.005%
14	3.042	603	607	610	rBV3	957	854	0.03%	0.004%
15	3.074	615	617	621	rBV3	1517	1200	0.04%	0.005%
16	3.244	666	670	674	rBV2	1268	1341	0.04%	0.006%
17	3.322	691	694	697	rBV3	1260	987	0.03%	0.004%
18	3.354	697	704	707	rVV4	736	713	0.02%	0.003%
19	3.376	707	711	712	rBV2	996	765	0.02%	0.003%
20	3.469	734	740	742	rVV3	1303	1136	0.04%	0.005%
21	3.553	764	766	770	rVB	1215	712	0.02%	0.003%
22	3.576	770	773	778	rBV3	1405	973	0.03%	0.004%
23	3.605	778	782	786	rBV2	705	718	0.02%	0.003%
24	3.717	813	817	820	rVB4	1229	903	0.03%	0.004%
25	3.752	825	828	832	rVB3	1554	1312	0.04%	0.005%
26	3.781	832	837	841	rVB2	1550	1347	0.04%	0.006%
27	3.826	848	851	855	rBV3	1039	780	0.02%	0.003%
28	3.875	862	866	867	rBV	893	668	0.02%	0.003%
29	3.913	873	878	881	rBV2	1249	1475	0.05%	0.006%
30	3.942	881	887	892	rVV3	1348	1646	0.05%	0.007%
31	4.119	939	942	947	rVB3	929	862	0.03%	0.004%
32	4.183	950	962	1002	rBV	286644	887733	27.88%	3.717%
33	4.643	1084	1105	1128	rBV	519419	1237687	38.87%	5.183%
34	5.003	1215	1217	1221	rVB3	1975	1283	0.04%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031611.D
 Acq On : 30 Apr 2019 01:36
 Operator : JC/SP
 Sample : K2593-01DL 500X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XB2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.100	1244	1247	1248	rBV2	1164	684	0.02%	0.003%
36	5.161	1262	1266	1270	rBV3	1369	1591	0.05%	0.007%
37	5.334	1297	1320	1357	rBV2	1055536	3184494	100.00%	13.335%
38	5.765	1451	1454	1455	rBV3	1286	794	0.02%	0.003%
39	5.830	1470	1474	1478	rVB5	1222	1065	0.03%	0.004%
40	5.884	1478	1491	1519	rBV	788300	1651551	51.86%	6.916%
41	6.183	1570	1584	1606	rBV	627925	1265826	39.75%	5.301%
42	6.325	1616	1628	1664	rVB	710825	1469627	46.15%	6.154%
43	6.553	1697	1699	1701	rBV3	1073	653	0.02%	0.003%
44	6.624	1719	1721	1723	rBV2	1258	648	0.02%	0.003%
45	6.698	1742	1744	1749	rVB3	1457	914	0.03%	0.004%
46	6.804	1774	1777	1784	rBV6	1613	1485	0.05%	0.006%
47	6.836	1784	1787	1790	rBV3	1099	736	0.02%	0.003%
48	6.874	1796	1799	1802	rBV4	844	663	0.02%	0.003%
49	6.977	1825	1831	1835	rBV6	1387	1680	0.05%	0.007%
50	7.000	1836	1838	1843	rVB2	1775	1062	0.03%	0.004%
51	7.096	1864	1868	1870	rBV3	1218	828	0.03%	0.003%
52	7.109	1870	1872	1876	rVB2	1378	989	0.03%	0.004%
53	7.174	1889	1892	1893	rBV2	1107	656	0.02%	0.003%
54	7.225	1896	1908	1934	rVV	332633	639919	20.09%	2.680%
55	7.563	2000	2013	2053	rBV	1222493	2280686	71.62%	9.550%
56	7.733	2064	2066	2069	rBV3	2264	1567	0.05%	0.007%
57	7.849	2092	2102	2126	rBV	227289	418379	13.14%	1.752%
58	8.109	2181	2183	2187	rBV3	1035	897	0.03%	0.004%
59	8.145	2191	2194	2196	rBV3	1037	684	0.02%	0.003%
60	8.231	2213	2221	2233	rVB3	8132	14919	0.47%	0.062%
61	8.312	2233	2246	2281	rBV	926291	1896931	59.57%	7.943%
62	8.839	2408	2410	2415	rVB4	1718	1247	0.04%	0.005%
63	9.087	2471	2487	2521	rBV	1173050	2081479	65.36%	8.716%
64	9.463	2600	2604	2608	rBV6	1203	1241	0.04%	0.005%
65	9.537	2624	2627	2630	rBV3	1511	847	0.03%	0.004%
66	9.588	2639	2643	2650	rBV5	1874	2179	0.07%	0.009%
67	9.649	2660	2662	2665	rVB2	1213	683	0.02%	0.003%
68	9.733	2685	2688	2691	rBV2	1461	1009	0.03%	0.004%
69	9.768	2695	2699	2708	rVV4	1466	2196	0.07%	0.009%
70	9.804	2708	2710	2713	rVB4	1844	946	0.03%	0.004%
71	9.958	2754	2758	2761	rBV2	1146	1097	0.03%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031611.D
 Acq On : 30 Apr 2019 01:36
 Operator : JC/SP
 Sample : K2593-01DL 500X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XB2DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.016	2773	2776	2783	rBV3	1061	1038	0.03%	0.004%
73	10.260	2849	2852	2854	rBV3	1085	851	0.03%	0.004%
74	10.292	2858	2862	2863	rBV2	1500	1131	0.04%	0.005%
75	10.337	2872	2876	2879	rBV4	1487	1127	0.04%	0.005%
76	10.427	2889	2904	2931	rBV	875283	1435194	45.07%	6.010%
77	10.646	2969	2972	2974	rBV3	1453	1030	0.03%	0.004%
78	10.813	3020	3024	3025	rBV2	1163	752	0.02%	0.003%
79	10.842	3030	3033	3037	rVB2	1046	775	0.02%	0.003%
80	10.961	3067	3070	3072	rBV2	923	680	0.02%	0.003%
81	11.022	3087	3089	3092	rBV2	1654	916	0.03%	0.004%
82	11.042	3092	3095	3099	rBV3	1108	814	0.03%	0.003%
83	11.070	3102	3104	3111	rVB4	1138	920	0.03%	0.004%
84	11.164	3131	3133	3136	rBV2	902	645	0.02%	0.003%
85	11.373	3194	3198	3202	rBV4	1211	1130	0.04%	0.005%
86	11.482	3219	3232	3254	rBV	912242	1493590	46.90%	6.254%
87	11.858	3337	3349	3372	rBV	980635	1647459	51.73%	6.899%
88	12.151	3438	3440	3443	rBV3	1558	825	0.03%	0.003%
89	12.450	3531	3533	3536	rBV	1100	649	0.02%	0.003%
90	12.601	3577	3580	3582	rBV3	1474	815	0.03%	0.003%
91	12.710	3611	3614	3617	rBV4	1908	1535	0.05%	0.006%
92	12.771	3630	3633	3635	rVB3	1393	776	0.02%	0.003%
93	12.836	3651	3653	3658	rVB2	1642	901	0.03%	0.004%
94	12.942	3684	3686	3690	rVB2	2017	1270	0.04%	0.005%
95	13.115	3737	3740	3744	rBV4	1364	1206	0.04%	0.005%
96	13.463	3846	3848	3852	rBV2	1886	1218	0.04%	0.005%
97	13.549	3872	3875	3877	rBV	1852	966	0.03%	0.004%
98	13.980	4006	4009	4011	rBV	1540	1095	0.03%	0.005%
99	14.347	4120	4123	4126	rBV3	1518	955	0.03%	0.004%
100	14.646	4213	4216	4219	rBV3	2075	1473	0.05%	0.006%


Sum of corrected areas: 23881031

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042919\
Data File : VU031611.D
Acq On : 30 Apr 2019 01:36
Operator : JC/SP
Sample : K2593-01DL 500X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XB2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

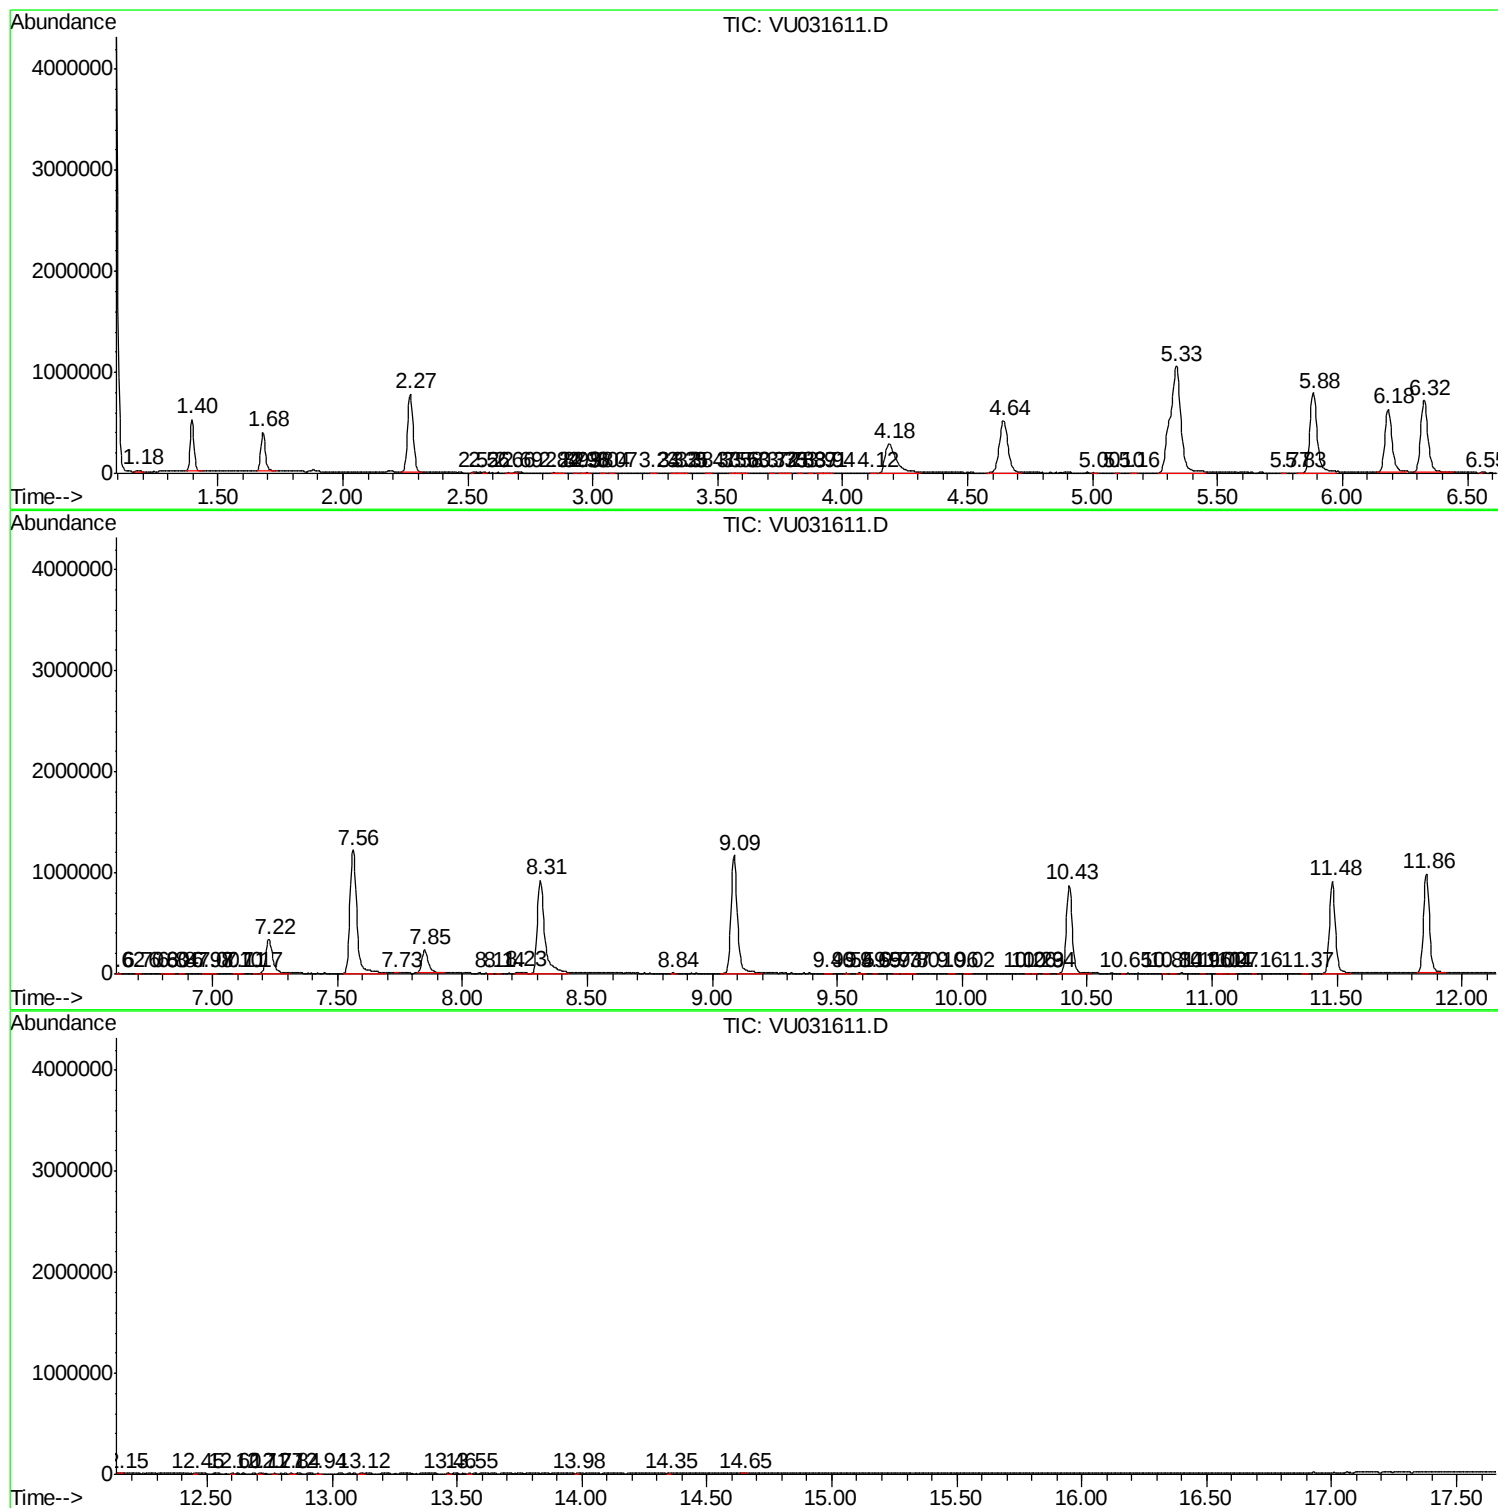

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042919\
Data File : VU031611.D
Acq On : 30 Apr 2019 01:36
Operator : JC/SP
Sample : K2593-01DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XB2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042919\
Data File : VU031611.D
Acq On : 30 Apr 2019 01:36
Operator : JC/SP
Sample : K2593-01DL 500X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XB2DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc