

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031612.D
 Acq On : 30 Apr 2019 01:59
 Operator : JC/SP
 Sample : K2592-12DL 1000X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X72DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	25	28	36	rVB3	15586	14132	0.45%	0.057%
2	1.396	88	95	110	rBV	493763	522989	16.71%	2.121%
3	1.682	176	184	200	rVB	358111	449107	14.35%	1.822%
4	1.884	242	247	259	rVB5	24068	34909	1.12%	0.142%
5	2.190	336	342	349	rVB6	8760	12683	0.41%	0.051%
6	2.270	356	367	381	rVB	752177	1143980	36.54%	4.640%
7	2.415	410	412	418	rVB5	3005	2165	0.07%	0.009%
8	2.447	419	422	424	rBV3	1665	1065	0.03%	0.004%
9	2.572	458	461	464	rBV3	1916	1198	0.04%	0.005%
10	2.695	496	499	501	rBV2	1437	1005	0.03%	0.004%
11	2.743	510	514	516	rBV3	1420	1085	0.03%	0.004%
12	2.807	531	534	540	rBV4	1130	1073	0.03%	0.004%
13	2.968	579	584	589	rBV5	1619	2091	0.07%	0.008%
14	3.016	593	599	603	rBV4	1429	2055	0.07%	0.008%
15	3.209	653	659	661	rBV3	864	974	0.03%	0.004%
16	3.283	677	682	684	rBV3	1246	1044	0.03%	0.004%
17	3.392	713	716	720	rBV2	1443	1070	0.03%	0.004%
18	3.540	760	762	764	rBV4	1335	780	0.02%	0.003%
19	3.579	770	774	777	rBV	867	729	0.02%	0.003%
20	3.630	785	790	794	rBV4	1015	1168	0.04%	0.005%
21	3.659	794	799	801	rBV2	1353	1281	0.04%	0.005%
22	3.675	801	804	808	rBV2	915	690	0.02%	0.003%
23	3.730	818	821	829	rVB4	1369	1341	0.04%	0.005%
24	3.778	829	836	839	rBV2	1104	972	0.03%	0.004%
25	3.807	841	845	849	rBV4	1552	1389	0.04%	0.006%
26	3.907	874	876	880	rVB2	1415	773	0.02%	0.003%
27	3.984	897	900	903	rVB3	1067	641	0.02%	0.003%
28	4.006	903	907	912	rVB4	1111	789	0.03%	0.003%
29	4.051	918	921	924	rVB	877	639	0.02%	0.003%
30	4.080	924	930	932	rBV2	851	1001	0.03%	0.004%
31	4.186	951	963	1000	rBV2	274041	871013	27.82%	3.533%
32	4.502	1057	1061	1069	rVB5	2210	2821	0.09%	0.011%
33	4.643	1088	1105	1127	rBV	504205	1204182	38.47%	4.884%
34	4.772	1143	1145	1148	rBV3	1208	677	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031612.D
 Acq On : 30 Apr 2019 01:59
 Operator : JC/SP
 Sample : K2592-12DL 1000X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X72DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	4.984	1203	1211	1214	rBV7	2077	2843	0.09%	0.012%
36	5.138	1257	1259	1262	rVB3	1351	717	0.02%	0.003%
37	5.167	1262	1268	1273	rVB6	1473	1806	0.06%	0.007%
38	5.193	1273	1276	1279	rBV3	942	799	0.03%	0.003%
39	5.231	1285	1288	1293	rVB4	1983	1735	0.06%	0.007%
40	5.334	1298	1320	1352	rBV2	1031006	3130484	100.00%	12.697%
41	5.746	1445	1448	1450	rBV2	1143	706	0.02%	0.003%
42	5.772	1453	1456	1459	rVB2	2248	1433	0.05%	0.006%
43	5.810	1465	1468	1473	rVB4	2186	1624	0.05%	0.007%
44	5.884	1476	1491	1533	rBV	772352	1658891	52.99%	6.728%
45	6.183	1569	1584	1615	rBV	1176076	2394999	76.51%	9.714%
46	6.325	1616	1628	1655	rVB	688924	1420237	45.37%	5.760%
47	6.608	1713	1716	1719	rVB2	1748	1063	0.03%	0.004%
48	6.633	1719	1724	1728	rVB5	1855	1552	0.05%	0.006%
49	6.685	1737	1740	1744	rBV2	1533	1069	0.03%	0.004%
50	6.707	1744	1747	1749	rBV3	1227	697	0.02%	0.003%
51	6.736	1754	1756	1759	rVB2	1470	676	0.02%	0.003%
52	6.755	1759	1762	1767	rBV5	969	975	0.03%	0.004%
53	6.897	1803	1806	1809	rVB3	1527	981	0.03%	0.004%
54	6.916	1809	1812	1817	rBV4	1492	1188	0.04%	0.005%
55	7.064	1856	1858	1862	rVV3	977	690	0.02%	0.003%
56	7.103	1867	1870	1872	rVV3	1211	884	0.03%	0.004%
57	7.167	1888	1890	1893	rVB2	1143	633	0.02%	0.003%
58	7.225	1893	1908	1932	rBV	335277	632926	20.22%	2.567%
59	7.460	1977	1981	1984	rBV5	1436	1245	0.04%	0.005%
60	7.562	1996	2013	2043	rBV	1203624	2236179	71.43%	9.070%
61	7.849	2092	2102	2128	rBV	216173	399947	12.78%	1.622%
62	8.083	2172	2175	2179	rBV3	1396	1047	0.03%	0.004%
63	8.225	2212	2219	2232	rBV7	13418	22933	0.73%	0.093%
64	8.312	2234	2246	2283	rBV2	909735	1857640	59.34%	7.534%
65	8.697	2361	2366	2368	rBV5	2232	2073	0.07%	0.008%
66	8.759	2382	2385	2389	rBV3	1200	872	0.03%	0.004%
67	8.913	2430	2433	2438	rBV5	1320	919	0.03%	0.004%
68	9.087	2473	2487	2518	rBV	1149282	2032938	64.94%	8.245%
69	9.296	2549	2552	2556	rVB4	1737	1157	0.04%	0.005%
70	9.373	2571	2576	2578	rBV3	1751	1619	0.05%	0.007%
71	9.617	2649	2652	2656	rBV3	1203	974	0.03%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031612.D
 Acq On : 30 Apr 2019 01:59
 Operator : JC/SP
 Sample : K2592-12DL 1000X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0X72DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	9.662	2664	2666	2671	rVB3	1129	636	0.02%	0.003%
73	10.003	2769	2772	2774	rBV	1010	652	0.02%	0.003%
74	10.025	2777	2779	2783	rVB3	1386	855	0.03%	0.003%
75	10.109	2800	2805	2806	rBV2	924	832	0.03%	0.003%
76	10.180	2823	2827	2829	rBV2	786	646	0.02%	0.003%
77	10.196	2829	2832	2836	rBV3	1109	790	0.03%	0.003%
78	10.260	2850	2852	2858	rVB3	1297	1084	0.03%	0.004%
79	10.295	2861	2863	2866	rVB2	1410	787	0.03%	0.003%
80	10.427	2892	2904	2932	rVV	863884	1401075	44.76%	5.683%
81	10.553	2939	2943	2945	rBV3	1425	1153	0.04%	0.005%
82	10.662	2973	2977	2981	rVB4	2165	1972	0.06%	0.008%
83	10.688	2981	2985	2987	rBV3	917	845	0.03%	0.003%
84	10.897	3047	3050	3053	rBV2	1090	821	0.03%	0.003%
85	11.003	3079	3083	3085	rBV4	1375	1078	0.03%	0.004%
86	11.096	3109	3112	3115	rBV4	1394	786	0.03%	0.003%
87	11.267	3162	3165	3168	rBV2	785	695	0.02%	0.003%
88	11.479	3219	3231	3253	rBV	894095	1488019	47.53%	6.035%
89	11.755	3315	3317	3322	rBV5	1520	1250	0.04%	0.005%
90	11.855	3335	3348	3372	rBV	960358	1635725	52.25%	6.634%
91	12.279	3478	3480	3485	rBV4	1376	703	0.02%	0.003%
92	12.720	3614	3617	3624	rBV3	1357	1375	0.04%	0.006%
93	12.791	3637	3639	3642	rBV4	1157	812	0.03%	0.003%
94	13.045	3716	3718	3722	rBV2	1023	875	0.03%	0.004%
95	13.511	3859	3863	3867	rBV4	1785	1726	0.06%	0.007%
96	13.533	3867	3870	3872	rVV2	1308	792	0.03%	0.003%
97	13.781	3943	3947	3949	rBV3	1537	1473	0.05%	0.006%
98	14.167	4064	4067	4072	rBV4	1983	2094	0.07%	0.008%
99	14.823	4269	4271	4274	rBV3	1701	1004	0.03%	0.004%
100	15.720	4547	4550	4554	rBV6	2411	2612	0.08%	0.011%


Sum of corrected areas: 24655829

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042919\
Data File : VU031612.D
Acq On : 30 Apr 2019 01:59
Operator : JC/SP
Sample : K2592-12DL 1000X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X72DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

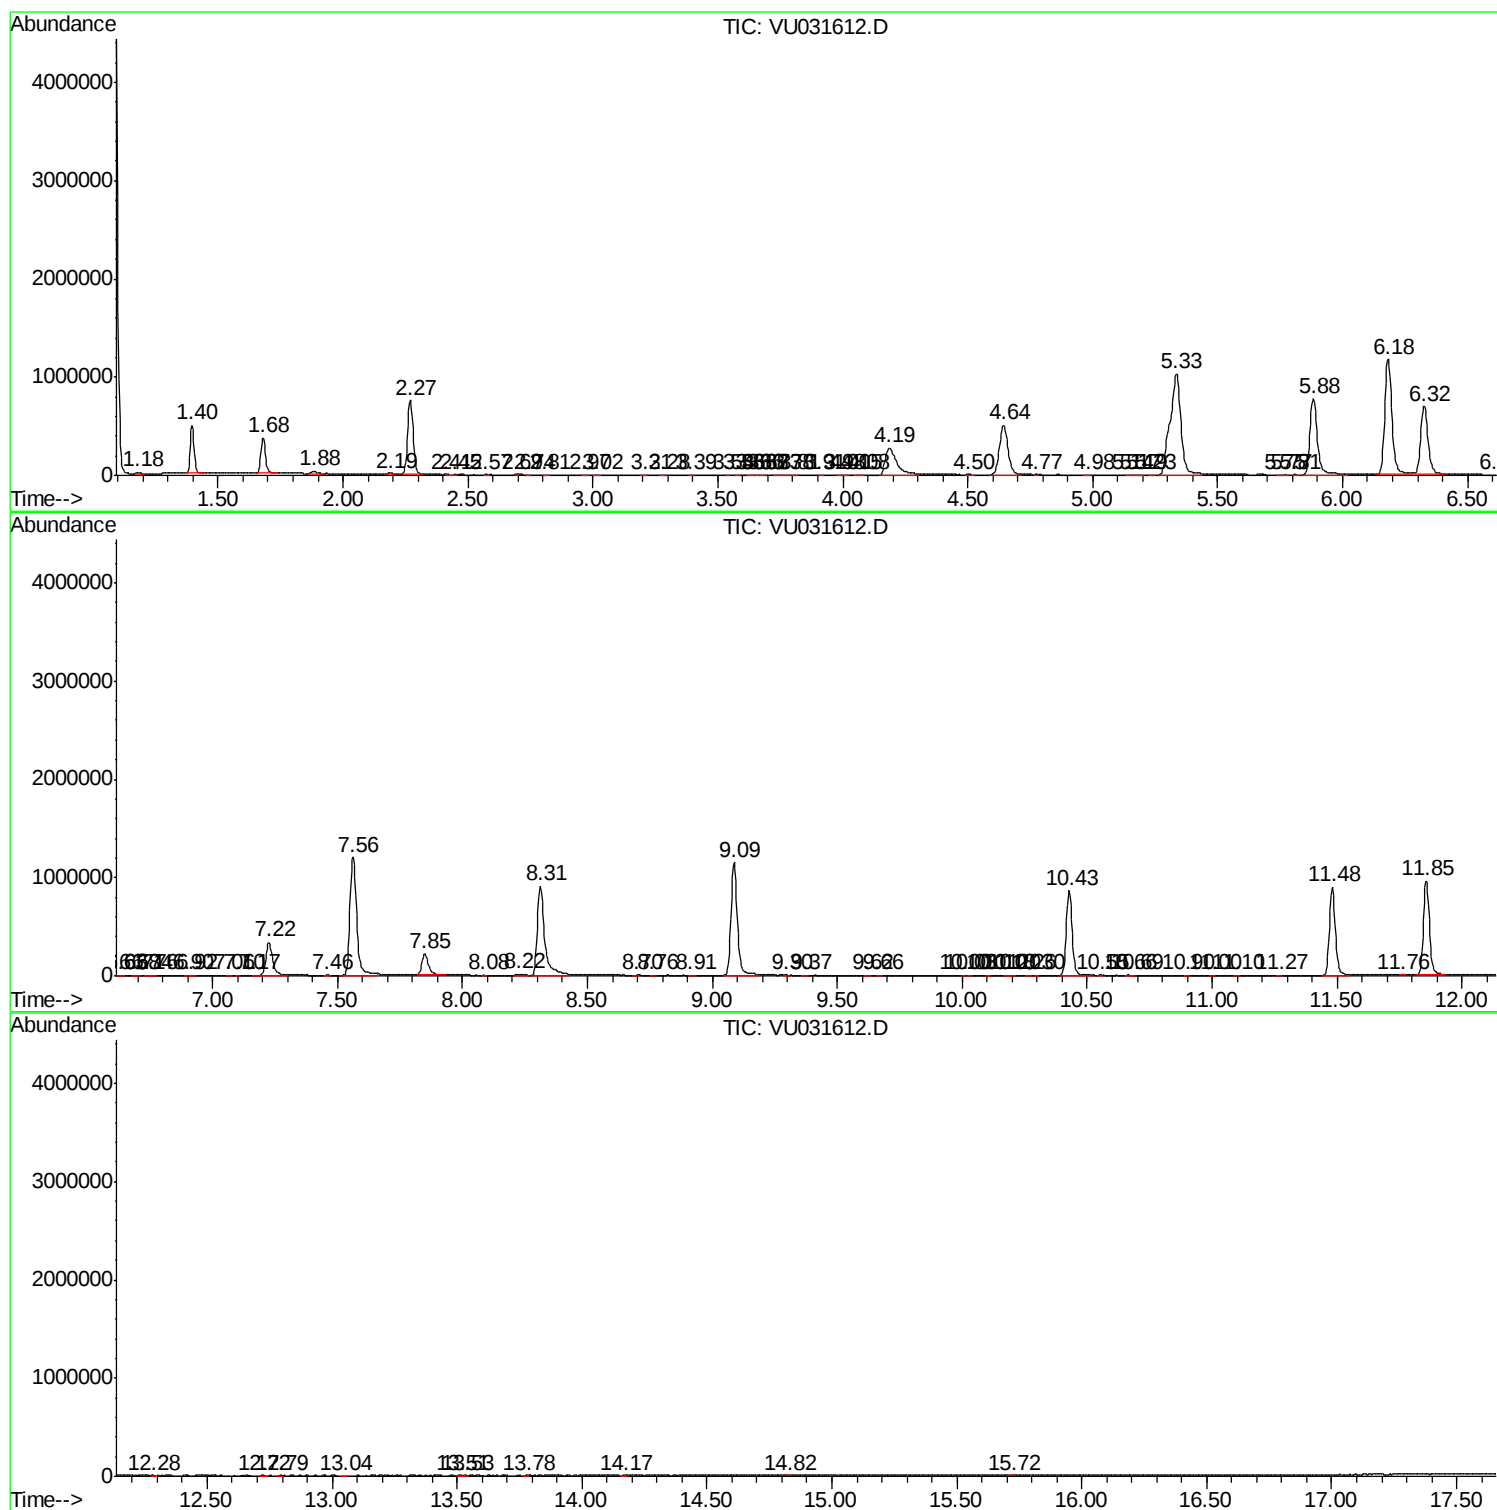

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042919\
Data File : VU031612.D
Acq On : 30 Apr 2019 01:59
Operator : JC/SP
Sample : K2592-12DL 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X72DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042919\
Data File : VU031612.D
Acq On : 30 Apr 2019 01:59
Operator : JC/SP
Sample : K2592-12DL 1000X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0X72DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc