

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031614.D
 Acq On : 30 Apr 2019 02:46
 Operator : JC/SP
 Sample : K2593-02 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XB4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	35	rBV4	14640	14360	0.21%	0.050%
2	1.299	60	65	69	rBV2	13448	13722	0.20%	0.048%
3	1.396	88	95	107	rVB	471626	507421	7.32%	1.770%
4	1.679	176	183	196	rBV	348719	442128	6.38%	1.542%
5	1.881	239	246	258	rVB	59143	82885	1.20%	0.289%
6	2.270	356	367	381	rVB	717834	1094169	15.78%	3.816%
7	2.447	420	422	425	rVB3	1378	676	0.01%	0.002%
8	2.646	480	484	492	rVB5	2413	2670	0.04%	0.009%
9	2.701	492	501	513	rVB5	6807	15440	0.22%	0.054%
10	2.762	516	520	522	rBV3	1960	1625	0.02%	0.006%
11	2.846	543	546	550	rVB4	1678	1350	0.02%	0.005%
12	2.891	557	560	562	rBV3	1169	692	0.01%	0.002%
13	2.936	571	574	579	rVV4	1461	1348	0.02%	0.005%
14	2.987	586	590	598	rVB4	2996	3143	0.05%	0.011%
15	3.097	620	624	627	rVB2	1332	1120	0.02%	0.004%
16	3.116	627	630	633	rBV4	1166	984	0.01%	0.003%
17	3.248	667	671	677	rBV4	1545	1620	0.02%	0.006%
18	3.354	701	704	707	rBV2	1093	764	0.01%	0.003%
19	3.386	711	714	717	rVB3	957	704	0.01%	0.002%
20	3.466	735	739	741	rBV	1812	1416	0.02%	0.005%
21	3.659	796	799	803	rBV2	944	672	0.01%	0.002%
22	3.698	807	811	814	rVB	974	896	0.01%	0.003%
23	3.733	817	822	824	rBV3	932	709	0.01%	0.002%
24	3.875	862	866	873	rBV	2126	2045	0.03%	0.007%
25	3.913	875	878	882	rBV4	850	830	0.01%	0.003%
26	4.093	931	934	937	rBV2	1909	1487	0.02%	0.005%
27	4.190	951	964	1005	rVV	261461	883374	12.74%	3.081%
28	4.518	1064	1066	1073	rVB3	1115	900	0.01%	0.003%
29	4.643	1088	1105	1134	rBV	491353	1176492	16.97%	4.103%
30	4.881	1177	1179	1184	rVB3	1345	965	0.01%	0.003%
31	4.997	1212	1215	1219	rVV4	1455	1041	0.02%	0.004%
32	5.032	1223	1226	1235	rVB4	901	1073	0.02%	0.004%
33	5.074	1236	1239	1243	rBV3	1365	950	0.01%	0.003%
34	5.103	1245	1248	1252	rVB3	1497	1140	0.02%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031614.D
 Acq On : 30 Apr 2019 02:46
 Operator : JC/SP
 Sample : K2593-02 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XB4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.129	1252	1256	1262	rVB4	1591	1797	0.03%	0.006%
36	5.170	1266	1269	1272	rBV	1093	673	0.01%	0.002%
37	5.193	1272	1276	1278	rBV2	1489	1068	0.02%	0.004%
38	5.334	1293	1320	1341	rBV2	990564	2993545	43.18%	10.440%
39	5.711	1434	1437	1441	rVB3	1259	905	0.01%	0.003%
40	5.743	1442	1447	1451	rBV4	1753	1853	0.03%	0.006%
41	5.813	1466	1469	1473	rVB4	1564	1065	0.02%	0.004%
42	5.881	1477	1490	1511	rBV	750877	1545653	22.30%	5.390%
43	6.180	1568	1583	1616	rBV	3482500	6932342	100.00%	24.177%
44	6.328	1617	1629	1658	rVB	681799	1445811	20.86%	5.042%
45	6.887	1799	1803	1805	rBV2	1334	1073	0.02%	0.004%
46	6.903	1805	1808	1810	rVV2	1025	650	0.01%	0.002%
47	6.936	1816	1818	1824	rBV4	868	863	0.01%	0.003%
48	7.000	1834	1838	1841	rBV4	1440	1051	0.02%	0.004%
49	7.170	1889	1891	1895	rVB2	1148	811	0.01%	0.003%
50	7.225	1895	1908	1928	rBV	328649	620809	8.96%	2.165%
51	7.440	1973	1975	1978	rBV3	1255	703	0.01%	0.002%
52	7.460	1978	1981	1984	rVB3	1577	900	0.01%	0.003%
53	7.563	2000	2013	2053	rBV	1138590	2150991	31.03%	7.502%
54	7.849	2091	2102	2136	rBV	223520	420102	6.06%	1.465%
55	8.112	2181	2184	2186	rBV3	1148	924	0.01%	0.003%
56	8.225	2209	2219	2234	rVB4	38238	67715	0.98%	0.236%
57	8.312	2234	2246	2294	rBV2	896537	1857852	26.80%	6.479%
58	8.698	2364	2366	2371	rVB4	1651	1215	0.02%	0.004%
59	8.727	2372	2375	2378	rBV4	1759	1315	0.02%	0.005%
60	8.810	2398	2401	2403	rBV3	1203	860	0.01%	0.003%
61	8.862	2413	2417	2421	rVB4	1856	1714	0.02%	0.006%
62	9.087	2472	2487	2515	rBV	1115741	1967110	28.38%	6.860%
63	9.373	2573	2576	2578	rBV3	2065	1161	0.02%	0.004%
64	9.463	2598	2604	2607	rBV5	939	1083	0.02%	0.004%
65	9.489	2608	2612	2617	rVB5	1326	1368	0.02%	0.005%
66	9.572	2636	2638	2640	rBV3	1370	800	0.01%	0.003%
67	9.681	2669	2672	2674	rVB2	1296	662	0.01%	0.002%
68	9.717	2679	2683	2686	rBV3	1588	1091	0.02%	0.004%
69	9.752	2692	2694	2698	rVB3	1489	982	0.01%	0.003%
70	9.916	2743	2745	2748	rBV3	1238	724	0.01%	0.003%
71	9.942	2748	2753	2756	rBV2	1493	1309	0.02%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031614.D
 Acq On : 30 Apr 2019 02:46
 Operator : JC/SP
 Sample : K2593-02 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XB4

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.080	2793	2796	2801	rVB3	1135	978	0.01%	0.003%
73	10.112	2801	2806	2810	rBV2	2083	1714	0.02%	0.006%
74	10.215	2833	2838	2842	rBV2	2105	2066	0.03%	0.007%
75	10.427	2891	2904	2928	rBV	849821	1377475	19.87%	4.804%
76	10.575	2948	2950	2956	rBV3	1231	1191	0.02%	0.004%
77	10.656	2971	2975	2977	rBV3	1065	826	0.01%	0.003%
78	10.739	2999	3001	3004	rBV2	1175	821	0.01%	0.003%
79	10.788	3014	3016	3019	rVB	1658	818	0.01%	0.003%
80	10.810	3021	3023	3032	rVB3	1340	1329	0.02%	0.005%
81	10.865	3037	3040	3043	rBV	1319	945	0.01%	0.003%
82	10.884	3043	3046	3047	rBV	1117	655	0.01%	0.002%
83	10.952	3064	3067	3070	rBV2	775	706	0.01%	0.002%
84	11.054	3095	3099	3103	rBV5	1177	1372	0.02%	0.005%
85	11.286	3169	3171	3176	rVB	1017	764	0.01%	0.003%
86	11.312	3176	3179	3183	rVB2	958	665	0.01%	0.002%
87	11.373	3196	3198	3205	rVB4	1088	856	0.01%	0.003%
88	11.405	3205	3208	3213	rBV3	1997	2363	0.03%	0.008%
89	11.482	3220	3232	3251	rBV	851257	1413984	20.40%	4.931%
90	11.858	3336	3349	3370	rBV	927164	1562417	22.54%	5.449%
91	12.324	3491	3494	3495	rBV2	1387	792	0.01%	0.003%
92	12.386	3511	3513	3516	rBV3	1119	677	0.01%	0.002%
93	12.569	3567	3570	3571	rBV2	1359	673	0.01%	0.002%
94	12.668	3598	3601	3604	rBV2	1087	1014	0.01%	0.004%
95	12.714	3612	3615	3618	rBV3	1399	1178	0.02%	0.004%
96	12.877	3661	3666	3670	rBV4	1506	1535	0.02%	0.005%
97	13.041	3713	3717	3719	rBV2	1691	1566	0.02%	0.005%
98	13.103	3733	3736	3738	rBV2	1786	892	0.01%	0.003%
99	13.630	3898	3900	3905	rBV4	1233	1167	0.02%	0.004%
100	13.781	3945	3947	3953	rBV2	1516	1004	0.01%	0.004%


Sum of corrected areas: 28673804

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042919\
Data File : VU031614.D
Acq On : 30 Apr 2019 02:46
Operator : JC/SP
Sample : K2593-02 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XB4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

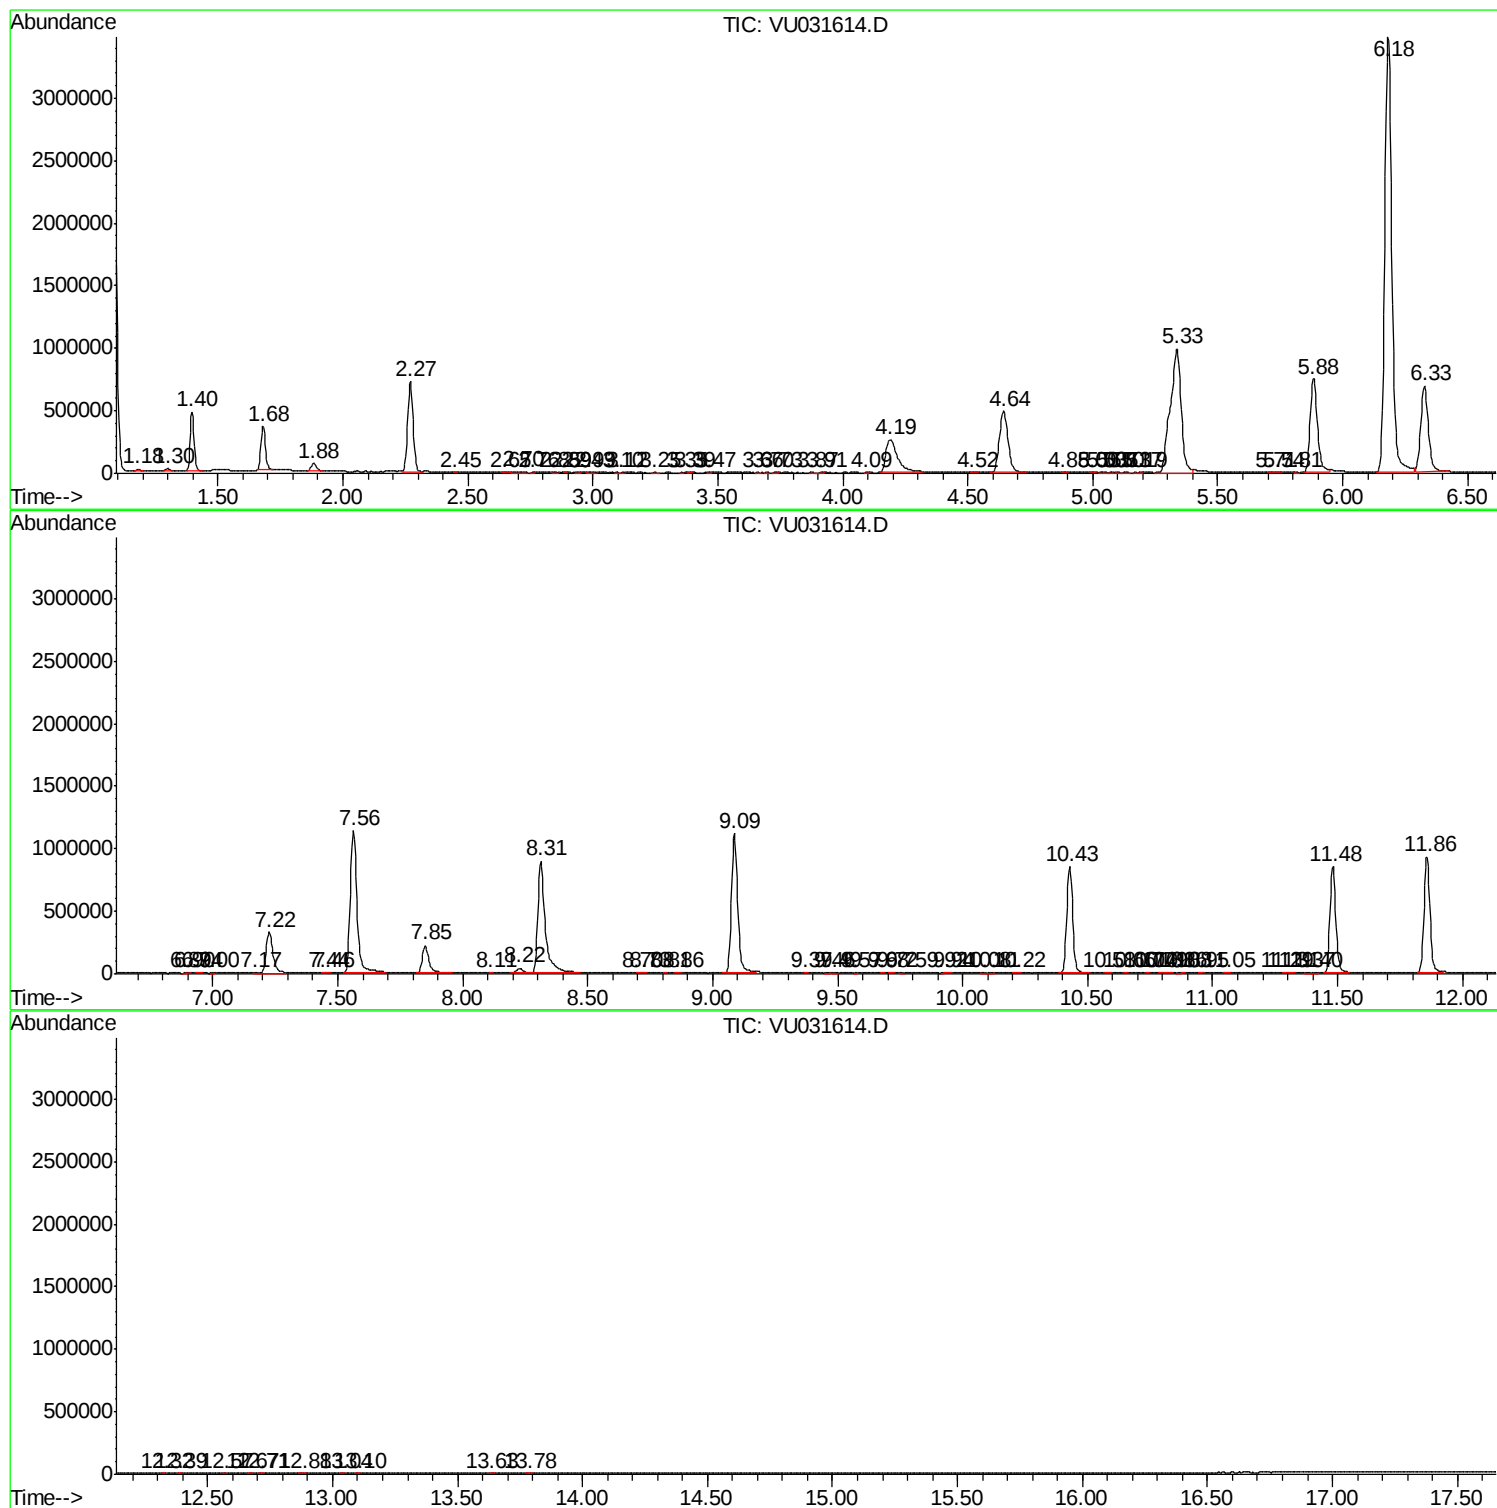

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042919\
Data File : VU031614.D
Acq On : 30 Apr 2019 02:46
Operator : JC/SP
Sample : K2593-02 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XB4

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU042919\
Data File : VU031614.D
Acq On : 30 Apr 2019 02:46
Operator : JC/SP
Sample : K2593-02 50X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
C0XB4

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc