

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031615.D
 Acq On : 30 Apr 2019 03:09
 Operator : JC/SP
 Sample : K2593-03 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XB7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	36	rVB3	14656	13577	0.13%	0.040%
2	1.395	88	95	108	rBV	485884	523436	4.85%	1.559%
3	1.678	176	183	196	rBV	374338	458241	4.24%	1.364%
4	1.884	239	247	262	rVB	89012	123137	1.14%	0.367%
5	2.270	356	367	380	rBV	752288	1146862	10.62%	3.415%
6	2.463	424	427	429	rBV2	1458	989	0.01%	0.003%
7	2.598	461	469	470	rBV7	999	1251	0.01%	0.004%
8	2.698	494	500	512	rVB5	5772	11028	0.10%	0.033%
9	2.852	545	548	552	rVB2	1397	980	0.01%	0.003%
10	2.968	580	584	585	rBV4	1616	1181	0.01%	0.004%
11	2.984	585	589	596	rVB7	2725	3459	0.03%	0.010%
12	3.022	596	601	603	rBV2	1092	928	0.01%	0.003%
13	3.109	622	628	631	rBV4	768	852	0.01%	0.003%
14	3.157	636	643	644	rBV4	1088	1082	0.01%	0.003%
15	3.215	656	661	670	rBV6	1417	2231	0.02%	0.007%
16	3.331	693	697	701	rVB4	1366	1205	0.01%	0.004%
17	3.370	707	709	713	rVB2	1597	952	0.01%	0.003%
18	3.411	719	722	725	rVB3	1234	799	0.01%	0.002%
19	3.434	725	729	731	rBV2	1166	813	0.01%	0.002%
20	3.479	738	743	745	rBV2	876	777	0.01%	0.002%
21	3.511	750	753	755	rBV3	1115	801	0.01%	0.002%
22	3.601	778	781	788	rVB4	721	805	0.01%	0.002%
23	3.707	811	814	818	rBV4	1284	1004	0.01%	0.003%
24	3.736	818	823	828	rBV3	1302	1511	0.01%	0.004%
25	3.788	836	839	843	rVB3	1205	1020	0.01%	0.003%
26	3.829	849	852	856	rVB3	1034	770	0.01%	0.002%
27	3.858	856	861	864	rBV3	1269	1194	0.01%	0.004%
28	3.891	867	871	874	rVB2	1123	852	0.01%	0.003%
29	3.916	874	879	880	rBV2	1131	786	0.01%	0.002%
30	3.971	894	896	900	rBV2	1131	884	0.01%	0.003%
31	4.055	918	922	926	rBV4	943	794	0.01%	0.002%
32	4.112	935	940	943	rBV2	995	914	0.01%	0.003%
33	4.186	951	963	1003	rBV	277707	894703	8.29%	2.664%
34	4.518	1064	1066	1071	rVB2	2067	1591	0.01%	0.005%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031615.D
 Acq On : 30 Apr 2019 03:09
 Operator : JC/SP
 Sample : K2593-03 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XB7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	4.643	1088	1105	1135	rBV	515956	1240203	11.48%	3.693%
36	4.929	1192	1194	1199	rVB4	1328	920	0.01%	0.003%
37	4.952	1199	1201	1203	rBV2	1572	887	0.01%	0.003%
38	5.180	1269	1272	1275	rVB2	1252	863	0.01%	0.003%
39	5.218	1281	1284	1288	rBV2	1385	1285	0.01%	0.004%
40	5.334	1297	1320	1361	rBV2	1038763	3174871	29.40%	9.454%
41	5.595	1398	1401	1405	rVB	2487	2128	0.02%	0.006%
42	5.620	1405	1409	1415	rVB6	1657	1993	0.02%	0.006%
43	5.649	1415	1418	1420	rVB2	1529	891	0.01%	0.003%
44	5.665	1420	1423	1425	rBV4	1113	752	0.01%	0.002%
45	5.704	1432	1435	1440	rVB4	1855	1566	0.01%	0.005%
46	5.746	1445	1448	1451	rVB3	1786	1070	0.01%	0.003%
47	5.810	1463	1468	1470	rBV5	1090	1019	0.01%	0.003%
48	5.884	1475	1491	1520	rBV2	794642	1665080	15.42%	4.958%
49	6.180	1568	1583	1616	rBV	5466699	10798662	100.00%	32.155%
50	6.328	1618	1629	1654	rVB	717179	1491345	13.81%	4.441%
51	6.878	1797	1800	1806	rBV4	1855	1535	0.01%	0.005%
52	6.916	1809	1812	1815	rVV4	1375	1047	0.01%	0.003%
53	6.980	1829	1832	1836	rVB4	1270	1132	0.01%	0.003%
54	7.122	1872	1876	1880	rBV3	977	855	0.01%	0.003%
55	7.225	1894	1908	1935	rBV	344528	655296	6.07%	1.951%
56	7.460	1979	1981	1988	rVB3	3164	3132	0.03%	0.009%
57	7.501	1991	1994	1996	rBV3	1359	965	0.01%	0.003%
58	7.562	2000	2013	2033	rBV	1213888	2221490	20.57%	6.615%
59	7.849	2090	2102	2122	rBV2	231743	426414	3.95%	1.270%
60	8.103	2179	2181	2184	rVB4	1523	791	0.01%	0.002%
61	8.125	2185	2188	2193	rVB3	1688	1539	0.01%	0.005%
62	8.151	2193	2196	2199	rBV	1784	991	0.01%	0.003%
63	8.225	2209	2219	2234	rBV4	69274	126562	1.17%	0.377%
64	8.312	2235	2246	2291	rVV	918707	1875086	17.36%	5.583%
65	8.836	2407	2409	2413	rVB4	1733	1124	0.01%	0.003%
66	8.861	2413	2417	2418	rBV	1259	886	0.01%	0.003%
67	8.894	2423	2427	2435	rBV5	1824	2779	0.03%	0.008%
68	9.086	2474	2487	2515	rBV	1177485	2063703	19.11%	6.145%
69	9.537	2623	2627	2630	rBV4	1356	1513	0.01%	0.005%
70	9.646	2657	2661	2663	rBV3	1722	1203	0.01%	0.004%
71	9.697	2671	2677	2682	rVB4	1195	1378	0.01%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031615.D
 Acq On : 30 Apr 2019 03:09
 Operator : JC/SP
 Sample : K2593-03 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XB7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	9.730	2682	2687	2689	rBV4	988	880	0.01%	0.003%
73	9.771	2697	2700	2703	rBV4	1284	903	0.01%	0.003%
74	9.820	2712	2715	2718	rBV2	1561	960	0.01%	0.003%
75	9.919	2743	2746	2751	rBV4	720	774	0.01%	0.002%
76	9.993	2766	2769	2772	rBV3	1308	1054	0.01%	0.003%
77	10.038	2780	2783	2786	rBV3	1048	745	0.01%	0.002%
78	10.080	2794	2796	2799	rVB3	1412	816	0.01%	0.002%
79	10.427	2892	2904	2927	rVV	875951	1414173	13.10%	4.211%
80	10.546	2938	2941	2950	rVB2	2822	3373	0.03%	0.010%
81	10.588	2950	2954	2955	rBV2	1412	937	0.01%	0.003%
82	10.646	2969	2972	2974	rBV2	1682	1067	0.01%	0.003%
83	10.726	2994	2997	3001	rVB2	2223	1304	0.01%	0.004%
84	10.826	3025	3028	3033	rVB3	1438	1024	0.01%	0.003%
85	10.987	3075	3078	3080	rBV	1345	747	0.01%	0.002%
86	11.016	3084	3087	3090	rBV2	1556	1133	0.01%	0.003%
87	11.086	3106	3109	3117	rVB4	2004	2411	0.02%	0.007%
88	11.218	3147	3150	3153	rBV2	1340	1025	0.01%	0.003%
89	11.479	3220	3231	3255	rBV	914302	1504932	13.94%	4.481%
90	11.855	3336	3348	3371	rBV	990842	1657177	15.35%	4.935%
91	12.180	3445	3449	3453	rBV3	2298	2189	0.02%	0.007%
92	12.311	3487	3490	3494	rBV5	1749	1443	0.01%	0.004%
93	12.392	3513	3515	3517	rBV3	1533	935	0.01%	0.003%
94	12.575	3569	3572	3575	rBV3	1696	1338	0.01%	0.004%
95	12.720	3615	3617	3620	rVB3	1459	797	0.01%	0.002%
96	12.749	3621	3626	3628	rBV3	1489	1515	0.01%	0.005%
97	13.324	3802	3805	3807	rBV2	1332	879	0.01%	0.003%
98	13.405	3827	3830	3832	rBV3	1679	983	0.01%	0.003%
99	14.517	4173	4176	4179	rBV3	2345	1988	0.02%	0.006%
100	14.729	4239	4242	4244	rBV2	1739	1284	0.01%	0.004%


Sum of corrected areas: 33583151

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042919\
Data File : VU031615.D
Acq On : 30 Apr 2019 03:09
Operator : JC/SP
Sample : K2593-03 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XB7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

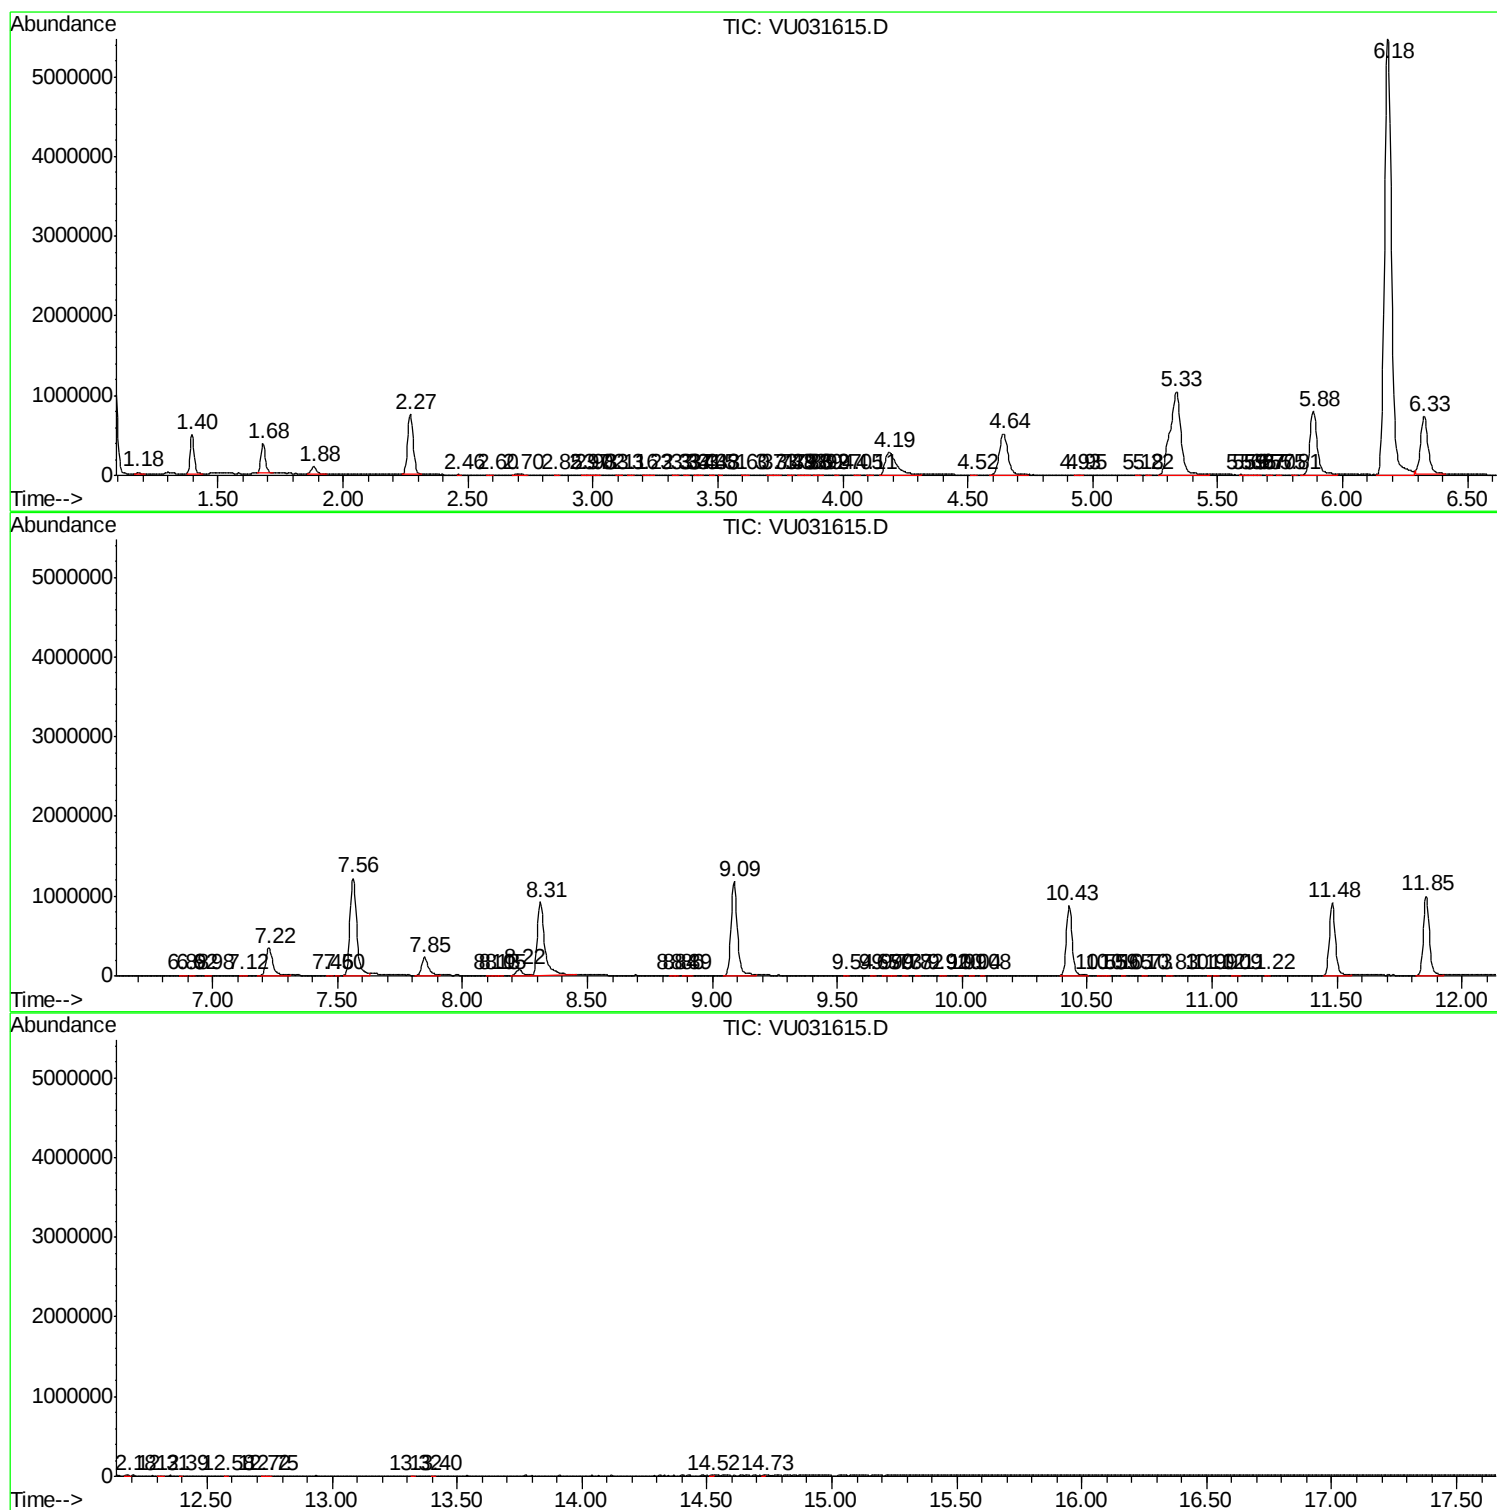

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042919\
Data File : VU031615.D
Acq On : 30 Apr 2019 03:09
Operator : JC/SP
Sample : K2593-03 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XB7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU042919\
Data File : VU031615.D
Acq On : 30 Apr 2019 03:09
Operator : JC/SP
Sample : K2593-03 50X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 48 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
C0XB7

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc