

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031617.D
 Acq On : 30 Apr 2019 03:55
 Operator : JC/SP
 Sample : K2593-05 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XD7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.180	24	28	34	rVB2	16684	14770	0.01%	0.011%
2	1.396	88	95	107	rBV	492703	524968	0.47%	0.375%
3	1.678	176	183	195	rBV	360886	445069	0.40%	0.318%
4	1.881	237	246	263	rVB	696603	961589	0.86%	0.688%
5	2.267	356	366	381	rVB	735374	1126923	1.00%	0.806%
6	2.453	420	424	425	rBV4	2125	1503	0.00%	0.001%
7	2.617	472	475	478	rVB3	1292	731	0.00%	0.001%
8	2.637	478	481	491	rVB7	1915	2045	0.00%	0.001%
9	2.701	491	501	515	rVB4	9465	16456	0.01%	0.012%
10	2.768	519	522	526	rVB3	1416	1157	0.00%	0.001%
11	2.820	534	538	546	rVB8	2106	2716	0.00%	0.002%
12	2.855	546	549	555	rBV6	2156	2268	0.00%	0.002%
13	2.974	581	586	588	rBV3	3876	3435	0.00%	0.002%
14	3.148	634	640	642	rBV5	948	785	0.00%	0.001%
15	3.228	663	665	668	rVB3	1244	733	0.00%	0.001%
16	3.270	675	678	687	rBV2	1879	2015	0.00%	0.001%
17	3.444	730	732	735	rVV2	1546	1015	0.00%	0.001%
18	3.466	735	739	747	rVB4	1826	2191	0.00%	0.002%
19	3.502	747	750	753	rBV2	1148	863	0.00%	0.001%
20	3.530	757	759	763	rVV2	1180	835	0.00%	0.001%
21	3.595	774	779	782	rBV2	1560	1177	0.00%	0.001%
22	3.630	787	790	797	rVB	1184	1269	0.00%	0.001%
23	3.739	820	824	826	rVV3	1261	752	0.00%	0.001%
24	3.794	837	841	852	rVB3	2003	3149	0.00%	0.002%
25	4.083	928	931	933	rBV2	933	730	0.00%	0.001%
26	4.100	933	936	941	rVB	980	874	0.00%	0.001%
27	4.186	951	963	997	rBV	291196	944931	0.84%	0.676%
28	4.437	1037	1041	1047	rVB5	2276	2341	0.00%	0.002%
29	4.582	1082	1086	1088	rBV3	1320	1122	0.00%	0.001%
30	4.643	1088	1105	1128	rVV	523223	1238772	1.10%	0.886%
31	4.984	1207	1211	1215	rBV5	1587	1457	0.00%	0.001%
32	5.135	1239	1258	1271	rBV3	15852	39642	0.04%	0.028%
33	5.334	1293	1320	1350	rBV2	1047038	3176628	2.83%	2.272%
34	5.585	1395	1398	1400	rBV4	1435	850	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031617.D
 Acq On : 30 Apr 2019 03:55
 Operator : JC/SP
 Sample : K2593-05 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XD7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

35	5.694	1429	1432	1436	rVB4	1440	1057	0.00%	0.001%
36	5.714	1436	1438	1443	rVB5	1277	1177	0.00%	0.001%
37	5.743	1443	1447	1448	rBV3	2102	1248	0.00%	0.001%
38	5.881	1476	1490	1519	rBV	796376	1659242	1.48%	1.187%
39	6.112	1559	1562	1566	rVB5	1767	1003	0.00%	0.001%
40	6.183	1566	1584	1618	rBV3	57380939	112198375	100.00%	80.246%
41	6.325	1621	1628	1661	rVB	806215	1806859	1.61%	1.292%
42	6.865	1793	1796	1802	rBV6	2187	2625	0.00%	0.002%
43	6.952	1820	1823	1825	rBV4	1271	963	0.00%	0.001%
44	7.058	1853	1856	1861	rVB4	1755	1406	0.00%	0.001%
45	7.112	1867	1873	1874	rBV3	932	915	0.00%	0.001%
46	7.177	1890	1893	1896	rBV3	1693	1005	0.00%	0.001%
47	7.225	1896	1908	1932	rBV	358513	670279	0.60%	0.479%
48	7.501	1991	1994	1997	rVB4	1359	837	0.00%	0.001%
49	7.562	1997	2013	2030	rBV	1201855	2207417	1.97%	1.579%
50	7.849	2090	2102	2126	rBV	238216	443525	0.40%	0.317%
51	8.070	2165	2171	2183	rVB10	5453	9359	0.01%	0.007%
52	8.116	2183	2185	2188	rVB4	1944	1187	0.00%	0.001%
53	8.138	2188	2192	2194	rBV4	1686	1284	0.00%	0.001%
54	8.222	2203	2218	2236	rBV	1844321	3229858	2.88%	2.310%
55	8.312	2236	2246	2287	rVB	986050	2003731	1.79%	1.433%
56	8.884	2419	2424	2428	rBV5	1352	1530	0.00%	0.001%
57	8.919	2433	2435	2437	rBV3	1382	811	0.00%	0.001%
58	9.032	2467	2470	2473	rBV2	1803	1211	0.00%	0.001%
59	9.087	2475	2487	2529	rBV	1184548	2107046	1.88%	1.507%
60	9.257	2534	2540	2551	rVB4	9088	15400	0.01%	0.011%
61	9.376	2566	2577	2594	rBV	34437	61182	0.05%	0.044%
62	9.720	2681	2684	2689	rBV4	1884	1578	0.00%	0.001%
63	9.781	2694	2703	2716	rBV2	28105	47337	0.04%	0.034%
64	10.019	2774	2777	2782	rVB4	1586	1316	0.00%	0.001%
65	10.128	2809	2811	2816	rVB3	2069	1456	0.00%	0.001%
66	10.164	2816	2822	2824	rBV4	4460	4694	0.00%	0.003%
67	10.273	2852	2856	2858	rBV	865	728	0.00%	0.001%
68	10.302	2863	2865	2869	rVB3	1573	1126	0.00%	0.001%
69	10.324	2869	2872	2875	rBV2	1932	1401	0.00%	0.001%
70	10.347	2875	2879	2883	rVB4	1275	1305	0.00%	0.001%
71	10.369	2883	2886	2890	rBV4	1082	1024	0.00%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
 Data File : VU031617.D
 Acq On : 30 Apr 2019 03:55
 Operator : JC/SP
 Sample : K2593-05 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0XD7

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis

72	10.427	2891	2904	2928	rBV	887835	1447206	1.29%	1.035%
73	10.588	2950	2954	2955	rBV3	2353	1738	0.00%	0.001%
74	10.652	2970	2974	2975	rBV3	1193	839	0.00%	0.001%
75	10.685	2975	2984	2998	rVV6	11473	24306	0.02%	0.017%
76	10.765	3002	3009	3012	rBV7	4483	5287	0.00%	0.004%
77	10.971	3065	3073	3086	rVB4	11511	18727	0.02%	0.013%
78	11.099	3109	3113	3116	rBV3	2025	2043	0.00%	0.001%
79	11.148	3121	3128	3138	rVB4	19985	31871	0.03%	0.023%
80	11.241	3155	3157	3160	rVB2	1892	892	0.00%	0.001%
81	11.260	3160	3163	3167	rBV3	2238	1802	0.00%	0.001%
82	11.482	3219	3232	3252	rBV	937222	1542395	1.37%	1.103%
83	11.569	3253	3259	3269	rVB2	26947	40679	0.04%	0.029%
84	11.855	3336	3348	3371	rBV	993035	1660705	1.48%	1.188%
85	12.234	3464	3466	3468	rBV3	1331	803	0.00%	0.001%
86	12.402	3515	3518	3521	rBV	1389	861	0.00%	0.001%
87	12.668	3598	3601	3603	rBV3	1370	891	0.00%	0.001%
88	12.935	3681	3684	3686	rBV2	2451	1644	0.00%	0.001%
89	13.118	3738	3741	3747	rVB4	1732	1864	0.00%	0.001%
90	13.279	3788	3791	3795	rBV3	1649	1237	0.00%	0.001%
91	13.501	3856	3860	3863	rBV2	1994	1719	0.00%	0.001%
92	13.681	3912	3916	3922	rBV3	2414	2824	0.00%	0.002%
93	13.710	3922	3925	3928	rVB2	1552	943	0.00%	0.001%
94	13.736	3930	3933	3935	rBV2	1324	840	0.00%	0.001%
95	13.810	3952	3956	3958	rBV4	1517	1319	0.00%	0.001%
96	14.032	4022	4025	4027	rBV2	1479	881	0.00%	0.001%
97	14.491	4165	4168	4170	rBV	2178	1483	0.00%	0.001%
98	14.768	4252	4254	4256	rBV3	1362	802	0.00%	0.001%
99	14.807	4262	4266	4269	rBV3	1976	1548	0.00%	0.001%
100	15.202	4386	4389	4392	rBV3	1993	1444	0.00%	0.001%


Sum of corrected areas: 139817851

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042919\
Data File : VU031617.D
Acq On : 30 Apr 2019 03:55
Operator : JC/SP
Sample : K2593-05 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XD7

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

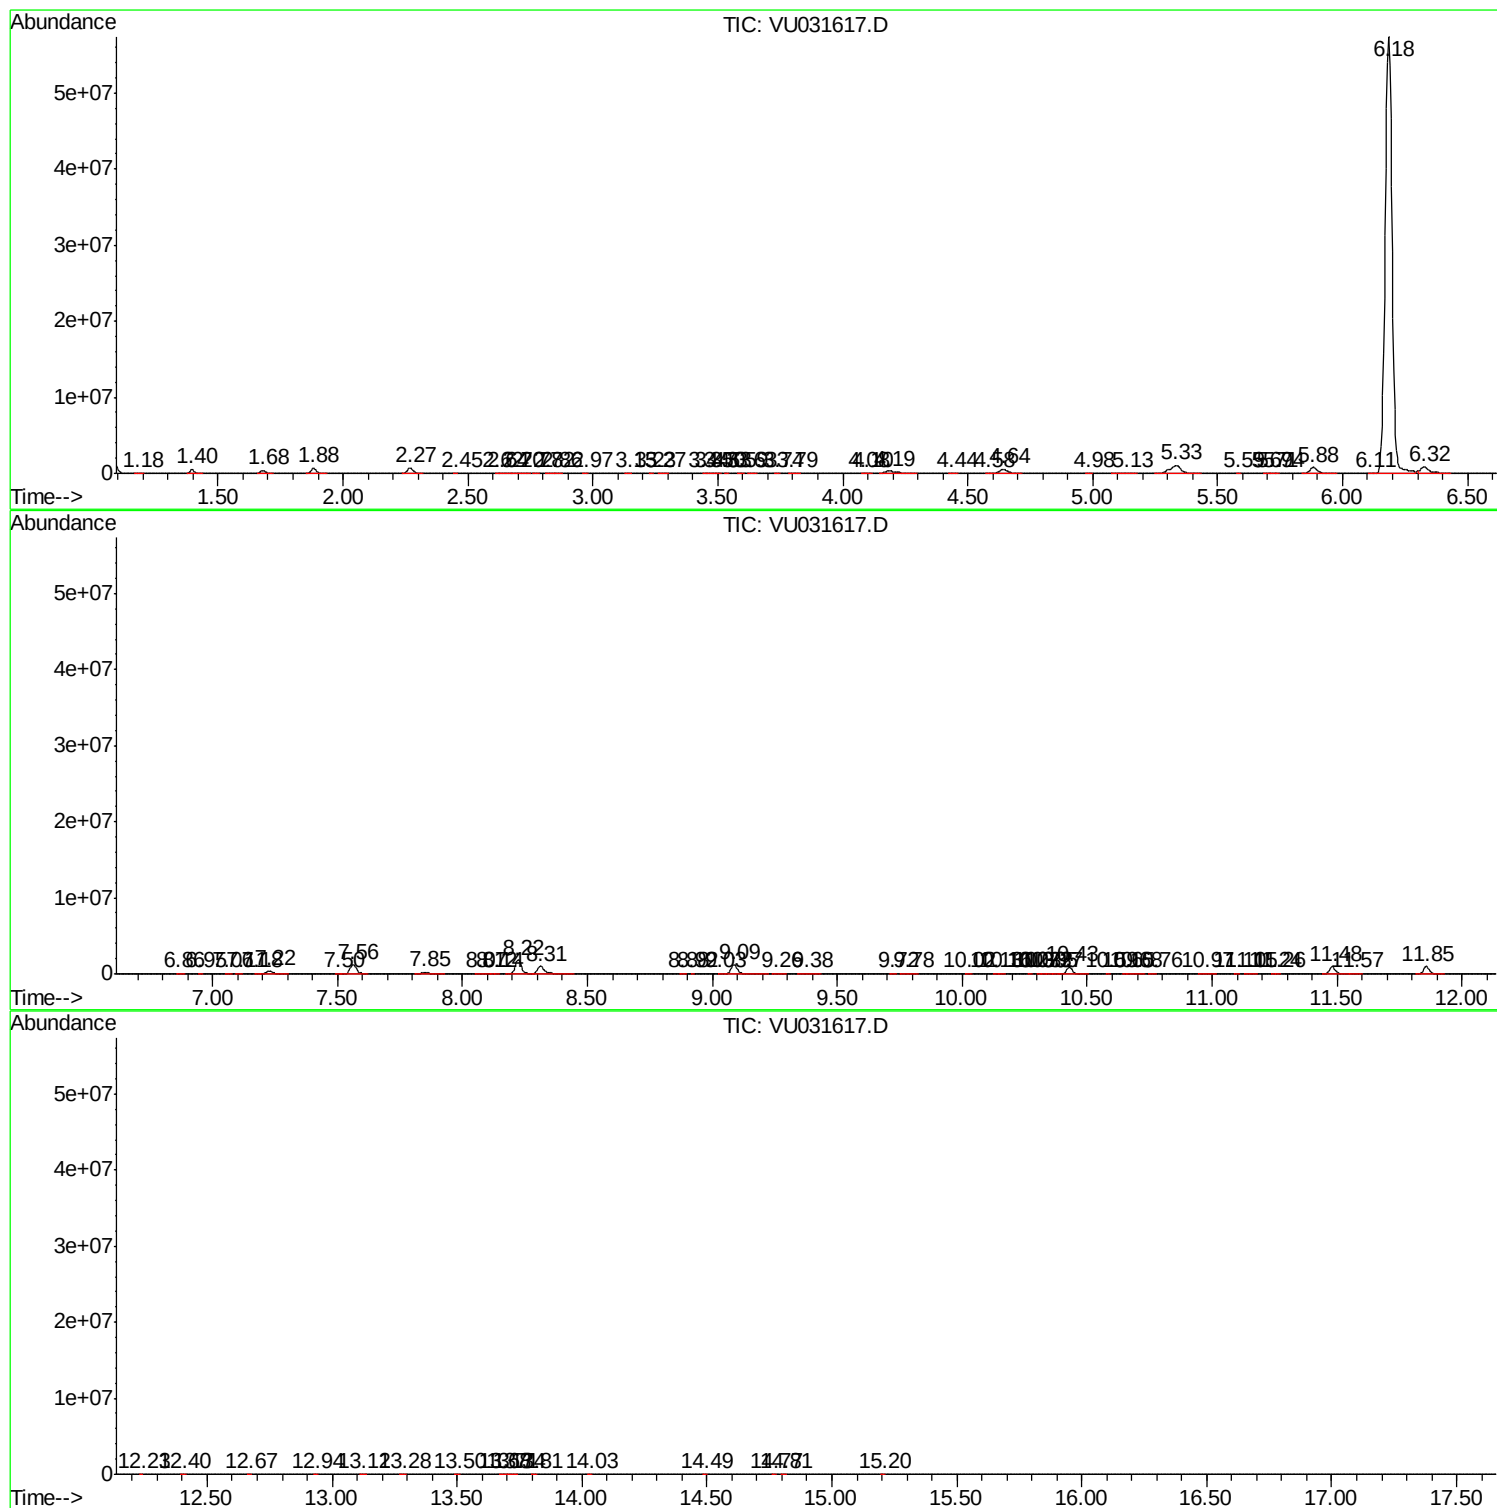

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042919\
Data File : VU031617.D
Acq On : 30 Apr 2019 03:55
Operator : JC/SP
Sample : K2593-05 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XD7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042919\
Data File : VU031617.D
Acq On : 30 Apr 2019 03:55
Operator : JC/SP
Sample : K2593-05 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0XD7

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc