


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU042919\
 Data File : VU031570.D
 Acq On : 29 Apr 2019 08:50
 Operator : JC/SP
 Sample : BFB33
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB33

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042719WMA.M
 Title : VOC Analysis
 Last Update : Tue Apr 30 04:50:11 2019

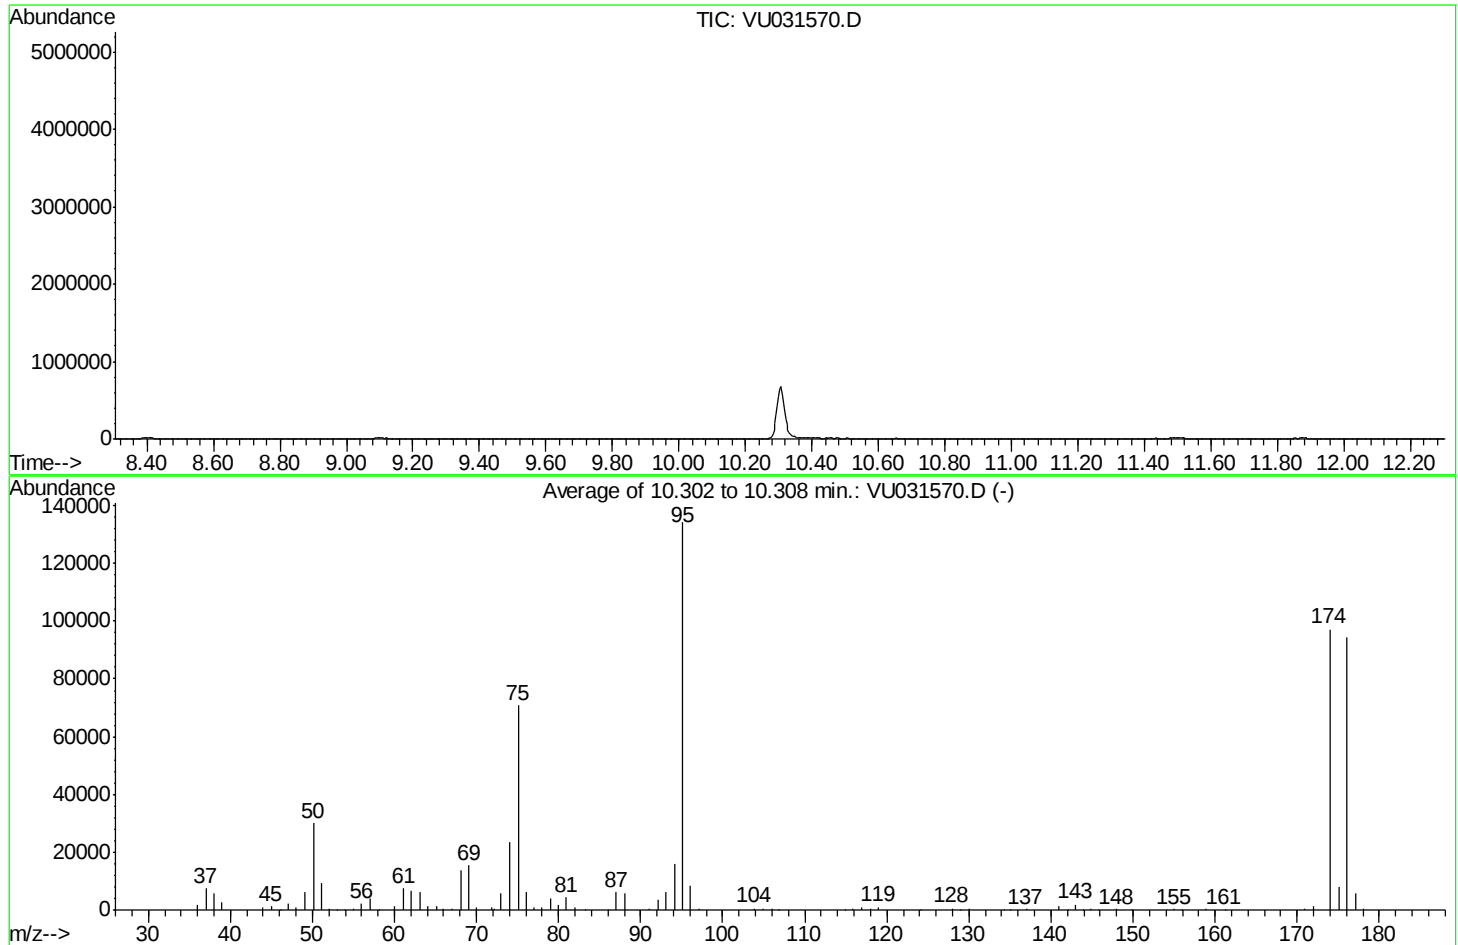

AutoFind: Scans 2865, 2866, 2867; Background Corrected with Scan 2853

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.3	29992	PASS
75	95	30	80	52.7	70704	PASS
95	95	100	100	100.0	134194	PASS
96	95	5	9	6.2	8301	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.4	97173	PASS
175	174	5	9	8.2	7974	PASS
176	174	95	101	97.3	94552	PASS
177	176	5	9	6.2	5852	PASS

Scan 2853 (10.263 min): VU031570.D
BFB33

m/z	Abundance
39.00	120.0
40.00	6027.0
42.90	141.0
43.90	794.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33

m/z	Abundance
36.00	1376.0
37.00	7317.0
38.00	6115.0
39.00	2951.0
40.00	6267.0
42.90	132.0
43.90	1776.0
45.00	1282.0
46.10	166.0
47.10	2060.0
48.10	855.0
49.10	6053.0
50.10	29784.0
51.10	9758.0
52.10	496.0
52.90	135.0
55.00	325.0
56.00	2096.0
57.10	3840.0
58.00	163.0
60.00	1277.0
61.10	7615.0
62.00	6281.0
63.00	6269.0
64.00	1156.0
65.10	1288.0
66.00	363.0
67.00	470.0
68.10	13570.0
69.10	15070.0
70.00	1174.0
71.90	842.0
73.00	5439.0
74.10	23320.0
75.10	69168.0
76.10	5946.0
77.10	835.0
77.90	819.0
78.90	3898.0
80.00	1439.0
80.90	4480.0
82.00	766.0
83.20	222.0
86.10	199.0
87.00	5626.0
88.00	5578.0
91.10	680.0
92.10	3709.0
93.00	6104.0
94.10	16053.0
95.10	130776.0
96.10	8267.0
97.10	366.0
104.00	554.0
105.00	259.0
105.90	393.0
114.90	125.0
115.90	408.0
117.00	785.0
117.90	505.0
119.00	1018.0
128.10	700.0
128.90	197.0
129.90	467.0
135.00	229.0
137.00	307.0
141.00	1427.0
142.10	211.0
143.00	1853.0
143.90	159.0
144.80	698.0
145.80	127.0
148.00	409.0
149.90	263.0
155.10	274.0
158.90	224.0
161.10	137.0
170.90	363.0
172.00	1291.0
174.00	92664.0
175.00	7631.0
176.00	89976.0
177.10	5748.0
178.10	361.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33

m/z	Abundance
36.00	1788.0
37.10	7757.0
38.10	6197.0
39.00	2869.0
40.00	6037.0
42.90	134.0
43.90	1775.0
45.00	1218.0
46.10	244.0
47.10	2288.0
48.10	676.0
49.10	6424.0
50.10	31056.0
51.10	9351.0
52.10	570.0
52.90	180.0
55.00	335.0
56.00	2242.0
57.00	4064.0
58.00	208.0
60.00	1274.0
61.10	7718.0
62.00	6579.0
63.10	6587.0
64.00	1197.0
65.10	1597.0
66.00	484.0
67.10	445.0
68.10	14189.0
69.10	16193.0
70.10	1101.0
71.90	909.0
73.00	6099.0
74.10	23944.0
75.10	73160.0
76.10	6510.0
77.10	757.0
78.00	899.0
78.90	4227.0
80.00	1643.0
81.00	4617.0
81.90	704.0
83.20	207.0
86.10	216.0
87.00	6333.0
88.00	5909.0
91.10	642.0
92.10	3843.0
93.10	6507.0
94.10	16354.0
95.10	138112.0
96.10	8476.0
97.10	371.0
103.80	638.0
105.00	251.0
106.00	549.0
106.70	122.0
115.00	103.0
115.90	544.0
117.00	816.0
118.00	496.0
119.00	1017.0
128.00	521.0
129.00	190.0
130.00	466.0
134.20	140.0
135.10	268.0
137.00	306.0
141.00	1496.0
142.10	228.0
143.00	2092.0
144.90	649.0
145.80	204.0
148.00	326.0
149.90	192.0
155.00	314.0
155.90	122.0
158.90	260.0
161.20	101.0
170.90	433.0
172.00	1440.0
174.00	100576.0
175.00	8104.0
176.00	98120.0
177.00	5990.0
178.00	254.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33

m/z	Abundance
36.00	1934.0
37.10	7309.0
38.10	5674.0
39.00	2749.0
40.00	5623.0
42.90	149.0
44.00	1844.0
44.90	1125.0
46.20	227.0
47.10	2077.0
48.00	684.0
49.10	6018.0
50.10	29136.0
51.00	8390.0
52.10	523.0
52.90	176.0
53.90	105.0
55.00	379.0
56.00	2071.0
57.00	3888.0
58.10	178.0
60.00	1310.0
61.10	6917.0
62.00	6518.0
63.10	6383.0
64.00	1095.0
65.10	1594.0
66.00	445.0
67.00	367.0
68.10	13626.0
69.10	14845.0
70.10	959.0
71.90	793.0
72.20	778.0
73.00	6219.0
74.00	22624.0
75.10	69784.0
76.10	6320.0
76.90	695.0
78.00	842.0
79.00	4255.0
80.00	1701.0
80.90	4160.0
82.00	816.0
83.20	123.0
86.10	212.0
87.00	6049.0
88.00	5380.0
91.10	568.0
92.10	3496.0
93.00	6077.0
94.10	15773.0
95.10	133696.0
96.10	8161.0
97.10	353.0
103.80	637.0
104.90	247.0
106.00	639.0
106.80	129.0
115.90	595.0
117.00	869.0
118.00	478.0
119.00	927.0
124.10	117.0
127.90	385.0
129.00	161.0
130.10	499.0
134.20	134.0
135.00	221.0
137.00	313.0
141.00	1259.0
142.10	198.0
143.00	2062.0
145.00	544.0
145.80	188.0
148.00	259.0
149.90	143.0
154.00	124.0
154.90	454.0
155.90	131.0
158.90	246.0
170.90	438.0
172.00	1555.0
174.00	98280.0
175.10	8187.0
176.00	95560.0
177.10	5820.0
178.00	115.0

Instrument :
MSVOA_U
ClientSampleId :
BFB33