

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042920\
 Data File : VU037912.D
 Acq On : 29 Apr 2020 15:28
 Operator : JC/MD
 Sample : L2395-15DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DA0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.613	77	85	94	rBV	324245	348498	10.41%	1.462%
2	1.929	175	183	196	rVB	270755	350755	10.48%	1.472%
3	2.591	376	389	408	rBV2	530893	945242	28.25%	3.966%
4	2.703	422	424	426	rBV3	885	495	0.01%	0.002%
5	2.861	471	473	477	rBV3	822	750	0.02%	0.003%
6	3.019	518	522	524	rBV2	591	392	0.01%	0.002%
7	3.076	528	540	557	rVV2	29581	55598	1.66%	0.233%
8	3.218	573	584	598	rVB2	11088	26256	0.78%	0.110%
9	3.379	628	634	636	rBV4	1721	1928	0.06%	0.008%
10	3.437	648	652	655	rBV3	491	391	0.01%	0.002%
11	3.478	663	665	670	rVB3	738	602	0.02%	0.003%
12	3.511	670	675	678	rBV3	750	728	0.02%	0.003%
13	3.588	695	699	703	rVB2	533	359	0.01%	0.002%
14	3.610	703	706	710	rBV3	391	385	0.01%	0.002%
15	3.649	716	718	722	rVB3	507	372	0.01%	0.002%
16	3.813	766	769	774	rBV2	571	366	0.01%	0.002%
17	3.838	775	777	786	rVB3	572	499	0.01%	0.002%
18	3.880	786	790	791	rBV2	722	418	0.01%	0.002%
19	3.909	796	799	802	rBV3	934	801	0.02%	0.003%
20	3.977	817	820	829	rVB2	879	683	0.02%	0.003%
21	4.015	829	832	838	rBV2	586	647	0.02%	0.003%
22	4.067	844	848	850	rBV	555	404	0.01%	0.002%
23	4.131	861	868	871	rBV3	515	671	0.02%	0.003%
24	4.179	879	883	885	rVV2	614	492	0.01%	0.002%
25	4.208	889	892	896	rVV2	540	506	0.02%	0.002%
26	4.501	979	983	986	rBV3	587	491	0.01%	0.002%
27	4.572	1003	1005	1014	rVB5	445	495	0.01%	0.002%
28	4.665	1016	1034	1065	rBV2	319947	817198	24.42%	3.429%
29	4.993	1133	1136	1138	rBV3	626	389	0.01%	0.002%
30	5.102	1152	1170	1195	rBV	448650	973929	29.11%	4.087%
31	5.272	1219	1223	1228	rVB2	765	582	0.02%	0.002%
32	5.353	1231	1248	1262	rBV2	71366	163071	4.87%	0.684%
33	5.562	1310	1313	1314	rBV	783	420	0.01%	0.002%
34	5.594	1318	1323	1326	rVB2	403	457	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042920\
 Data File : VU037912.D
 Acq On : 29 Apr 2020 15:28
 Operator : JC/MD
 Sample : L2395-15DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DA0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

35	5.620	1326	1331	1337	rBV2	591	822	0.02%	0.003%
36	5.758	1351	1374	1407	rBV2	965085	2586377	77.29%	10.853%
37	6.006	1448	1451	1459	rBV6	666	753	0.02%	0.003%
38	6.131	1487	1490	1492	rBV2	945	643	0.02%	0.003%
39	6.279	1521	1536	1567	rVV	773419	1500159	44.83%	6.295%
40	6.433	1580	1584	1587	rVB3	637	577	0.02%	0.002%
41	6.571	1608	1627	1654	rBV	1796176	3346258	100.00%	14.041%
42	6.723	1660	1674	1694	rVB	608937	1190243	35.57%	4.994%
43	7.022	1764	1767	1773	rVB2	728	733	0.02%	0.003%
44	7.137	1800	1803	1807	rVB3	507	463	0.01%	0.002%
45	7.208	1816	1825	1835	rVB6	2512	4737	0.14%	0.020%
46	7.494	1910	1914	1919	rBV2	407	365	0.01%	0.002%
47	7.591	1930	1944	1960	rBV	312033	539281	16.12%	2.263%
48	7.922	2032	2047	2081	rVV	1151684	2113989	63.17%	8.871%
49	8.112	2103	2106	2111	rVB5	816	637	0.02%	0.003%
50	8.202	2120	2134	2148	rBV	224435	366120	10.94%	1.536%
51	8.420	2196	2202	2203	rBV3	1280	1045	0.03%	0.004%
52	8.491	2216	2224	2230	rBV5	1382	1666	0.05%	0.007%
53	8.575	2242	2250	2261	rBV6	3396	5263	0.16%	0.022%
54	8.655	2261	2275	2313	rBV	846386	1574360	47.05%	6.606%
55	8.935	2352	2362	2375	rVV10	4295	9158	0.27%	0.038%
56	9.054	2393	2399	2400	rBV3	454	437	0.01%	0.002%
57	9.179	2431	2438	2446	rVB4	869	1283	0.04%	0.005%
58	9.250	2451	2460	2462	rBV2	620	705	0.02%	0.003%
59	9.349	2490	2491	2495	rVB	713	408	0.01%	0.002%
60	9.436	2504	2518	2547	rBV	1109116	1901351	56.82%	7.978%
61	9.584	2561	2564	2571	rVB4	614	514	0.02%	0.002%
62	9.652	2582	2585	2587	rBV2	784	410	0.01%	0.002%
63	9.671	2587	2591	2594	rBV2	585	360	0.01%	0.002%
64	9.764	2615	2620	2622	rBV2	482	509	0.02%	0.002%
65	10.038	2696	2705	2708	rBV2	556	946	0.03%	0.004%
66	10.118	2720	2730	2741	rVB4	5318	8628	0.26%	0.036%
67	10.198	2750	2755	2757	rBV2	499	480	0.01%	0.002%
68	10.237	2761	2767	2770	rVB	410	378	0.01%	0.002%
69	10.263	2770	2775	2778	rBV4	521	525	0.02%	0.002%
70	10.391	2813	2815	2824	rVB2	487	457	0.01%	0.002%
71	10.501	2842	2849	2858	rVB3	2812	3834	0.11%	0.016%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042920\
 Data File : VU037912.D
 Acq On : 29 Apr 2020 15:28
 Operator : JC/MD
 Sample : L2395-15DL 100X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DA0DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

72	10.661	2893	2899	2902	rBV2	438	389	0.01%	0.002%
73	10.771	2920	2933	2953	rBV	822893	1303681	38.96%	5.470%
74	10.899	2971	2973	2976	rVV2	959	471	0.01%	0.002%
75	11.076	3023	3028	3032	rBV4	726	657	0.02%	0.003%
76	11.124	3034	3043	3053	rVB4	7881	12021	0.36%	0.050%
77	11.169	3054	3057	3060	rVB3	645	375	0.01%	0.002%
78	11.234	3074	3077	3082	rBV2	456	426	0.01%	0.002%
79	11.298	3094	3097	3101	rVB	706	414	0.01%	0.002%
80	11.330	3101	3107	3113	rBV4	428	656	0.02%	0.003%
81	11.423	3132	3136	3142	rBV4	990	1119	0.03%	0.005%
82	11.481	3150	3154	3160	rVB6	1028	1357	0.04%	0.006%
83	11.713	3221	3226	3228	rBV3	634	527	0.02%	0.002%
84	11.758	3228	3240	3247	rVV6	4893	7419	0.22%	0.031%
85	11.825	3247	3261	3278	rBV	1110038	1762188	52.66%	7.394%
86	12.073	3332	3338	3340	rBV3	664	678	0.02%	0.003%
87	12.205	3365	3379	3398	rBV	1165043	1852913	55.37%	7.775%
88	12.327	3415	3417	3423	rVB4	637	425	0.01%	0.002%
89	12.481	3460	3465	3469	rBV3	605	531	0.02%	0.002%
90	12.613	3502	3506	3513	rBV2	517	575	0.02%	0.002%
91	12.828	3571	3573	3578	rVB	754	532	0.02%	0.002%
92	13.005	3625	3628	3630	rBV2	586	406	0.01%	0.002%
93	13.037	3633	3638	3641	rBV4	1211	1216	0.04%	0.005%
94	13.099	3655	3657	3662	rVB	784	506	0.02%	0.002%
95	13.301	3717	3720	3724	rBV3	641	455	0.01%	0.002%
96	13.510	3781	3785	3788	rBV2	645	567	0.02%	0.002%
97	13.709	3842	3847	3850	rBV2	905	789	0.02%	0.003%
98	13.864	3887	3895	3904	rVB3	11101	16327	0.49%	0.069%
99	14.105	3968	3970	3979	rVB6	2178	3164	0.09%	0.013%
100	15.240	4321	4323	4326	rVB3	1087	508	0.02%	0.002%


Sum of corrected areas: 23831436

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042920\
Data File : VU037912.D
Acq On : 29 Apr 2020 15:28
Operator : JC/MD
Sample : L2395-15DL 100X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DA0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

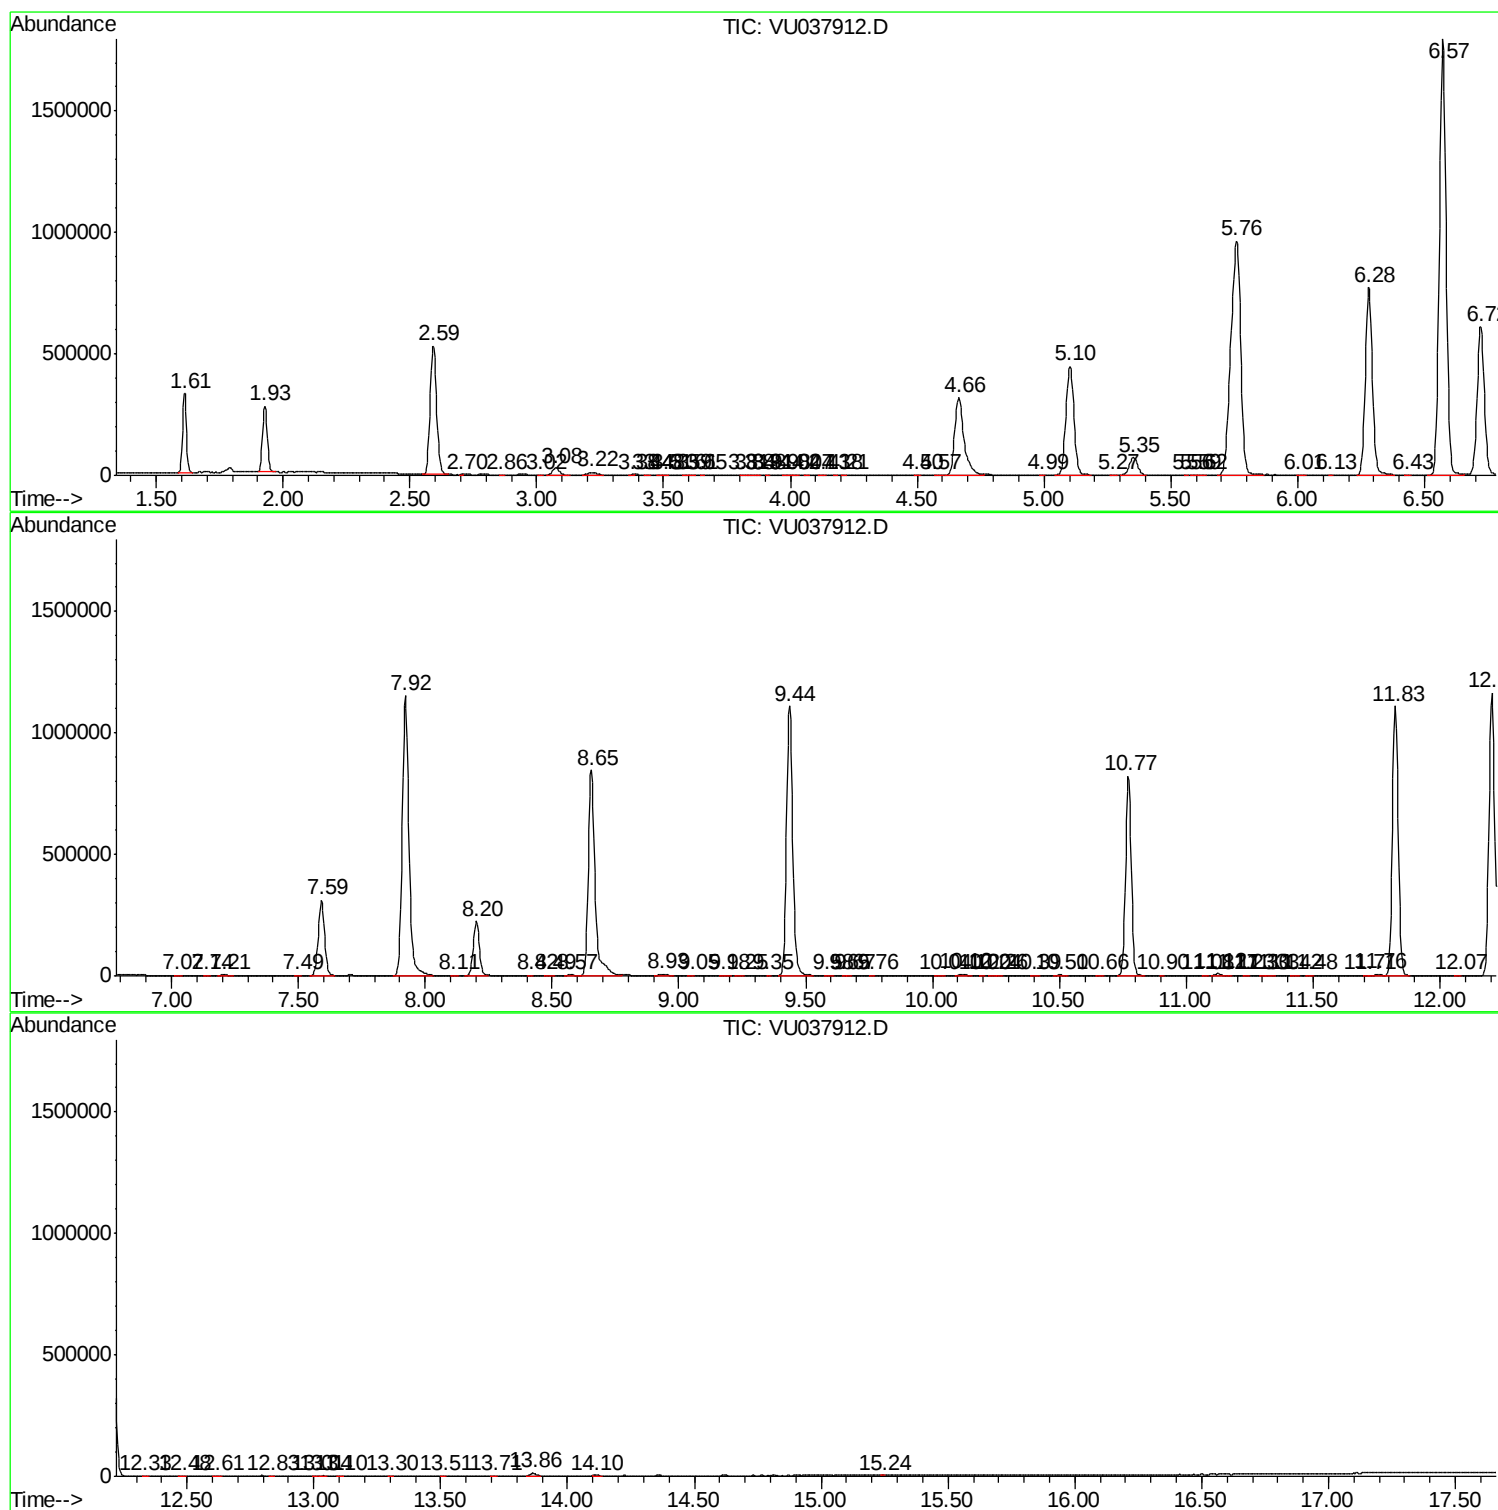

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042920\
Data File : VU037912.D
Acq On : 29 Apr 2020 15:28
Operator : JC/MD
Sample : L2395-15DL 100X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DA0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU042920\
Data File : VU037912.D
Acq On : 29 Apr 2020 15:28
Operator : JC/MD
Sample : L2395-15DL 100X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
C0DA0DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc