

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042920\
 Data File : VU037917.D
 Acq On : 29 Apr 2020 17:21
 Operator : JC/MD
 Sample : L2410-15
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBFF3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.610	78	84	98	rBV	222976	239583	6.66%	1.138%
2	1.929	175	183	197	rVB	198915	260348	7.24%	1.236%
3	2.591	377	389	402	rBV	340381	560801	15.59%	2.663%
4	2.652	403	408	419	rVB2	9342	14599	0.41%	0.069%
5	2.787	441	450	456	rBV6	3186	6129	0.17%	0.029%
6	2.867	472	475	481	rVB6	879	822	0.02%	0.004%
7	2.983	500	511	526	rVB3	4304	8738	0.24%	0.041%
8	3.064	533	536	538	rBV3	1135	807	0.02%	0.004%
9	3.160	561	566	573	rVB4	758	833	0.02%	0.004%
10	3.215	573	583	598	rVB3	3841	8670	0.24%	0.041%
11	3.285	602	605	610	rBV4	571	617	0.02%	0.003%
12	3.388	627	637	645	rBV7	2603	4952	0.14%	0.024%
13	3.552	683	688	689	rBV2	598	428	0.01%	0.002%
14	3.793	758	763	766	rBV3	483	481	0.01%	0.002%
15	3.883	780	791	793	rBV5	1413	1788	0.05%	0.008%
16	4.089	850	855	860	rBV4	933	959	0.03%	0.005%
17	4.141	868	871	878	rVB3	820	897	0.02%	0.004%
18	4.173	878	881	884	rBV3	627	475	0.01%	0.002%
19	4.346	928	935	943	rVV2	1009	1726	0.05%	0.008%
20	4.581	1005	1008	1011	rBV4	704	554	0.02%	0.003%
21	4.665	1016	1034	1037	rBV	299623	532036	14.79%	2.526%
22	4.967	1126	1128	1131	rBV3	715	448	0.01%	0.002%
23	5.047	1148	1153	1154	rBV2	1125	891	0.02%	0.004%
24	5.102	1154	1170	1188	rVV	343389	747043	20.76%	3.547%
25	5.215	1202	1205	1214	rVB6	1323	1311	0.04%	0.006%
26	5.263	1217	1220	1226	rBV4	779	846	0.02%	0.004%
27	5.324	1234	1239	1240	rBV4	1982	1475	0.04%	0.007%
28	5.414	1257	1267	1273	rBV4	1935	3531	0.10%	0.017%
29	5.758	1349	1374	1400	rBV2	714951	1940621	53.94%	9.214%
30	6.022	1453	1456	1459	rVB4	784	550	0.02%	0.003%
31	6.089	1459	1477	1479	rBV4	15894	34534	0.96%	0.164%
32	6.279	1524	1536	1574	rVB	674013	1351841	37.58%	6.419%
33	6.571	1613	1627	1646	rBV	610394	1141862	31.74%	5.422%
34	6.723	1659	1674	1697	rBV	466939	912242	25.36%	4.331%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042920\
 Data File : VU037917.D
 Acq On : 29 Apr 2020 17:21
 Operator : JC/MD
 Sample : L2410-15
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBFF3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

35	7.070	1771	1782	1795	rBV2	18534	32741	0.91%	0.155%
36	7.208	1813	1825	1837	rBV9	4012	8280	0.23%	0.039%
37	7.385	1877	1880	1884	rBV3	619	418	0.01%	0.002%
38	7.459	1900	1903	1909	rVB6	667	549	0.02%	0.003%
39	7.591	1931	1944	1961	rBV	275468	474354	13.19%	2.252%
40	7.706	1973	1980	1985	rBV5	3013	4109	0.11%	0.020%
41	7.764	1994	1998	2003	rVB6	1808	1908	0.05%	0.009%
42	7.922	2030	2047	2065	rBV	849979	1524430	42.37%	7.238%
43	8.202	2120	2134	2149	rBV	194266	325776	9.06%	1.547%
44	8.372	2184	2187	2192	rBV5	623	507	0.01%	0.002%
45	8.488	2214	2223	2235	rVB3	10961	19432	0.54%	0.092%
46	8.575	2235	2250	2264	rBV	2083774	3597675	100.00%	17.082%
47	8.655	2265	2275	2298	rVB	841495	1490444	41.43%	7.077%
48	8.883	2341	2346	2350	rVB4	1325	1388	0.04%	0.007%
49	8.948	2362	2366	2372	rBV5	807	937	0.03%	0.004%
50	9.076	2403	2406	2409	rBV2	706	599	0.02%	0.003%
51	9.185	2431	2440	2446	rVV4	2729	4161	0.12%	0.020%
52	9.230	2446	2454	2468	rVB5	8098	13109	0.36%	0.062%
53	9.353	2486	2492	2496	rBV4	850	959	0.03%	0.005%
54	9.436	2500	2518	2542	rBV	924829	1603754	44.58%	7.615%
55	9.581	2558	2563	2564	rBV3	2574	2010	0.06%	0.010%
56	9.642	2576	2582	2584	rBV6	2701	2897	0.08%	0.014%
57	10.047	2698	2708	2717	rBV6	5673	11026	0.31%	0.052%
58	10.182	2748	2750	2755	rBV4	653	549	0.02%	0.003%
59	10.259	2765	2774	2777	rBV4	1999	2708	0.08%	0.013%
60	10.340	2793	2799	2800	rBV2	888	647	0.02%	0.003%
61	10.369	2801	2808	2825	rVB2	4253	11214	0.31%	0.053%
62	10.478	2837	2842	2844	rBV4	1093	1018	0.03%	0.005%
63	10.501	2844	2849	2853	rVB5	1355	1413	0.04%	0.007%
64	10.642	2890	2893	2896	rBV3	667	502	0.01%	0.002%
65	10.700	2907	2911	2913	rBV2	1100	955	0.03%	0.005%
66	10.771	2920	2933	2948	rBV	686583	1095903	30.46%	5.204%
67	10.902	2966	2974	2983	rBV5	4640	7447	0.21%	0.035%
68	10.964	2991	2993	2999	rVB3	1048	792	0.02%	0.004%
69	11.121	3038	3042	3056	rVB7	4589	7581	0.21%	0.036%
70	11.176	3056	3059	3062	rBV2	560	478	0.01%	0.002%
71	11.192	3062	3064	3068	rVV2	695	446	0.01%	0.002%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042920\
 Data File : VU037917.D
 Acq On : 29 Apr 2020 17:21
 Operator : JC/MD
 Sample : L2410-15
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBFF3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

72	11.317	3090	3103	3104	rBV5	3780	4334	0.12%	0.021%
73	11.481	3146	3154	3159	rBV7	2585	3635	0.10%	0.017%
74	11.581	3183	3185	3190	rVB3	924	622	0.02%	0.003%
75	11.697	3216	3221	3224	rBV4	762	961	0.03%	0.005%
76	11.755	3235	3239	3247	rVB5	2291	3253	0.09%	0.015%
77	11.825	3248	3261	3277	rBV	951328	1512744	42.05%	7.183%
78	11.944	3295	3298	3300	rBV4	649	443	0.01%	0.002%
79	12.076	3329	3339	3352	rBV	24396	43357	1.21%	0.206%
80	12.205	3366	3379	3395	rVB	890616	1422978	39.55%	6.756%
81	12.324	3413	3416	3418	rBV3	1236	825	0.02%	0.004%
82	12.517	3474	3476	3480	rVB3	857	493	0.01%	0.002%
83	12.539	3480	3483	3485	rBV4	938	633	0.02%	0.003%
84	12.674	3522	3525	3531	rBV4	540	456	0.01%	0.002%
85	12.700	3531	3533	3539	rVB2	587	588	0.02%	0.003%
86	12.732	3539	3543	3545	rBV2	928	679	0.02%	0.003%
87	12.767	3548	3554	3556	rBV5	1228	1109	0.03%	0.005%
88	12.790	3556	3561	3571	rVB2	3326	5440	0.15%	0.026%
89	12.909	3594	3598	3605	rVB3	1198	1405	0.04%	0.007%
90	13.008	3625	3629	3630	rBV	713	460	0.01%	0.002%
91	13.050	3639	3642	3645	rBV2	899	561	0.02%	0.003%
92	13.124	3662	3665	3667	rBV	849	450	0.01%	0.002%
93	13.230	3693	3698	3699	rBV4	1397	1074	0.03%	0.005%
94	13.497	3778	3781	3785	rBV2	564	525	0.01%	0.002%
95	13.754	3858	3861	3863	rBV3	844	532	0.01%	0.003%
96	13.864	3888	3895	3904	rBV8	4508	7151	0.20%	0.034%
97	14.108	3967	3971	3974	rBV4	2373	1944	0.05%	0.009%
98	14.176	3987	3992	3996	rBV6	1073	1254	0.03%	0.006%
99	14.626	4124	4132	4139	rVB2	3654	5731	0.16%	0.027%
100	15.507	4403	4406	4409	rBV2	1206	689	0.02%	0.003%


Sum of corrected areas: 21060880

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042920\
Data File : VU037917.D
Acq On : 29 Apr 2020 17:21
Operator : JC/MD
Sample : L2410-15
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBFF3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

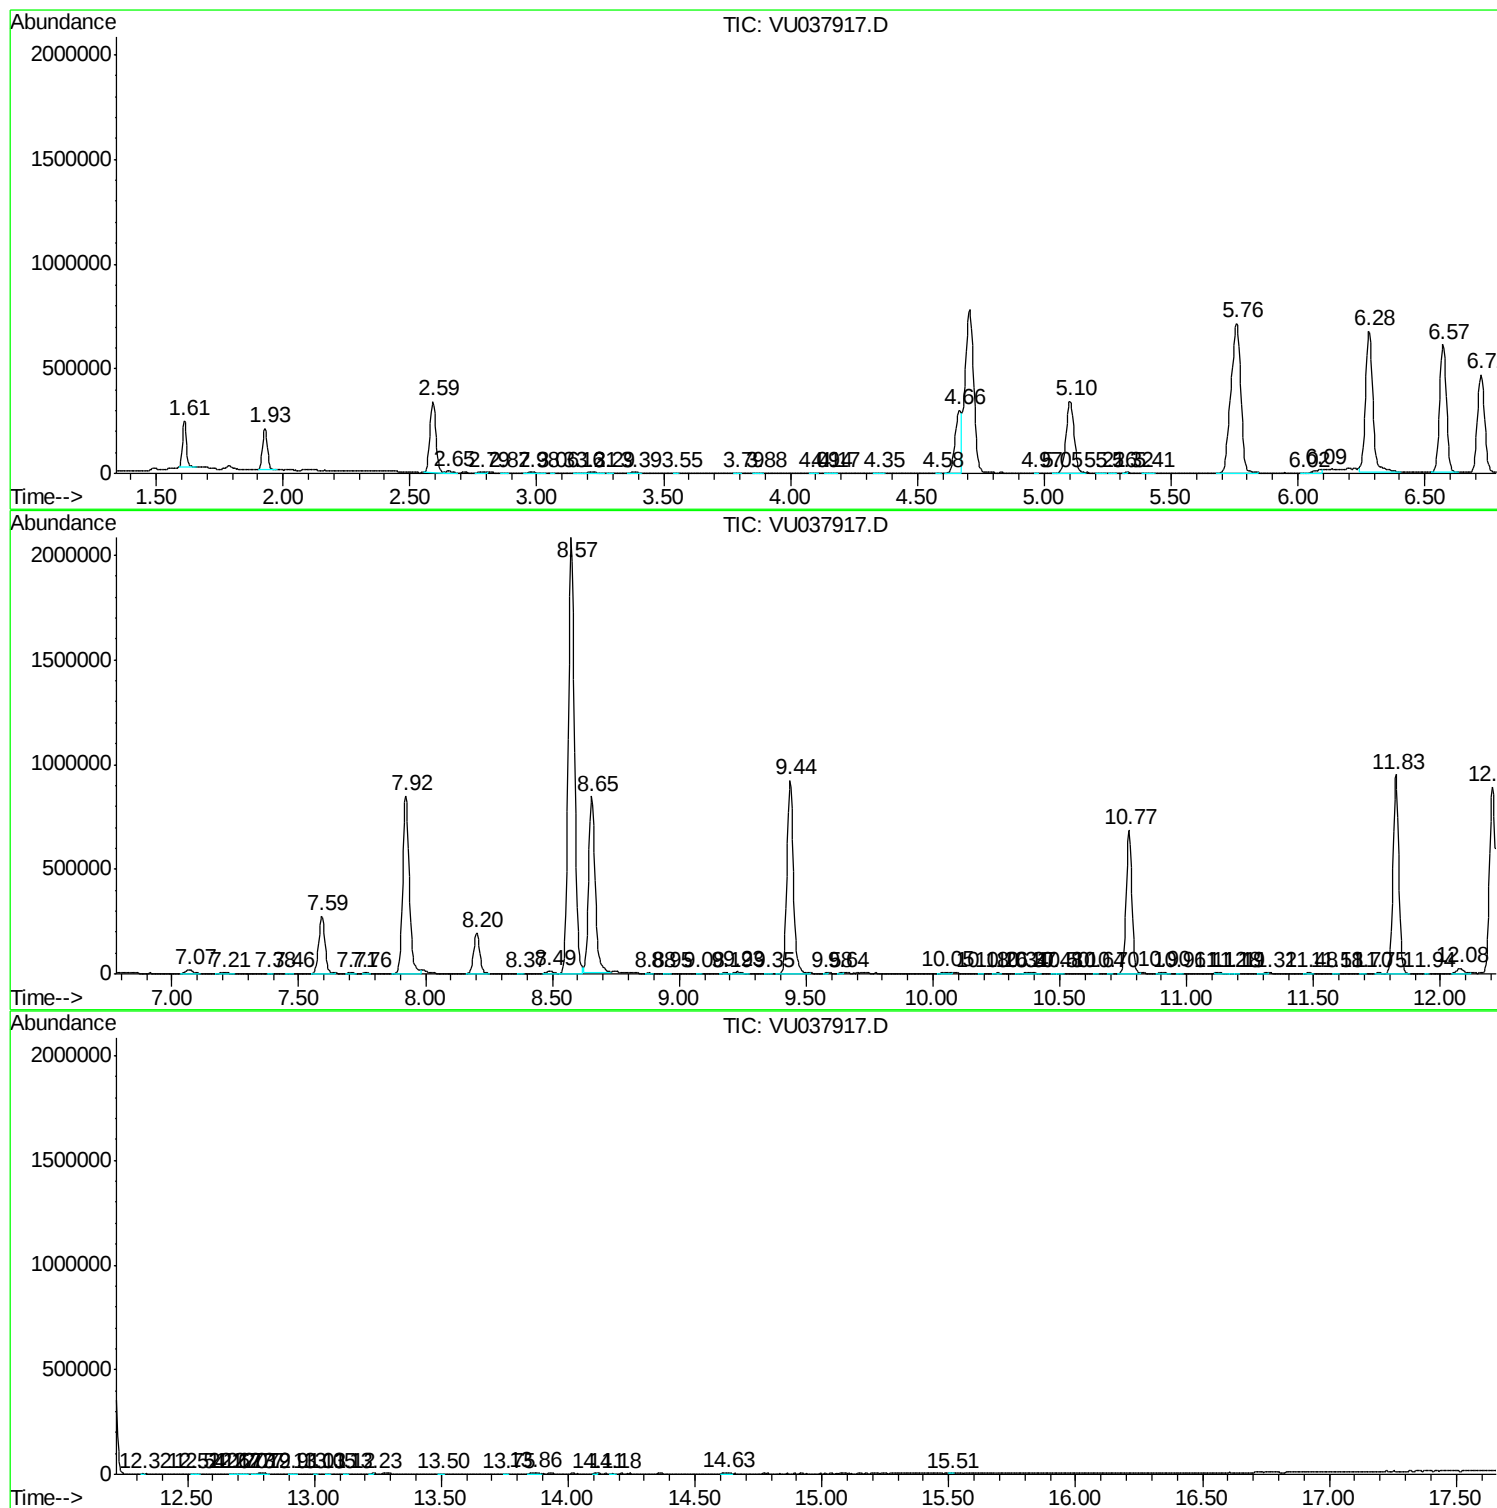

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042920\
Data File : VU037917.D
Acq On : 29 Apr 2020 17:21
Operator : JC/MD
Sample : L2410-15
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBFF3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU042920\
Data File : VU037917.D
Acq On : 29 Apr 2020 17:21
Operator : JC/MD
Sample : L2410-15
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
DBFF3

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc