

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042920\
 Data File : VU037921.D
 Acq On : 29 Apr 2020 18:51
 Operator : JC/MD
 Sample : L2395-02DL 400X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D87DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.610	77	84	93	rBV	311035	332544	13.43%	1.512%
2	1.928	175	183	196	rVB	263131	341279	13.78%	1.552%
3	2.591	376	389	408	rBV2	482591	849656	34.31%	3.864%
4	2.723	423	430	436	rVB6	2329	2986	0.12%	0.014%
5	2.790	444	451	455	rVV7	1426	2055	0.08%	0.009%
6	2.848	466	469	471	rVB3	978	595	0.02%	0.003%
7	2.867	471	475	477	rBV3	367	328	0.01%	0.001%
8	3.076	527	540	554	rVB	40236	75091	3.03%	0.341%
9	3.221	569	585	602	rBV	19414	45566	1.84%	0.207%
10	3.446	649	655	659	rBV3	472	501	0.02%	0.002%
11	3.472	659	663	666	rBV2	586	502	0.02%	0.002%
12	3.906	789	798	801	rBV5	1427	2110	0.09%	0.010%
13	4.157	871	876	882	rVB3	480	559	0.02%	0.003%
14	4.189	882	886	890	rBV3	476	459	0.02%	0.002%
15	4.411	952	955	960	rBV3	505	456	0.02%	0.002%
16	4.452	964	968	973	rVB4	400	416	0.02%	0.002%
17	4.494	979	981	985	rBV3	563	352	0.01%	0.002%
18	4.517	985	988	992	rBV3	434	402	0.02%	0.002%
19	4.665	1015	1034	1064	rBV2	342328	860137	34.73%	3.911%
20	4.928	1114	1116	1119	rBV4	464	376	0.02%	0.002%
21	5.102	1154	1170	1190	rVV	435884	937135	37.84%	4.262%
22	5.279	1222	1225	1228	rVB2	685	453	0.02%	0.002%
23	5.353	1229	1248	1266	rBV2	83362	193278	7.81%	0.879%
24	5.452	1278	1279	1286	rVB2	479	443	0.02%	0.002%
25	5.639	1335	1337	1341	rVB2	630	362	0.01%	0.002%
26	5.661	1341	1344	1350	rBV2	688	652	0.03%	0.003%
27	5.758	1350	1374	1405	rBV2	919313	2476304	100.00%	11.261%
28	5.896	1413	1417	1419	rBV4	1034	668	0.03%	0.003%
29	6.076	1467	1473	1475	rBV4	2257	2455	0.10%	0.011%
30	6.279	1523	1536	1569	rVB	733796	1407700	56.85%	6.401%
31	6.571	1611	1627	1655	rBV	1220466	2302580	92.98%	10.471%
32	6.719	1660	1673	1696	rVB	595491	1161530	46.91%	5.282%
33	6.828	1704	1707	1708	rBV2	1836	1096	0.04%	0.005%
34	6.906	1729	1731	1734	rVB2	1206	728	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042920\
 Data File : VU037921.D
 Acq On : 29 Apr 2020 18:51
 Operator : JC/MD
 Sample : L2395-02DL 400X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D87DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

35	6.931	1734	1739	1742	rBV5	1105	924	0.04%	0.004%
36	7.070	1776	1782	1788	rVB6	1704	2427	0.10%	0.011%
37	7.208	1813	1825	1834	rVB5	3998	6266	0.25%	0.028%
38	7.246	1834	1837	1839	rBV	553	346	0.01%	0.002%
39	7.259	1839	1841	1846	rVB2	570	408	0.02%	0.002%
40	7.298	1849	1853	1856	rBV3	651	448	0.02%	0.002%
41	7.362	1869	1873	1874	rBV2	624	416	0.02%	0.002%
42	7.590	1930	1944	1965	rBV	306937	528549	21.34%	2.404%
43	7.706	1977	1980	1984	rBV6	1276	1097	0.04%	0.005%
44	7.812	2008	2013	2016	rBV6	697	571	0.02%	0.003%
45	7.861	2025	2028	2030	rVB2	851	534	0.02%	0.002%
46	7.922	2030	2047	2066	rBV	1063090	1923016	77.66%	8.745%
47	8.201	2121	2134	2152	rBV	222976	364217	14.71%	1.656%
48	8.417	2196	2201	2202	rBV2	1361	882	0.04%	0.004%
49	8.491	2213	2224	2232	rBV6	2924	4665	0.19%	0.021%
50	8.574	2240	2250	2262	rVB4	15600	25559	1.03%	0.116%
51	8.655	2262	2275	2314	rBV	911943	1624555	65.60%	7.388%
52	8.854	2333	2337	2341	rBV4	845	598	0.02%	0.003%
53	8.928	2348	2360	2372	rBV2	12870	24058	0.97%	0.109%
54	8.999	2380	2382	2387	rVB3	917	544	0.02%	0.002%
55	9.053	2397	2399	2403	rBV2	510	412	0.02%	0.002%
56	9.079	2403	2407	2412	rVB5	861	711	0.03%	0.003%
57	9.137	2420	2425	2428	rBV2	465	398	0.02%	0.002%
58	9.230	2445	2454	2457	rBV5	1569	1999	0.08%	0.009%
59	9.436	2503	2518	2547	rBV	1020476	1754914	70.87%	7.980%
60	9.549	2552	2553	2556	rVV3	736	406	0.02%	0.002%
61	9.590	2559	2566	2574	rBV4	1697	2199	0.09%	0.010%
62	9.709	2592	2603	2614	rVB3	10092	15717	0.63%	0.071%
63	10.021	2698	2700	2705	rVB	649	490	0.02%	0.002%
64	10.050	2705	2709	2713	rBV2	391	409	0.02%	0.002%
65	10.118	2716	2730	2739	rBV3	9204	16155	0.65%	0.073%
66	10.407	2815	2820	2822	rBV2	492	383	0.02%	0.002%
67	10.494	2842	2847	2851	rBV3	806	833	0.03%	0.004%
68	10.668	2898	2901	2904	rBV2	620	396	0.02%	0.002%
69	10.770	2920	2933	2954	rBV	807051	1280168	51.70%	5.821%
70	10.864	2959	2962	2967	rBV2	647	467	0.02%	0.002%
71	10.896	2967	2972	2973	rBV	1021	707	0.03%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042920\
 Data File : VU037921.D
 Acq On : 29 Apr 2020 18:51
 Operator : JC/MD
 Sample : L2395-02DL 400X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0D87DL

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

72	11.008	3002	3007	3011	rVB2	547	370	0.01%	0.002%
73	11.031	3012	3014	3018	rVB	709	400	0.02%	0.002%
74	11.053	3018	3021	3023	rBV	471	360	0.01%	0.002%
75	11.118	3032	3041	3045	rBV5	1184	2247	0.09%	0.010%
76	11.314	3095	3102	3106	rBV3	761	829	0.03%	0.004%
77	11.426	3134	3137	3143	rVB2	637	517	0.02%	0.002%
78	11.481	3151	3154	3157	rVB2	934	476	0.02%	0.002%
79	11.732	3228	3232	3234	rBV2	487	429	0.02%	0.002%
80	11.761	3236	3241	3244	rVV2	1093	1229	0.05%	0.006%
81	11.822	3247	3260	3280	rBV	1031643	1644066	66.39%	7.476%
82	11.896	3280	3283	3287	rVB3	814	650	0.03%	0.003%
83	11.934	3292	3295	3299	rVB2	738	460	0.02%	0.002%
84	11.967	3301	3305	3307	rBV3	482	491	0.02%	0.002%
85	12.073	3332	3338	3346	rBV6	2239	3120	0.13%	0.014%
86	12.204	3364	3379	3399	rBV	1089273	1735573	70.09%	7.892%
87	12.362	3424	3428	3430	rBV4	715	333	0.01%	0.002%
88	12.616	3504	3507	3512	rBV3	490	448	0.02%	0.002%
89	12.703	3531	3534	3538	rBV2	529	426	0.02%	0.002%
90	12.725	3538	3541	3545	rVB2	561	361	0.01%	0.002%
91	12.796	3560	3563	3566	rBV3	829	492	0.02%	0.002%
92	12.909	3595	3598	3600	rBV2	699	369	0.01%	0.002%
93	13.301	3717	3720	3723	rBV2	686	490	0.02%	0.002%
94	13.429	3758	3760	3764	rVB2	616	404	0.02%	0.002%
95	13.536	3790	3793	3795	rBV2	515	404	0.02%	0.002%
96	13.626	3817	3821	3826	rBV5	480	477	0.02%	0.002%
97	13.860	3888	3894	3903	rBV5	2630	3504	0.14%	0.016%
98	13.896	3903	3905	3909	rVB2	587	354	0.01%	0.002%
99	14.111	3966	3972	3978	rBV6	1476	2065	0.08%	0.009%
100	14.552	4107	4109	4112	rBV3	647	446	0.02%	0.002%


Sum of corrected areas: 21990388

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042920\
Data File : VU037921.D
Acq On : 29 Apr 2020 18:51
Operator : JC/MD
Sample : L2395-02DL 400X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D87DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

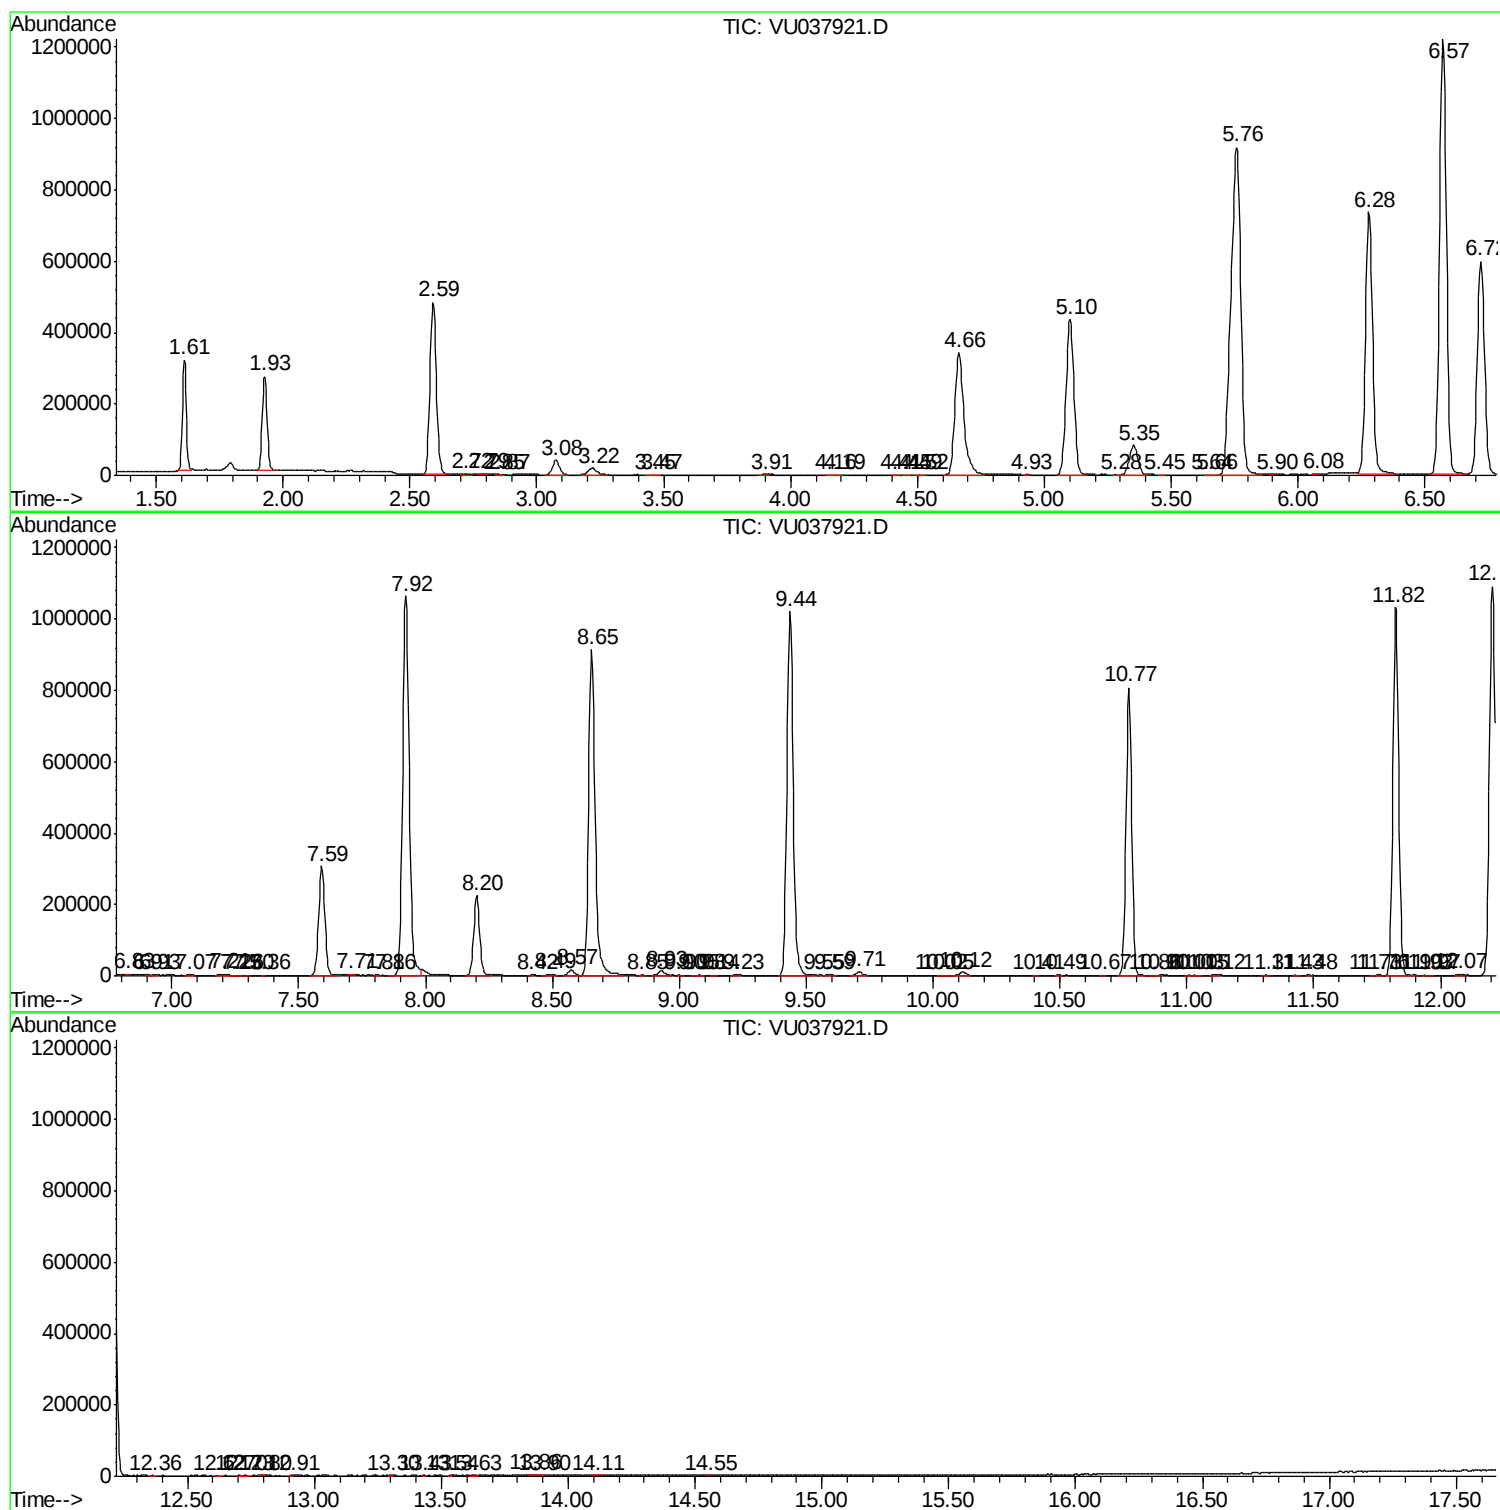

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042920\
Data File : VU037921.D
Acq On : 29 Apr 2020 18:51
Operator : JC/MD
Sample : L2395-02DL 400X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0D87DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU042920\
Data File : VU037921.D
Acq On : 29 Apr 2020 18:51
Operator : JC/MD
Sample : L2395-02DL 400X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
C0D87DL

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc