

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042920\
 Data File : VU037927.D
 Acq On : 29 Apr 2020 21:54
 Operator : JC/MD
 Sample : L2395-18 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DA3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.610	77	84	93	rBV	293111	307779	7.42%	1.202%
2	1.925	174	182	197	rVB	248959	328121	7.91%	1.282%
3	2.591	376	389	409	rBV3	517866	971741	23.41%	3.795%
4	2.710	423	426	428	rBV2	1281	1009	0.02%	0.004%
5	2.774	443	446	447	rBV2	798	510	0.01%	0.002%
6	2.964	502	505	507	rBV3	671	434	0.01%	0.002%
7	3.006	515	518	521	rBV	517	391	0.01%	0.002%
8	3.076	525	540	556	rVV	255325	474310	11.43%	1.853%
9	3.218	571	584	600	rVV2	23499	51736	1.25%	0.202%
10	3.289	604	606	610	rVB4	600	357	0.01%	0.001%
11	3.385	629	636	637	rBV2	1611	1356	0.03%	0.005%
12	3.453	653	657	660	rBV3	565	454	0.01%	0.002%
13	3.594	699	701	706	rVB3	797	545	0.01%	0.002%
14	3.623	706	710	715	rBV3	729	740	0.02%	0.003%
15	3.697	730	733	735	rBV	514	327	0.01%	0.001%
16	3.752	747	750	759	rVB3	767	701	0.02%	0.003%
17	3.912	785	800	812	rBV2	15295	36392	0.88%	0.142%
18	4.125	862	866	868	rBV2	453	477	0.01%	0.002%
19	4.224	895	897	900	rVB2	511	318	0.01%	0.001%
20	4.298	917	920	923	rBV3	523	430	0.01%	0.002%
21	4.314	923	925	929	rVV	476	337	0.01%	0.001%
22	4.665	1017	1034	1040	rBV2	352392	804013	19.37%	3.140%
23	4.941	1117	1120	1125	rVB2	960	586	0.01%	0.002%
24	5.102	1153	1170	1193	rBV	426995	949874	22.89%	3.710%
25	5.353	1231	1248	1267	rBV	174555	396147	9.55%	1.547%
26	5.427	1270	1271	1275	rVV2	1115	699	0.02%	0.003%
27	5.501	1292	1294	1297	rVB2	788	387	0.01%	0.002%
28	5.526	1297	1302	1304	rBV2	859	609	0.01%	0.002%
29	5.588	1318	1321	1328	rVB2	559	590	0.01%	0.002%
30	5.758	1350	1374	1406	rBV2	916536	2449967	59.03%	9.569%
31	5.957	1432	1436	1438	rBV2	644	492	0.01%	0.002%
32	6.044	1461	1463	1466	rBV3	487	336	0.01%	0.001%
33	6.121	1483	1487	1489	rBV3	643	464	0.01%	0.002%
34	6.141	1489	1493	1494	rBV2	990	643	0.02%	0.003%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042920\
 Data File : VU037927.D
 Acq On : 29 Apr 2020 21:54
 Operator : JC/MD
 Sample : L2395-18 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DA3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

35	6.279	1521	1536	1557	rBV	844145	1613615	38.88%	6.302%
36	6.571	1611	1627	1647	rBV	2239152	4150255	100.00%	16.210%
37	6.723	1659	1674	1695	rVB	598781	1155919	27.85%	4.515%
38	6.935	1737	1740	1743	rVB3	923	513	0.01%	0.002%
39	7.211	1815	1826	1838	rVB5	4596	8579	0.21%	0.034%
40	7.369	1869	1875	1878	rBV	612	469	0.01%	0.002%
41	7.388	1878	1881	1883	rBV2	1049	652	0.02%	0.003%
42	7.433	1889	1895	1896	rBV2	483	379	0.01%	0.001%
43	7.591	1930	1944	1961	rBV	340829	586598	14.13%	2.291%
44	7.706	1972	1980	1990	rVV5	3208	5277	0.13%	0.021%
45	7.858	2025	2027	2032	rVB2	513	462	0.01%	0.002%
46	7.922	2032	2047	2082	rBV	1076736	1941792	46.79%	7.584%
47	8.076	2091	2095	2102	rBV4	846	935	0.02%	0.004%
48	8.134	2110	2113	2121	rBV3	340	424	0.01%	0.002%
49	8.202	2121	2134	2152	rBV	238883	395945	9.54%	1.546%
50	8.346	2176	2179	2181	rBV3	606	324	0.01%	0.001%
51	8.420	2194	2202	2209	rBV5	6180	9795	0.24%	0.038%
52	8.469	2214	2217	2219	rBV2	625	421	0.01%	0.002%
53	8.488	2219	2223	2227	rBV2	707	662	0.02%	0.003%
54	8.536	2234	2238	2241	rBV3	677	602	0.01%	0.002%
55	8.578	2241	2251	2256	rVB7	2576	4160	0.10%	0.016%
56	8.655	2256	2275	2312	rBV	927552	1694165	40.82%	6.617%
57	8.980	2371	2376	2377	rBV3	631	531	0.01%	0.002%
58	9.221	2448	2451	2455	rVV2	556	348	0.01%	0.001%
59	9.436	2504	2518	2547	rBV	1207308	2046468	49.31%	7.993%
60	9.591	2560	2566	2574	rBV5	1570	2635	0.06%	0.010%
61	9.623	2574	2576	2579	rVB3	920	517	0.01%	0.002%
62	9.642	2579	2582	2585	rBV	753	555	0.01%	0.002%
63	9.710	2593	2603	2614	rVB2	12371	20666	0.50%	0.081%
64	9.803	2629	2632	2635	rVB2	515	387	0.01%	0.002%
65	9.899	2657	2662	2665	rBV2	409	365	0.01%	0.001%
66	9.960	2677	2681	2684	rBV2	583	454	0.01%	0.002%
67	10.118	2718	2730	2740	rBV5	7391	13181	0.32%	0.051%
68	10.504	2840	2850	2855	rBV3	1244	1897	0.05%	0.007%
69	10.771	2919	2933	2948	rBV	827686	1336136	32.19%	5.219%
70	10.906	2973	2975	2980	rVB2	997	621	0.01%	0.002%
71	10.928	2980	2982	2984	rBV	483	338	0.01%	0.001%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042920\
 Data File : VU037927.D
 Acq On : 29 Apr 2020 21:54
 Operator : JC/MD
 Sample : L2395-18 50X
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0DA3

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

72	10.989	2995	3001	3003	rBV2	568	571	0.01%	0.002%
73	11.108	3030	3038	3043	rBV5	1032	1573	0.04%	0.006%
74	11.250	3079	3082	3086	rBV3	565	348	0.01%	0.001%
75	11.452	3142	3145	3148	rBV3	402	330	0.01%	0.001%
76	11.481	3148	3154	3162	rVB4	1421	2220	0.05%	0.009%
77	11.665	3208	3211	3217	rVB2	930	876	0.02%	0.003%
78	11.758	3228	3240	3245	rBV6	2303	3933	0.09%	0.015%
79	11.825	3247	3261	3277	rBV	1253166	1969507	47.46%	7.692%
80	11.999	3313	3315	3319	rVB2	551	367	0.01%	0.001%
81	12.205	3365	3379	3397	rVV	1137468	1812821	43.68%	7.080%
82	12.349	3420	3424	3426	rBV3	608	416	0.01%	0.002%
83	12.439	3450	3452	3456	rBV2	443	360	0.01%	0.001%
84	12.523	3474	3478	3481	rBV3	545	444	0.01%	0.002%
85	12.568	3487	3492	3493	rBV2	386	341	0.01%	0.001%
86	12.639	3511	3514	3516	rBV3	580	401	0.01%	0.002%
87	12.796	3553	3563	3574	rVB	4896	8912	0.21%	0.035%
88	12.845	3574	3578	3582	rBV2	549	532	0.01%	0.002%
89	12.906	3591	3597	3601	rBV5	543	631	0.02%	0.002%
90	13.041	3633	3639	3645	rBV5	1970	2016	0.05%	0.008%
91	13.163	3674	3677	3681	rBV3	552	528	0.01%	0.002%
92	13.198	3685	3688	3690	rBV2	604	318	0.01%	0.001%
93	13.240	3695	3701	3705	rBV4	1904	2271	0.05%	0.009%
94	13.356	3734	3737	3743	rBV3	400	389	0.01%	0.002%
95	13.754	3858	3861	3863	rBV2	637	425	0.01%	0.002%
96	13.809	3876	3878	3887	rBV2	555	683	0.02%	0.003%
97	13.864	3889	3895	3903	rVB6	3440	4885	0.12%	0.019%
98	14.108	3966	3971	3980	rBV3	3232	4253	0.10%	0.017%
99	14.362	4043	4050	4053	rBV6	1223	1767	0.04%	0.007%
100	15.346	4352	4356	4360	rBV2	1139	1005	0.02%	0.004%


Sum of corrected areas: 25603437

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA U\DATA\VU042920\
Data File : VU037927.D
Acq On : 29 Apr 2020 21:54
Operator : JC/MD
Sample : L2395-18 50X
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DA3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

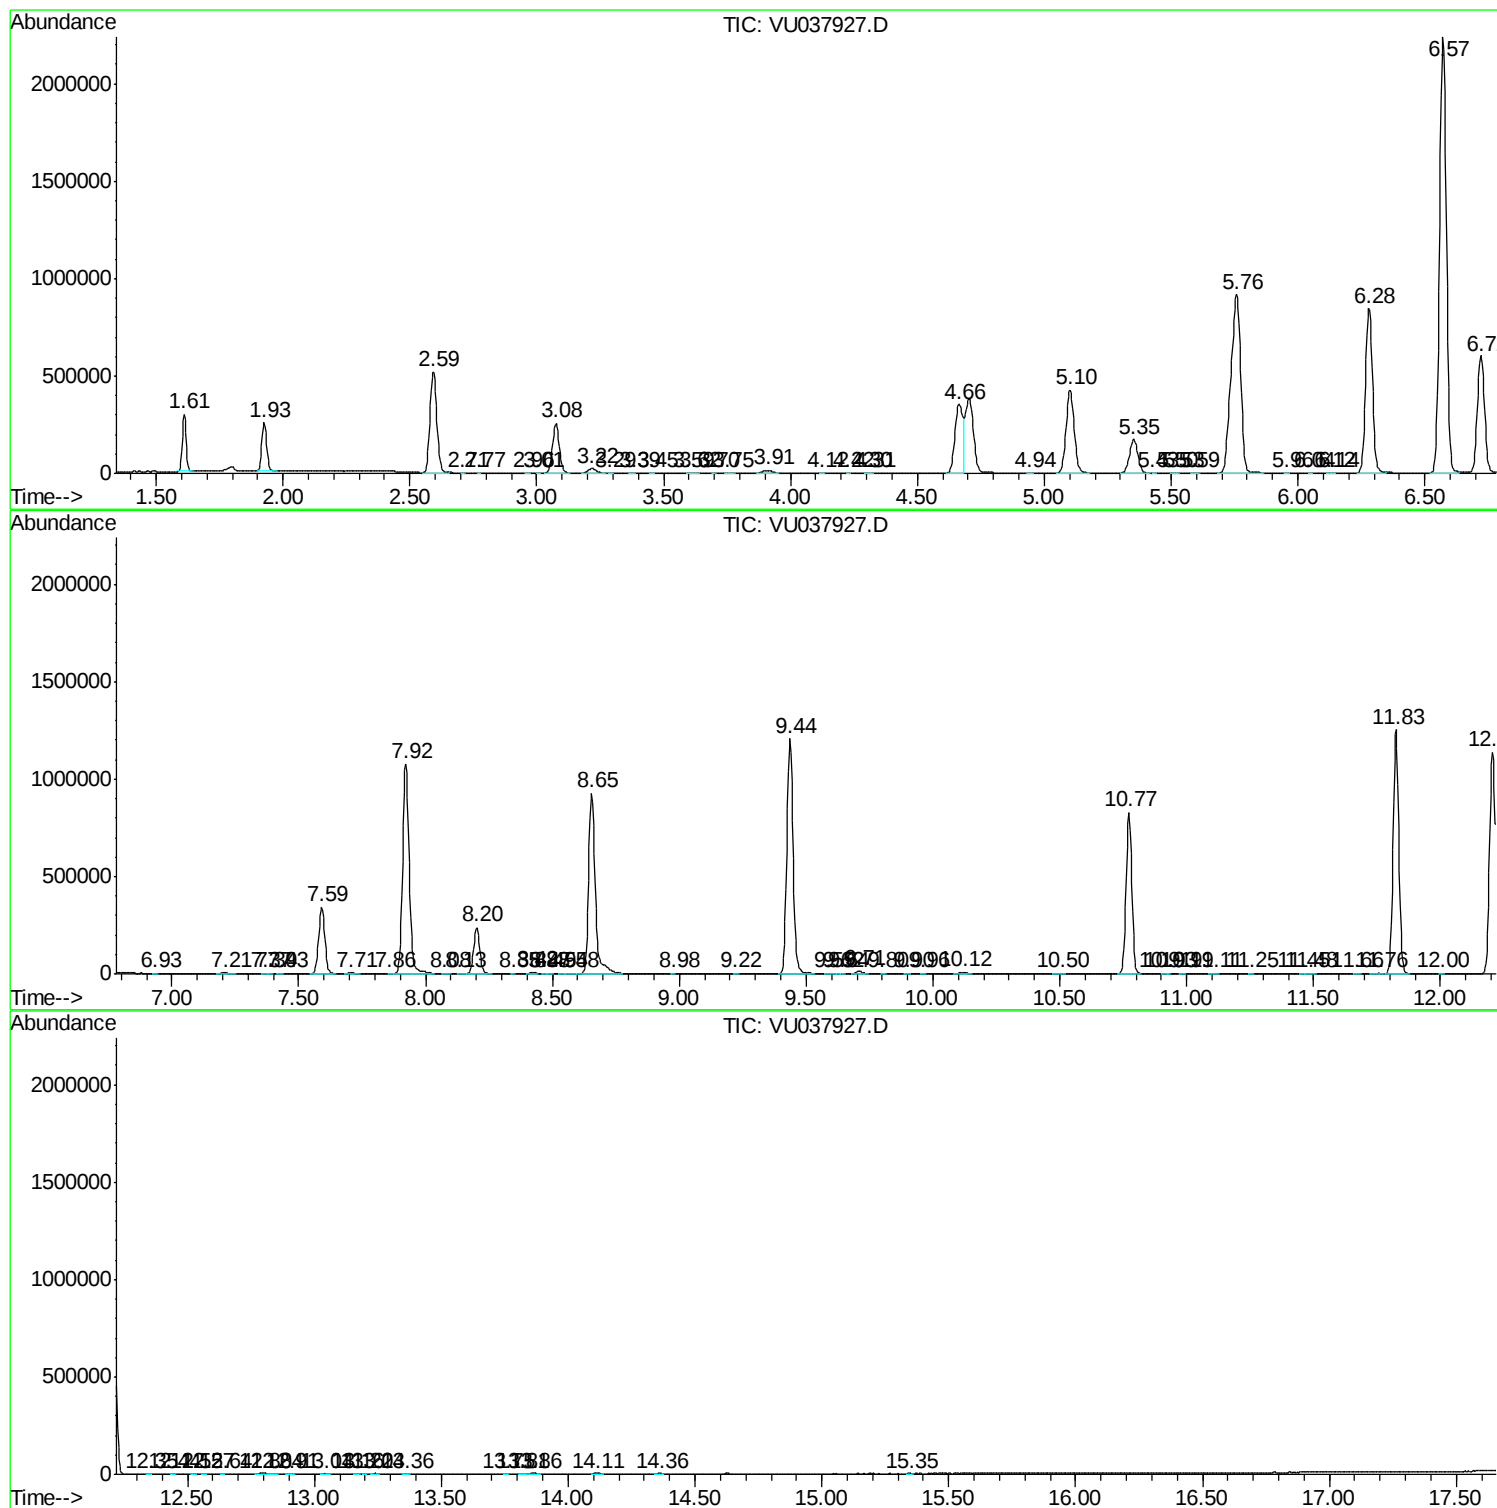

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042920\
Data File : VU037927.D
Acq On : 29 Apr 2020 21:54
Operator : JC/MD
Sample : L2395-18 50X
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0DA3

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSV0A_U\DATA\VU042920\
Data File : VU037927.D
Acq On : 29 Apr 2020 21:54
Operator : JC/MD
Sample : L2395-18 50X
Misc : 5.0mL/MSV0A_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSV0A_U
ClientSampleId :
C0DA3

Quant Method : Z:\V0ASRV\HPCHEM1\MSV0A_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc