

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042920\
 Data File : VU037936.D
 Acq On : 30 Apr 2020 01:18
 Operator : JC/MD
 Sample : L2410-11
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBFE6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.369	4	9	21	rBV2	29406	30632	0.06%	0.040%
2	1.610	76	84	95	rBV	390454	429179	0.79%	0.556%
3	1.928	175	183	197	rVB	310295	397154	0.73%	0.515%
4	2.591	376	389	404	rBV	543637	886733	1.62%	1.149%
5	2.755	435	440	441	rBV2	1019	774	0.00%	0.001%
6	2.977	506	509	511	rBV3	646	422	0.00%	0.001%
7	3.079	530	541	549	rBV5	2315	4907	0.01%	0.006%
8	3.218	573	584	586	rBV7	2760	4209	0.01%	0.005%
9	3.269	594	600	602	rBV3	659	626	0.00%	0.001%
10	3.623	697	710	716	rBV4	1693	2979	0.01%	0.004%
11	3.732	737	744	745	rBV3	1163	1138	0.00%	0.001%
12	3.858	778	783	787	rBV5	605	487	0.00%	0.001%
13	4.041	837	840	844	rVB2	675	475	0.00%	0.001%
14	4.195	882	888	890	rBV4	703	811	0.00%	0.001%
15	4.224	895	897	903	rVB	972	629	0.00%	0.001%
16	4.317	924	926	932	rVB2	500	440	0.00%	0.001%
17	4.382	941	946	952	rVB3	594	802	0.00%	0.001%
18	4.430	958	961	965	rBV2	491	432	0.00%	0.001%
19	4.504	980	984	987	rVB2	922	803	0.00%	0.001%
20	4.530	987	992	996	rBV3	705	738	0.00%	0.001%
21	4.665	1013	1034	1040	rBV	287370	637615	1.17%	0.826%
22	5.102	1153	1170	1190	rBV	466005	1027363	1.88%	1.332%
23	5.292	1226	1229	1232	rBV2	645	545	0.00%	0.001%
24	5.321	1233	1238	1244	rVV6	1337	1783	0.00%	0.002%
25	5.478	1283	1287	1289	rVV3	759	616	0.00%	0.001%
26	5.497	1291	1293	1298	rVB3	924	655	0.00%	0.001%
27	5.758	1348	1374	1406	rBV2	1023101	2716500	4.98%	3.521%
28	5.899	1414	1418	1419	rBV3	833	613	0.00%	0.001%
29	6.134	1483	1491	1493	rBV4	752	968	0.00%	0.001%
30	6.153	1494	1497	1501	rBV4	724	761	0.00%	0.001%
31	6.282	1522	1537	1557	rBV	840578	1575979	2.89%	2.043%
32	6.423	1579	1581	1585	rBV5	850	616	0.00%	0.001%
33	6.571	1612	1627	1646	rBV	640559	1193813	2.19%	1.547%
34	6.722	1658	1674	1693	rBV	646568	1242799	2.28%	1.611%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042920\
 Data File : VU037936.D
 Acq On : 30 Apr 2020 01:18
 Operator : JC/MD
 Sample : L2410-11
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBFE6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

35	6.909	1727	1732	1734	rBV4	1439	1393	0.00%	0.002%
36	7.128	1796	1800	1807	rVB4	531	547	0.00%	0.001%
37	7.211	1818	1826	1832	rBV8	1903	3115	0.01%	0.004%
38	7.266	1837	1843	1847	rVB5	495	572	0.00%	0.001%
39	7.324	1858	1861	1864	rVB3	690	450	0.00%	0.001%
40	7.520	1916	1922	1927	rBV4	630	748	0.00%	0.001%
41	7.591	1930	1944	1961	rBV	361710	624570	1.14%	0.810%
42	7.745	1990	1992	2000	rVB6	818	673	0.00%	0.001%
43	7.816	2008	2014	2023	rVB6	1472	2353	0.00%	0.003%
44	7.922	2033	2047	2068	rBV	1253958	2222478	4.07%	2.881%
45	8.201	2120	2134	2150	rBV	254653	421133	0.77%	0.546%
46	8.394	2189	2194	2199	rVB8	1924	2389	0.00%	0.003%
47	8.491	2214	2224	2234	rBV3	3704	5864	0.01%	0.008%
48	8.578	2234	2251	2267	rBV	32649995	54596382	100.00%	70.767%
49	8.655	2268	2275	2316	rVB2	859315	1778149	3.26%	2.305%
50	8.886	2340	2347	2356	rVB7	3833	5983	0.01%	0.008%
51	8.938	2358	2363	2365	rBV3	1595	1451	0.00%	0.002%
52	9.086	2407	2409	2414	rVB3	711	460	0.00%	0.001%
53	9.182	2432	2439	2446	rVV5	4645	6576	0.01%	0.009%
54	9.227	2451	2453	2454	rBV2	1024	480	0.00%	0.001%
55	9.346	2486	2490	2491	rBV3	560	466	0.00%	0.001%
56	9.436	2504	2518	2543	rBV	1168129	1982811	3.63%	2.570%
57	9.584	2557	2564	2575	rBV10	4763	8482	0.02%	0.011%
58	9.648	2577	2584	2591	rBV5	5703	8400	0.02%	0.011%
59	9.812	2633	2635	2640	rVB4	1176	725	0.00%	0.001%
60	10.047	2697	2708	2718	rBV6	10335	23124	0.04%	0.030%
61	10.259	2765	2774	2777	rBV5	2535	3732	0.01%	0.005%
62	10.288	2779	2783	2794	rVB4	4783	6089	0.01%	0.008%
63	10.375	2799	2810	2829	rVB4	7972	21630	0.04%	0.028%
64	10.623	2885	2887	2891	rBV4	887	765	0.00%	0.001%
65	10.655	2895	2897	2903	rVB3	1217	979	0.00%	0.001%
66	10.713	2908	2915	2919	rBV3	3131	3663	0.01%	0.005%
67	10.770	2921	2933	2947	rBV	812815	1297610	2.38%	1.682%
68	10.909	2967	2976	2981	rBV6	2794	3763	0.01%	0.005%
69	10.947	2985	2988	2990	rBV3	1055	634	0.00%	0.001%
70	10.963	2990	2993	2999	rVB5	1272	1271	0.00%	0.002%
71	11.076	3021	3028	3037	rBV5	2134	3095	0.01%	0.004%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042920\
 Data File : VU037936.D
 Acq On : 30 Apr 2020 01:18
 Operator : JC/MD
 Sample : L2410-11
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBFE6

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

72	11.246	3077	3081	3082	rBV2	627	461	0.00%	0.001%
73	11.317	3091	3103	3115	rVB6	9929	18647	0.03%	0.024%
74	11.388	3123	3125	3131	rVB3	736	518	0.00%	0.001%
75	11.481	3150	3154	3157	rBV2	1241	1359	0.00%	0.002%
76	11.516	3157	3165	3180	rVB8	6960	12320	0.02%	0.016%
77	11.642	3201	3204	3205	rBV2	874	426	0.00%	0.001%
78	11.725	3226	3230	3235	rBV6	1782	1680	0.00%	0.002%
79	11.825	3247	3261	3284	rBV	1211310	1920717	3.52%	2.490%
80	11.944	3294	3298	3300	rBV3	1739	1236	0.00%	0.002%
81	12.037	3324	3327	3329	rBV3	878	621	0.00%	0.001%
82	12.076	3334	3339	3347	rVB4	6005	8795	0.02%	0.011%
83	12.153	3360	3363	3366	rVV4	1770	1722	0.00%	0.002%
84	12.205	3366	3379	3401	rVB	1208609	1950403	3.57%	2.528%
85	12.327	3415	3417	3420	rBV3	827	502	0.00%	0.001%
86	12.706	3532	3535	3539	rVV2	682	525	0.00%	0.001%
87	12.761	3549	3552	3560	rBV6	2111	2620	0.00%	0.003%
88	12.851	3576	3580	3583	rBV3	670	512	0.00%	0.001%
89	12.883	3586	3590	3594	rVB2	524	476	0.00%	0.001%
90	12.912	3594	3599	3601	rBV3	1093	939	0.00%	0.001%
91	12.970	3609	3617	3625	rVB6	2709	3910	0.01%	0.005%
92	13.240	3699	3701	3706	rVB3	1216	819	0.00%	0.001%
93	13.336	3727	3731	3735	rVB	801	701	0.00%	0.001%
94	13.500	3779	3782	3785	rVB2	596	435	0.00%	0.001%
95	13.864	3891	3895	3900	rVB4	1490	1195	0.00%	0.002%
96	14.114	3966	3973	3982	rVB2	5962	8194	0.02%	0.011%
97	14.176	3990	3992	3997	rVB2	1057	672	0.00%	0.001%
98	14.221	4003	4006	4007	rBV2	828	461	0.00%	0.001%
99	14.494	4087	4091	4092	rBV3	644	493	0.00%	0.001%
100	14.777	4177	4179	4182	rBV2	597	439	0.00%	0.001%


Sum of corrected areas: 77149799

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042920\
Data File : VU037936.D
Acq On : 30 Apr 2020 01:18
Operator : JC/MD
Sample : L2410-11
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBFE6

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

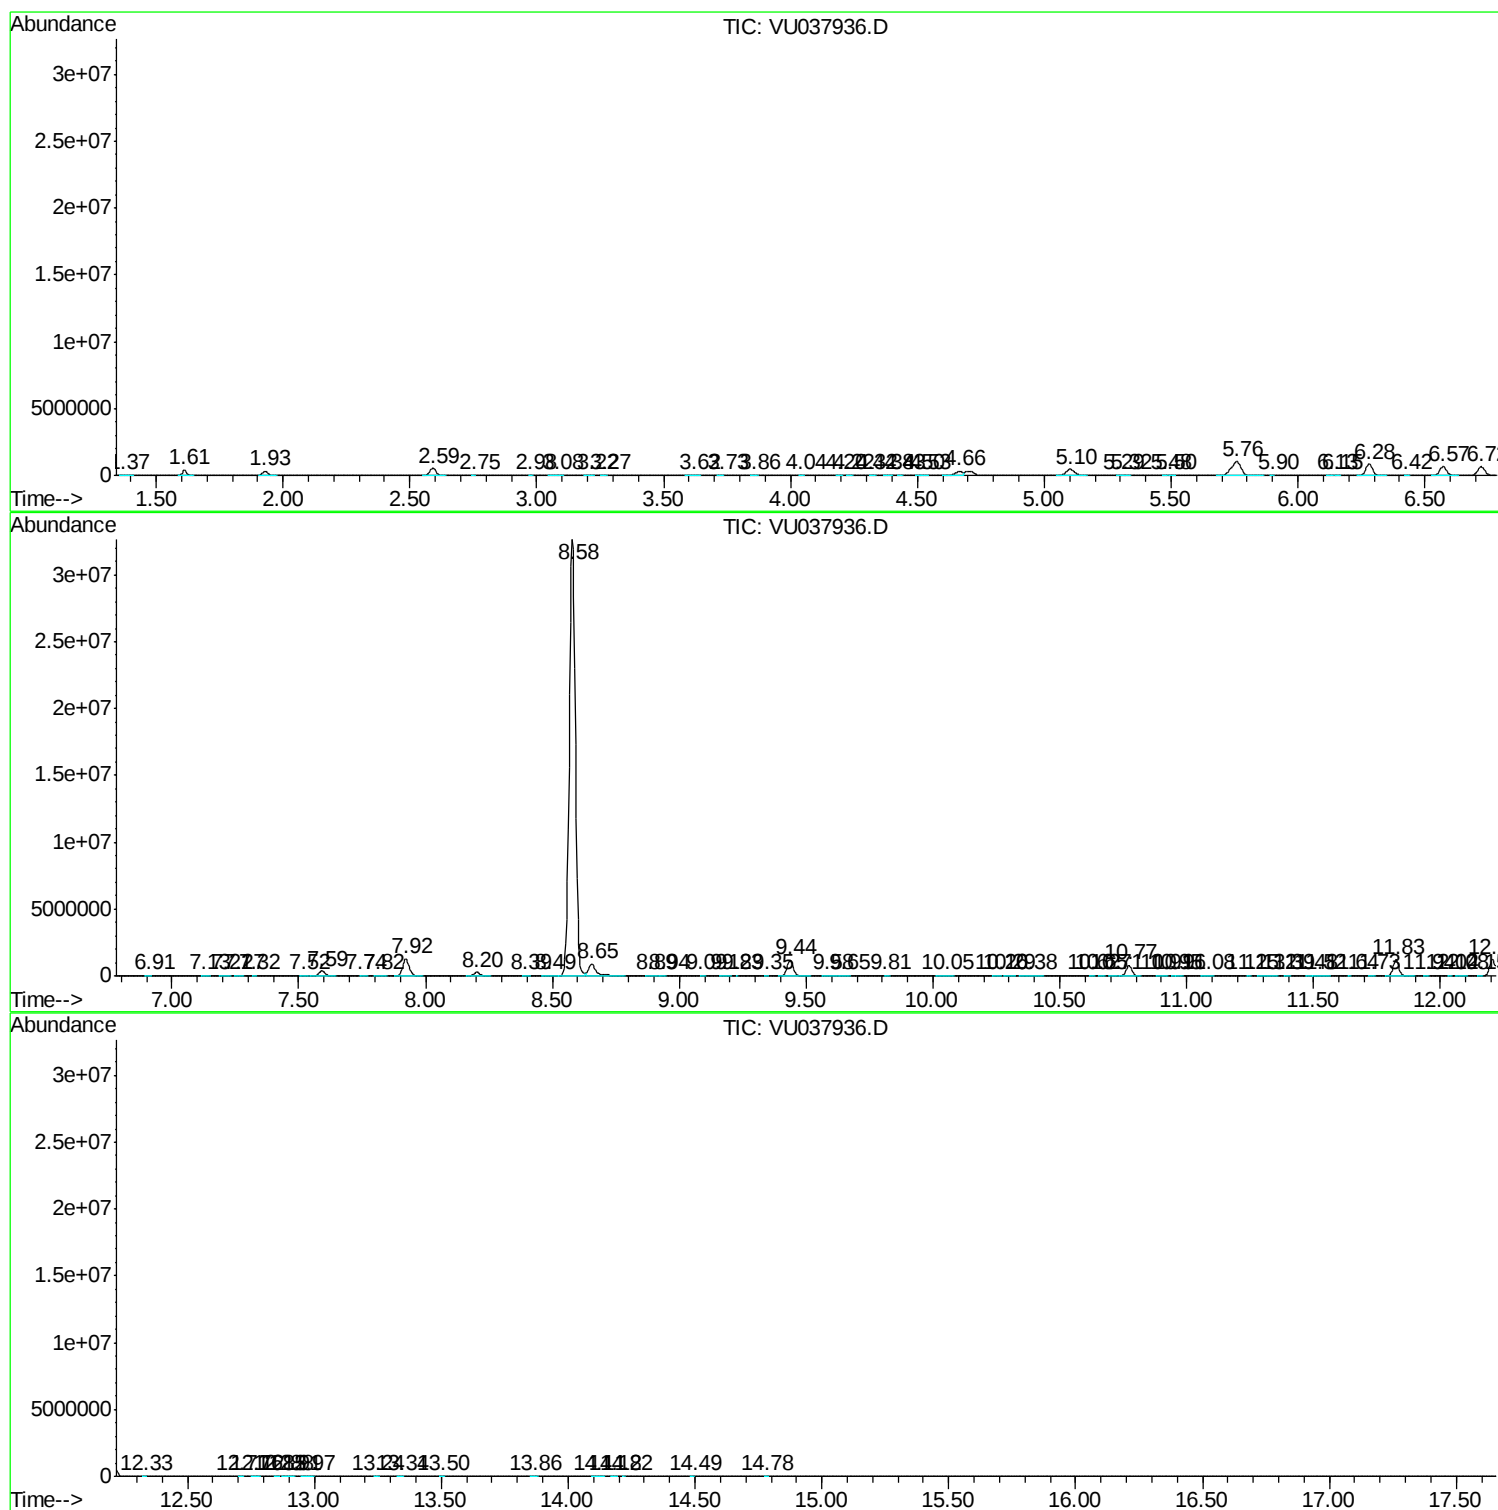

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042920\
Data File : VU037936.D
Acq On : 30 Apr 2020 01:18
Operator : JC/MD
Sample : L2410-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBFE6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042920\
Data File : VU037936.D
Acq On : 30 Apr 2020 01:18
Operator : JC/MD
Sample : L2410-11
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBFE6

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc