

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042920\
 Data File : VU037937.D
 Acq On : 30 Apr 2020 01:41
 Operator : JC/MD
 Sample : L2410-12
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBFF0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.610	77	84	96	rBV	378731	401432	0.21%	0.187%
2	1.928	175	183	196	rVB	303164	392057	0.20%	0.183%
3	2.591	375	389	402	rBV	537736	881166	0.46%	0.411%
4	2.716	424	428	429	rBV3	1105	767	0.00%	0.000%
5	2.787	439	450	457	rBV8	3141	6724	0.00%	0.003%
6	3.080	533	541	551	rVB6	3578	6117	0.00%	0.003%
7	3.131	555	557	563	rVB2	858	732	0.00%	0.000%
8	3.166	563	568	571	rBV4	902	788	0.00%	0.000%
9	3.324	612	617	620	rBV4	688	607	0.00%	0.000%
10	3.385	627	636	651	rVB2	7849	16337	0.01%	0.008%
11	3.543	682	685	691	rVB4	726	751	0.00%	0.000%
12	3.645	713	717	722	rVV3	515	579	0.00%	0.000%
13	3.703	731	735	738	rVB2	673	422	0.00%	0.000%
14	3.729	738	743	744	rBV2	389	381	0.00%	0.000%
15	3.912	796	800	802	rBV2	784	647	0.00%	0.000%
16	4.041	837	840	843	rBV2	577	396	0.00%	0.000%
17	4.073	847	850	853	rBV	673	537	0.00%	0.000%
18	4.118	862	864	868	rVB2	634	381	0.00%	0.000%
19	4.179	880	883	887	rVB3	534	506	0.00%	0.000%
20	4.279	910	914	916	rVV2	471	370	0.00%	0.000%
21	4.317	921	926	930	rVB2	330	354	0.00%	0.000%
22	4.353	934	937	941	rBV3	421	372	0.00%	0.000%
23	4.456	964	969	971	rBV	529	399	0.00%	0.000%
24	4.472	971	974	976	rVB2	553	358	0.00%	0.000%
25	4.533	990	993	996	rVB3	597	433	0.00%	0.000%
26	4.555	996	1000	1003	rBV3	647	637	0.00%	0.000%
27	4.668	1017	1035	1036	rBV	288807	457944	0.24%	0.214%
28	4.912	1109	1111	1115	rVB3	615	354	0.00%	0.000%
29	4.951	1120	1123	1127	rBV2	977	603	0.00%	0.000%
30	5.102	1151	1170	1193	rBV	462888	1073546	0.56%	0.501%
31	5.321	1232	1238	1239	rBV3	1130	1081	0.00%	0.001%
32	5.401	1256	1263	1265	rBV4	1107	1185	0.00%	0.001%
33	5.440	1271	1275	1280	rVB4	917	821	0.00%	0.000%
34	5.600	1320	1325	1328	rBV3	718	644	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042920\
 Data File : VU037937.D
 Acq On : 30 Apr 2020 01:41
 Operator : JC/MD
 Sample : L2410-12
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBFF0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

35	5.758	1352	1374	1396	rBV2	1016878	2708559	1.41%	1.263%
36	5.944	1429	1432	1433	rBV3	764	379	0.00%	0.000%
37	5.970	1437	1440	1444	rVB5	978	701	0.00%	0.000%
38	6.279	1520	1536	1555	rVV	879717	1639862	0.86%	0.765%
39	6.497	1599	1604	1607	rBV5	745	767	0.00%	0.000%
40	6.571	1612	1627	1642	rBV2	506020	939788	0.49%	0.438%
41	6.723	1659	1674	1693	rBV	644619	1236428	0.65%	0.577%
42	6.838	1706	1710	1718	rVB7	2846	3175	0.00%	0.001%
43	7.076	1781	1784	1788	rVB	771	473	0.00%	0.000%
44	7.131	1791	1801	1812	rBV3	5494	8838	0.00%	0.004%
45	7.205	1817	1824	1833	rVB6	1823	3192	0.00%	0.001%
46	7.240	1833	1835	1838	rVB2	580	356	0.00%	0.000%
47	7.266	1838	1843	1847	rBV4	840	858	0.00%	0.000%
48	7.414	1886	1889	1894	rBV2	724	712	0.00%	0.000%
49	7.494	1910	1914	1917	rVB3	443	361	0.00%	0.000%
50	7.591	1928	1944	1962	rBV	365935	628394	0.33%	0.293%
51	7.694	1973	1976	1978	rBV2	788	614	0.00%	0.000%
52	7.771	1996	2000	2003	rBV4	583	528	0.00%	0.000%
53	7.864	2025	2029	2032	rVB3	349	336	0.00%	0.000%
54	7.922	2032	2047	2065	rBV	1300358	2244079	1.17%	1.047%
55	8.144	2113	2116	2118	rBV	534	347	0.00%	0.000%
56	8.202	2121	2134	2148	rVV	259997	423633	0.22%	0.198%
57	8.423	2197	2203	2211	rVB6	1792	2457	0.00%	0.001%
58	8.491	2214	2224	2232	rBV4	2316	3663	0.00%	0.002%
59	8.587	2234	2254	2268	rBV3	104469930	191636839	100.00%	89.388%
60	8.655	2269	2275	2309	rVB3	955126	2176959	1.14%	1.015%
61	9.436	2504	2518	2542	rBV	1281049	2095233	1.09%	0.977%
62	9.552	2547	2554	2560	rVV4	6257	8486	0.00%	0.004%
63	9.684	2592	2595	2596	rBV3	1077	554	0.00%	0.000%
64	10.034	2698	2704	2709	rBV4	656	707	0.00%	0.000%
65	10.115	2723	2729	2733	rBV3	1170	1361	0.00%	0.001%
66	10.362	2802	2806	2809	rBV3	892	669	0.00%	0.000%
67	10.439	2826	2830	2833	rBV4	494	488	0.00%	0.000%
68	10.771	2920	2933	2951	rBV	817077	1309490	0.68%	0.611%
69	10.899	2967	2973	2984	rBV7	2156	3350	0.00%	0.002%
70	11.054	3016	3021	3024	rBV4	782	825	0.00%	0.000%
71	11.070	3024	3026	3029	rVB2	945	577	0.00%	0.000%

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042920\
 Data File : VU037937.D
 Acq On : 30 Apr 2020 01:41
 Operator : JC/MD
 Sample : L2410-12
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBFF0

Integration Parameters: LSCINT.P

Integrator: RTE
 Smoothing : OFF
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 0 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis

72	11.102	3034	3036	3040	rBV3	526	360	0.00%	0.000%
73	11.198	3060	3066	3070	rBV4	474	584	0.00%	0.000%
74	11.336	3107	3109	3114	rVB3	802	731	0.00%	0.000%
75	11.484	3149	3155	3160	rVB5	1170	1666	0.00%	0.001%
76	11.536	3168	3171	3173	rBV	531	338	0.00%	0.000%
77	11.603	3188	3192	3198	rVB3	550	562	0.00%	0.000%
78	11.703	3219	3223	3227	rBV3	609	541	0.00%	0.000%
79	11.735	3229	3233	3234	rBV3	887	617	0.00%	0.000%
80	11.825	3248	3261	3283	rBV	1282647	2041344	1.07%	0.952%
81	11.954	3297	3301	3303	rBV2	595	393	0.00%	0.000%
82	12.031	3321	3325	3327	rBV2	509	415	0.00%	0.000%
83	12.076	3331	3339	3348	rBV5	7415	12981	0.01%	0.006%
84	12.205	3366	3379	3399	rVB	1250895	1982152	1.03%	0.925%
85	12.336	3414	3420	3421	rBV4	704	661	0.00%	0.000%
86	12.529	3477	3480	3485	rVB2	700	542	0.00%	0.000%
87	12.590	3496	3499	3502	rBV2	522	424	0.00%	0.000%
88	12.751	3544	3549	3553	rBV2	527	546	0.00%	0.000%
89	12.796	3559	3563	3569	rVV3	1600	1503	0.00%	0.001%
90	12.902	3593	3596	3600	rBV2	650	554	0.00%	0.000%
91	12.996	3624	3625	3630	rBV	494	372	0.00%	0.000%
92	13.140	3668	3670	3674	rBV2	495	374	0.00%	0.000%
93	13.291	3713	3717	3718	rBV2	542	419	0.00%	0.000%
94	13.362	3737	3739	3741	rBV2	594	343	0.00%	0.000%
95	13.864	3890	3895	3903	rVB3	2421	3054	0.00%	0.001%
96	14.333	4039	4041	4044	rBV3	877	519	0.00%	0.000%
97	14.352	4044	4047	4049	rBV2	922	630	0.00%	0.000%
98	14.610	4125	4127	4130	rBV2	773	538	0.00%	0.000%
99	14.770	4175	4177	4181	rVB2	1053	585	0.00%	0.000%
100	14.828	4193	4195	4197	rBV3	686	380	0.00%	0.000%




Sum of corrected areas: 214388594

Data Path : Z:\VOASRV\HPCHEM1\MSVOA U\DATA\VU042920\
Data File : VU037937.D
Acq On : 30 Apr 2020 01:41
Operator : JC/MD
Sample : L2410-12
Misc : 5.0mL/MSVOA U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBFF0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

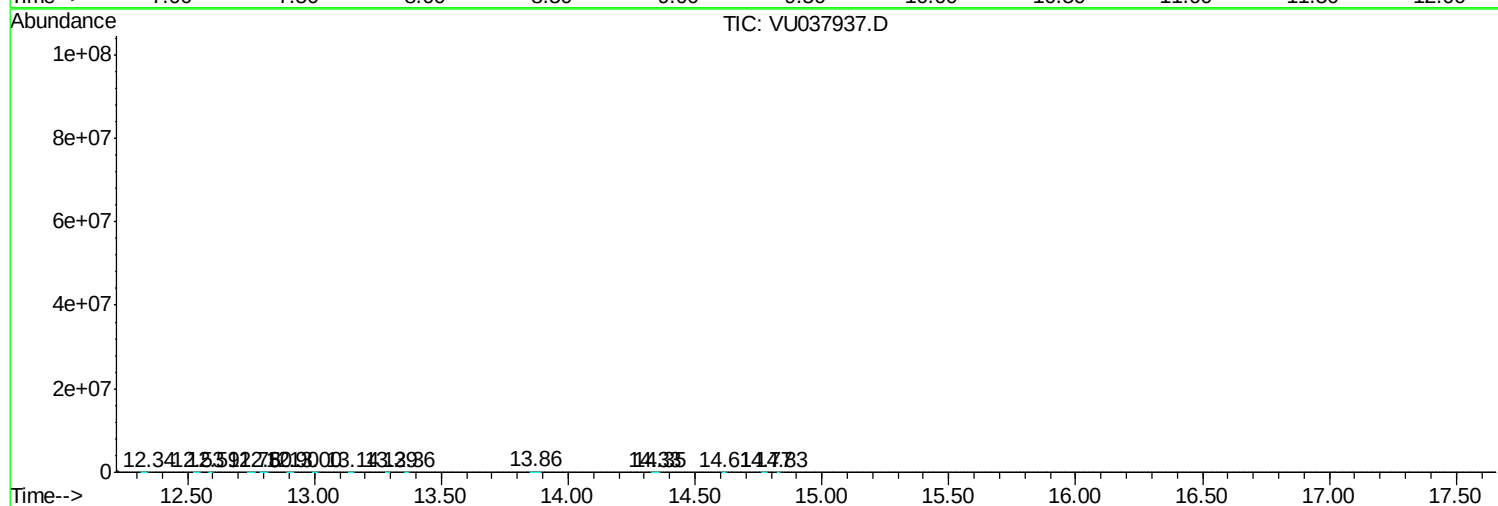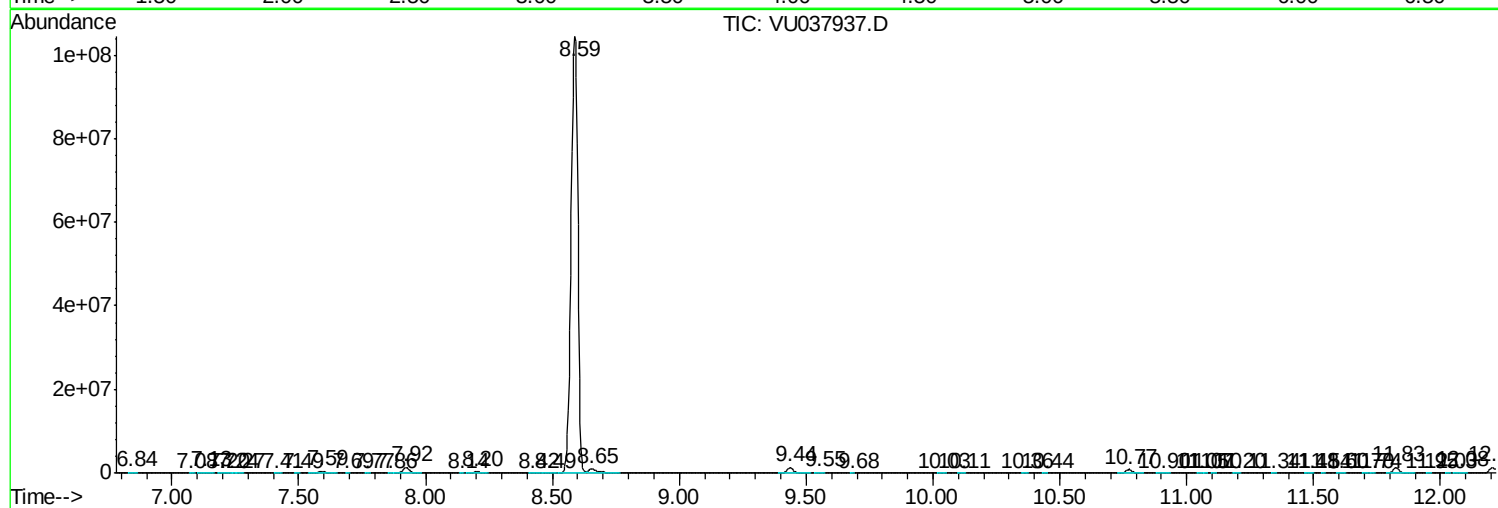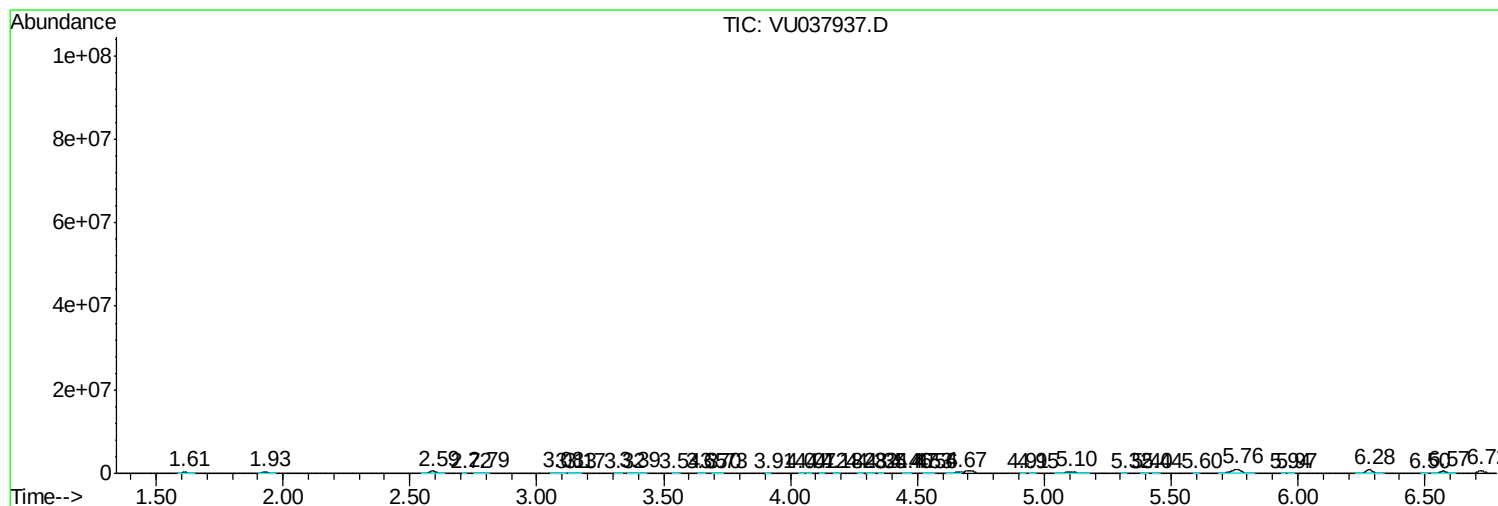

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_U\DATA\VU042920\
Data File : VU037937.D
Acq On : 30 Apr 2020 01:41
Operator : JC/MD
Sample : L2410-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBFF0

Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_U\DATA\VU042920\
Data File : VU037937.D
Acq On : 30 Apr 2020 01:41
Operator : JC/MD
Sample : L2410-12
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBFF0

Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc