


Data Path : Z:\voasrv\HPCHEM1\MSVOA U\Data\VU042920\
 Data File : VU037901.D
 Acq On : 29 Apr 2020 08:35
 Operator : JC/MD
 Sample : BFB44
 Misc : 5.0mL/MSVOA U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB44

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_U\METHOD\SOMULM042320WMA.M
 Title : VOC Analysis
 Last Update : Thu Apr 30 04:10:11 2020

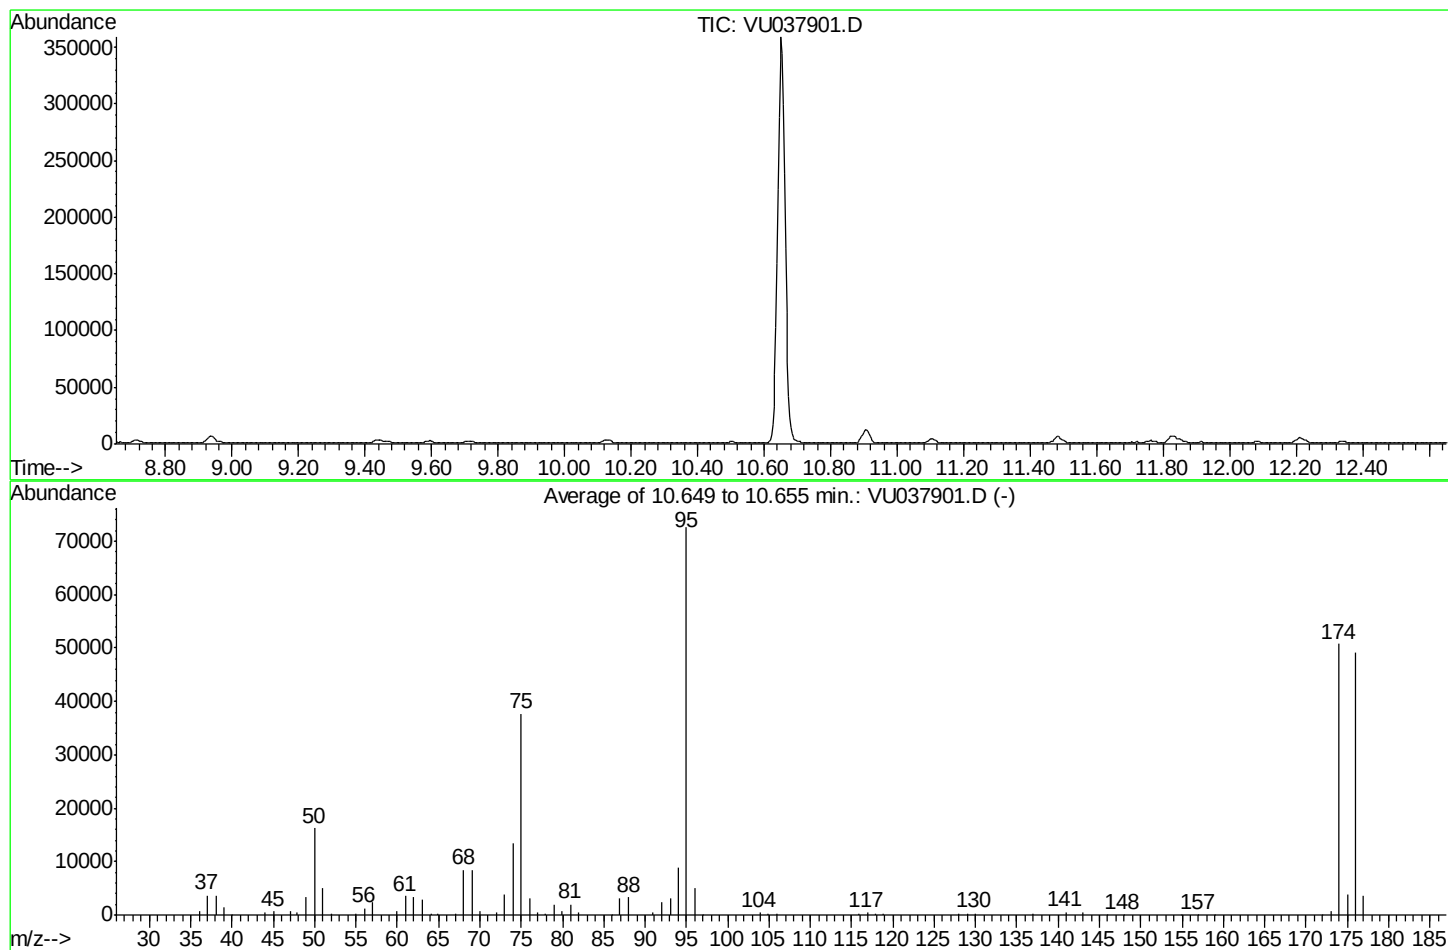

AutoFind: Scans 2895, 2896, 2897; Background Corrected with Scan 2883

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	22.4	16277	PASS
75	95	30	80	52.0	37765	PASS
95	95	100	100	100.0	72616	PASS
96	95	5	9	7.0	5062	PASS
173	174	0.00	2	1.3	659	PASS
174	95	50	120	69.9	50773	PASS
175	174	5	9	7.7	3896	PASS
176	174	95	101	96.8	49146	PASS
177	176	5	9	7.6	3720	PASS

m/z	Abundance
36.00	574.0
37.00	3556.0
38.10	3369.0
39.00	1451.0
40.00	257.0
44.00	1604.0
45.00	654.0
47.10	830.0
47.90	513.0
49.00	3290.0
50.00	16480.0
51.00	5114.0
52.00	294.0
54.90	351.0
56.00	1239.0
57.00	2370.0
60.00	750.0
61.00	3573.0
62.00	3485.0
63.00	2830.0
64.10	276.0
64.90	220.0
67.00	271.0
68.00	8280.0
69.00	8223.0
70.00	684.0
72.00	421.0
73.00	3662.0
74.00	13389.0
75.00	37544.0
76.00	3226.0
77.00	450.0
77.90	298.0
78.90	1982.0
79.90	703.0
81.00	1911.0
81.90	443.0
85.90	100.0
87.00	2803.0
88.00	3191.0
90.90	360.0
92.00	2043.0
93.00	2956.0
94.10	8703.0
95.00	71448.0
96.00	5165.0
97.00	107.0
103.90	423.0
104.90	150.0
106.00	220.0
115.90	317.0
116.90	443.0
117.90	259.0
118.80	288.0
128.00	191.0
129.00	137.0
129.90	268.0
136.90	108.0
140.90	509.0
143.00	442.0
147.90	116.0
171.90	117.0
173.10	669.0
174.00	48016.0
175.00	3709.0
176.00	46792.0
177.00	3808.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.00	626.0
37.00	3851.0
38.10	3605.0
39.00	1498.0
39.90	303.0
44.00	1510.0
45.00	737.0
47.00	793.0
47.90	574.0
49.00	3551.0
50.00	16920.0
51.00	5186.0
52.00	215.0
55.00	340.0
56.00	1355.0
57.00	2497.0
60.00	811.0
61.00	3637.0
62.00	3482.0
63.00	2940.0
64.10	338.0
65.00	208.0
67.00	259.0
68.00	8689.0
69.10	8567.0
70.00	700.0
72.00	491.0
73.00	4034.0
74.00	14024.0
75.00	38984.0
76.00	3317.0
77.00	551.0
78.00	330.0
79.00	1987.0
79.90	748.0
81.00	2095.0
81.90	473.0
85.90	106.0
86.90	3177.0
88.00	3535.0
90.90	438.0
92.00	2472.0
93.10	3266.0
94.00	9202.0
95.00	74904.0
96.00	5248.0
97.00	103.0
103.90	439.0
104.90	143.0
105.90	261.0
115.80	304.0
116.90	425.0
117.90	242.0
118.90	295.0
128.00	194.0
129.00	158.0
129.90	289.0
136.90	146.0
141.00	562.0
142.90	554.0
147.90	105.0
154.90	126.0
157.00	134.0
158.90	111.0
172.00	115.0
173.10	679.0
174.00	52360.0
175.00	4046.0
176.00	50800.0
177.00	3879.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

m/z	Abundance
36.00	640.0
37.00	3666.0
38.00	3575.0
39.00	1387.0
39.90	354.0
44.00	1426.0
45.00	675.0
47.00	780.0
47.90	563.0
49.00	3519.0
50.00	15431.0
51.00	4641.0
52.00	180.0
55.00	289.0
56.00	1340.0
57.00	2363.0
60.00	717.0
61.00	3423.0
62.00	3181.0
63.10	2745.0
64.00	392.0
65.00	187.0
67.00	267.0
68.00	8222.0
69.00	8064.0
70.00	639.0
72.00	389.0
73.00	4040.0
74.00	13141.0
75.00	36768.0
76.10	3152.0
76.90	574.0
77.90	326.0
79.00	1893.0
79.90	717.0
81.00	2064.0
81.90	494.0
85.90	125.0
87.00	3148.0
88.00	3350.0
91.00	393.0
92.00	2501.0
93.10	3198.0
94.00	8609.0
95.00	71496.0
96.00	4775.0
96.90	145.0
103.90	348.0
104.90	150.0
105.90	267.0
115.90	262.0
117.00	449.0
117.90	180.0
118.90	279.0
127.90	227.0
129.00	136.0
129.90	276.0
136.90	150.0
141.00	608.0
142.90	590.0
145.90	115.0
154.90	140.0
157.00	136.0
158.90	150.0
173.10	630.0
174.00	51944.0
175.00	3933.0
176.00	49848.0
177.00	3474.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44

Scan 2883 (10.610 min): VU037901.D
BFB44

m/z	Abundance
40.00	246.0
43.90	944.0

Instrument :
MSVOA_U
ClientSampleId :
BFB44